

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 23:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 00:47:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	13143205	34088816	22.362	21.519
28)	SA Decachlor...	11.640	10.387	12232390	29133198	22.814	21.230
Target Compounds							
7)	B delta-BHC	0.000	6.414	0	399165	N.D.	0.186 #
8)	B Heptachlo...	8.125	0.000	3107632	0	4.552	N.D. #
9)	A Endosulfan I	0.000	7.446f	0	107604	N.D.	0.064 #
11)	B alpha-Chl...	0.000	7.398f	0	213717	N.D.	0.117 #
13)	MA Dieldrin	0.000	7.754	0	2941220	N.D.	1.695 #
14)	MA Endrin	0.000	8.070f	0	987982	N.D.	0.635 #
15)	B Endosulfa...	9.306	0.000	101977	0	0.181	N.D. #
21)	B Endrin ke...	10.187f	0.000	513252	0	0.836	N.D. #
26)	Chlordane-4	0.000	7.398f	0	213717	N.D.	1.131 #
27)	Chlordane-5	0.000	8.161f	0	4406955	N.D.	88.314 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 23:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 00:47:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

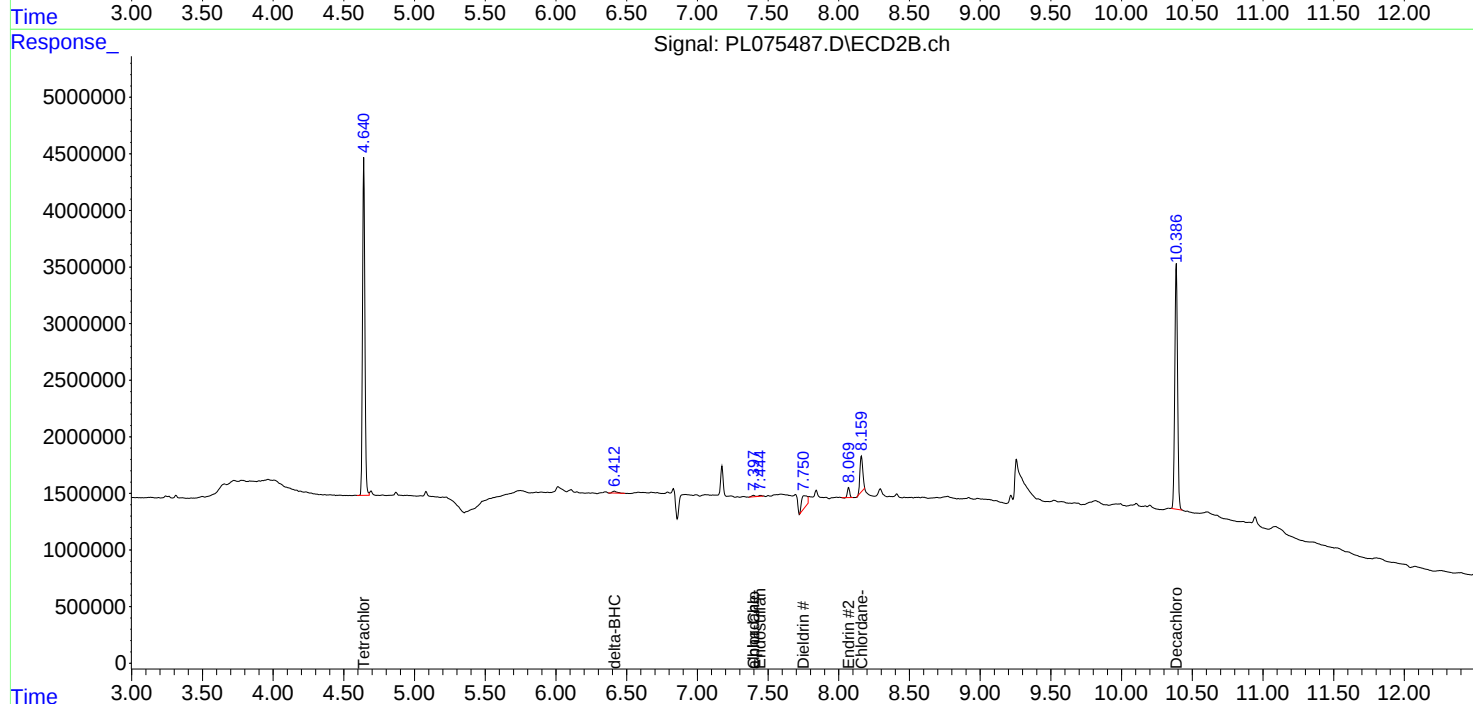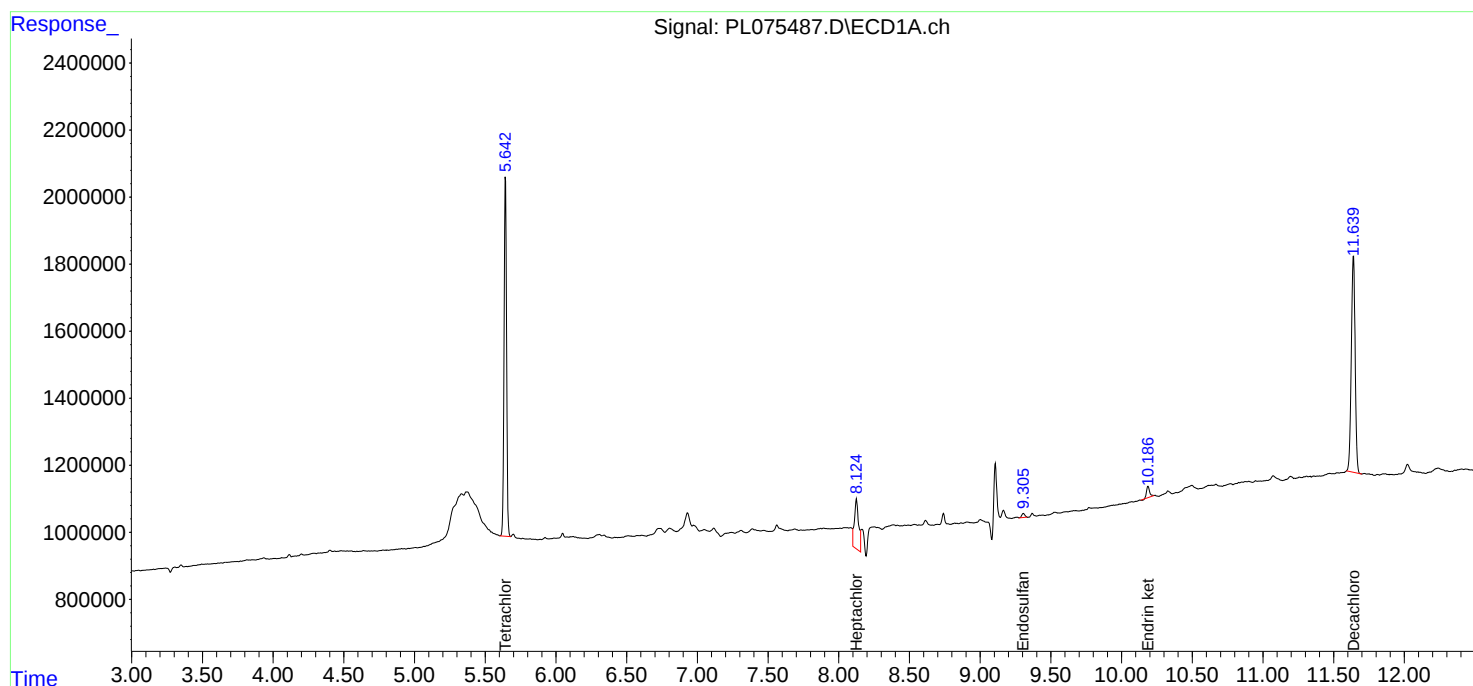


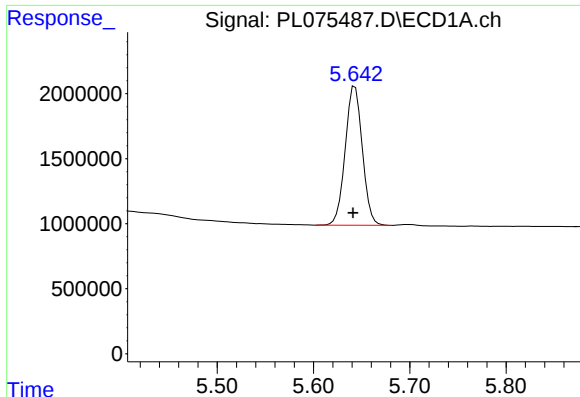

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 13143205
Conc: 22.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

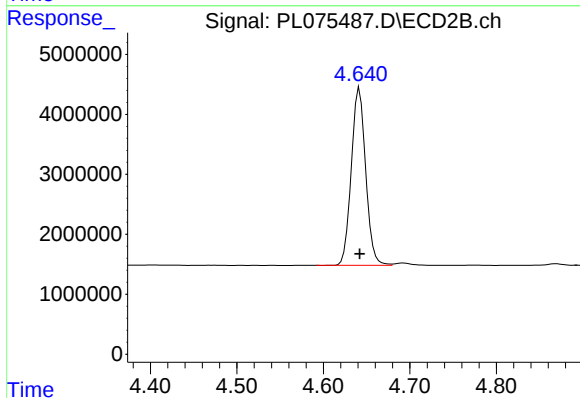


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 34088816
Conc: 21.52 ng/ml

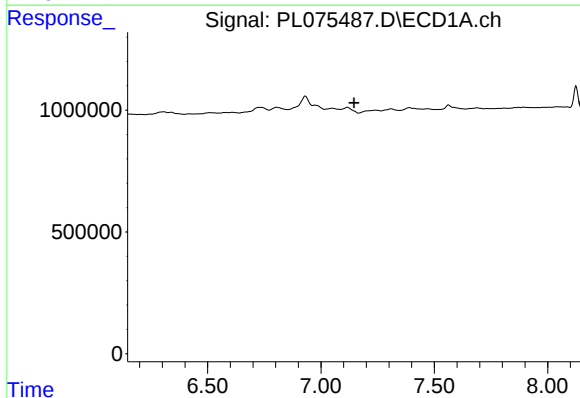


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

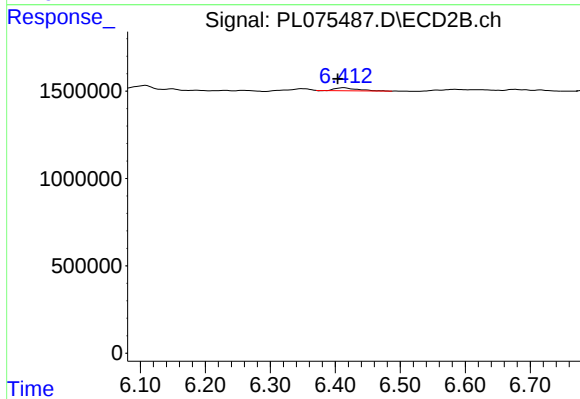

#7 delta-BHC


R.T.: 6.414 min
Delta R.T.: 0.010 min
Response: 399165
Conc: 0.19 ng/ml

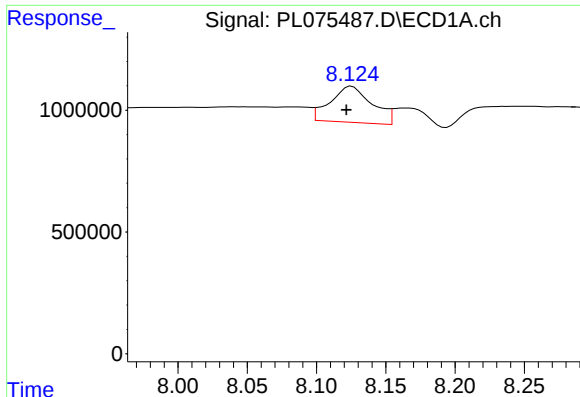

#8 Heptachlor epoxide


R.T.: 8.125 min
Delta R.T.: 0.004 min
Response: 3107632
Conc: 4.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

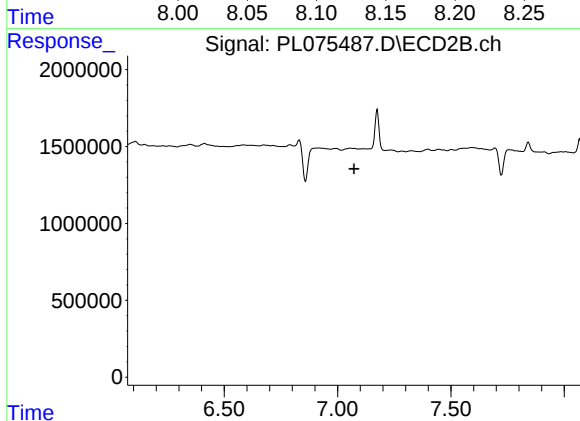


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

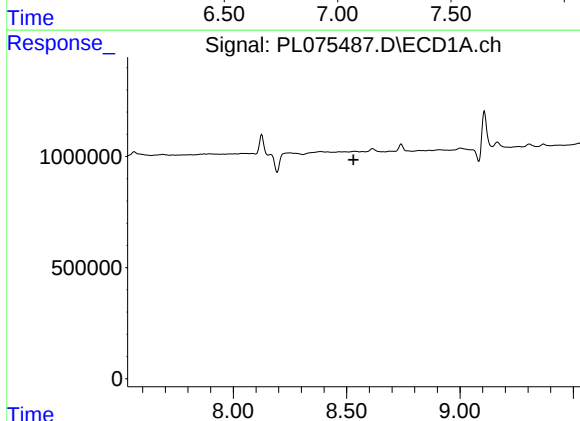


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

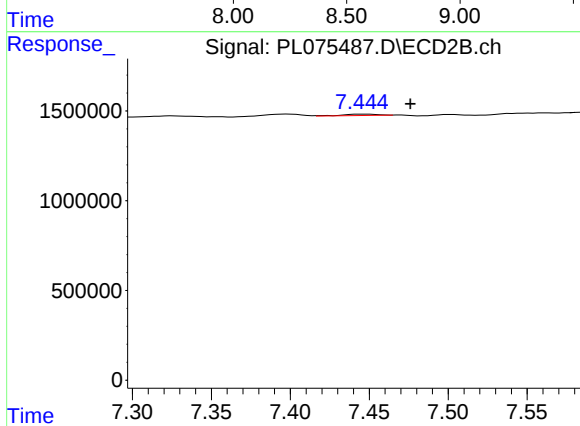

#9 Endosulfan I


R.T.: 7.446 min
Delta R.T.: -0.030 min
Response: 107604
Conc: 0.06 ng/ml

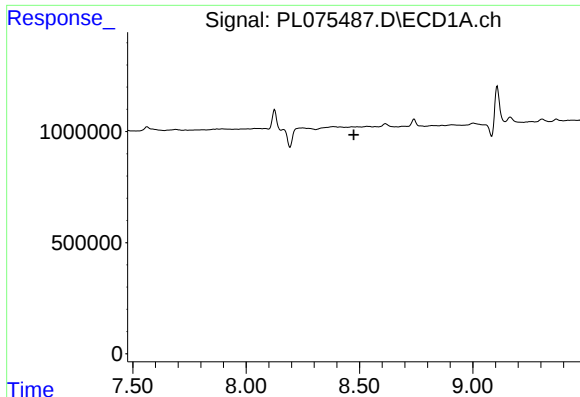

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

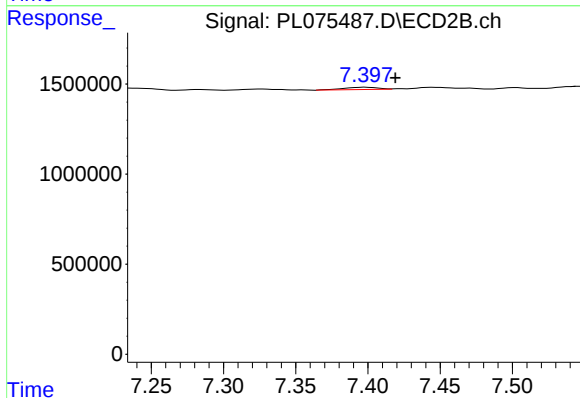


#11 alpha-Chlordane

R.T.: 7.398 min
Delta R.T.: -0.021 min
Response: 213717
Conc: 0.12 ng/ml

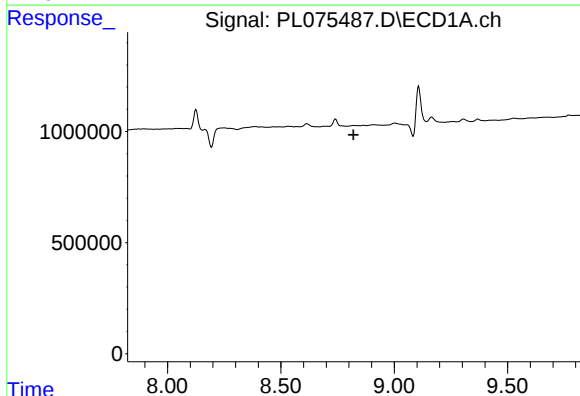


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

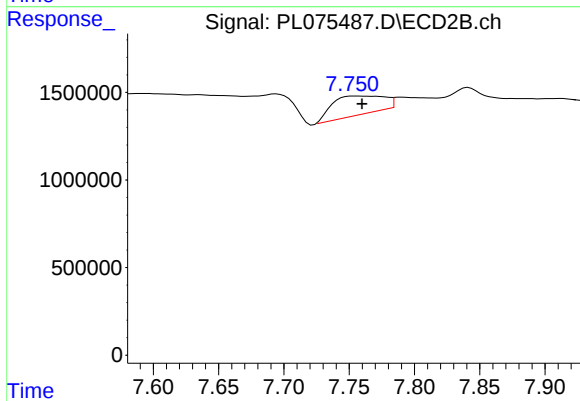

#13 Dieldrin


R.T.: 7.754 min
Delta R.T.: -0.006 min
Response: 2941220
Conc: 1.70 ng/ml

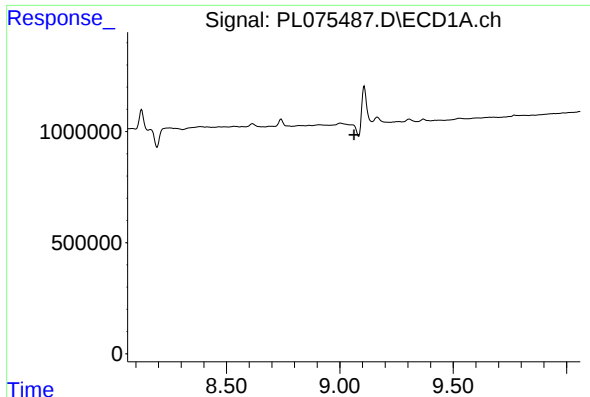

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

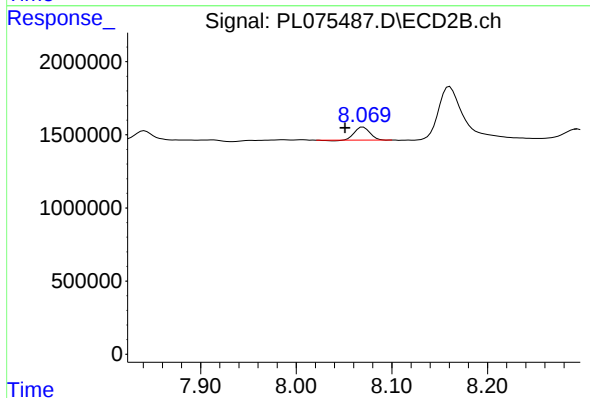


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 987982
Conc: 0.63 ng/ml

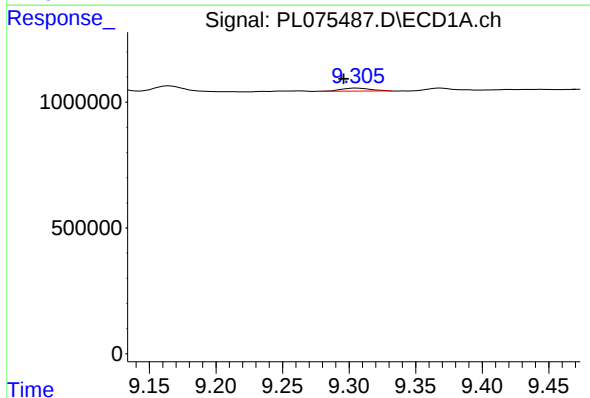


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 101977
Conc: 0.18 ng/ml

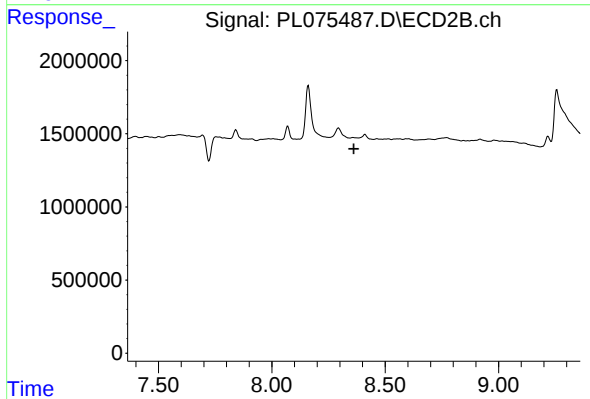

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

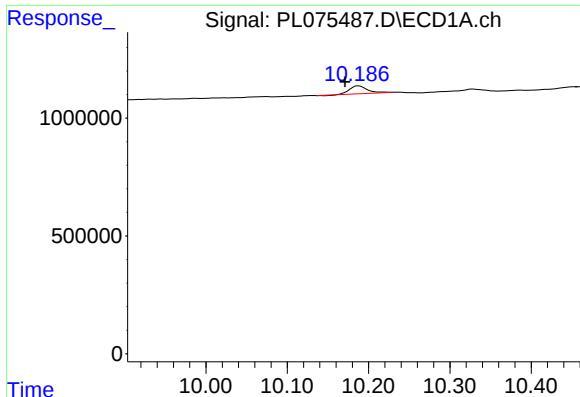

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 513252
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

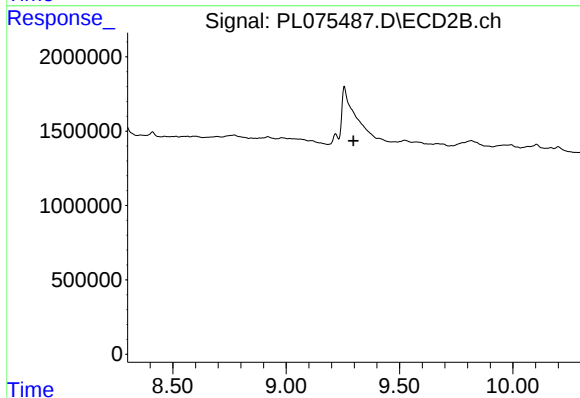


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.297 min
Response: 0
Conc: N.D.

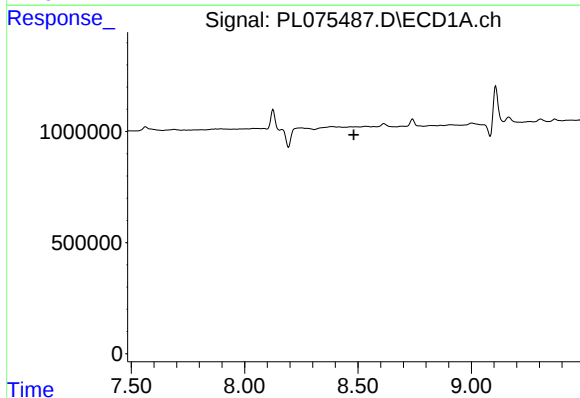


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

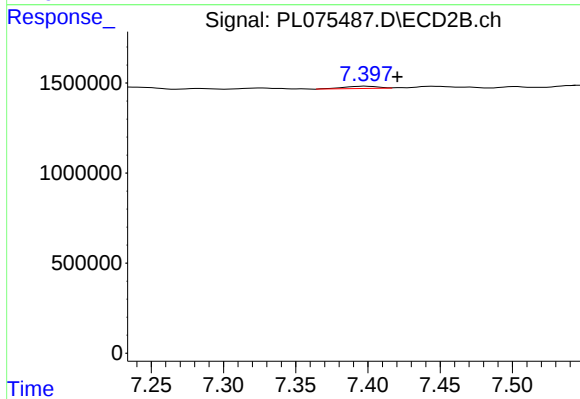

#26 Chlordane-4


R.T.: 7.398 min
Delta R.T.: -0.022 min
Response: 213717
Conc: 1.13 ng/ml

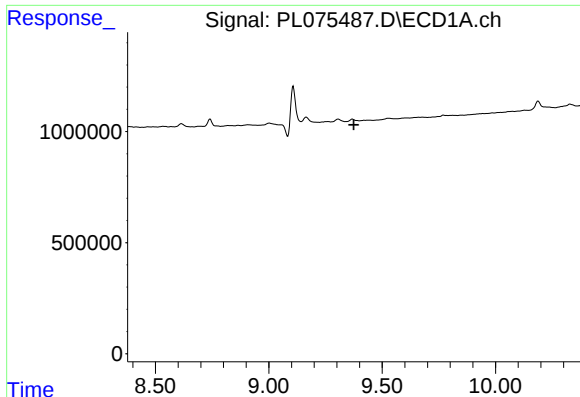

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

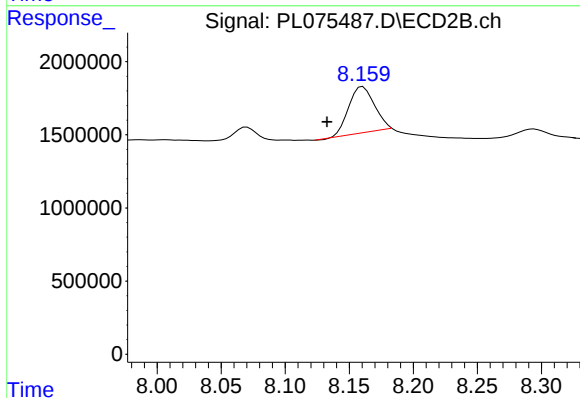


#27 Chlordane-5

R.T.: 8.161 min
Delta R.T.: 0.028 min
Response: 4406955
Conc: 88.31 ng/ml

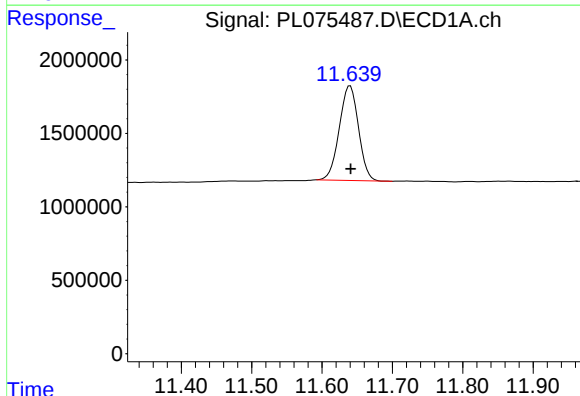

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 12232390
Conc: 22.81 ng/ml

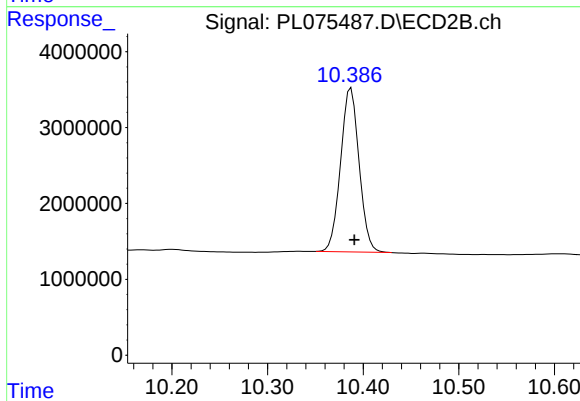

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 29133198
Conc: 21.23 ng/ml