

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2022 01:45
 Operator : AR\AJ
 Sample : PB145241BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 05:15:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	11865192	30259909	20.188	19.102
28)	SA Decachlor...	11.640	10.387	11142530	25592729	20.781	18.650
Target Compounds							
7)	B delta-BHC	0.000	6.409	0	358836	N.D.	0.167 #
11)	B alpha-Chl...	0.000	7.396f	0	209586	N.D.	0.115 #
14)	MA Endrin	0.000	8.071f	0	228609	N.D.	0.147 #
15)	B Endosulfa...	9.305	0.000	194097	0	0.344	N.D. #
17)	MA 4,4'-DDT	9.497f	0.000	77137	0	0.132	N.D. #
18)	B Endrin al...	0.000	8.573f	0	259763	N.D.	0.215 #
21)	B Endrin ke...	10.188f	0.000	355846	0	0.580	N.D. #
26)	Chlordane-4	0.000	7.396f	0	209586	N.D.	1.109 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2022 01:45
Operator : AR\AJ
Sample : PB145241BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 05:15:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

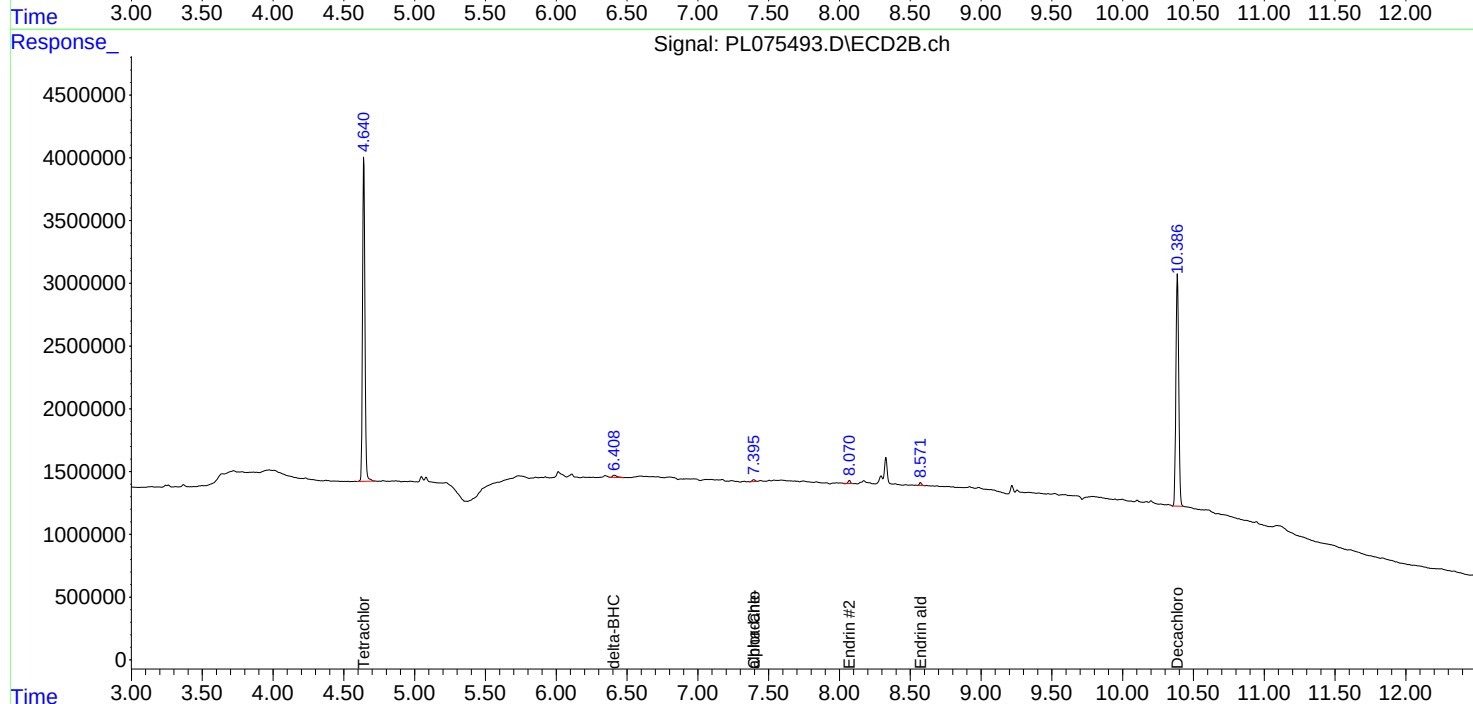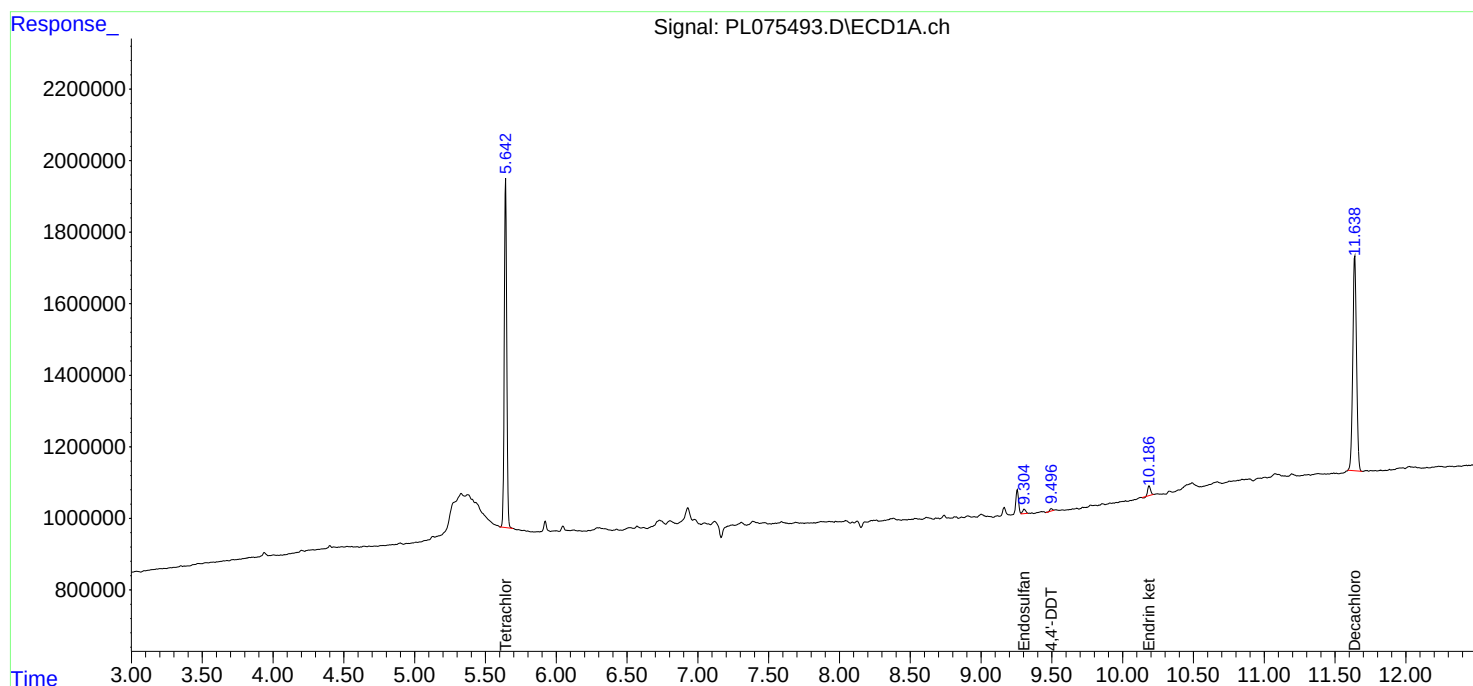


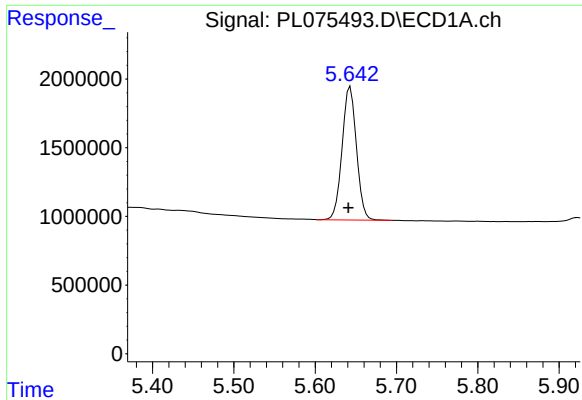

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11865192
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

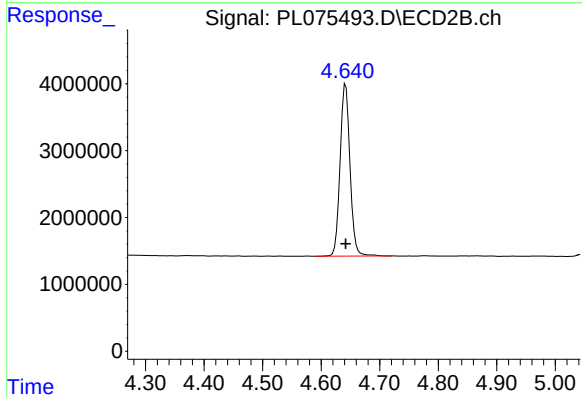


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 30259909
Conc: 19.10 ng/ml

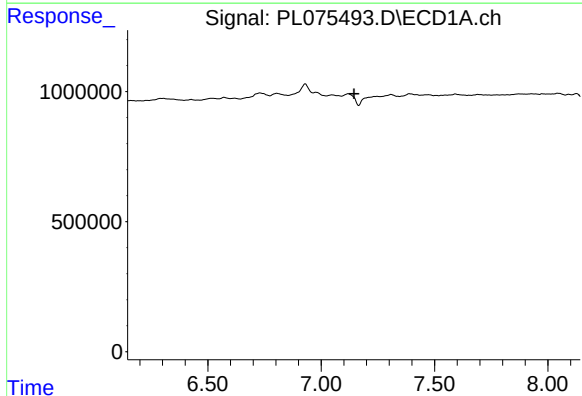


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

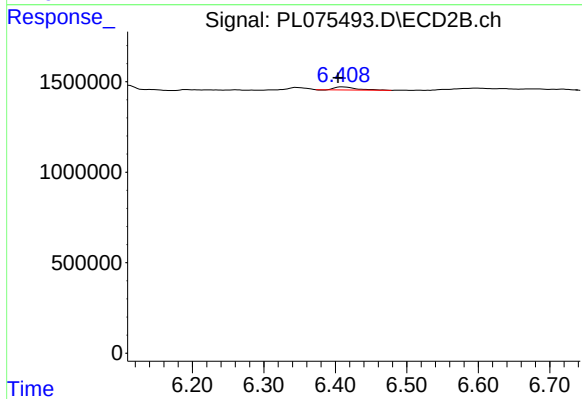

#7 delta-BHC


R.T.: 6.409 min
Delta R.T.: 0.005 min
Response: 358836
Conc: 0.17 ng/ml

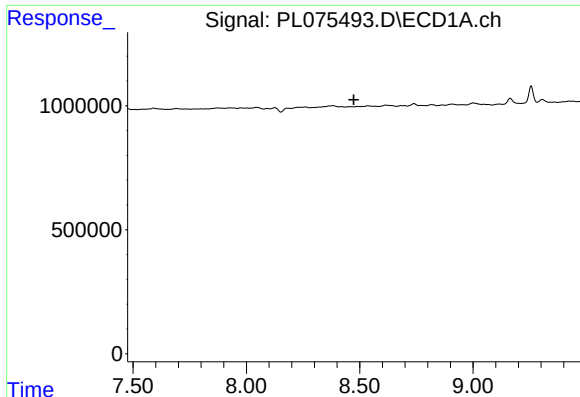

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

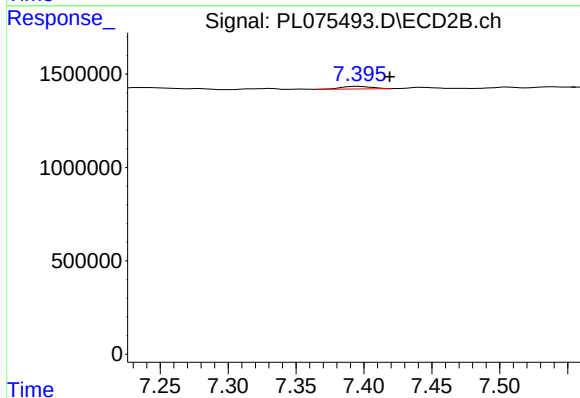


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.023 min
Response: 209586
Conc: 0.11 ng/ml

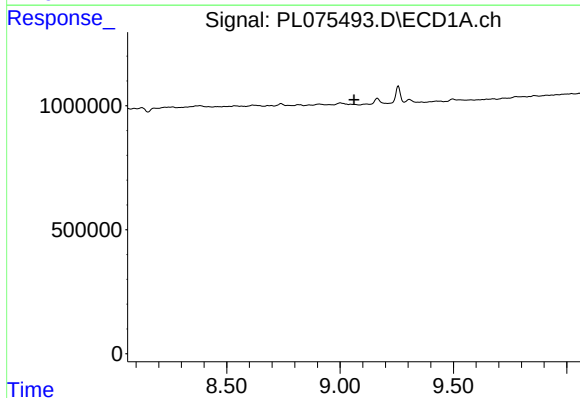


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

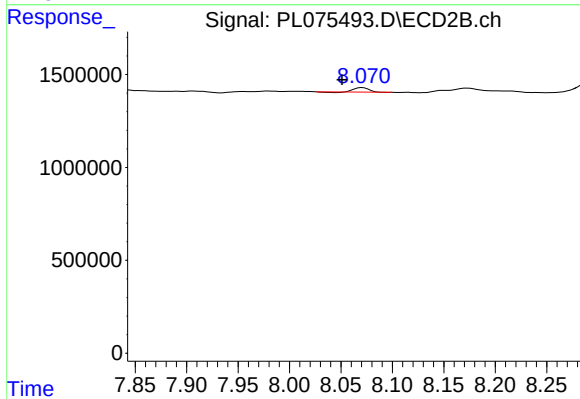

#14 Endrin


R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 228609
Conc: 0.15 ng/ml

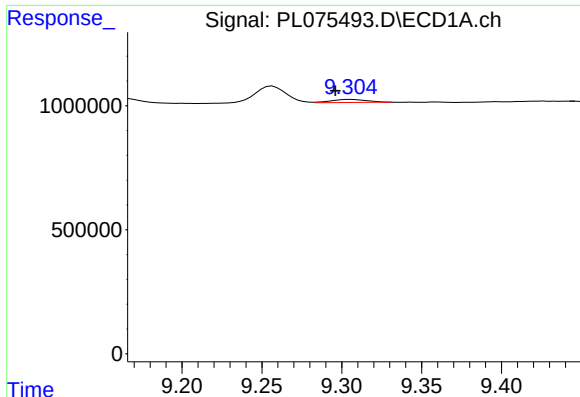

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 194097
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

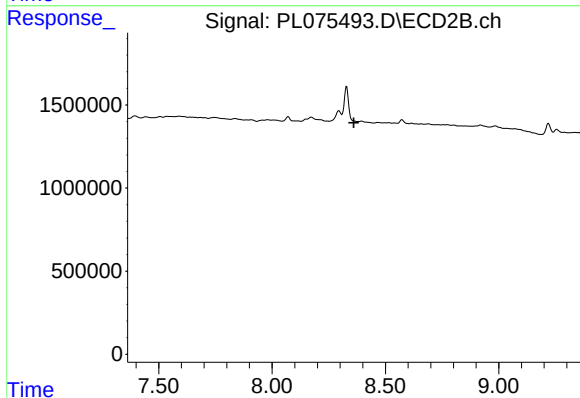


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

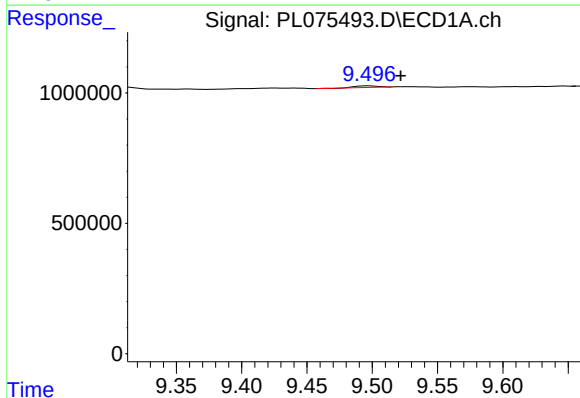


#17 4,4'-DDT

R.T.: 9.497 min
Delta R.T.: -0.025 min
Response: 77137
Conc: 0.13 ng/ml

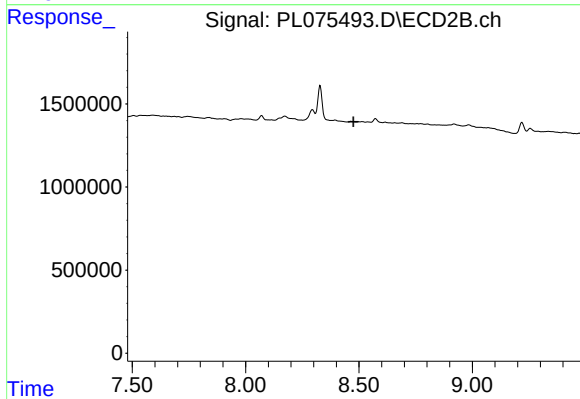

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

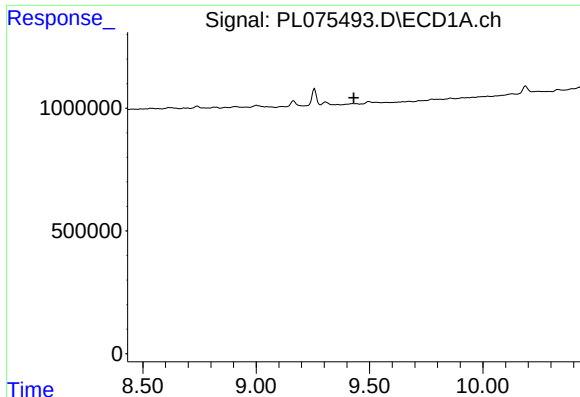

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

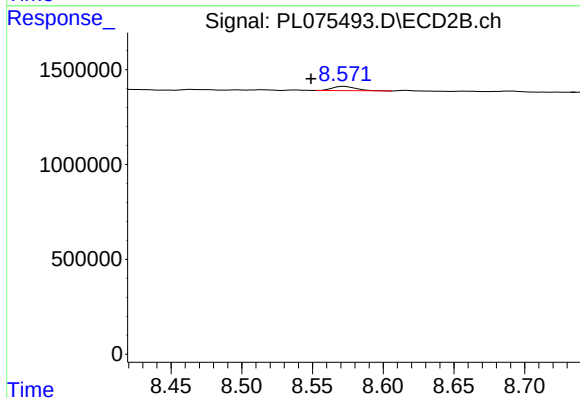


#18 Endrin aldehyde

R.T.: 8.573 min
Delta R.T.: 0.024 min
Response: 259763
Conc: 0.22 ng/ml

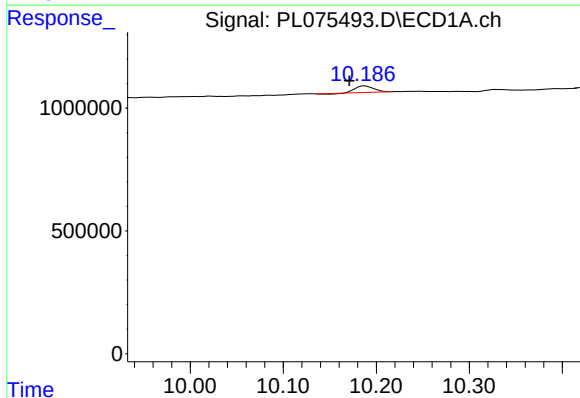


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.016 min
Response: 355846
Conc: 0.58 ng/ml

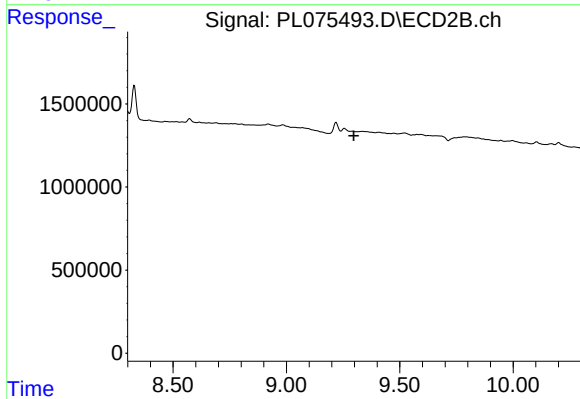

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.297 min
Response: 0
Conc: N.D.

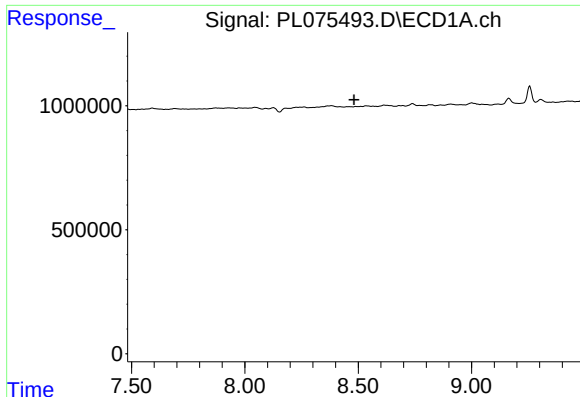

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

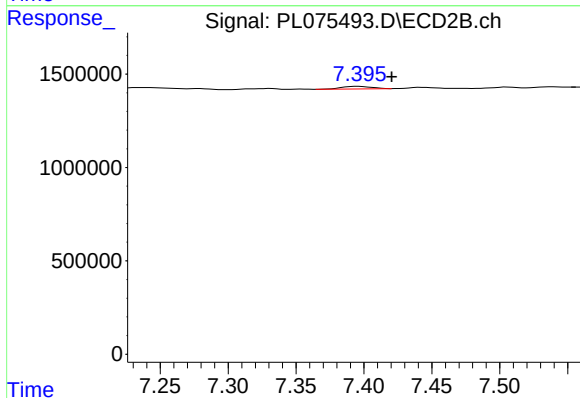


#26 Chlordane-4

R.T.: 7.396 min
Delta R.T.: -0.024 min
Response: 209586
Conc: 1.11 ng/ml

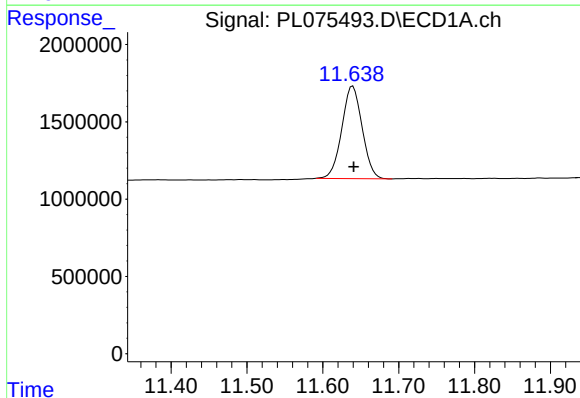

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 11142530
Conc: 20.78 ng/ml

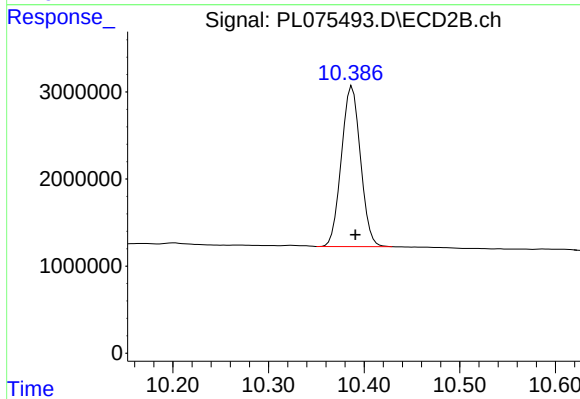

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 25592729
Conc: 18.65 ng/ml