

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
 Data File : PL075452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 12:48
 Operator : AR\AJ
 Sample : N3099-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20220426-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:53:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	9328347	24307934	15.872	15.345
28)	SA Decachlor...	11.639	10.386	4705952	11586901	8.777	8.444
Target Compounds							
12)	B 4,4'-DDE	8.658	7.627	402797	1126865	0.692	0.692



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060322\
Data File : PL075452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 12:48
Operator : AR\AJ
Sample : N3099-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20220426-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:53:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

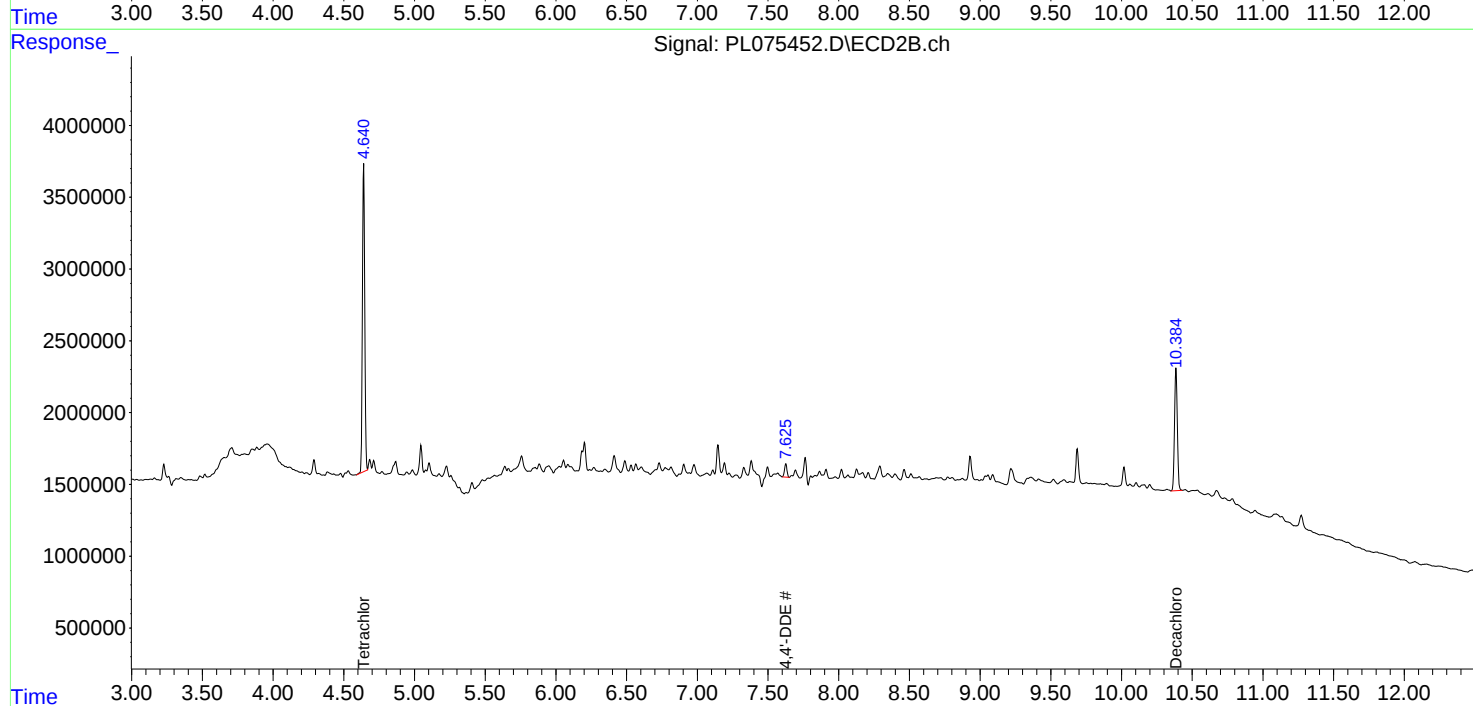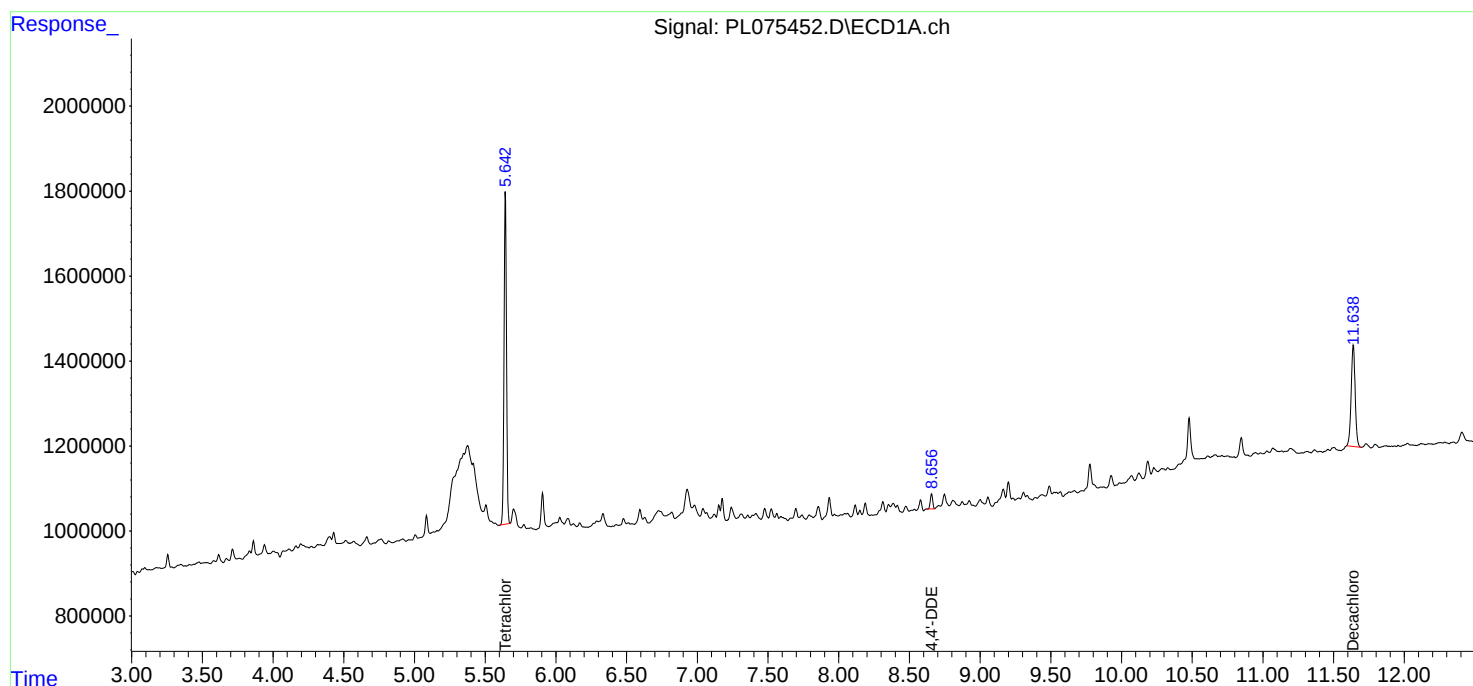


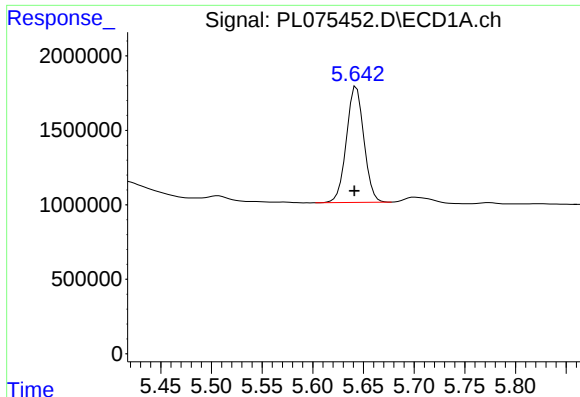

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 9328347
Conc: 15.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220426-AMENDED-COMPOSITE-F

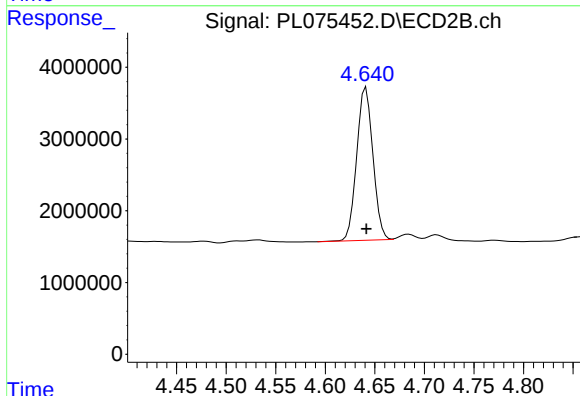


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 24307934
Conc: 15.34 ng/ml

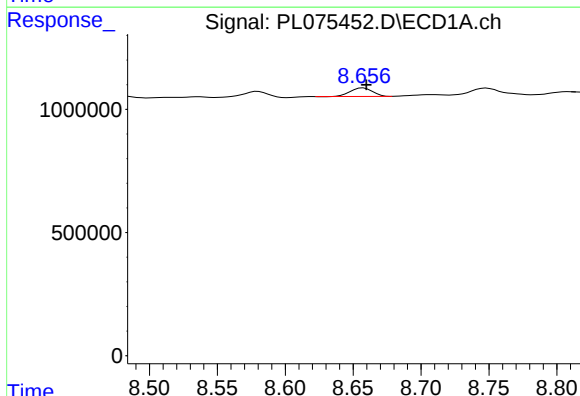


#12 4,4'-DDE

R.T.: 8.658 min
Delta R.T.: -0.002 min
Response: 402797
Conc: 0.69 ng/ml

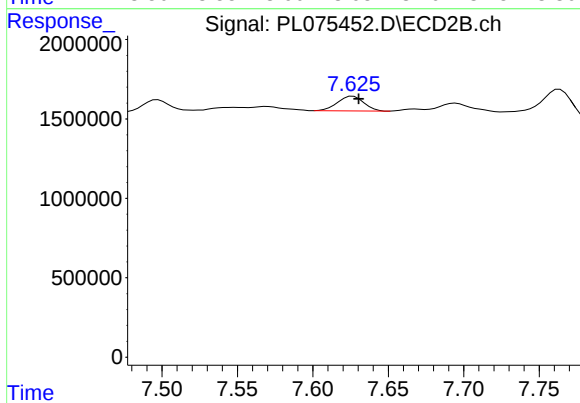

#12 4,4'-DDE


R.T.: 7.627 min
Delta R.T.: -0.004 min
Response: 1126865
Conc: 0.69 ng/ml

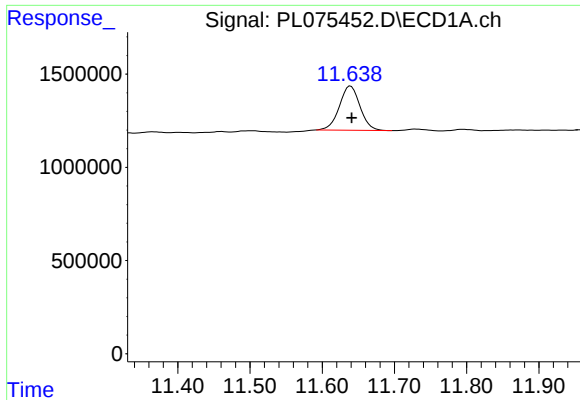

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 4705952
Conc: 8.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
20220426-AMENDED-COMPOSITE-F

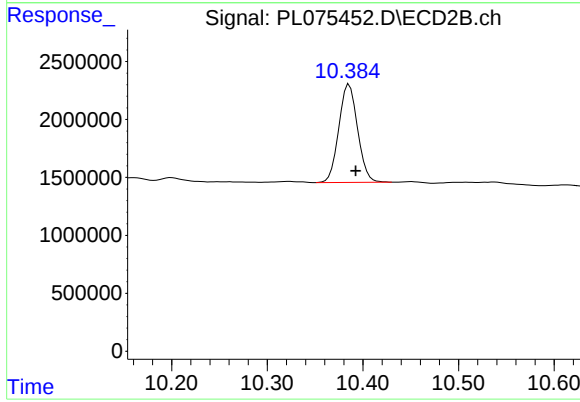

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.007 min
Response: 11586901
Conc: 8.44 ng/ml