

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
 Data File : PL075594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 01:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:54:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.639	12677189	30788939	18.784	18.346
28)	SA Decachlor...	11.635	10.383	12234280	27975233	19.983	19.855
Target Compounds							
7)	B delta-BHC	0.000	6.407	0	400170	N.D.	0.187 #
8)	B Heptachlo...	8.124	0.000	844745	0	1.093	N.D. #
9)	A Endosulfan I	8.533	0.000	273418	0	0.391	N.D. #
10)	B gamma-Chl...	8.383	0.000	1175130	0	1.513	N.D. #
13)	MA Dieldrin	0.000	7.754	0	463420	N.D.	0.274 #
14)	MA Endrin	0.000	8.067f	0	438259	N.D.	0.321 #
15)	B Endosulfa...	9.302	0.000	228355	0	0.367	N.D. #
21)	B Endrin ke...	10.184f	0.000	573901	0	0.816	N.D. #
25)	Chlordane-3	8.383	0.000	1175130	0	11.381	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
Data File : PL075594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 01:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:54:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

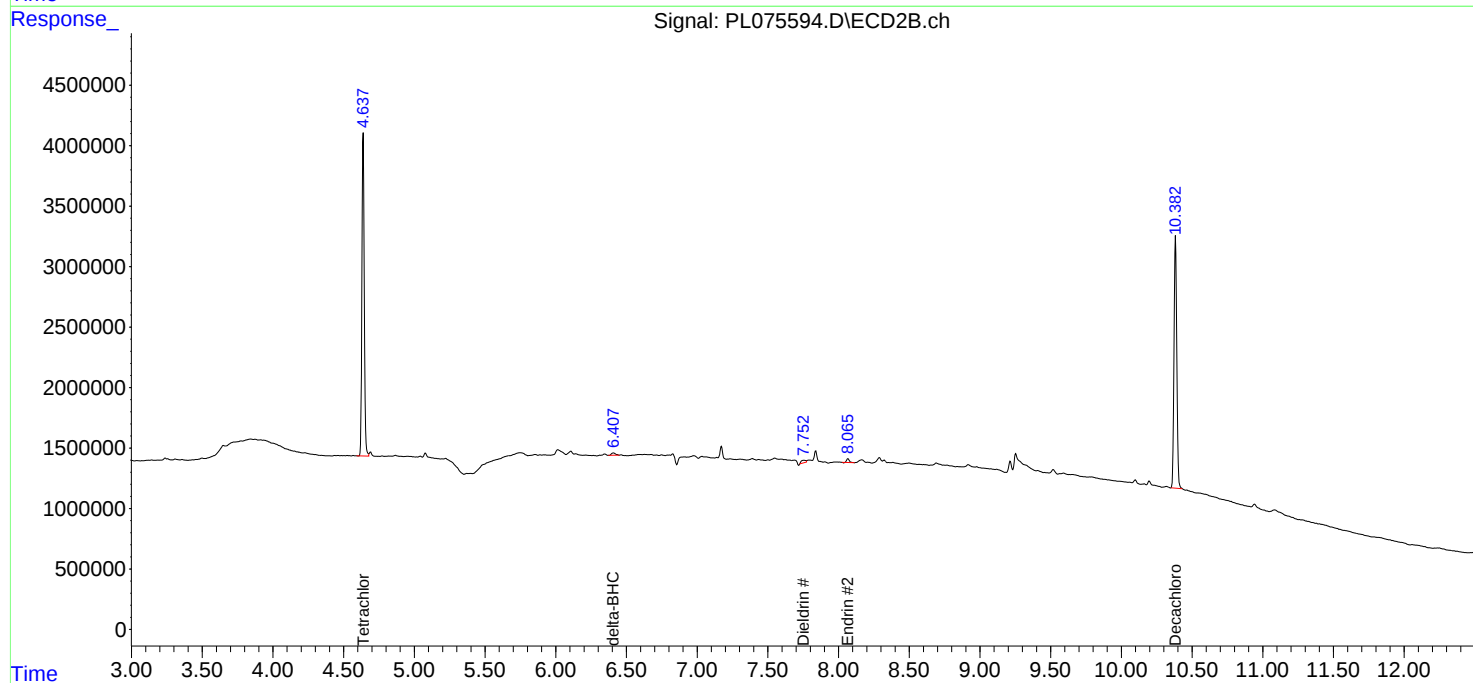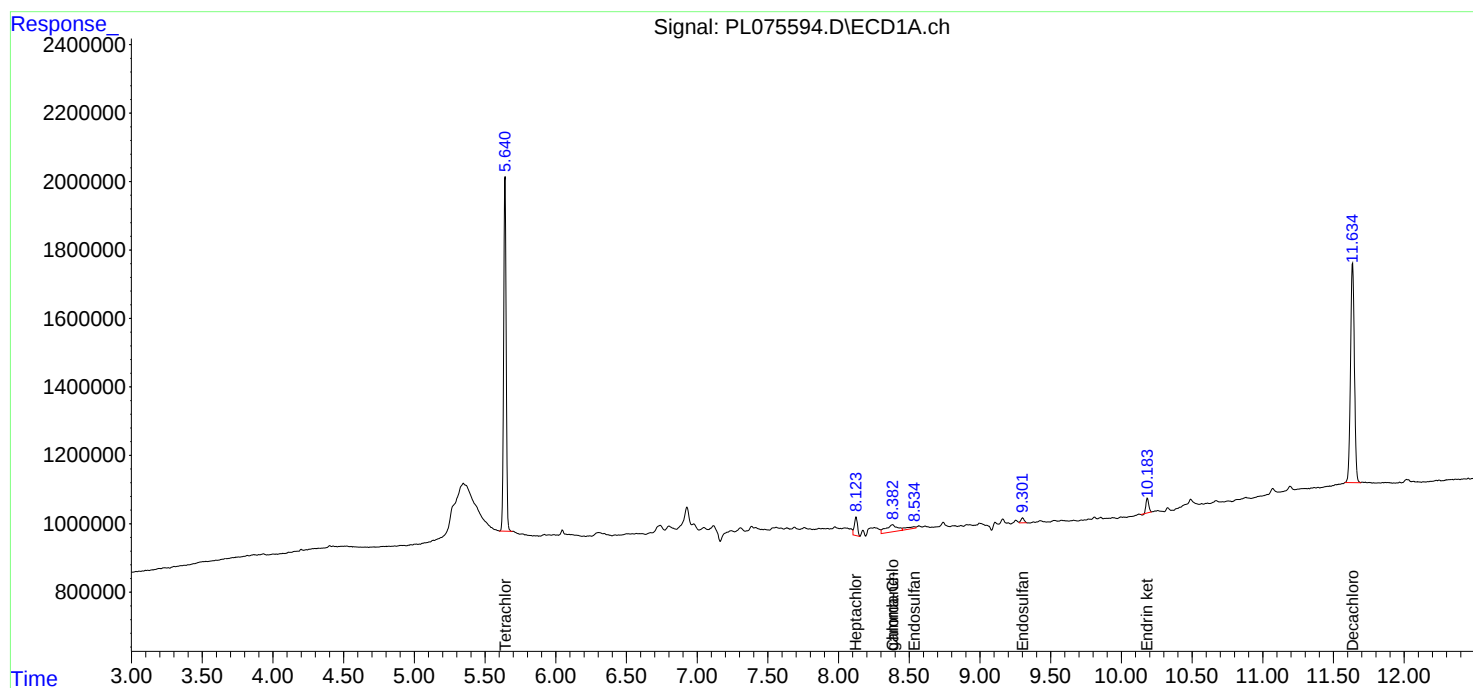


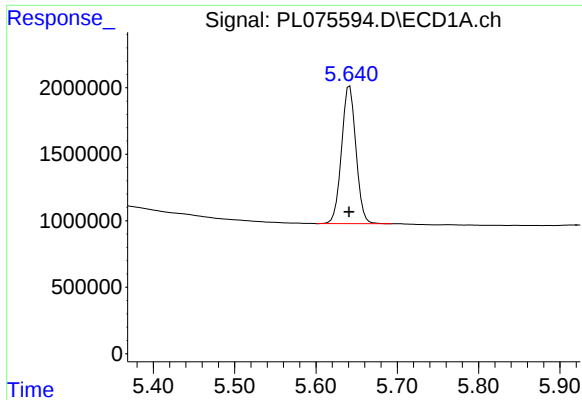

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 12677189
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

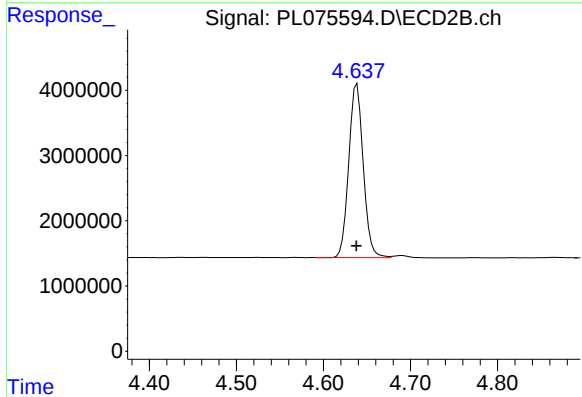


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 30788939
Conc: 18.35 ng/ml

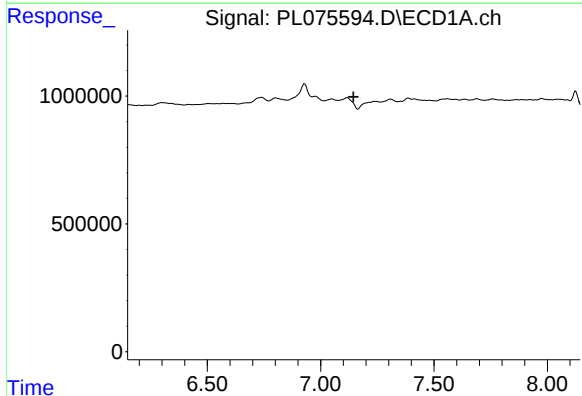


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

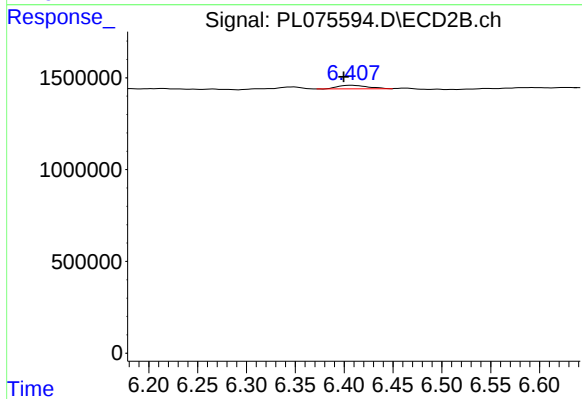

#7 delta-BHC


R.T.: 6.407 min
Delta R.T.: 0.008 min
Response: 400170
Conc: 0.19 ng/ml

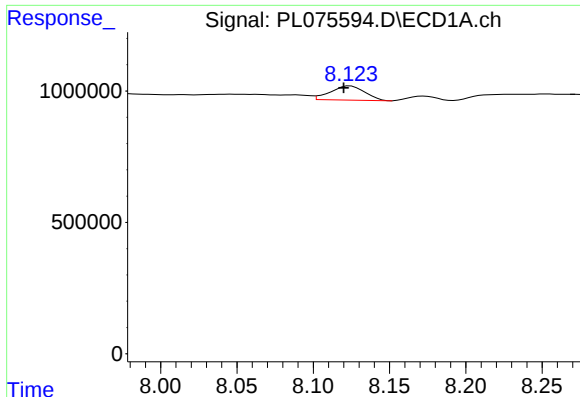

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.004 min
Response: 844745
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

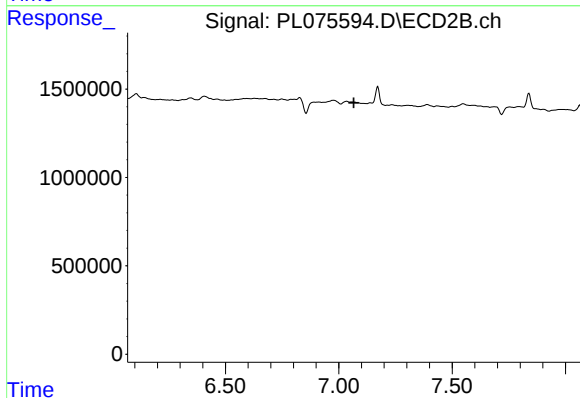


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

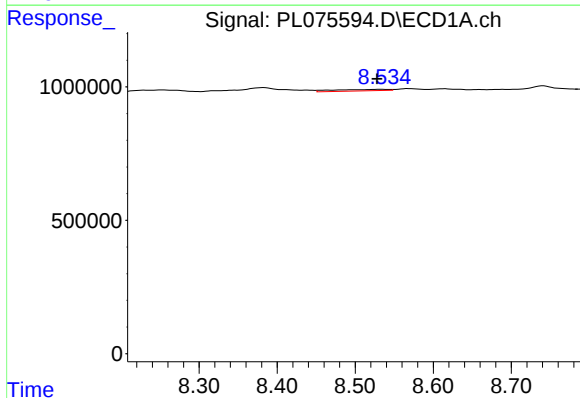


#9 Endosulfan I

R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 273418
Conc: 0.39 ng/ml

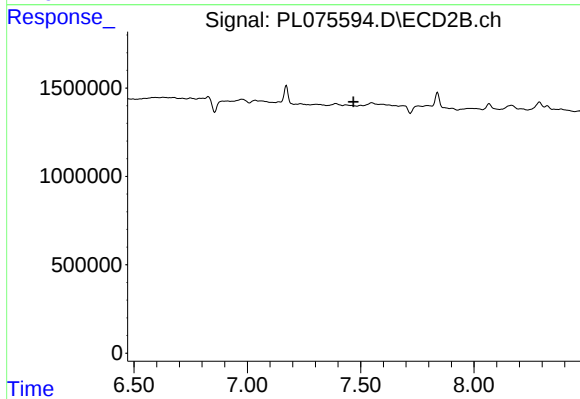

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

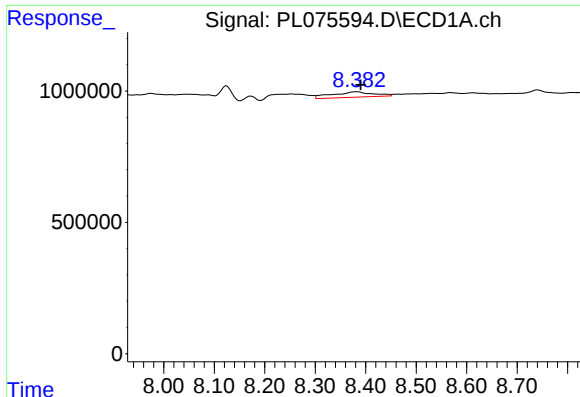

#10 gamma-Chlordane


R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1175130
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

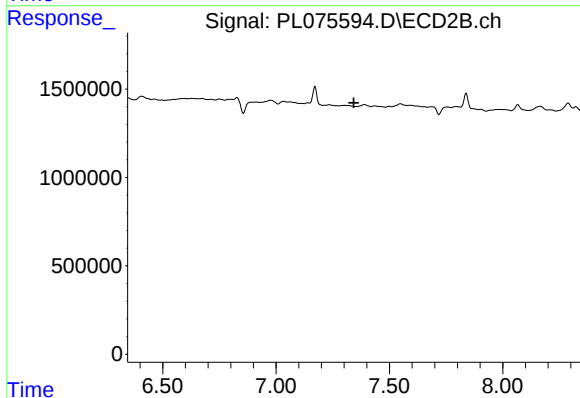


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

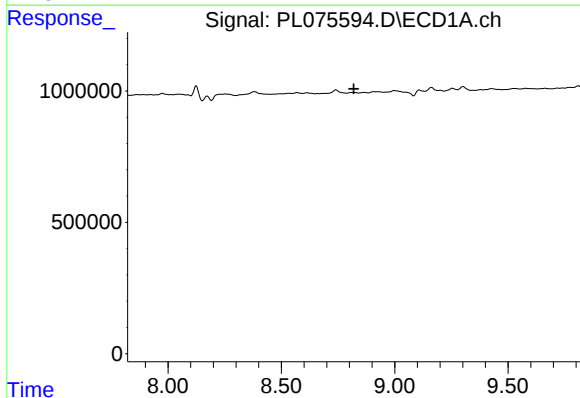


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.819 min
Response: 0
Conc: N.D.

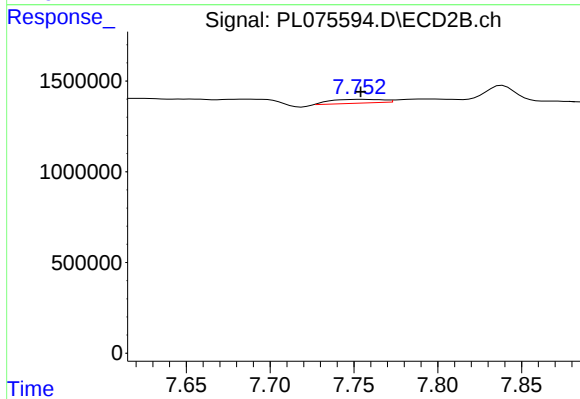

#13 Dieldrin


R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 463420
Conc: 0.27 ng/ml

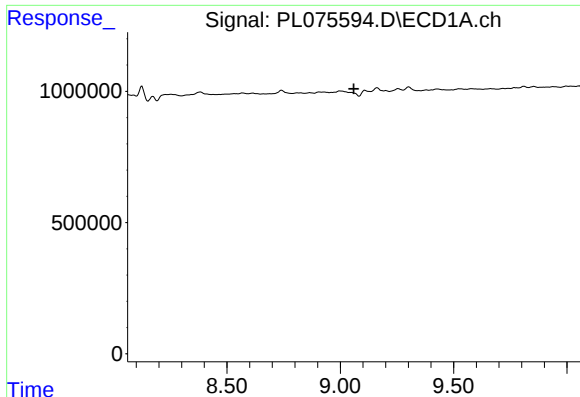

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

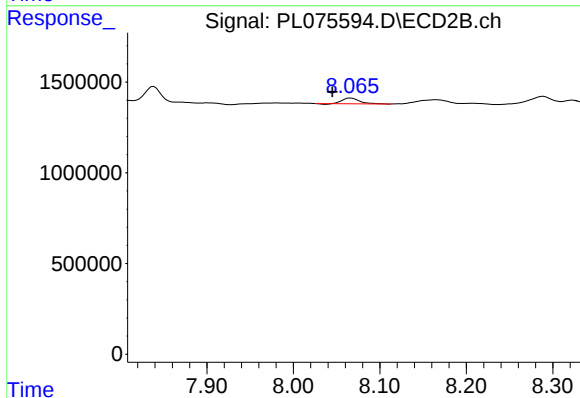


#14 Endrin

R.T.: 8.067 min
Delta R.T.: 0.022 min
Response: 438259
Conc: 0.32 ng/ml

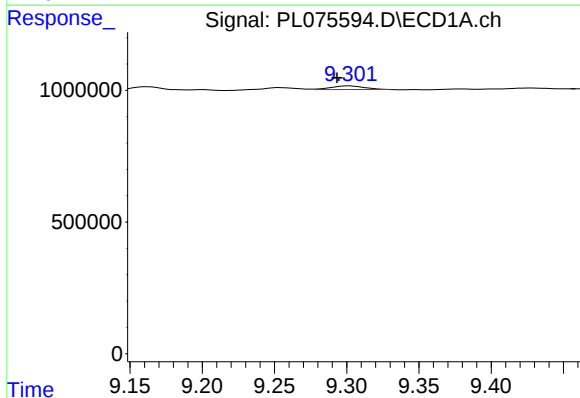


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.009 min
Response: 228355
Conc: 0.37 ng/ml

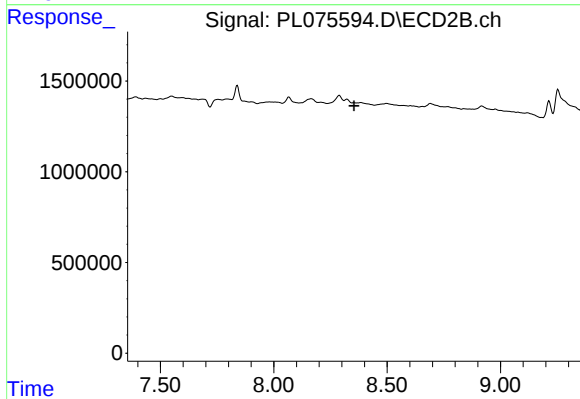

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

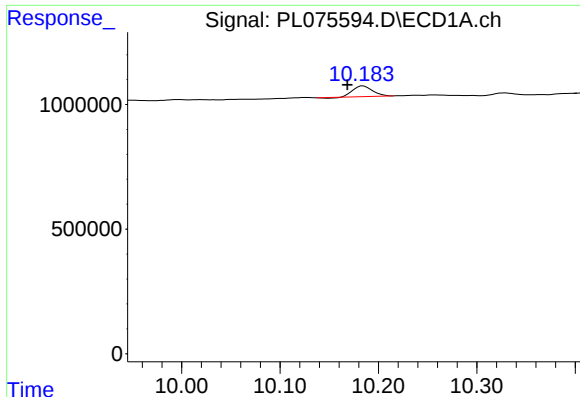

#21 Endrin ketone


R.T.: 10.184 min
Delta R.T.: 0.016 min
Response: 573901
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

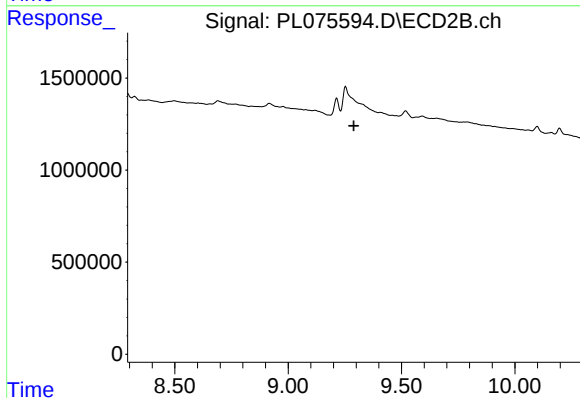


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

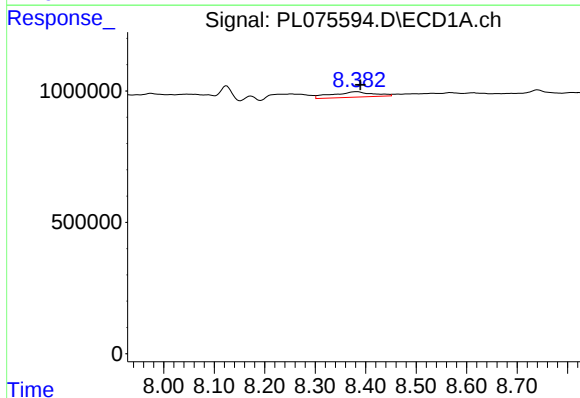


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 1175130
Conc: 11.38 ng/ml

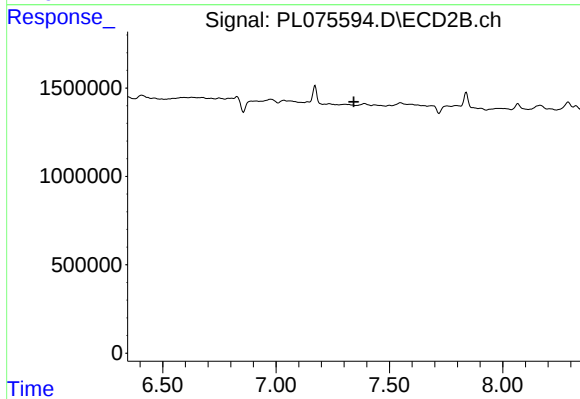

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

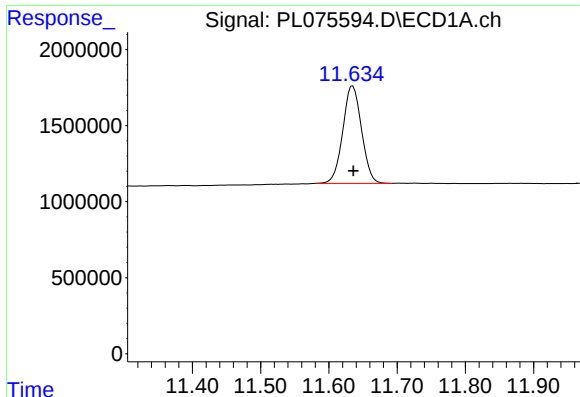

#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: -0.001 min
Response: 12234280
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

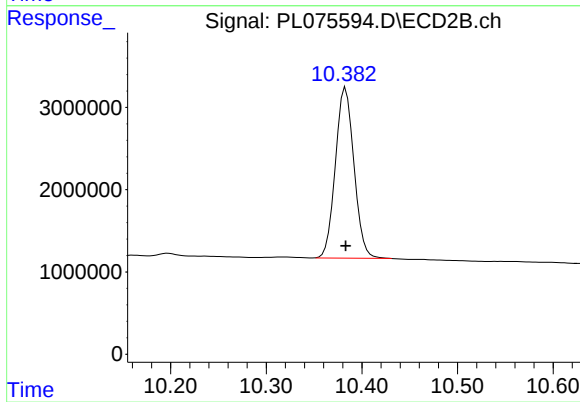

#28 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: 0.000 min
Response: 27975233
Conc: 19.86 ng/ml