

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
 Data File : PL075565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 15:48
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:52:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 01:43:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.638	70557061	206.9E6	99.888	99.862
28)	SA Decachlor...	11.636	10.383	58016638	135.2E6	95.166	95.489
Target Compounds							
23)	Chlordane-1	7.036	5.959	25303130	54259686	992.759	987.277
24)	Chlordane-2	7.630	6.645	29525815	62024873	967.893	966.362
25)	Chlordane-3	8.391	7.344	105.6E6	175.2E6	998.160	999.544
26)	Chlordane-4	8.474	7.412	126.8E6	185.0E6	987.473	995.090
27)	Chlordane-5	9.367	8.123	22090261	45997576	985.553	975.079



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
Data File : PL075565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 15:48
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:52:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 01:43:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

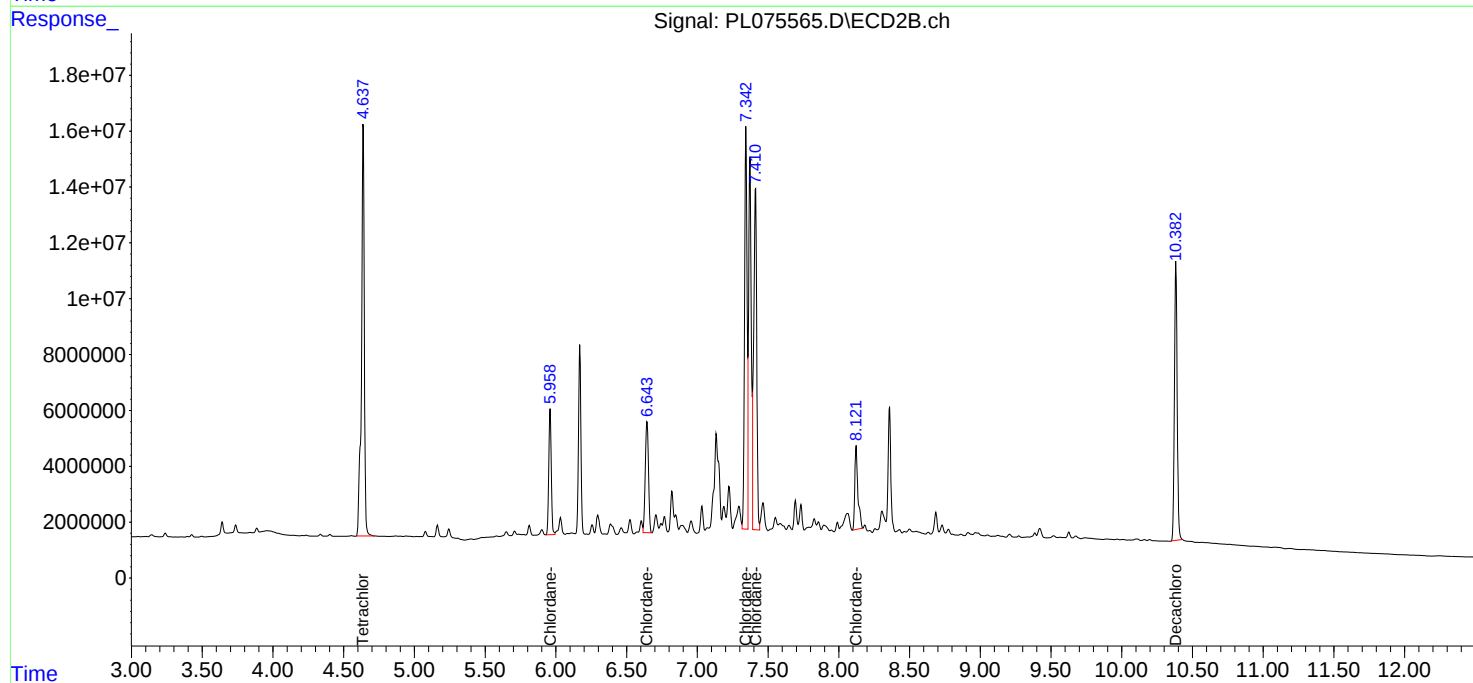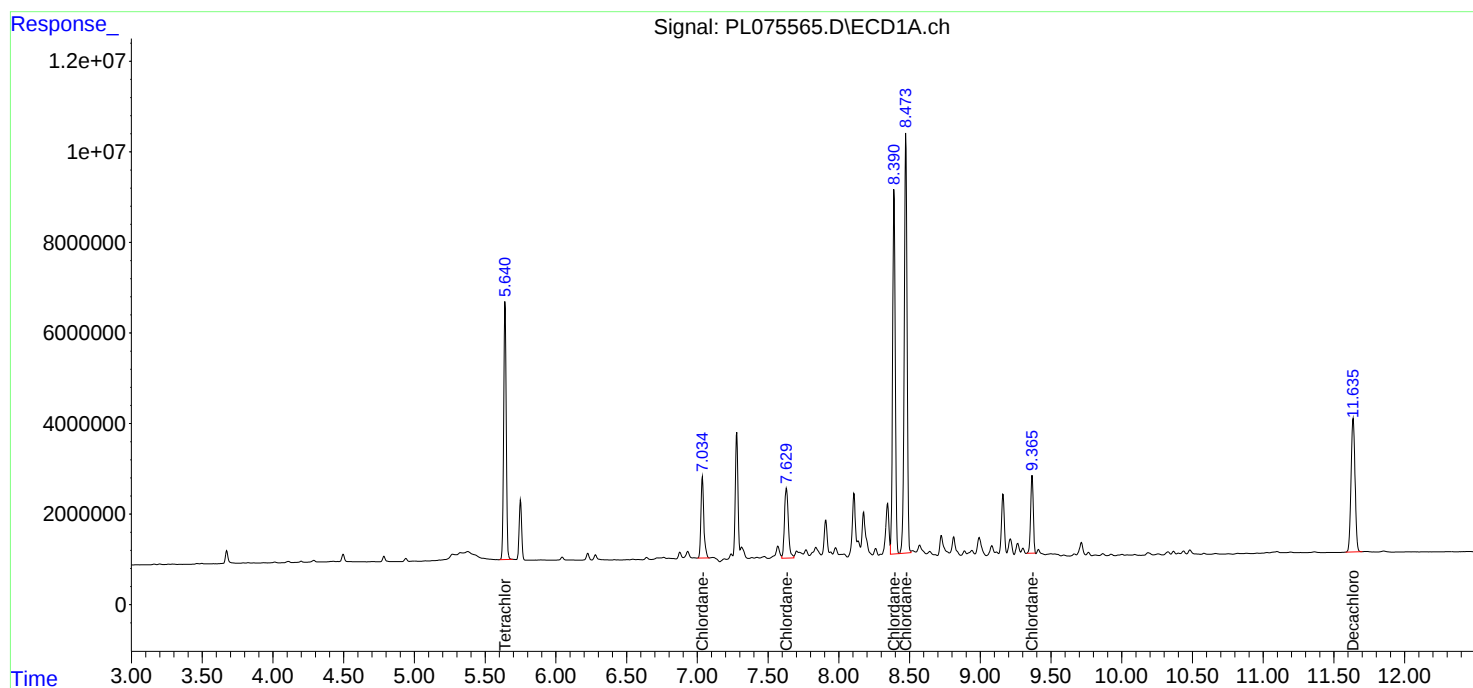


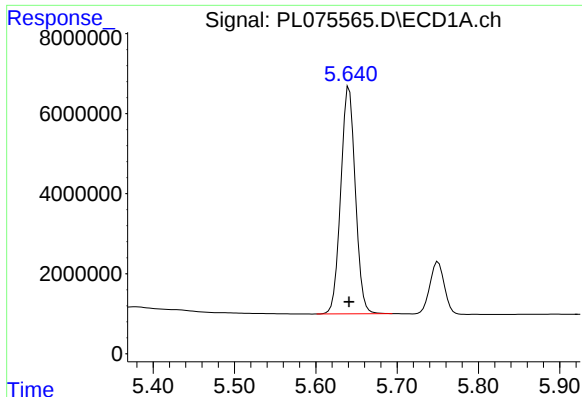

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 70557061
Conc: 99.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

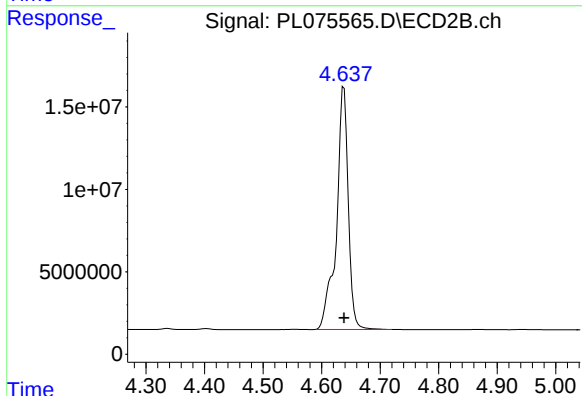


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 206933432
Conc: 99.86 ng/ml

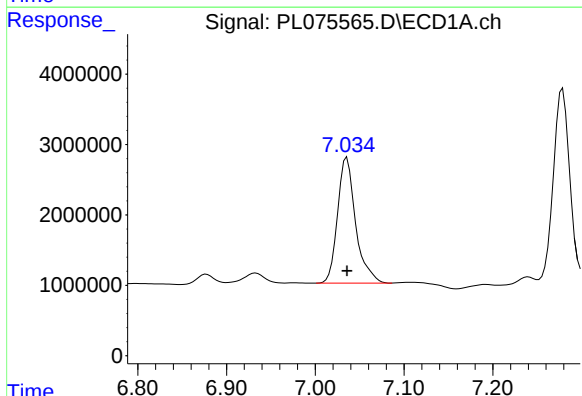


#23 Chlordane-1

R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 25303130
Conc: 992.76 ng/ml

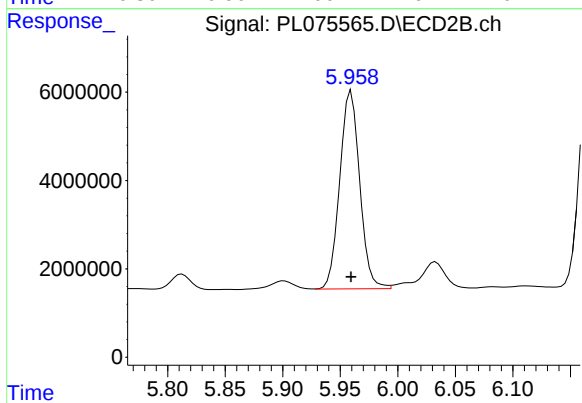

#23 Chlordane-1


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 54259686
Conc: 987.28 ng/ml

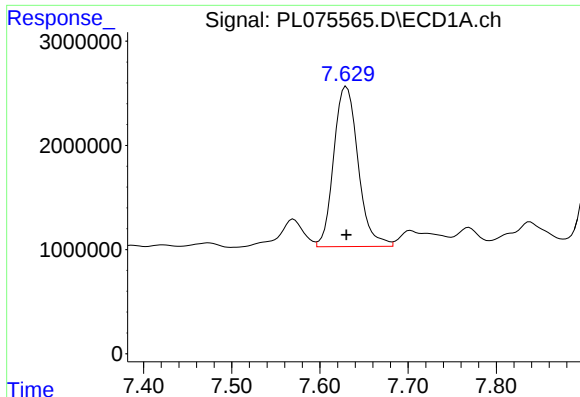

#24 Chlordane-2


R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 29525815
Conc: 967.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

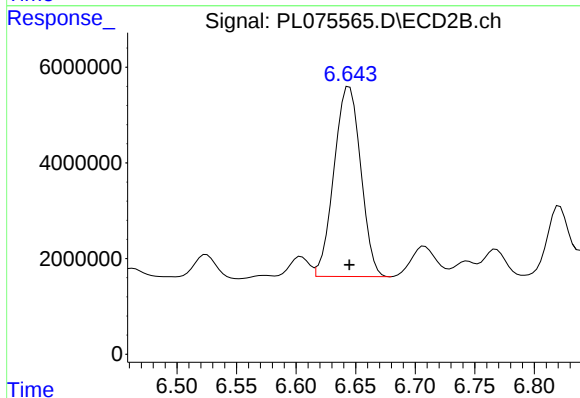


#24 Chlordane-2

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 62024873
Conc: 966.36 ng/ml

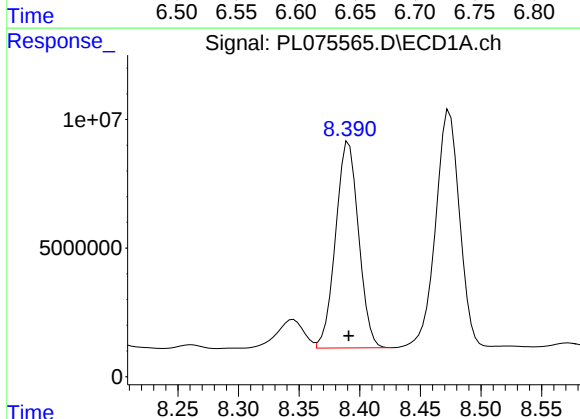


#25 Chlordane-3

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 105575833
Conc: 998.16 ng/ml

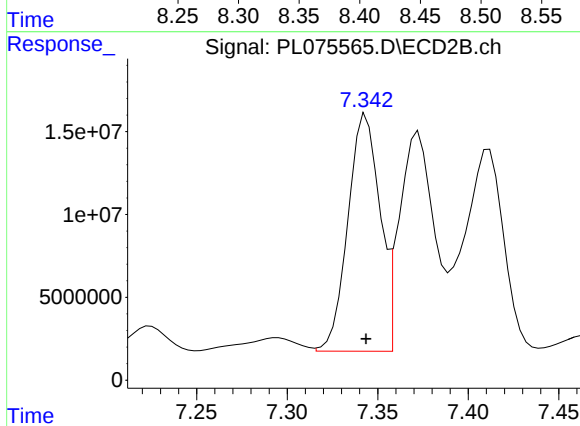

#25 Chlordane-3


R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 175211940
Conc: 999.54 ng/ml

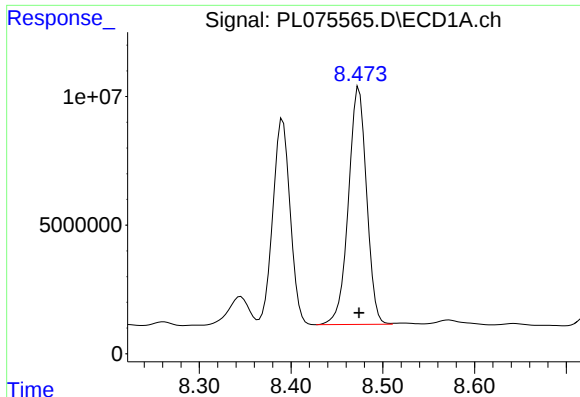

#26 Chlordane-4


R.T.: 8.474 min
Delta R.T.: 0.000 min
Response: 126756717
Conc: 987.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

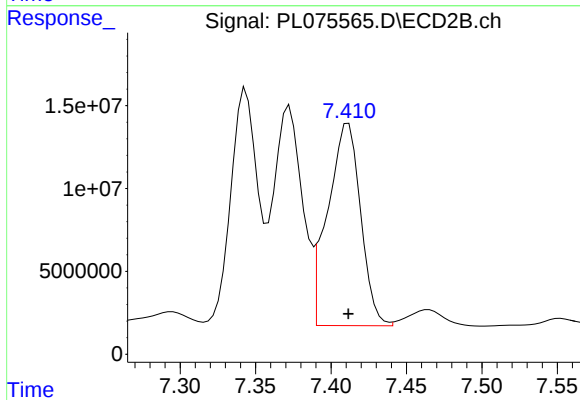


#26 Chlordane-4

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 184988063
Conc: 995.09 ng/ml

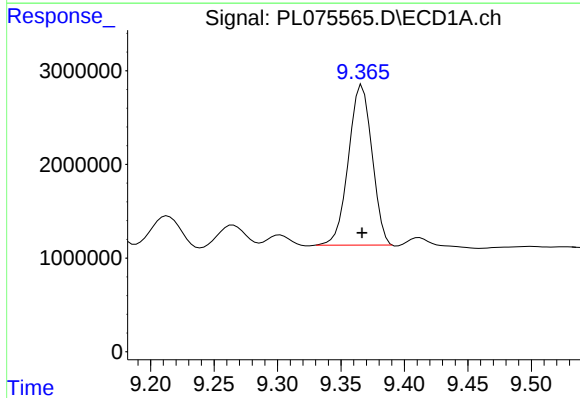


#27 Chlordane-5

R.T.: 9.367 min
Delta R.T.: 0.000 min
Response: 22090261
Conc: 985.55 ng/ml

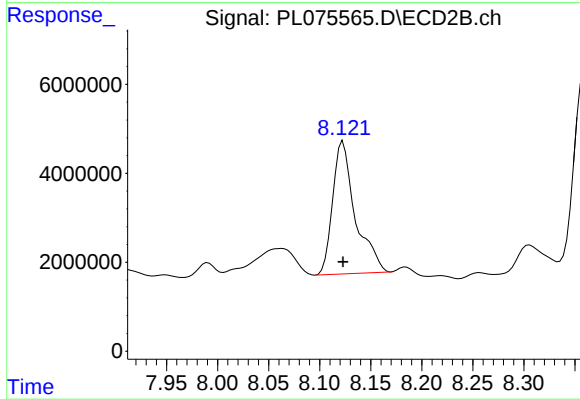

#27 Chlordane-5


R.T.: 8.123 min
Delta R.T.: 0.000 min
Response: 45997576
Conc: 975.08 ng/ml

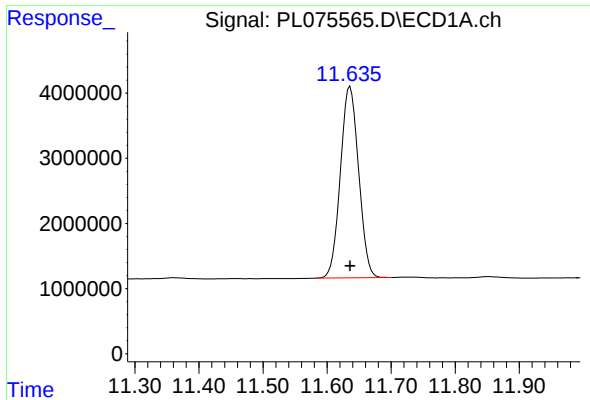

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 58016638
Conc: 95.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

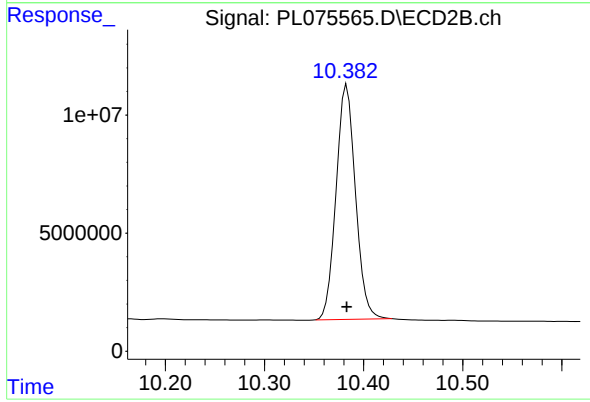

#28 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: 0.000 min
Response: 135228307
Conc: 95.49 ng/ml