

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
 Data File : PL075566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 16:04
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:54:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 01:54:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.638	51651833	149.1E6	73.739	72.928
28)	SA Decachlor...	11.636	10.383	44456728	102.3E6	73.603	73.155
Target Compounds							
23)	Chlordane-1	7.035	5.959	18649519	39894323	737.704	733.755
24)	Chlordane-2	7.630	6.645	22188757	46385128	734.764	731.570
25)	Chlordane-3	8.391	7.344	77496922	127.8E6	738.370	736.036
26)	Chlordane-4	8.474	7.412	93263248	135.1E6	734.201	734.442
27)	Chlordane-5	9.366	8.123	16214423	33912749	732.057	728.975



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
Data File : PL075566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 16:04
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:54:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 01:54:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

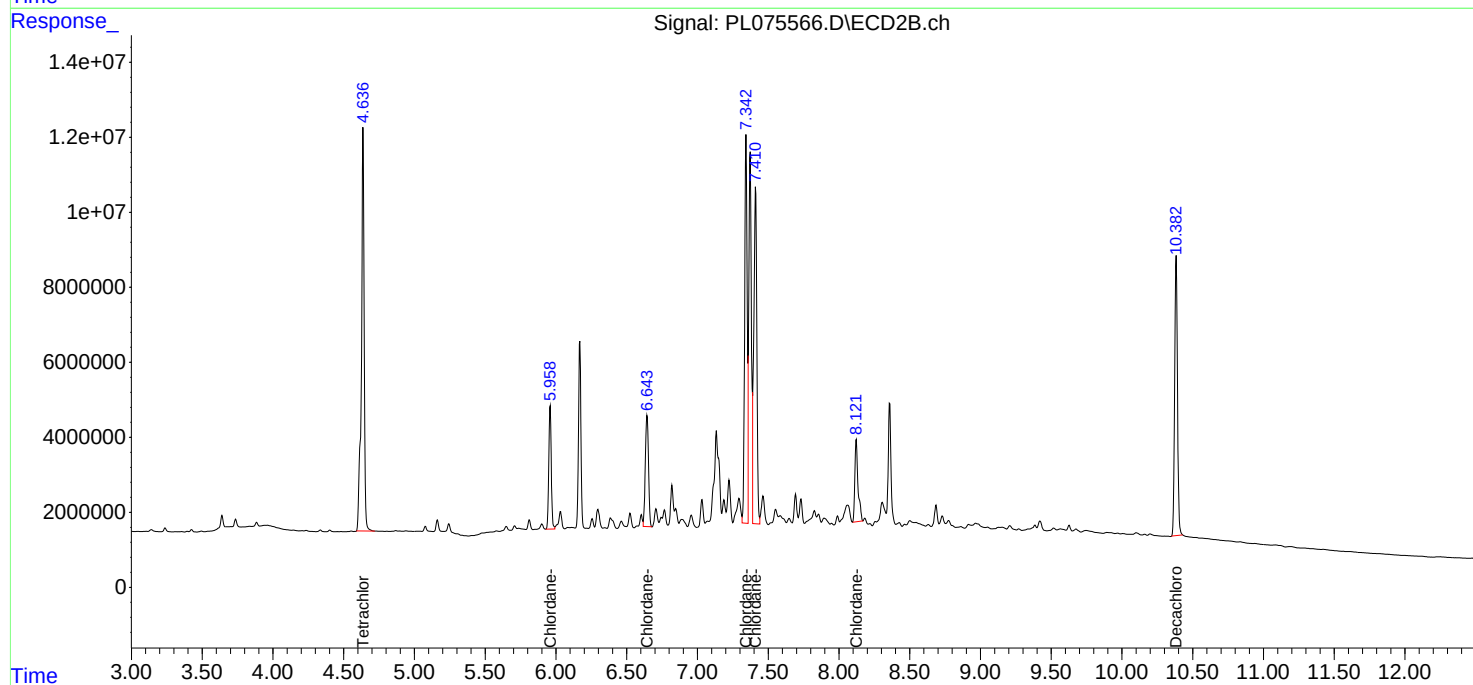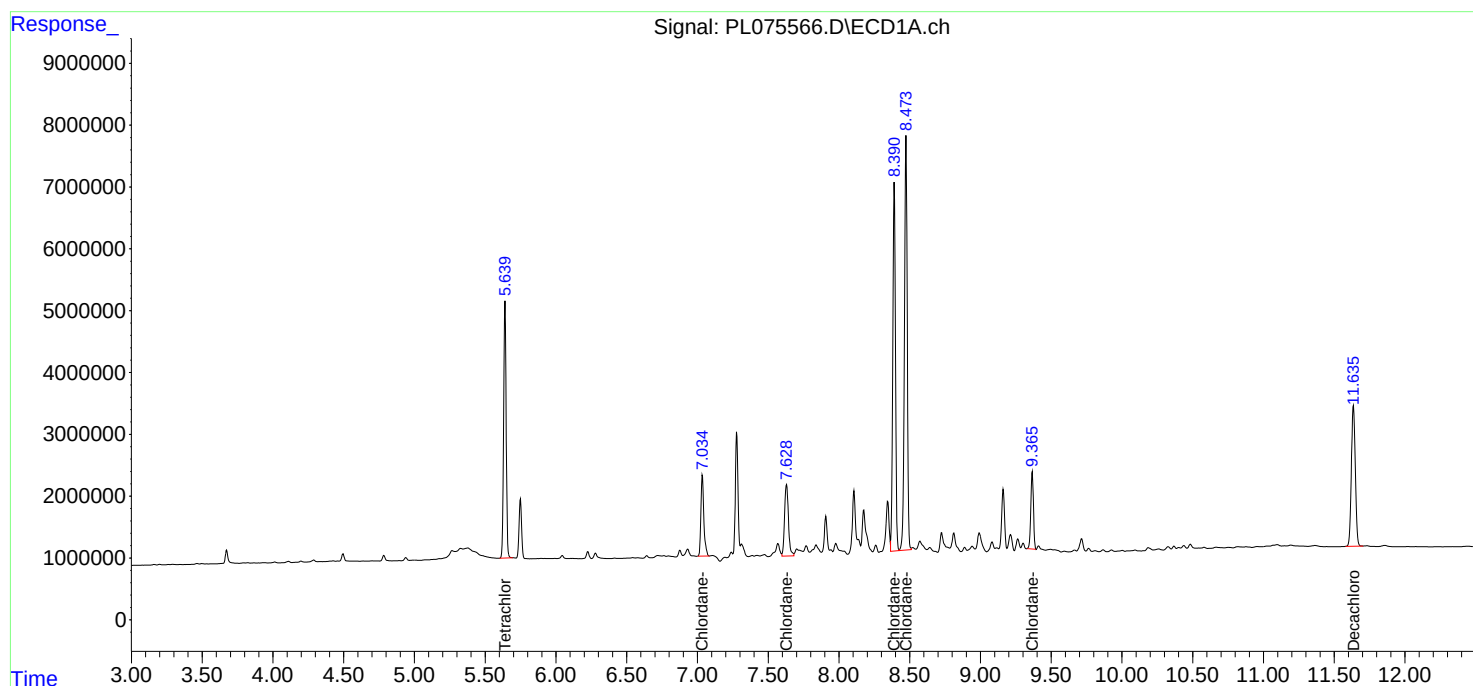


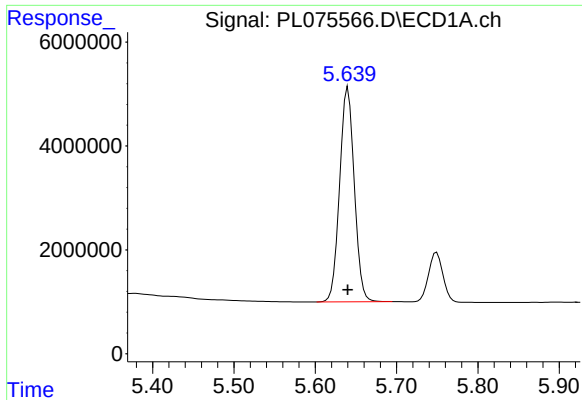

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 51651833
Conc: 73.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

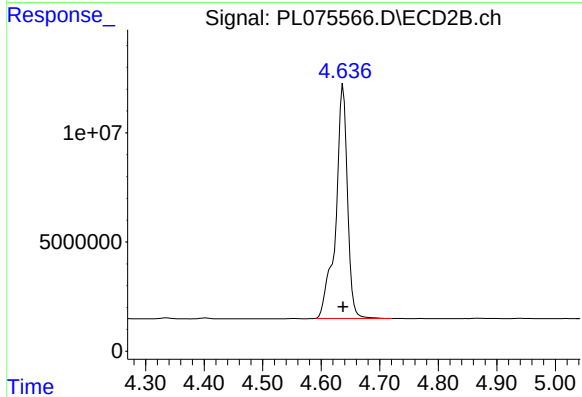


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 149062037
Conc: 72.93 ng/ml

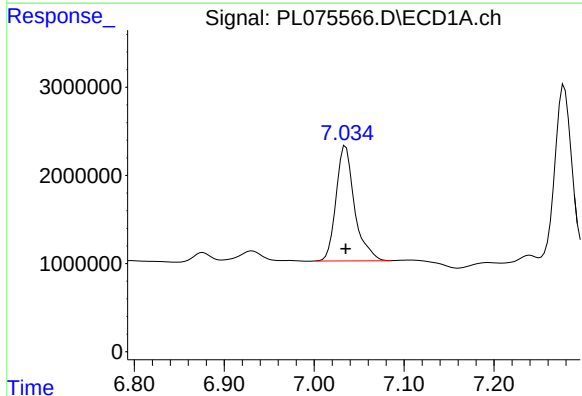


#23 Chlordane-1

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 18649519
Conc: 737.70 ng/ml

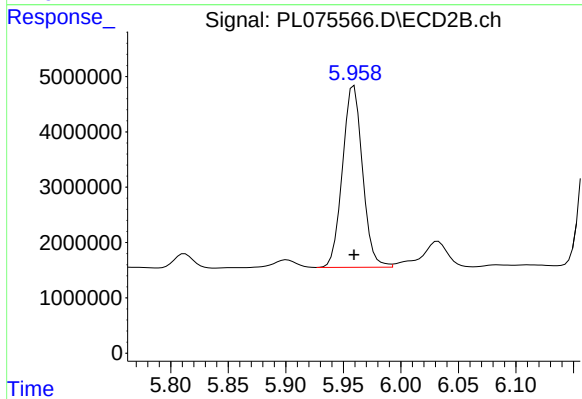

#23 Chlordane-1


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 39894323
Conc: 733.75 ng/ml

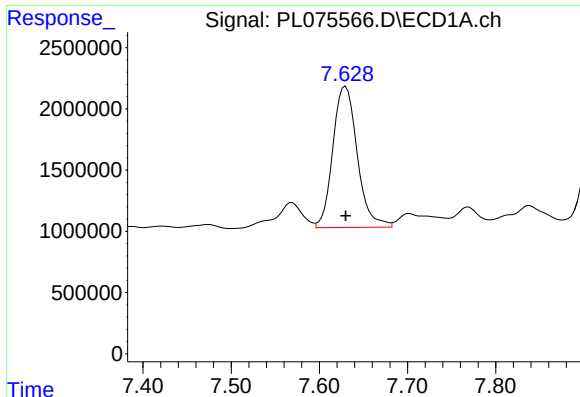

#24 Chlordane-2


R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 22188757
Conc: 734.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

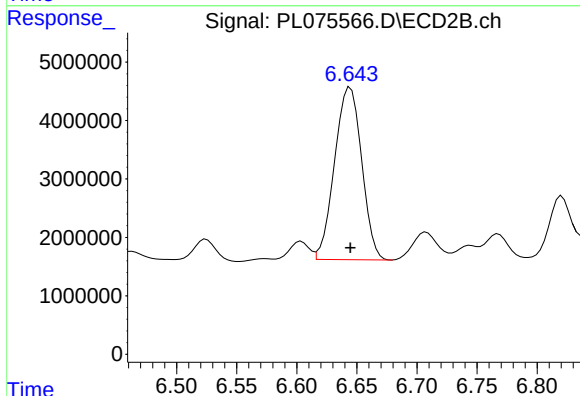


#24 Chlordane-2

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 46385128
Conc: 731.57 ng/ml

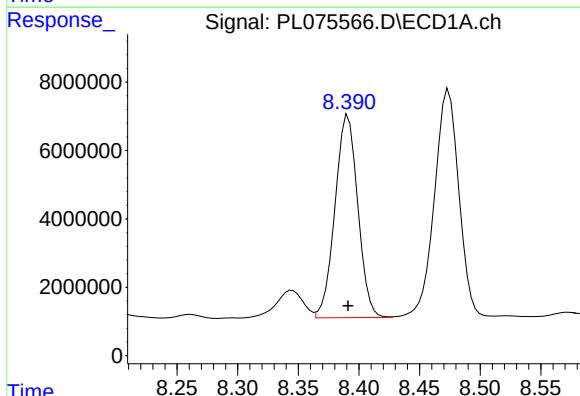


#25 Chlordane-3

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 77496922
Conc: 738.37 ng/ml

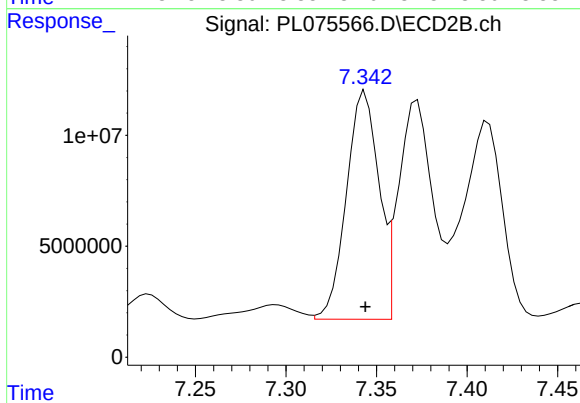

#25 Chlordane-3


R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 127831181
Conc: 736.04 ng/ml

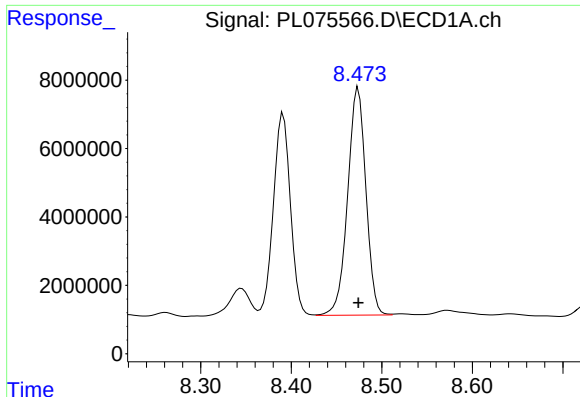

#26 Chlordane-4


R.T.: 8.474 min
Delta R.T.: 0.000 min
Response: 93263248
Conc: 734.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

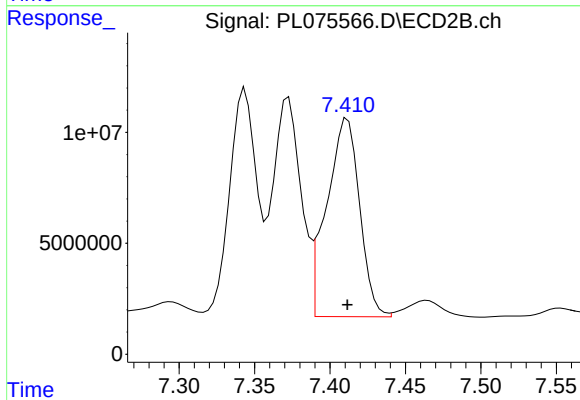


#26 Chlordane-4

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 135131662
Conc: 734.44 ng/ml

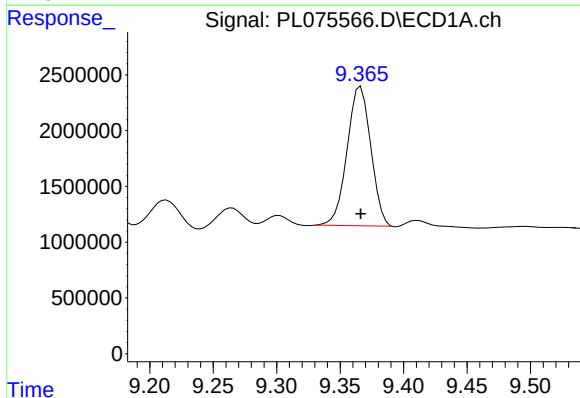


#27 Chlordane-5

R.T.: 9.366 min
Delta R.T.: 0.000 min
Response: 16214423
Conc: 732.06 ng/ml

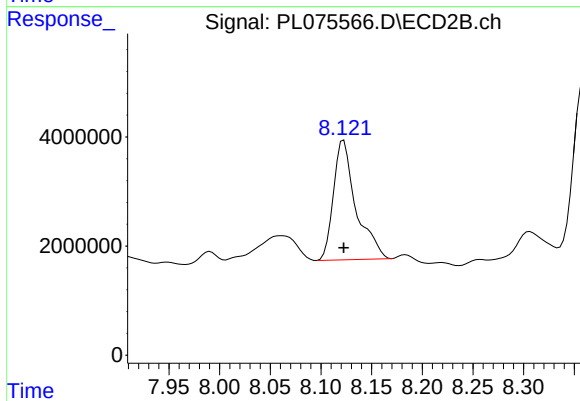

#27 Chlordane-5


R.T.: 8.123 min
Delta R.T.: 0.000 min
Response: 33912749
Conc: 728.98 ng/ml

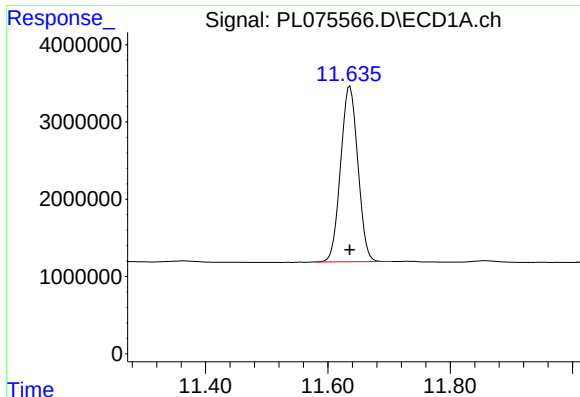

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 44456728
Conc: 73.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

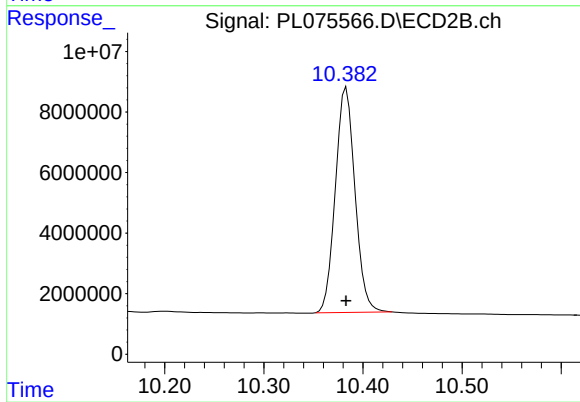

#28 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: 0.000 min
Response: 102340602
Conc: 73.15 ng/ml