

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
 Data File : PL075567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 16:21
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:47:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 01:43:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.637	35357871	103.8E6	50.000	50.000
28)	SA Decachlor...	11.635	10.382	31955334	74002803	50.000	50.000
Target Compounds							
23)	Chlordane-1	7.036	5.959	12836133	27829095	500.000	500.000
24)	Chlordane-2	7.629	6.644	15742330	33171457	500.000	500.000
25)	Chlordane-3	8.391	7.343	52982534	87685832	500.000	500.000
26)	Chlordane-4	8.474	7.411	64986412	93406748	500.000	500.000
27)	Chlordane-5	9.367	8.122	11368953	24174408	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
Data File : PL075567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 16:21
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:47:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 01:43:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

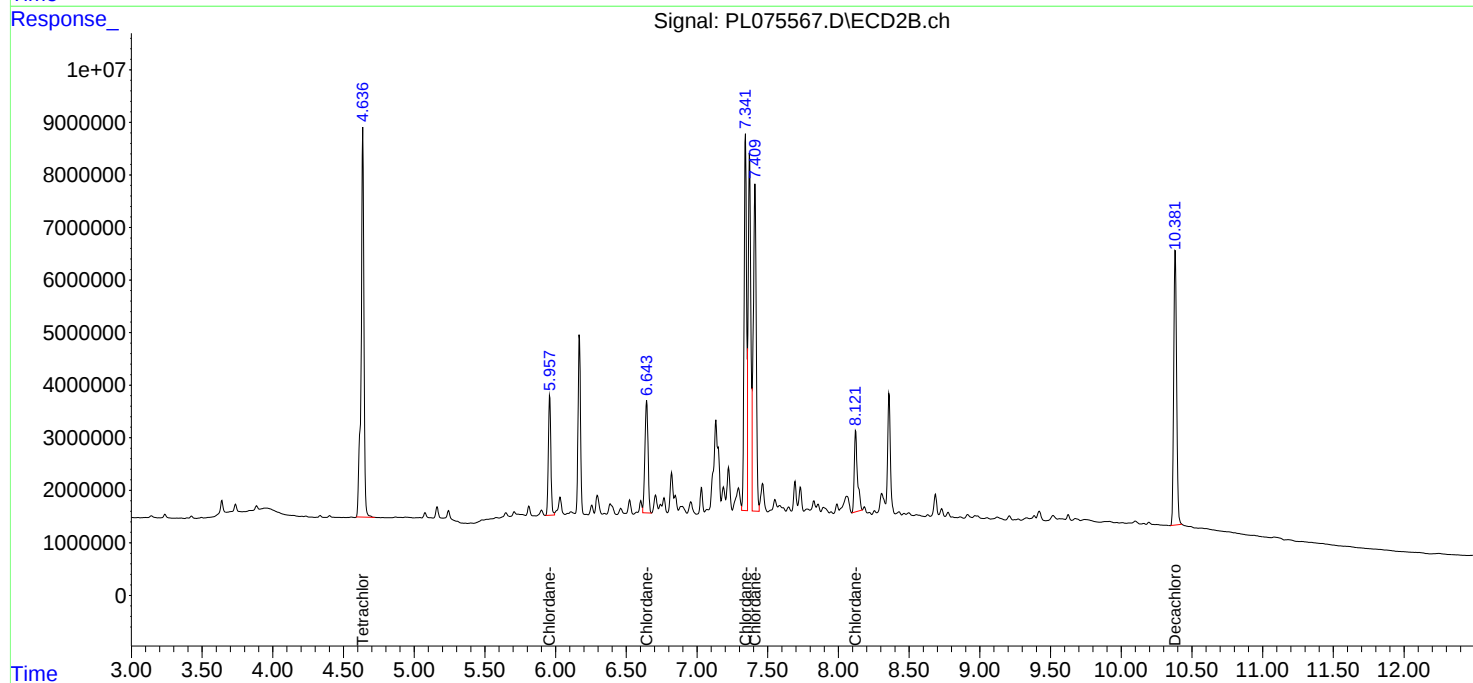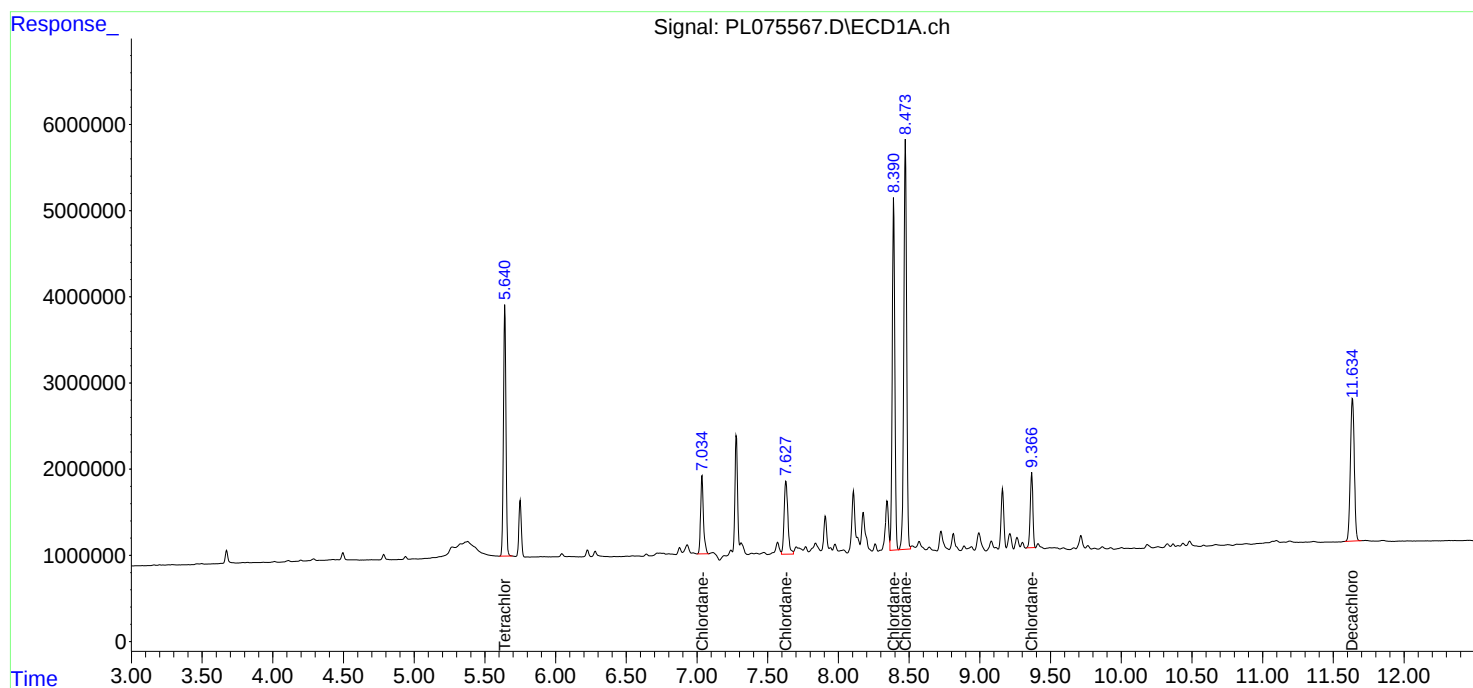


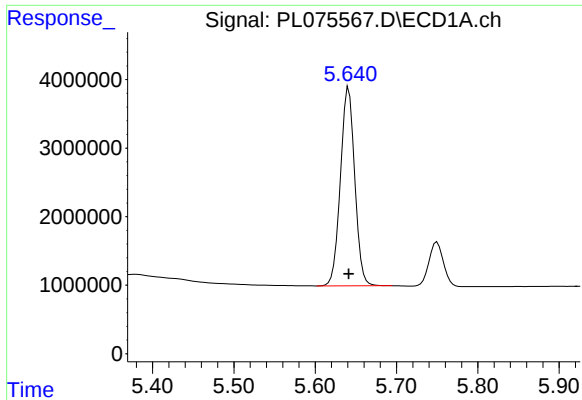

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 35357871
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

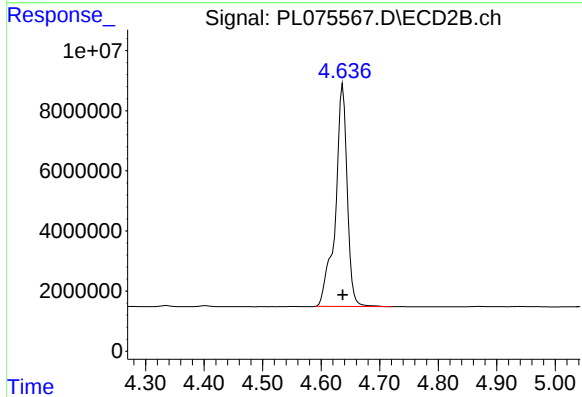


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 103752029
Conc: 50.00 ng/ml

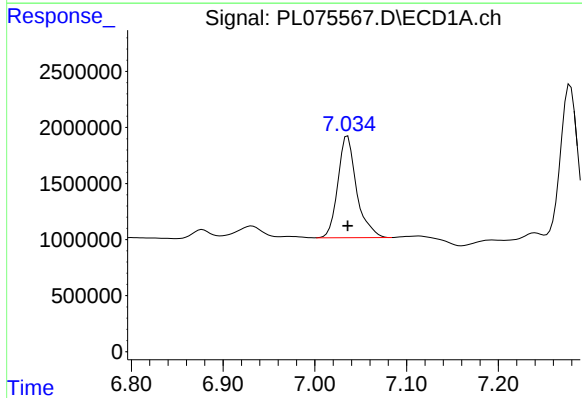


#23 Chlordane-1

R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 12836133
Conc: 500.00 ng/ml

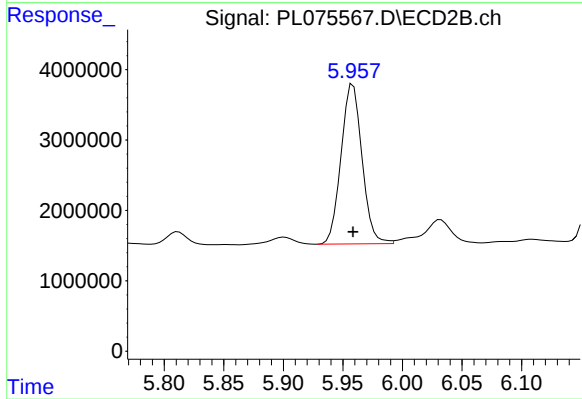

#23 Chlordane-1


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 27829095
Conc: 500.00 ng/ml

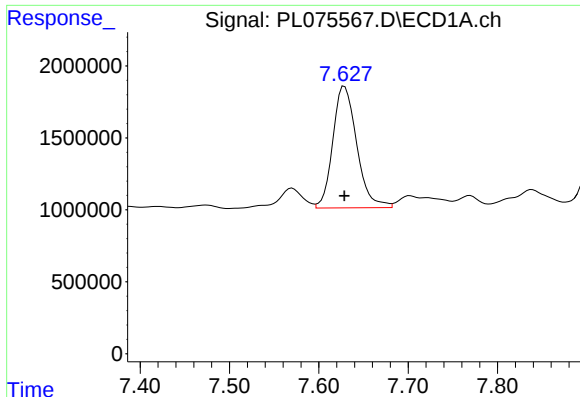

#24 Chlordane-2


R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 15742330
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

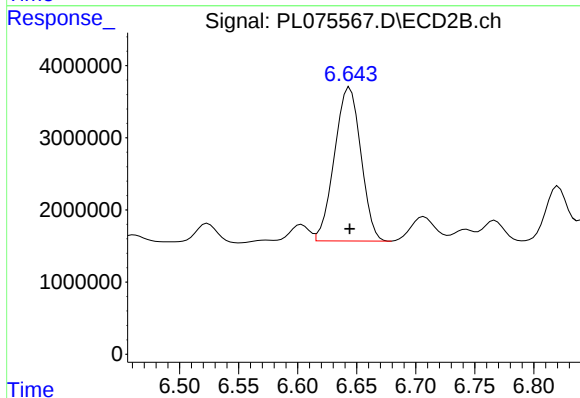


#24 Chlordane-2

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 33171457
Conc: 500.00 ng/ml

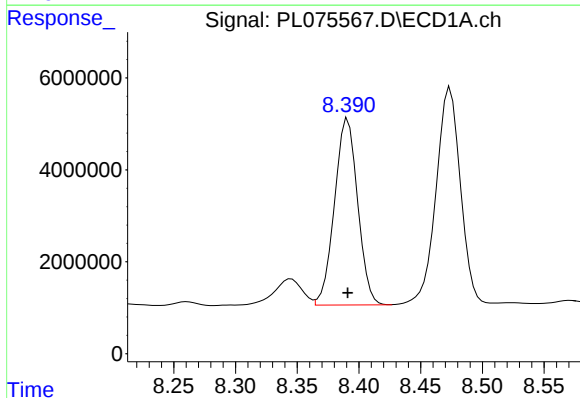


#25 Chlordane-3

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 52982534
Conc: 500.00 ng/ml

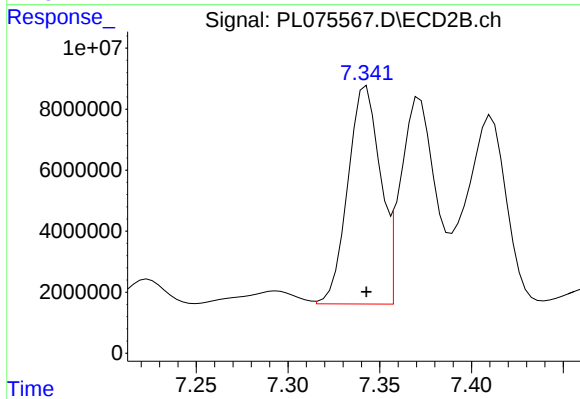

#25 Chlordane-3


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 87685832
Conc: 500.00 ng/ml

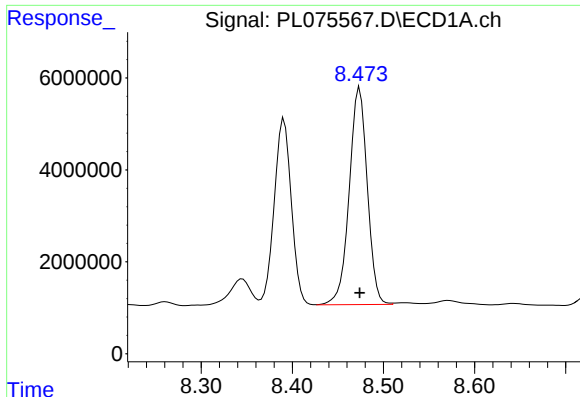

#26 Chlordane-4


R.T.: 8.474 min
Delta R.T.: 0.000 min
Response: 64986412
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

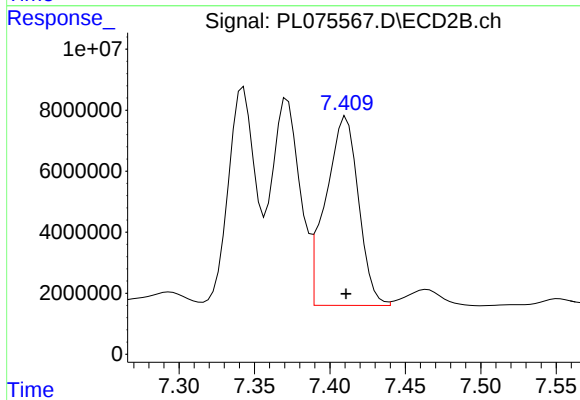


#26 Chlordane-4

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 93406748
Conc: 500.00 ng/ml

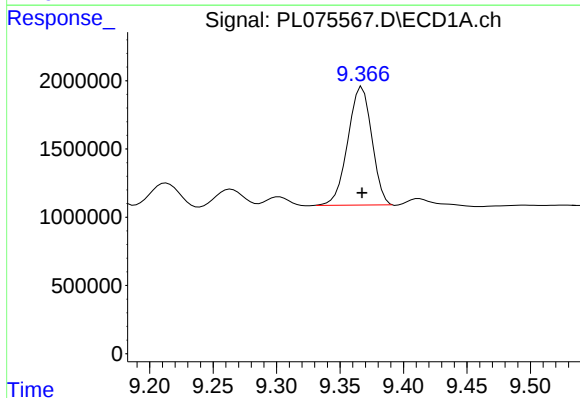


#27 Chlordane-5

R.T.: 9.367 min
Delta R.T.: 0.000 min
Response: 11368953
Conc: 500.00 ng/ml

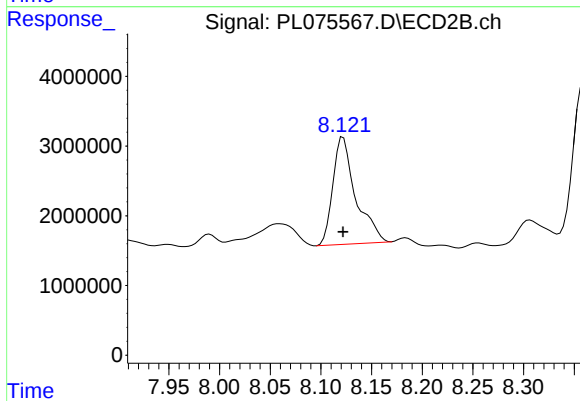

#27 Chlordane-5


R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 24174408
Conc: 500.00 ng/ml

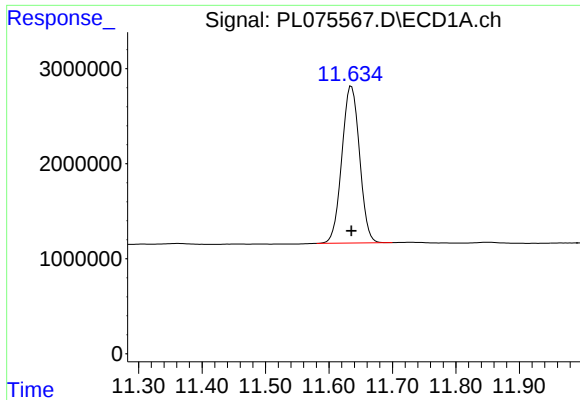

#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: 0.000 min
Response: 31955334
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

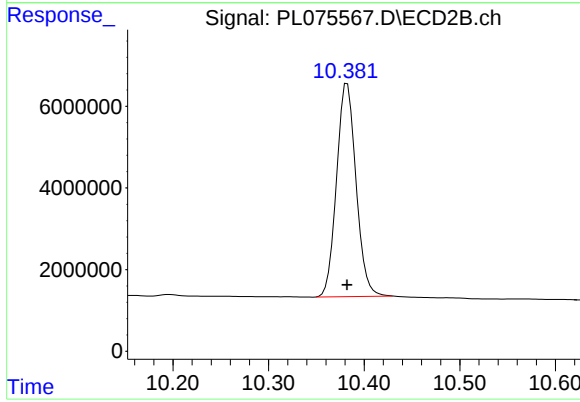

#28 Decachlorobiphenyl

R.T.: 10.382 min
Delta R.T.: 0.000 min
Response: 74002803
Conc: 50.00 ng/ml