

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
 Data File : PL075568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 16:37
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 01:57:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 01:56:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.637	17007088	50709750	24.456	24.857
28)	SA Decachlor...	11.636	10.383	16198588	37682314	26.339	26.424
Target Compounds							
23)	Chlordane-1	7.035	5.959	6078223	13758493	242.754	252.282
24)	Chlordane-2	7.629	6.645	7707506	17152683	253.901	265.085
25)	Chlordane-3	8.391	7.343	25121527	42006795	241.928	243.853
26)	Chlordane-4	8.474	7.411	31075816	44989517	245.958	245.866
27)	Chlordane-5	9.367	8.123	5383499	12132763	244.756	258.014



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060622\
Data File : PL075568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 16:37
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 01:57:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 01:56:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

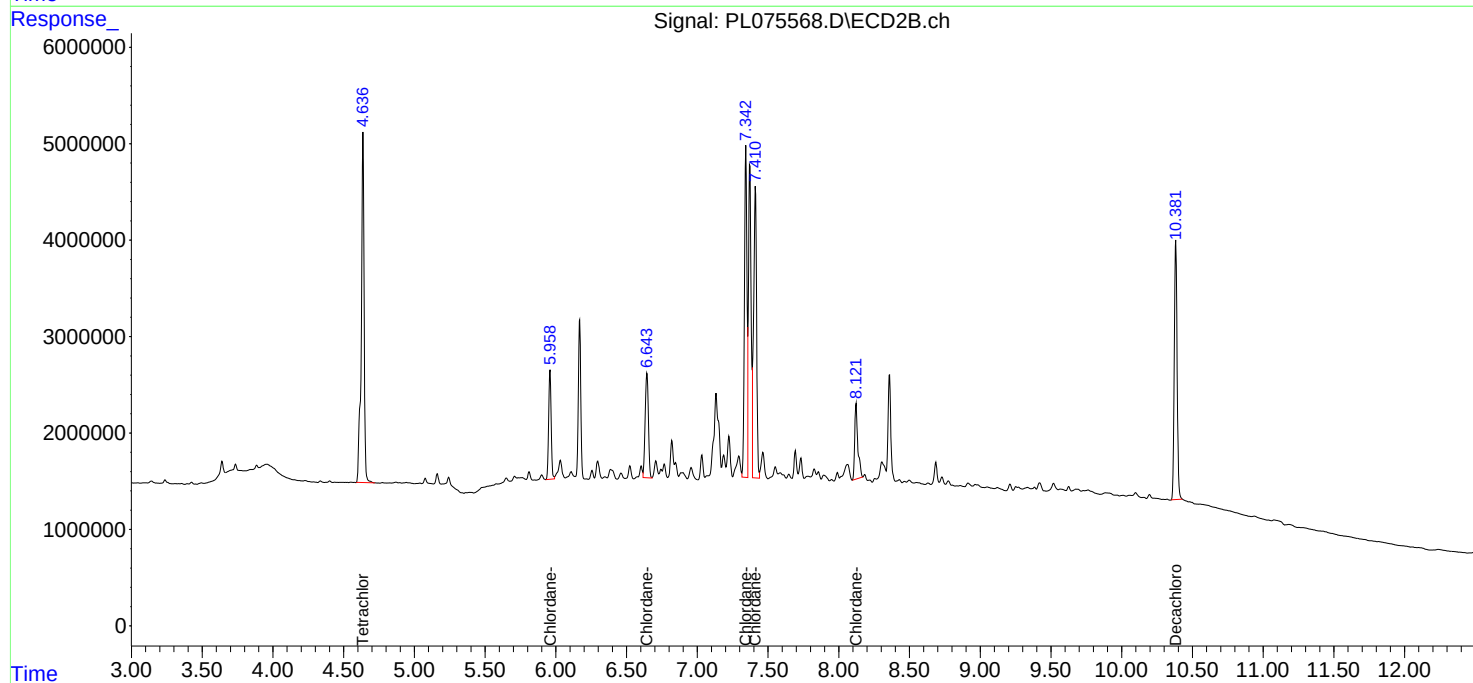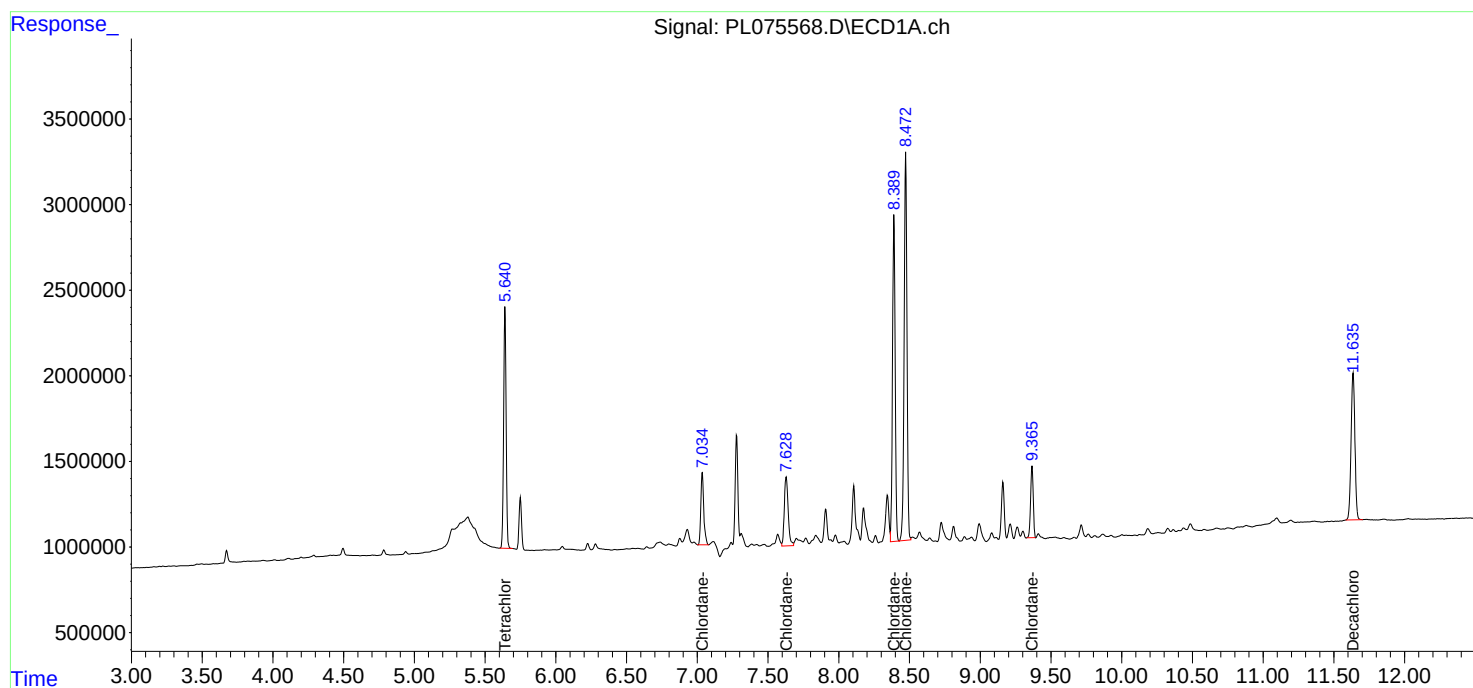


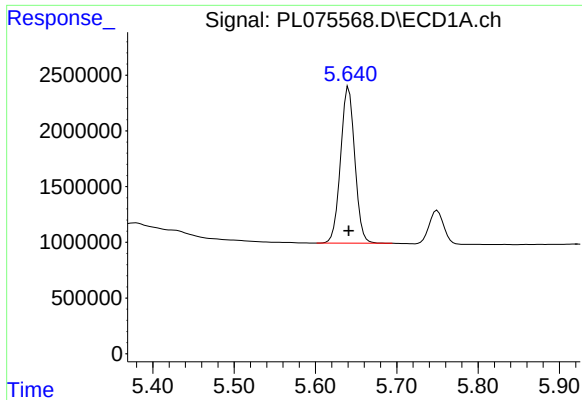

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 17007088
Conc: 24.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

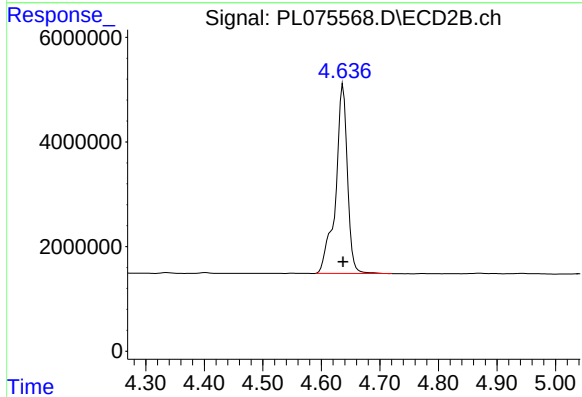


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 50709750
Conc: 24.86 ng/ml

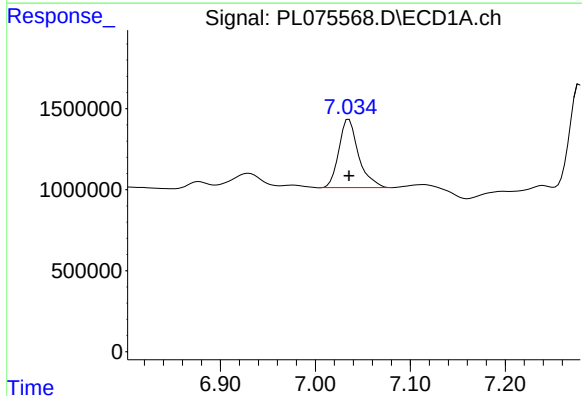


#23 Chlordane-1

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 6078223
Conc: 242.75 ng/ml

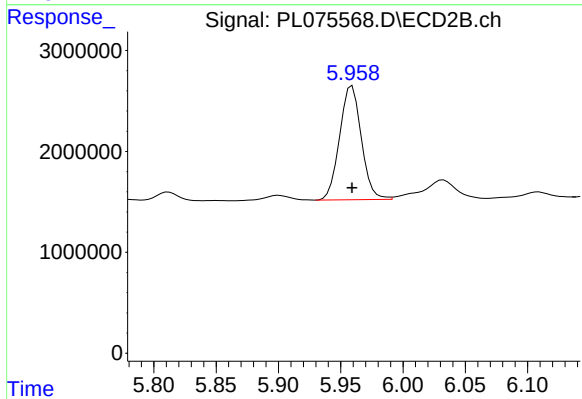

#23 Chlordane-1


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 13758493
Conc: 252.28 ng/ml

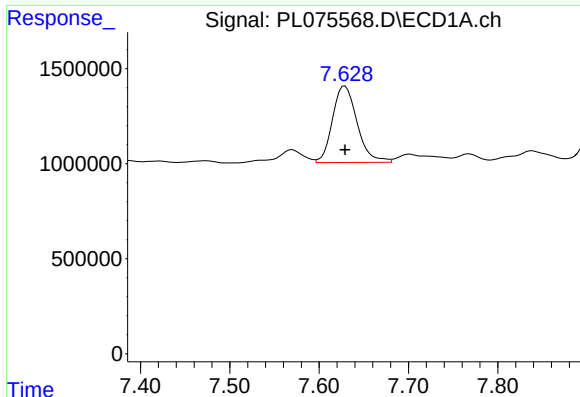

#24 Chlordane-2


R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 7707506
Conc: 253.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

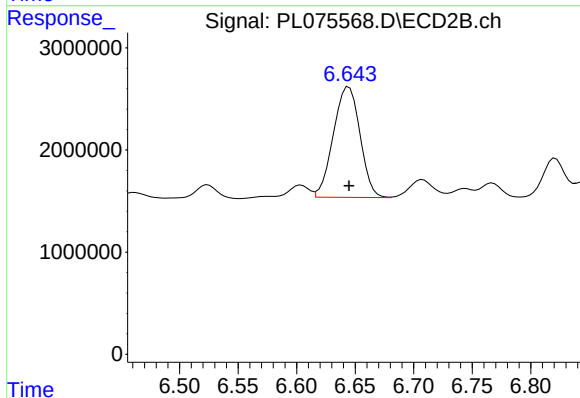


#24 Chlordane-2

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 17152683
Conc: 265.09 ng/ml

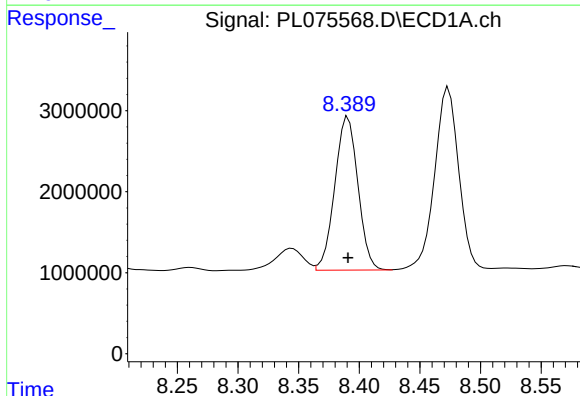


#25 Chlordane-3

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 25121527
Conc: 241.93 ng/ml

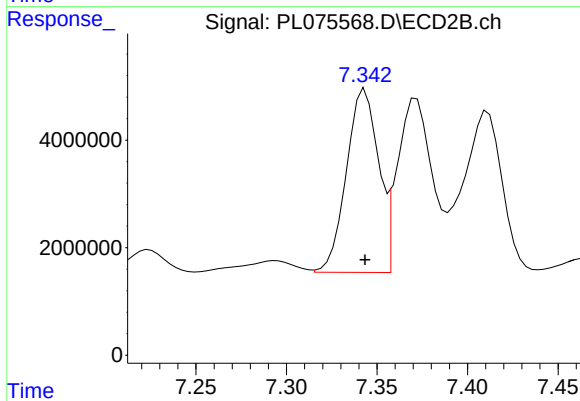

#25 Chlordane-3


R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 42006795
Conc: 243.85 ng/ml

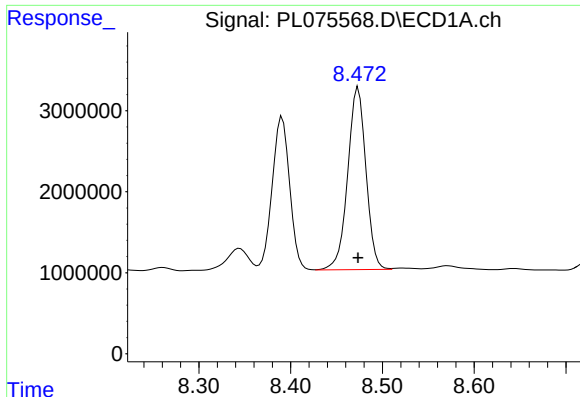

#26 Chlordane-4


R.T.: 8.474 min
Delta R.T.: 0.000 min
Response: 31075816
Conc: 245.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

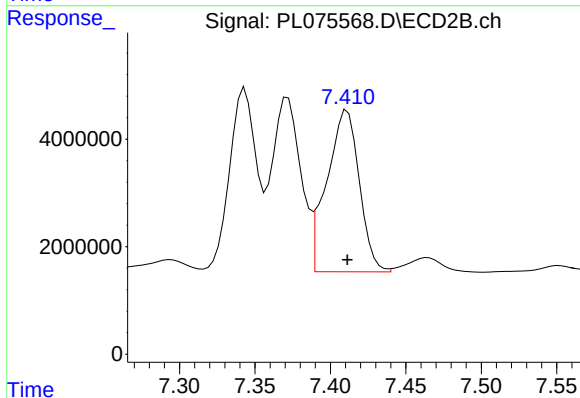


#26 Chlordane-4

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 44989517
Conc: 245.87 ng/ml

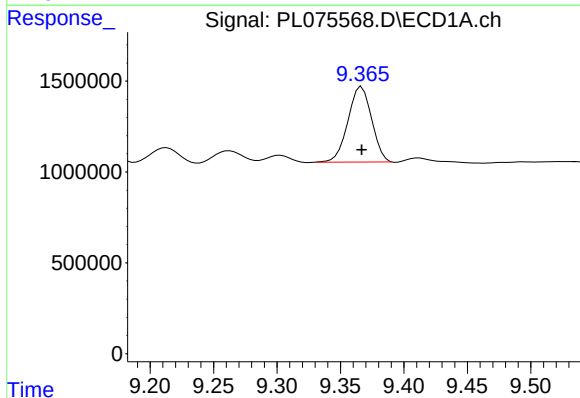


#27 Chlordane-5

R.T.: 9.367 min
Delta R.T.: 0.000 min
Response: 5383499
Conc: 244.76 ng/ml

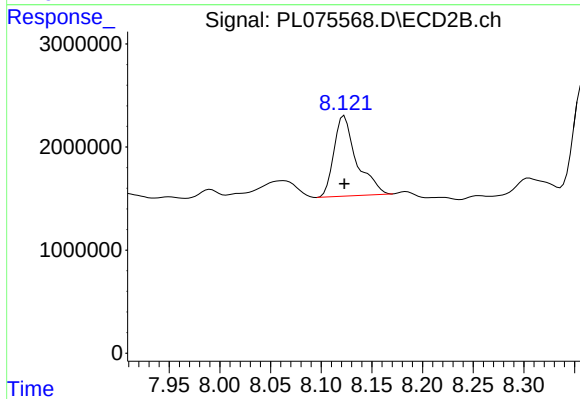

#27 Chlordane-5


R.T.: 8.123 min
Delta R.T.: 0.000 min
Response: 12132763
Conc: 258.01 ng/ml

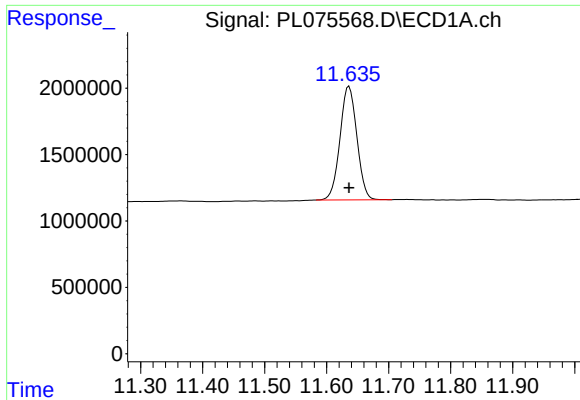

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 16198588
Conc: 26.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

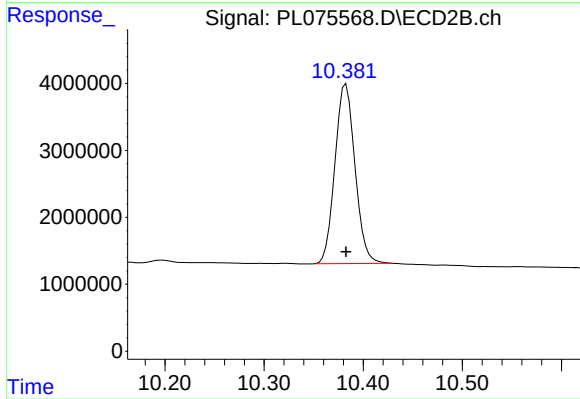

#28 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: 0.000 min
Response: 37682314
Conc: 26.42 ng/ml