

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060624\
 Data File : PL089998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2024 19:21
 Operator : AR\AJ
 Sample : P2591-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BHBQ3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2024
 Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 21:53:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 15:06:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.792	14424383	12583288	7.479m	9.269
2) SA Decachlor...	9.043	7.934	155.0E6	66464173	117.489m	47.937m#
Target Compounds						
9) A Endosulfan I	6.108	5.149	163.9E6	433.1E6	80.223m	288.384m#
13) MA Dieldrin	6.369	5.390	191.2E6	172.7E6	90.827m	104.264m
16) A 4,4'-DDD	6.698	5.808	68894254	49759496	45.258m	39.454
17) MA 4,4'-DDT	7.028	6.058	25042925	40091715	16.174m	29.706m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060624\
Data File : PL089998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2024 19:21
Operator : AR\AJ
Sample : P2591-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 21:53:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 15:06:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

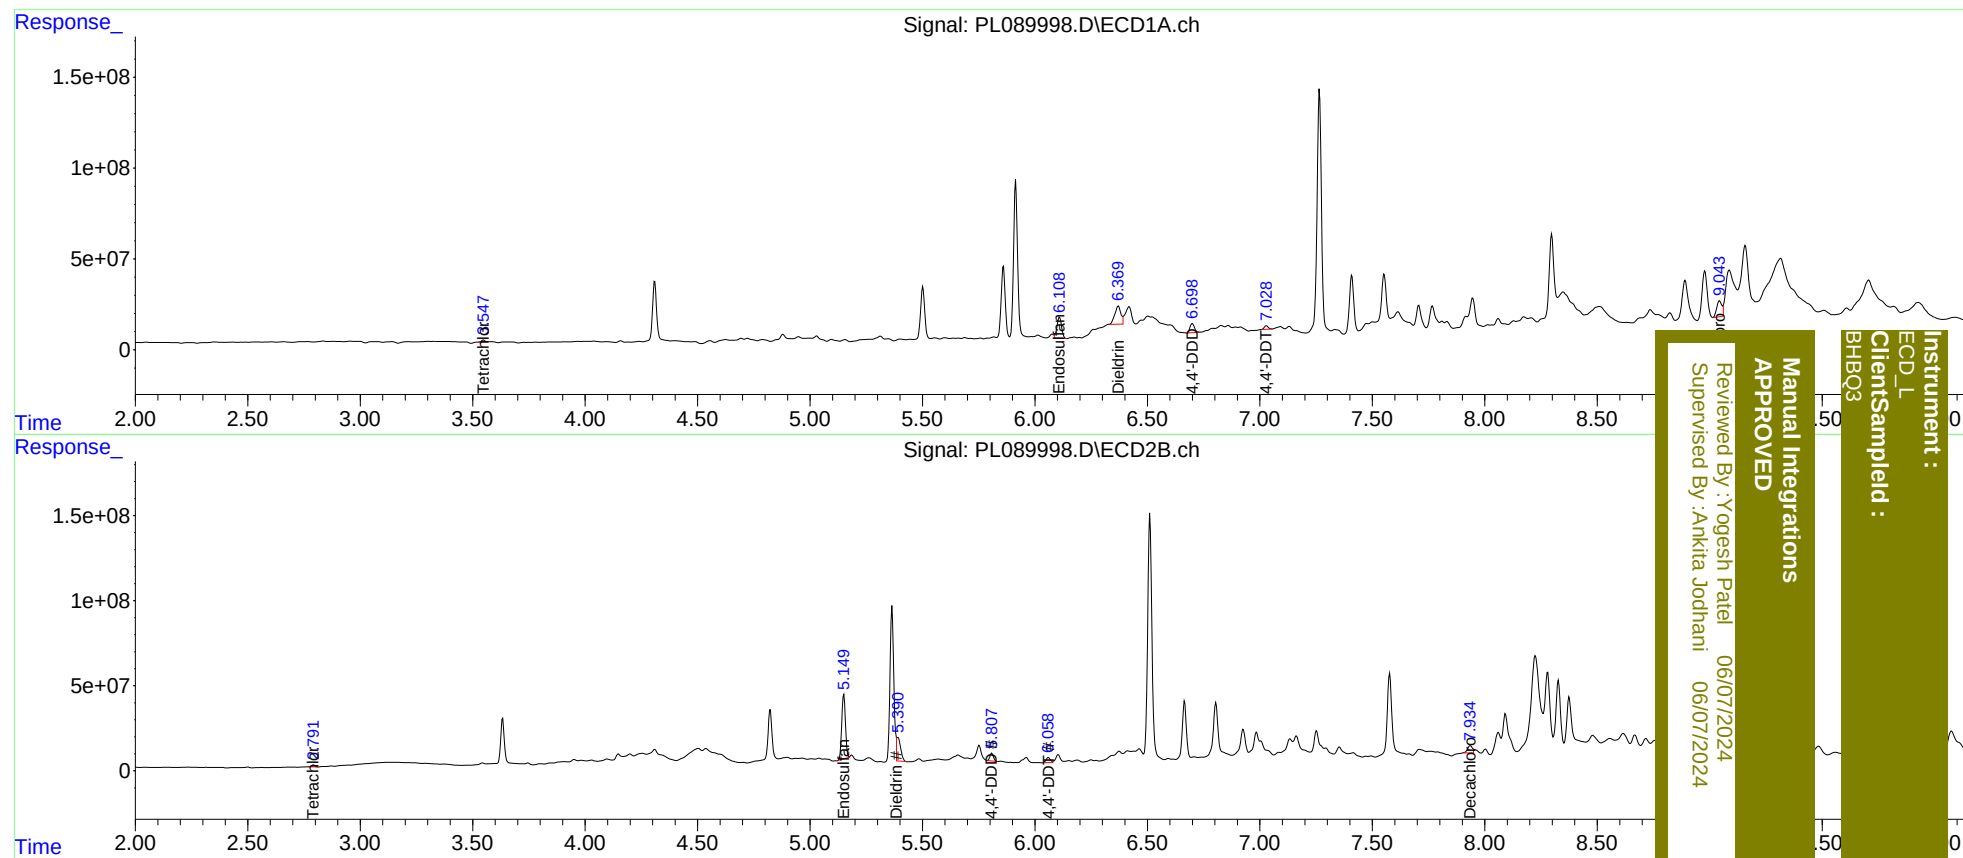

Instrument :
ECD_L
ClientSampled :
BHB03

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 06/07/2024
Supervised By : Ankita Jodhani 06/07/2024