

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060625\
 Data File : PL095970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2025 18:03
 Operator : AR\AJ
 Sample : Q2226-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 22:43:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.578	2.880	82917379	61021652	26.279	15.591 #
28)	SA Decachlor...	0.000	8.067	0	60581223	N.D.	13.849 #
Target Compounds							
10)	B gamma-Chl...	5.951f	0.000	5682752	0	1.460	N.D. #
12)	B 4,4'-DDE	6.233	5.370	30614271	46009266	8.347	8.580
13)	MA Dieldrin	0.000	5.533f	0	12543198	N.D.	2.367 #
14)	MA Endrin	0.000	5.788	0	14049682	N.D.	2.881 #
15)	B Endosulfa...	0.000	6.074	0	7008095	N.D.	1.475 #
16)	A 4,4'-DDD	6.746	5.925	36033423	36726190	12.296	8.376 #
17)	MA 4,4'-DDT	7.063	6.179	21588869	34584562	7.981	7.231
25)	Chlordane-3	5.951f	0.000	5682752	0	7.689	N.D. #
27)	Chlordane-5	0.000	6.074	0	7008095	N.D.	27.490 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060625\
Data File : PL095970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2025 18:03
Operator : AR\AJ
Sample : Q2226-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 22:43:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

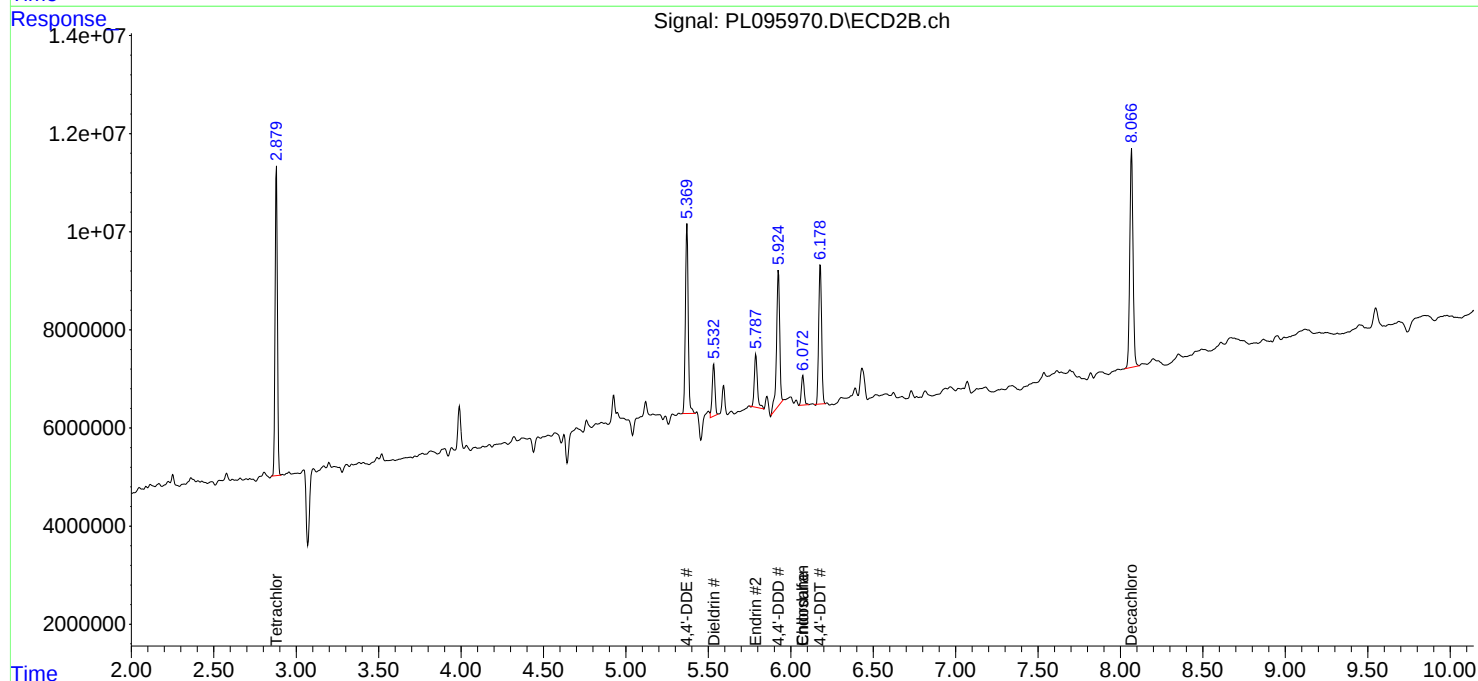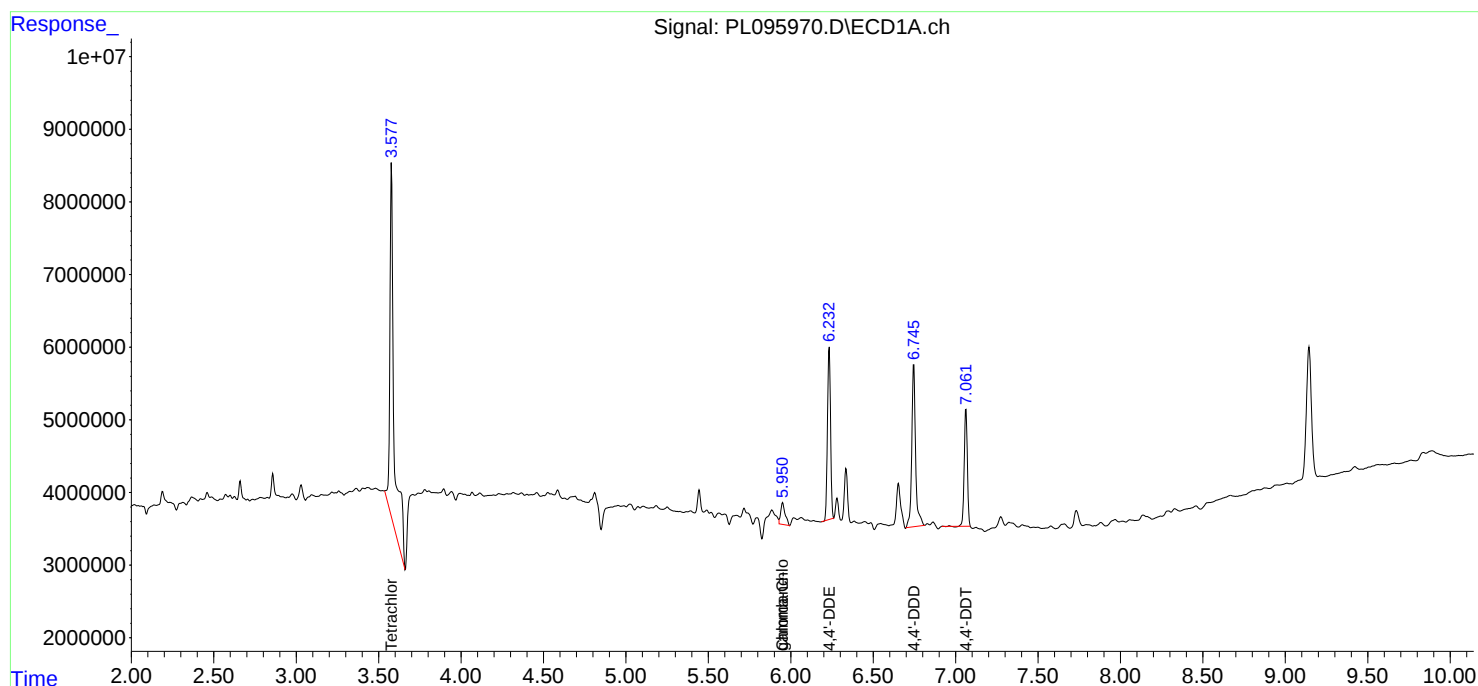


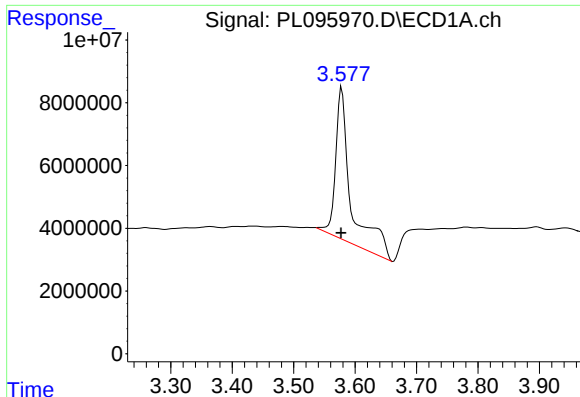

#1 Tetrachloro-m-xylene


R.T.: 3.578 min
Delta R.T.: 0.001 min
Response: 82917379
Conc: 26.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

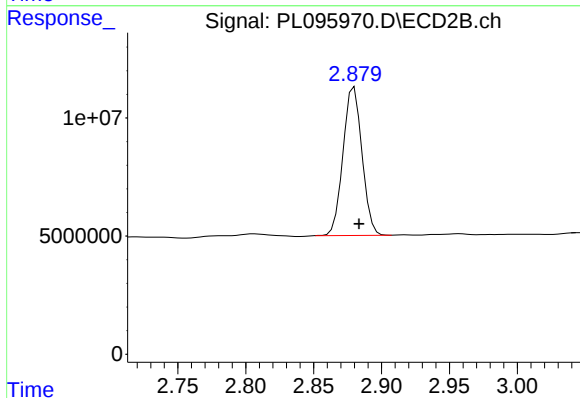


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: -0.004 min
Response: 61021652
Conc: 15.59 ng/ml

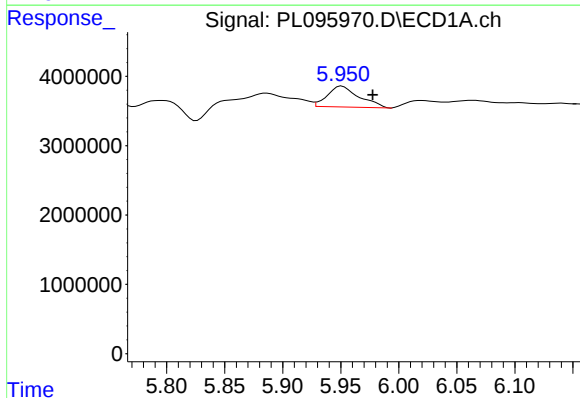


#10 gamma-Chlordane

R.T.: 5.951 min
Delta R.T.: -0.026 min
Response: 5682752
Conc: 1.46 ng/ml

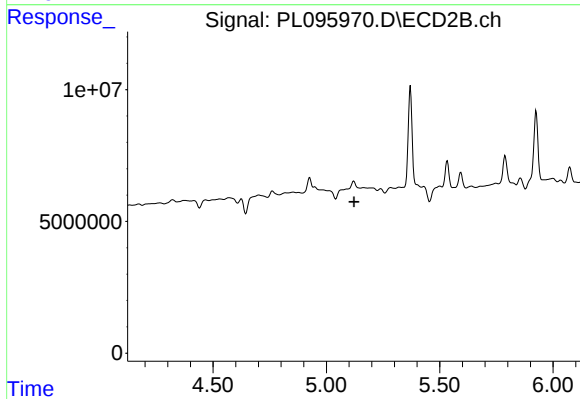

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

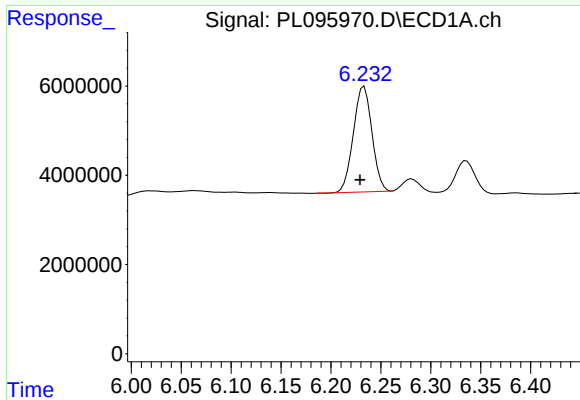

#12 4,4'-DDE


R.T.: 6.233 min
Delta R.T.: 0.004 min
Response: 30614271
Conc: 8.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

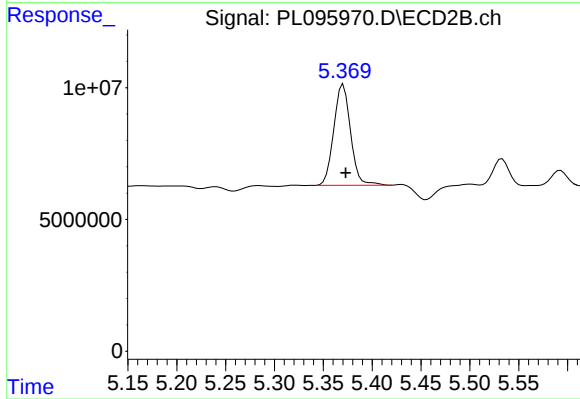


#12 4,4'-DDE

R.T.: 5.370 min
Delta R.T.: -0.002 min
Response: 46009266
Conc: 8.58 ng/ml

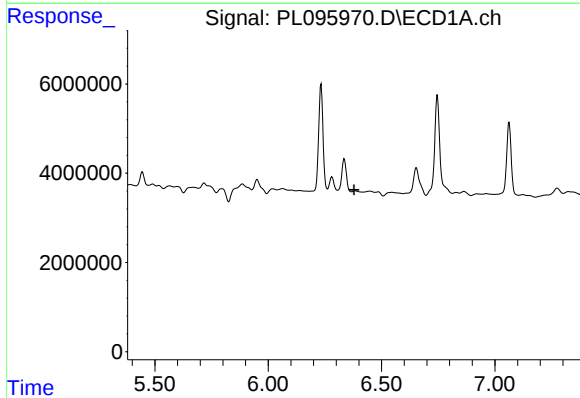


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

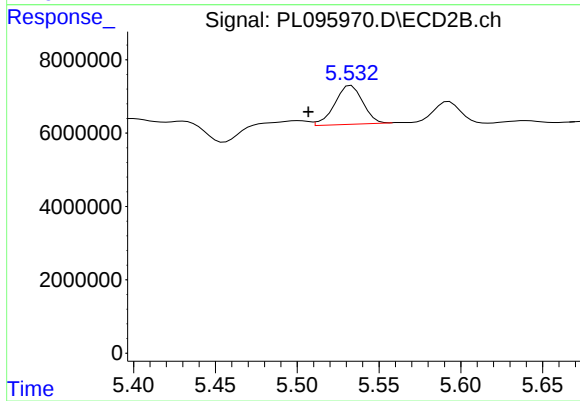

#13 Dieldrin


R.T.: 5.533 min
Delta R.T.: 0.026 min
Response: 12543198
Conc: 2.37 ng/ml

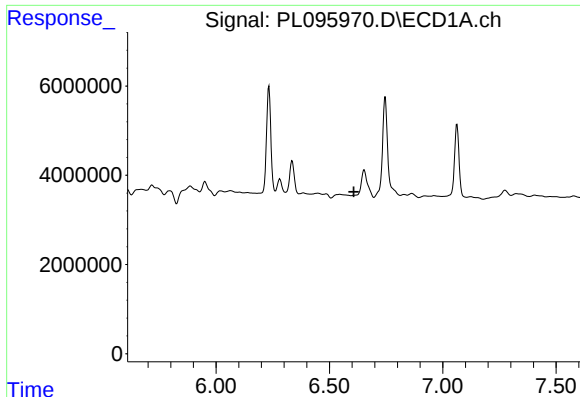

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.607 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

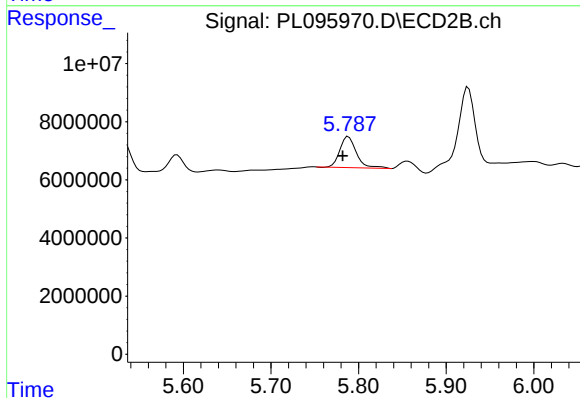


#14 Endrin

R.T.: 5.788 min
Delta R.T.: 0.007 min
Response: 14049682
Conc: 2.88 ng/ml

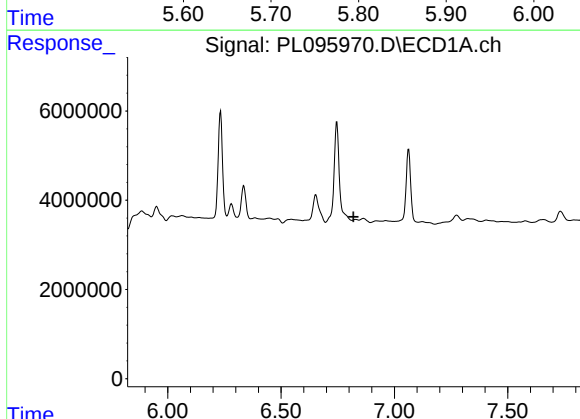


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.820 min
Response: 0
Conc: N.D.

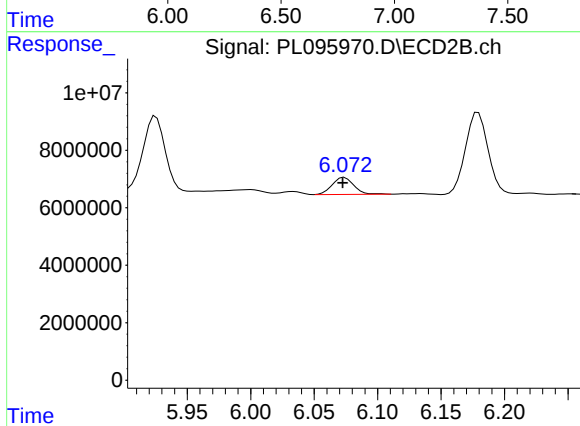

#15 Endosulfan II


R.T.: 6.074 min
Delta R.T.: 0.001 min
Response: 7008095
Conc: 1.47 ng/ml

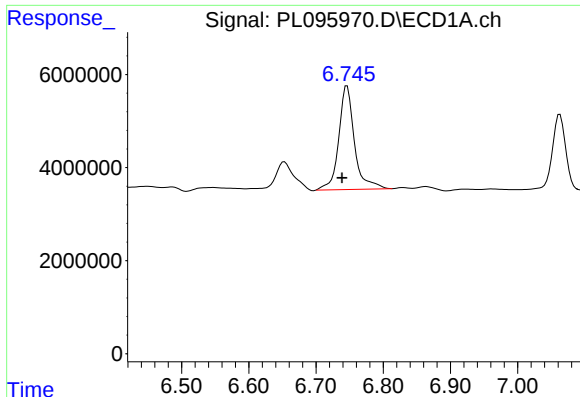

#16 4,4'-DDD


R.T.: 6.746 min
Delta R.T.: 0.007 min
Response: 36033423
Conc: 12.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

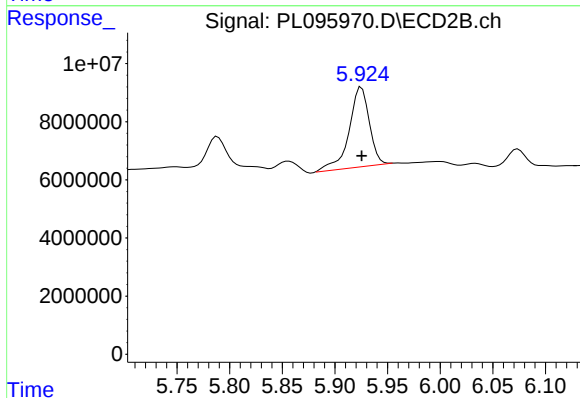


#16 4,4'-DDD

R.T.: 5.925 min
Delta R.T.: 0.000 min
Response: 36726190
Conc: 8.38 ng/ml

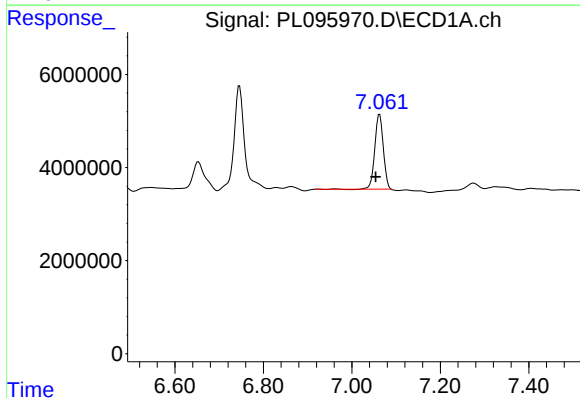


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: 0.009 min
Response: 21588869
Conc: 7.98 ng/ml

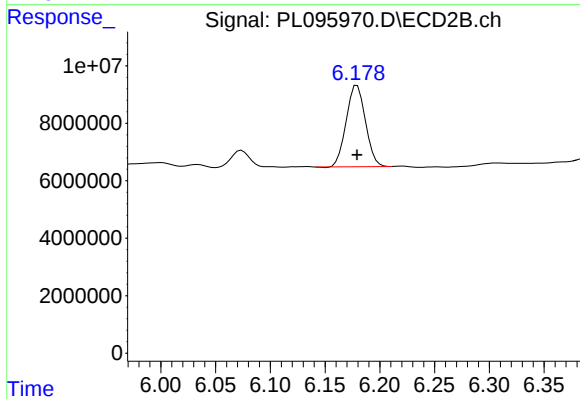

#17 4,4'-DDT


R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 34584562
Conc: 7.23 ng/ml

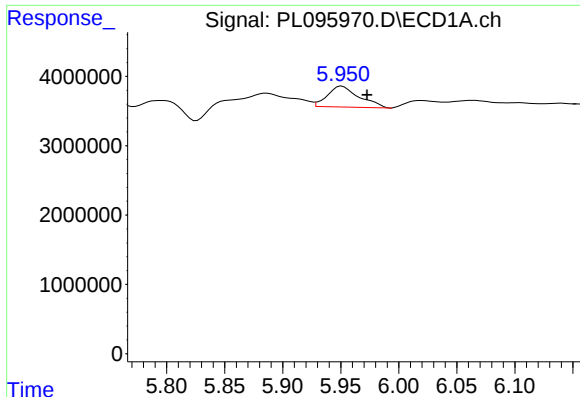

#25 Chlordane-3


R.T.: 5.951 min
Delta R.T.: -0.021 min
Response: 5682752
Conc: 7.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

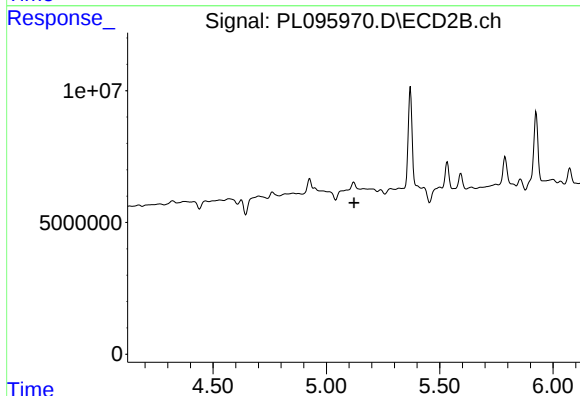


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

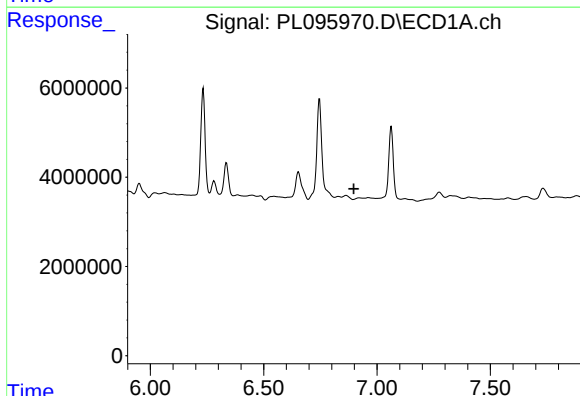


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.897 min
Response: 0
Conc: N.D.

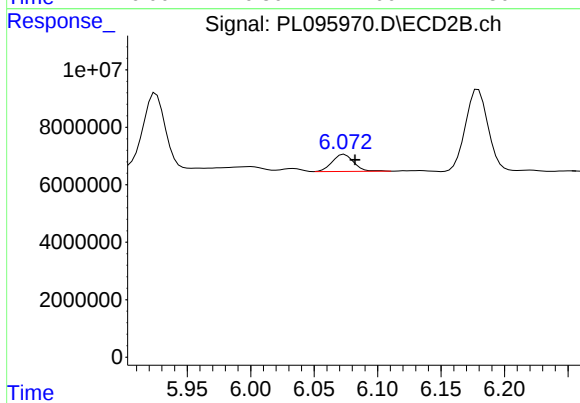

#27 Chlordane-5


R.T.: 6.074 min
Delta R.T.: -0.008 min
Response: 7008095
Conc: 27.49 ng/ml

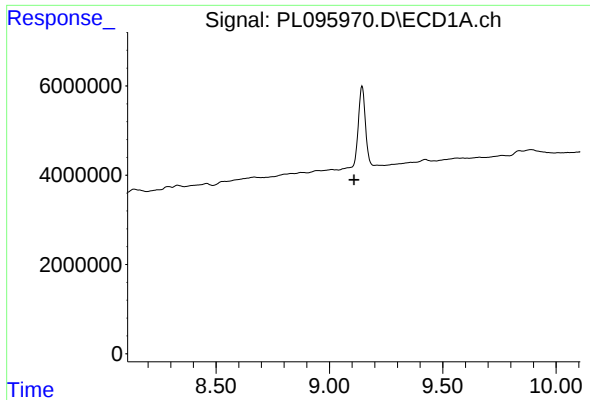

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

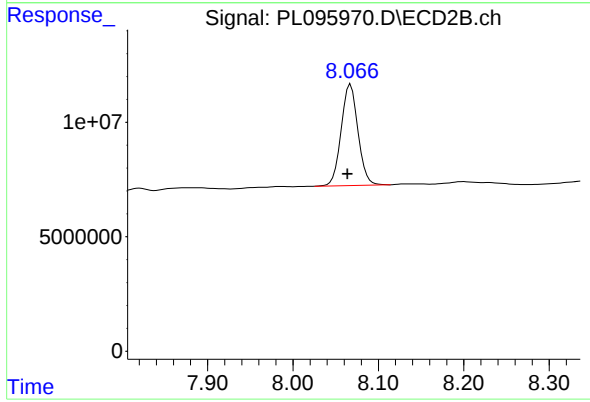

#28 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: 0.004 min
Response: 60581223
Conc: 13.85 ng/ml