

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060625\
 Data File : PL095971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2025 18:17
 Operator : AR\AJ
 Sample : Q2224-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 22:43:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.882	32318748	44069240	10.243	11.260
28)	SA Decachlor...	9.117	8.066	35478752	44283842	15.057	10.123 #
Target Compounds							
9)	A Endosulfan I	0.000	5.249	0	9046170	N.D.	1.898 #
10)	B gamma-Chl...	5.969	0.000	260427	0	0.067	N.D. #
11)	B alpha-Chl...	6.055	0.000	4172682	0	1.057	N.D. #
16)	A 4,4'-DDD	0.000	5.909f	0	10955540	N.D.	2.498 #
23)	Chlordane-1	0.000	3.891	0	10513421	N.D.	53.920 #
24)	Chlordane-2	0.000	4.510f	0	9891868	N.D.	44.407 #
25)	Chlordane-3	5.969	0.000	260427	0	0.352	N.D. #
26)	Chlordane-4	6.055	0.000	4172682	0	4.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060625\
Data File : PL095971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2025 18:17
Operator : AR\AJ
Sample : Q2224-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 22:43:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

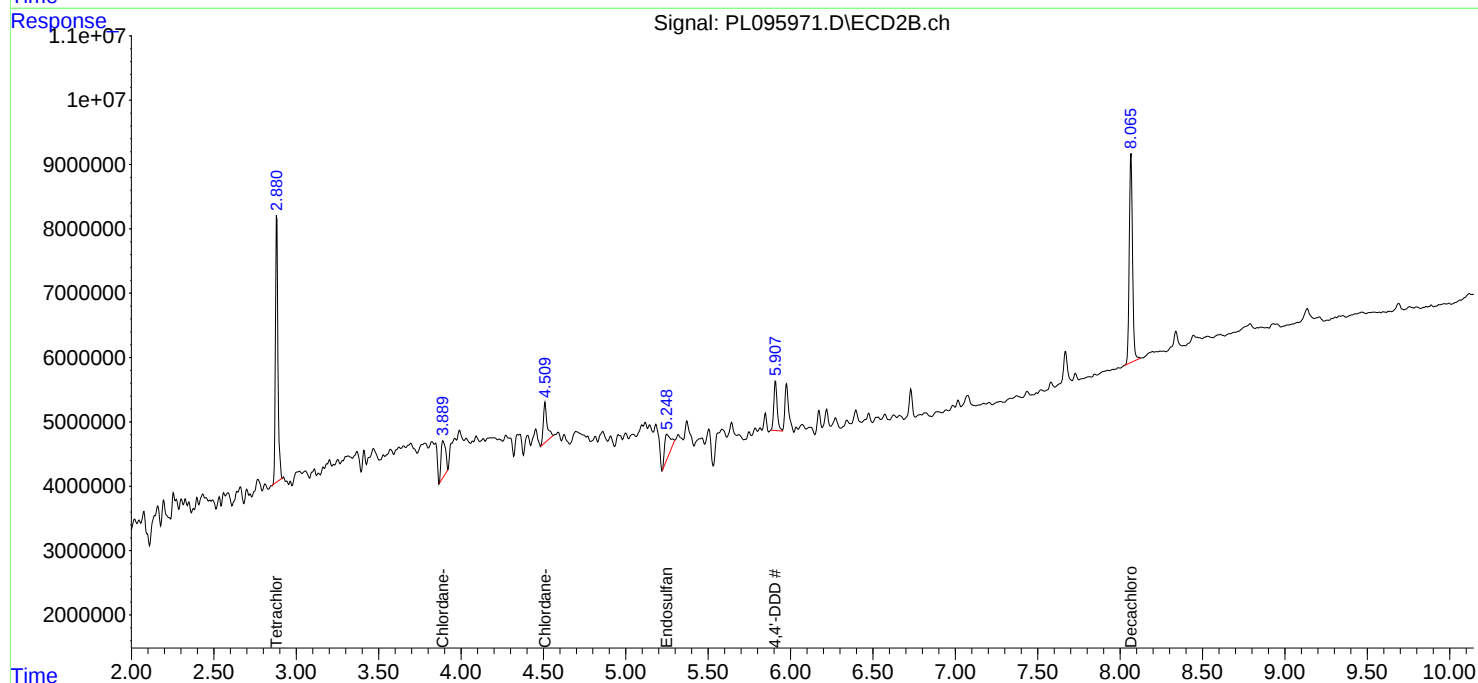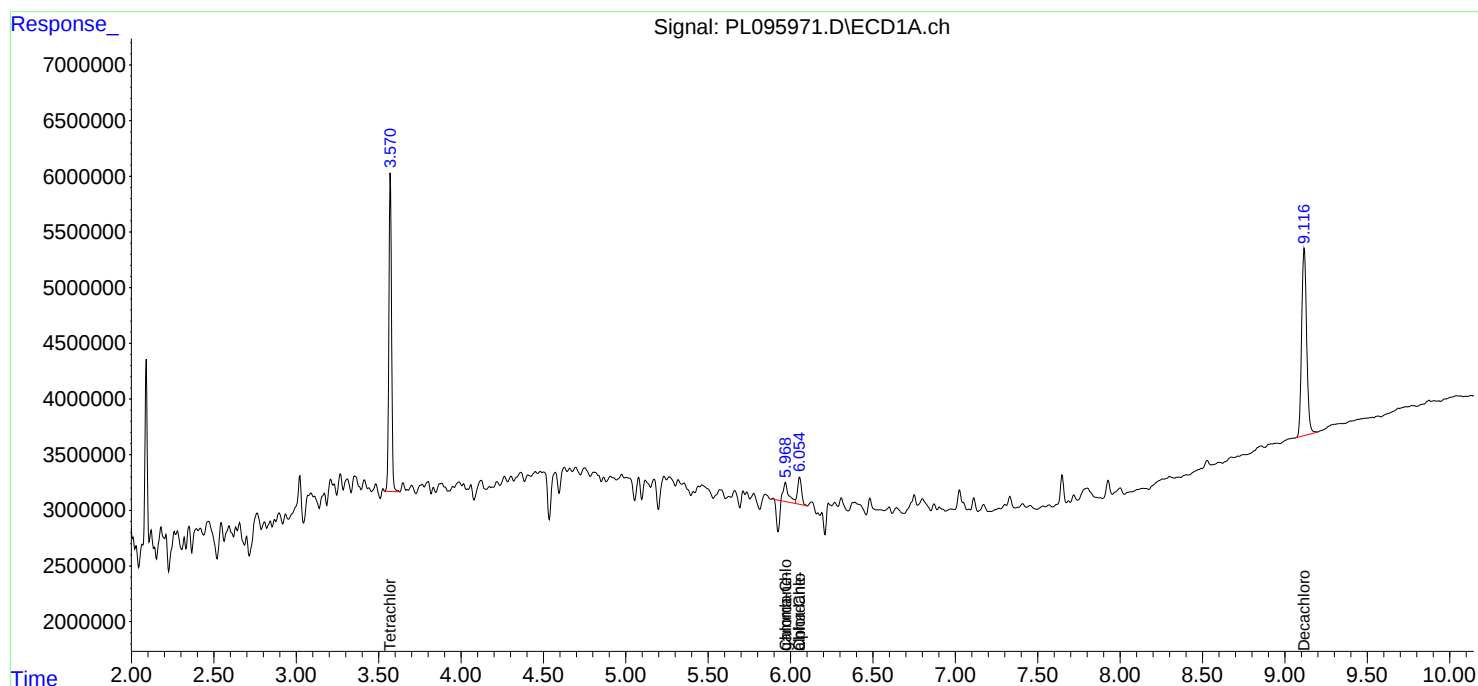


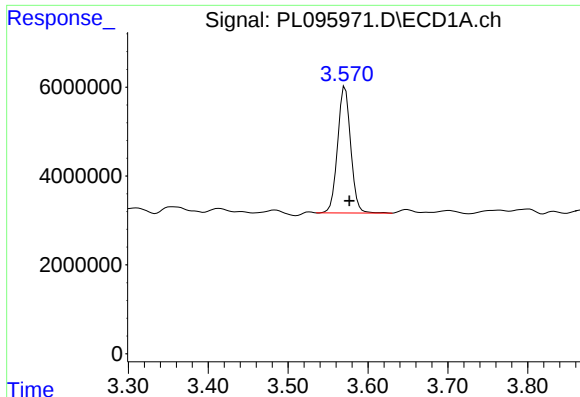

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: -0.006 min
Response: 32318748
Conc: 10.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

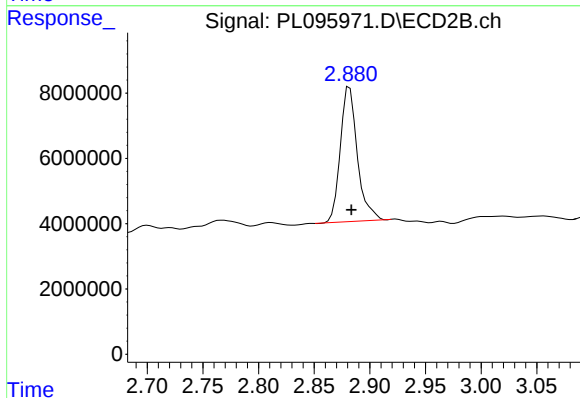


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: -0.002 min
Response: 44069240
Conc: 11.26 ng/ml

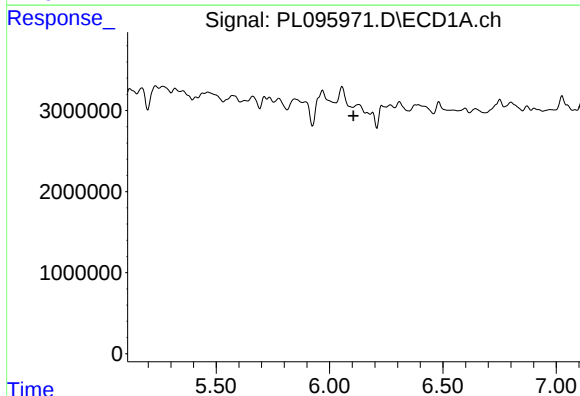


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.106 min
Response: 0
Conc: N.D.

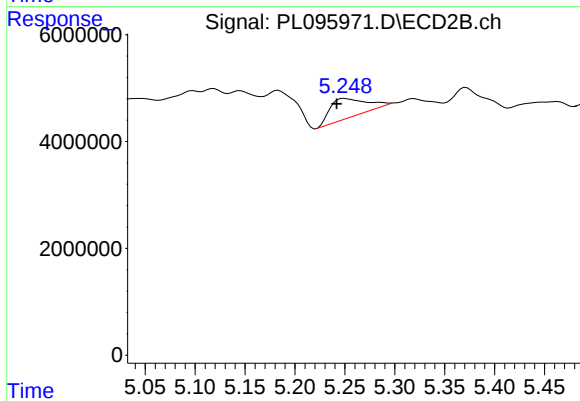

#9 Endosulfan I


R.T.: 5.249 min
Delta R.T.: 0.007 min
Response: 9046170
Conc: 1.90 ng/ml

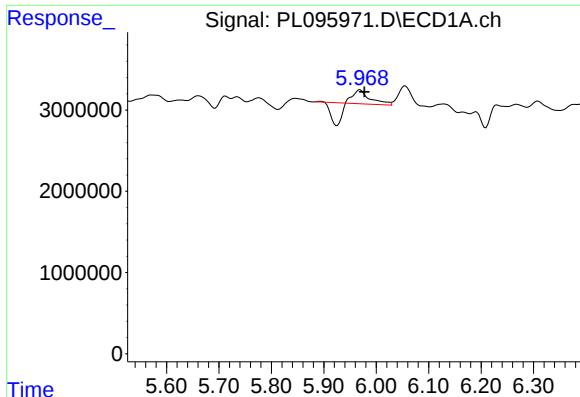

#10 gamma-Chlordane


R.T.: 5.969 min
Delta R.T.: -0.008 min
Response: 260427
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

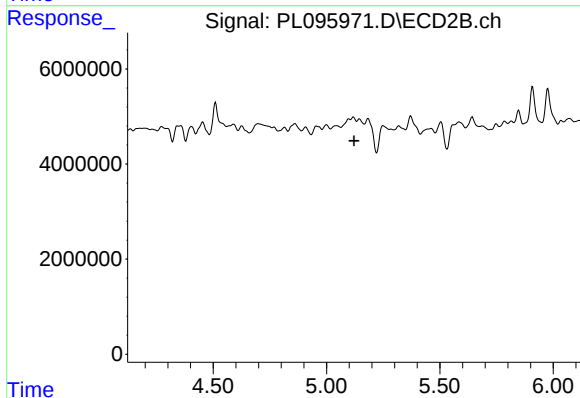


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.122 min
Response: 0
Conc: N.D.

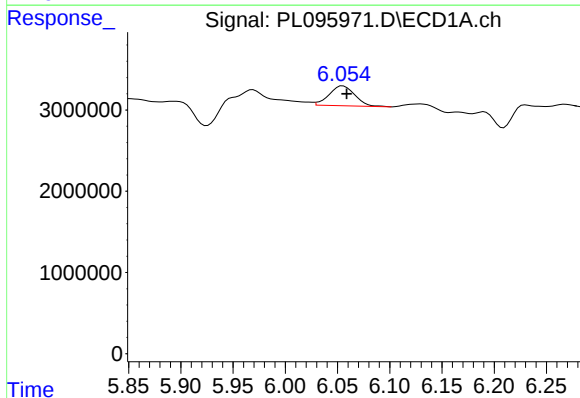


#11 alpha-Chlordane

R.T.: 6.055 min
Delta R.T.: -0.003 min
Response: 4172682
Conc: 1.06 ng/ml

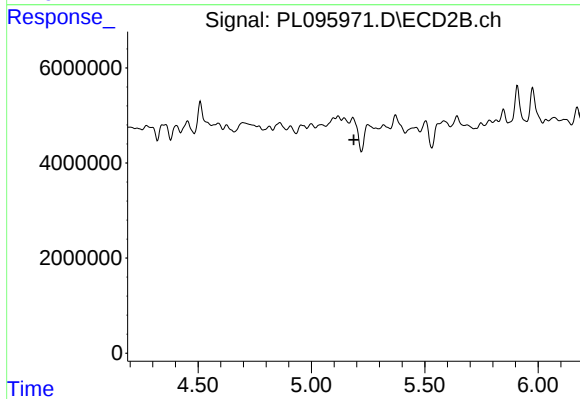

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.186 min
Response: 0
Conc: N.D.

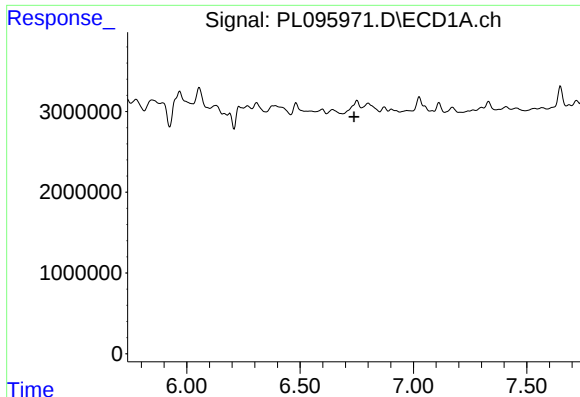

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.739 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

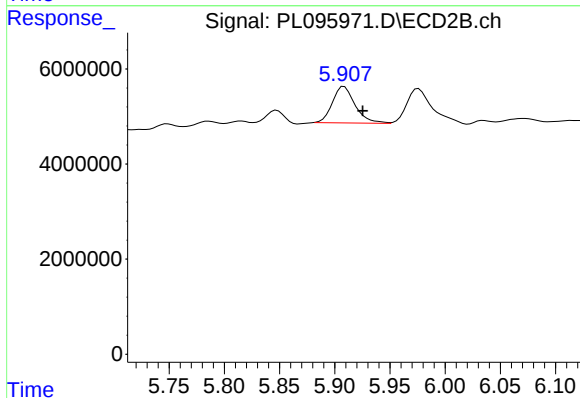


#16 4,4'-DDD

R.T.: 5.909 min
Delta R.T.: -0.017 min
Response: 10955540
Conc: 2.50 ng/ml

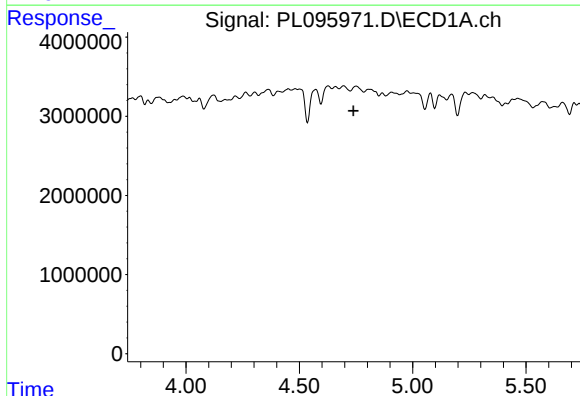


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.739 min
Response: 0
Conc: N.D.

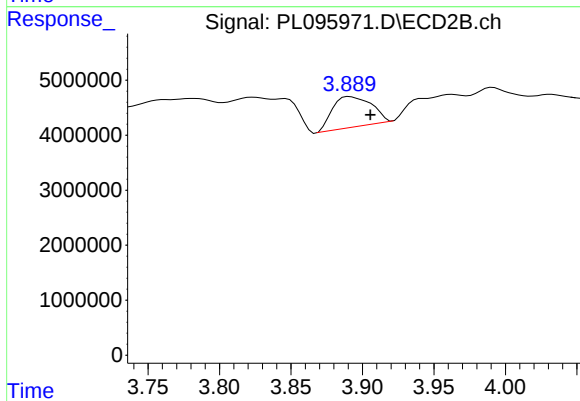

#23 Chlordane-1


R.T.: 3.891 min
Delta R.T.: -0.014 min
Response: 10513421
Conc: 53.92 ng/ml

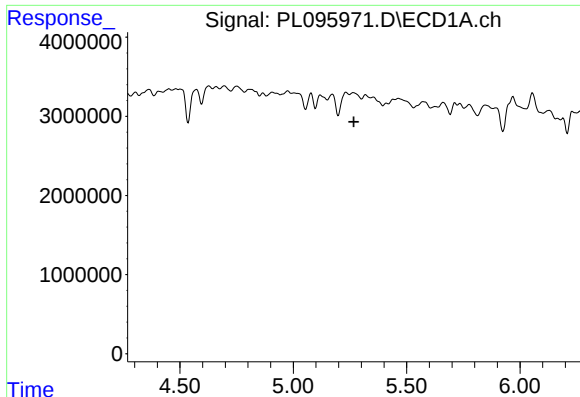

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

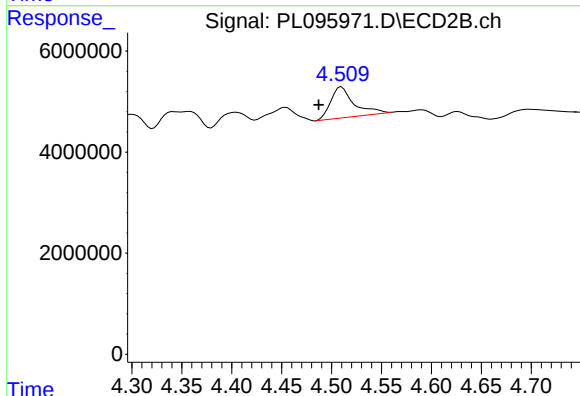


#24 Chlordane-2

R.T.: 4.510 min
Delta R.T.: 0.023 min
Response: 9891868
Conc: 44.41 ng/ml

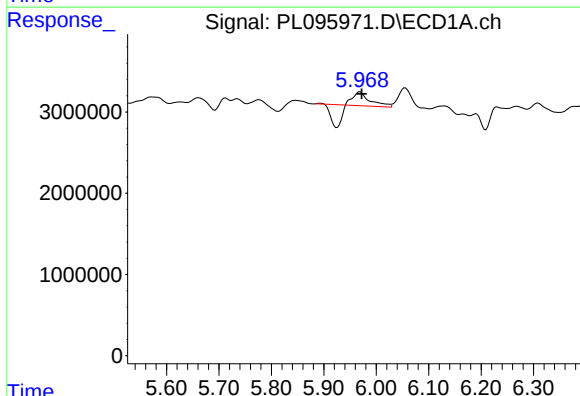


#25 Chlordane-3

R.T.: 5.969 min
Delta R.T.: -0.003 min
Response: 260427
Conc: 0.35 ng/ml

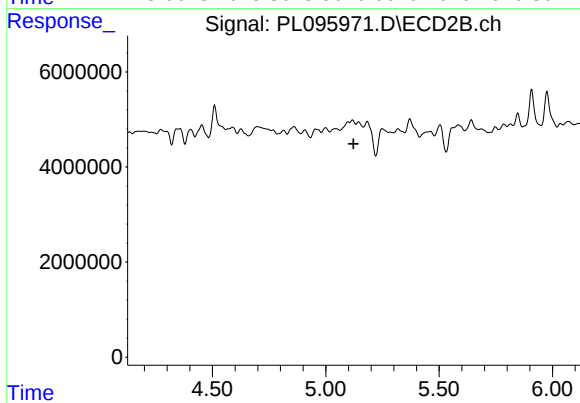

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

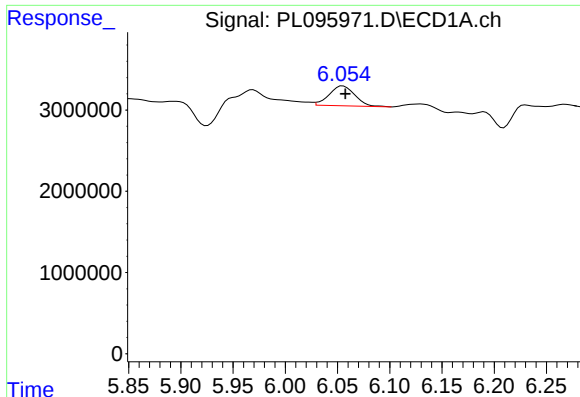

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: -0.002 min
Response: 4172682
Conc: 4.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

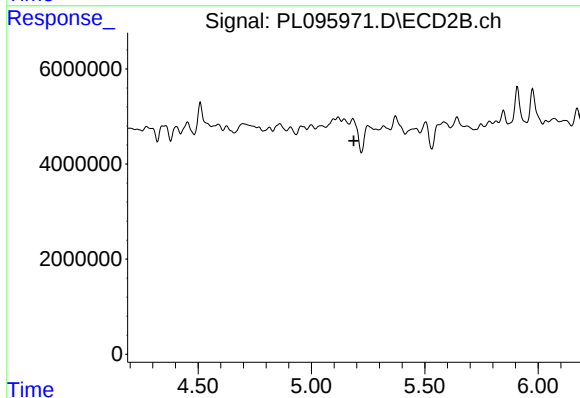


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

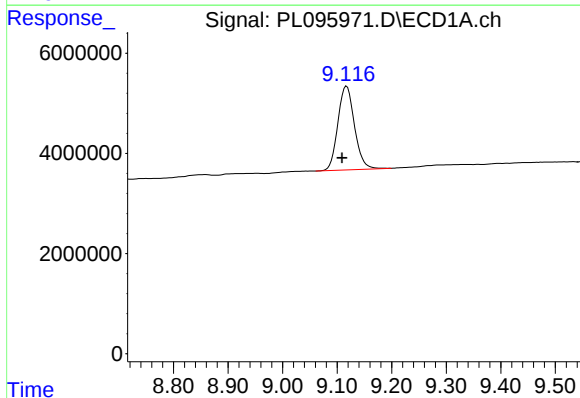

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.008 min
Response: 35478752
Conc: 15.06 ng/ml

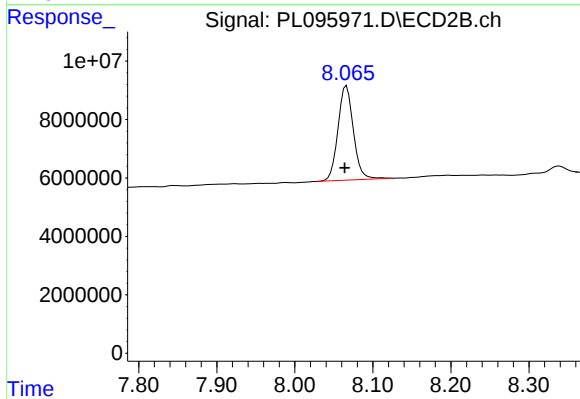

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.002 min
Response: 44283842
Conc: 10.12 ng/ml