

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
 Data File : PL067291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 14:58
 Operator : AR\AJ
 Sample : M2625-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:29:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	11858231	19634284	21.569	20.827
28)	SA Decachlor...	10.222	11.428	12458877	19585207	17.580	19.663
Target Compounds							
2)	A alpha-BHC	5.176	0.000	316842	0	0.431	N.D. #
4)	MA Heptachlor	5.992f	0.000	190687	0	0.253	N.D. #
6)	B beta-BHC	5.992	0.000	190687	0	0.533	N.D. #
7)	B delta-BHC	0.000	6.999f	0	1200057	N.D.	1.021 #
13)	MA Dieldrin	0.000	8.688	0	205906	N.D.	0.227 #
18)	B Endrin al...	8.378	0.000	1032156	0	2.039	N.D. #
19)	B Endosulfa...	8.591f	0.000	436980	0	0.688	N.D. #
21)	B Endrin ke...	9.129	10.005f	952733	439227	1.251	0.485 #
22)	Mirex	9.295	0.000	162632	0	0.258	N.D. #
24)	Chlordane-2	6.486	0.000	1204966	0	44.998	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
Data File : PL067291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 14:58
Operator : AR\AJ
Sample : M2625-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:29:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

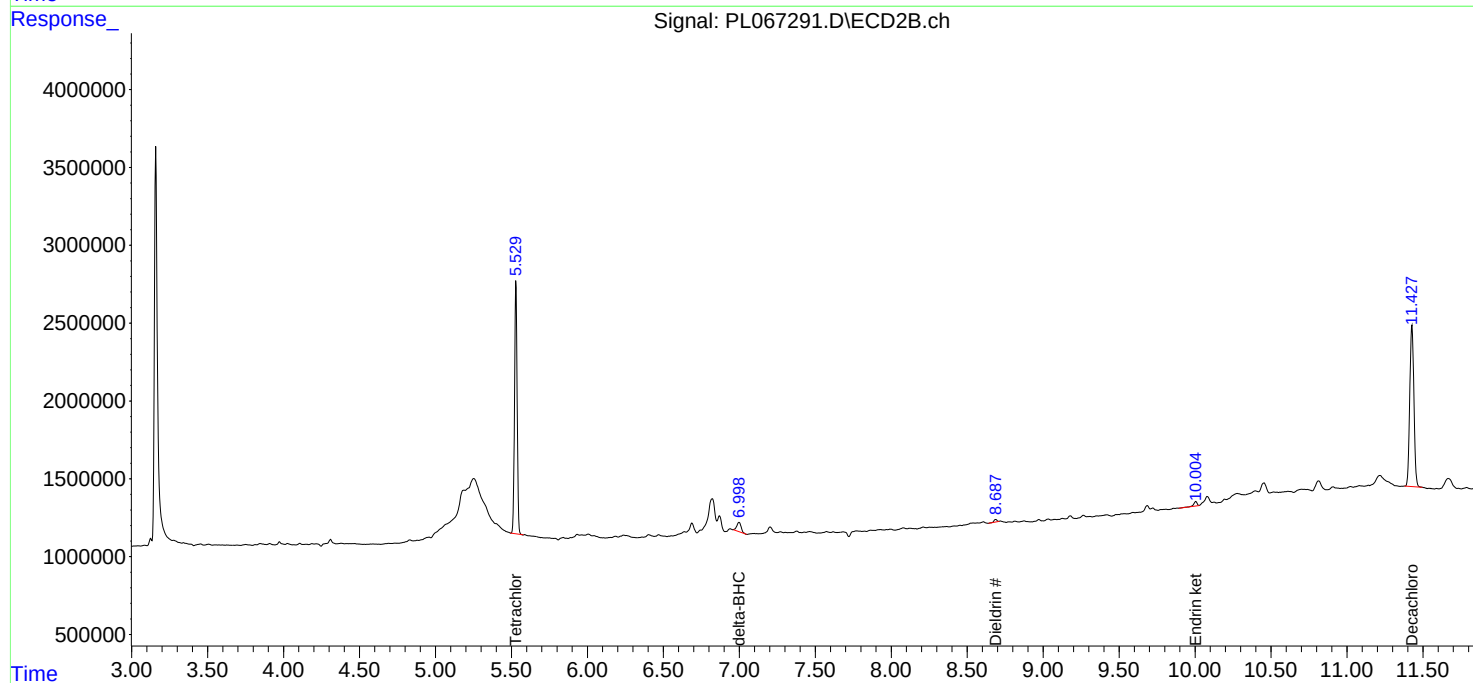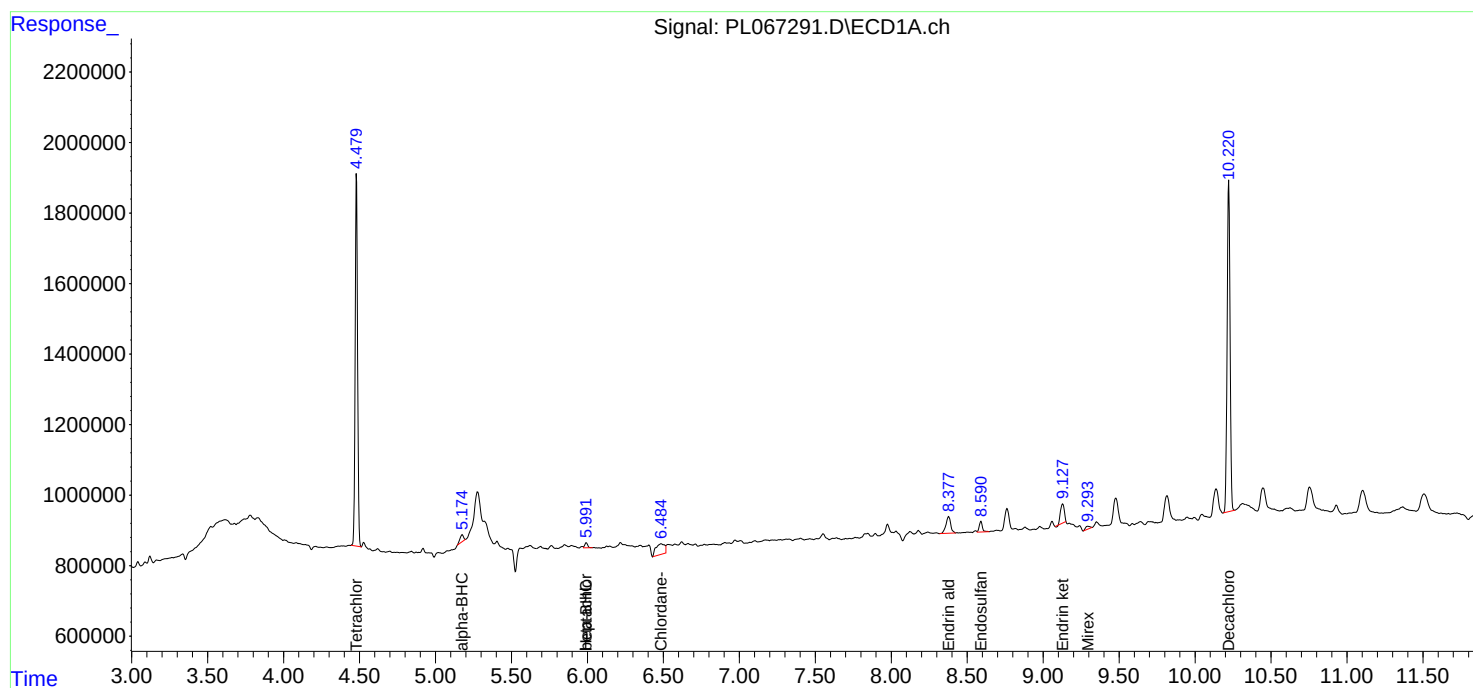


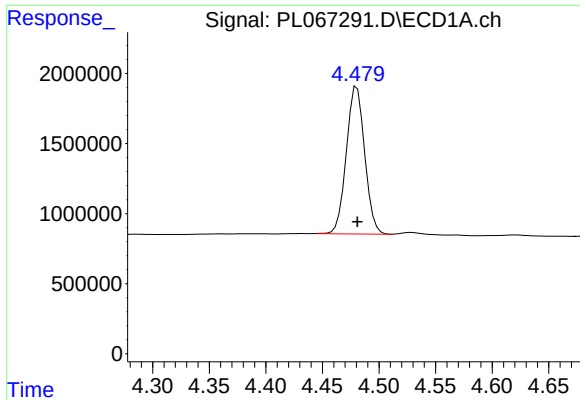

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 11858231
Conc: 21.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

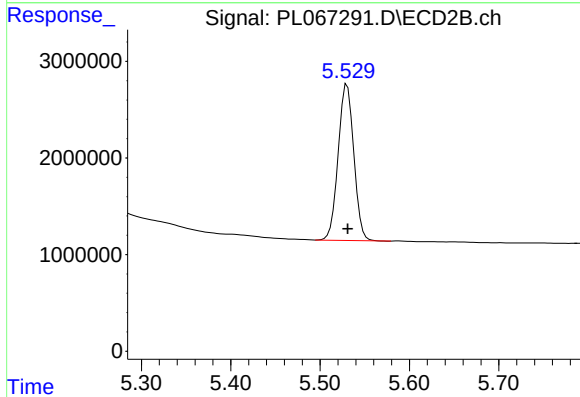


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 19634284
Conc: 20.83 ng/ml

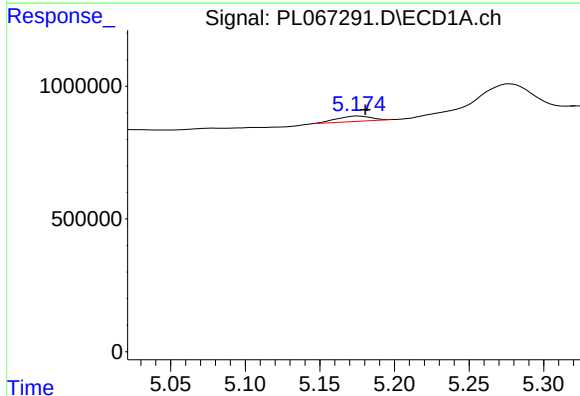


#2 alpha-BHC

R.T.: 5.176 min
Delta R.T.: -0.005 min
Response: 316842
Conc: 0.43 ng/ml

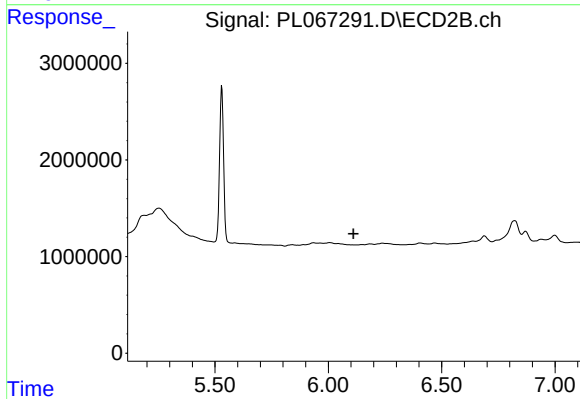

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

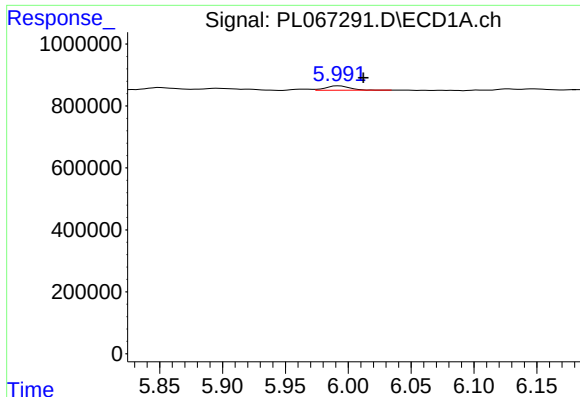

#4 Heptachlor


R.T.: 5.992 min
Delta R.T.: -0.020 min
Response: 190687
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

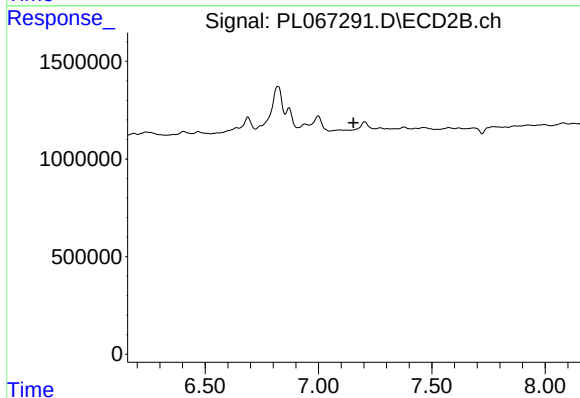


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

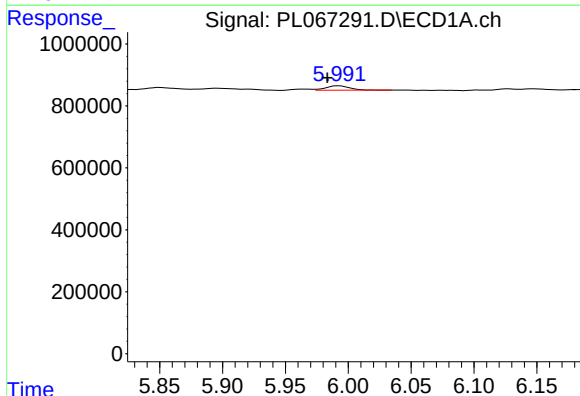


#6 beta-BHC

R.T.: 5.992 min
Delta R.T.: 0.009 min
Response: 190687
Conc: 0.53 ng/ml

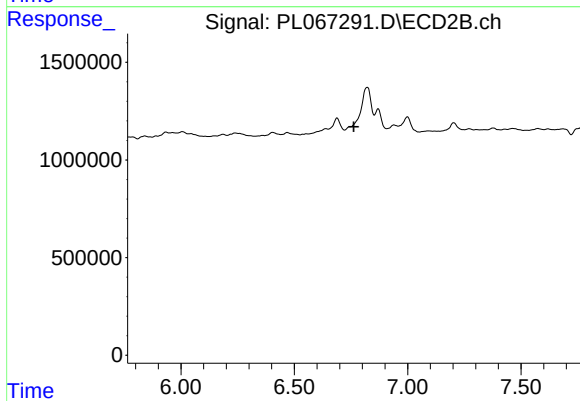

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

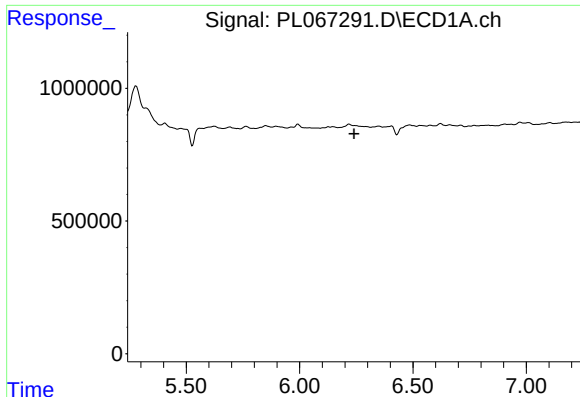

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

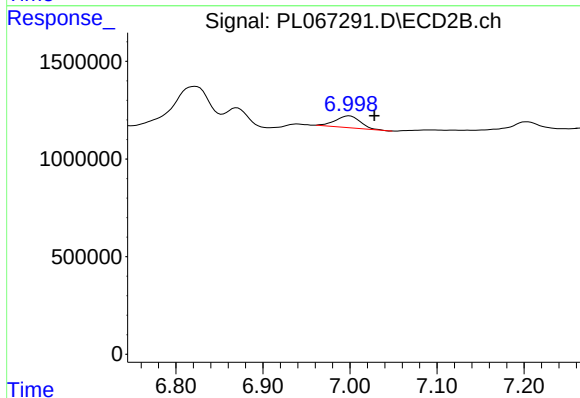


#7 delta-BHC

R.T.: 6.999 min
Delta R.T.: -0.029 min
Response: 1200057
Conc: 1.02 ng/ml

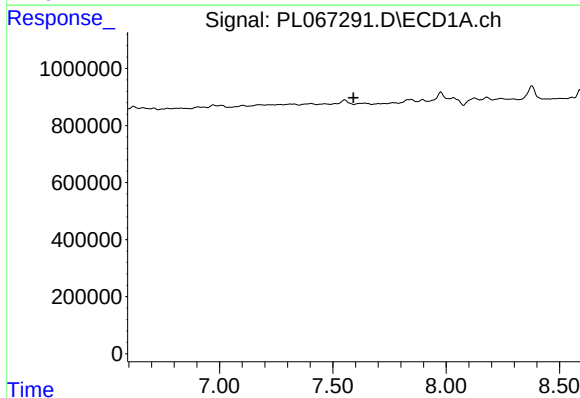


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

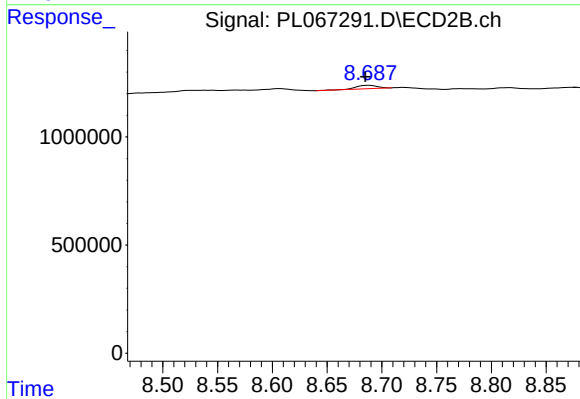

#13 Dieldrin


R.T.: 8.688 min
Delta R.T.: 0.003 min
Response: 205906
Conc: 0.23 ng/ml

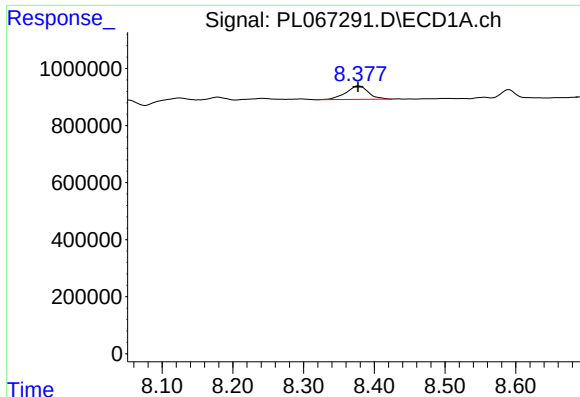

#18 Endrin aldehyde


R.T.: 8.378 min
Delta R.T.: 0.001 min
Response: 1032156
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

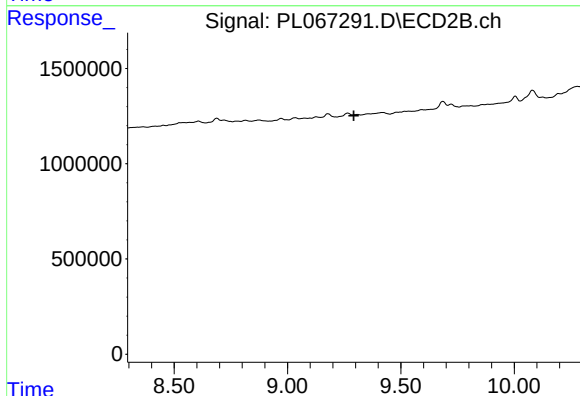


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

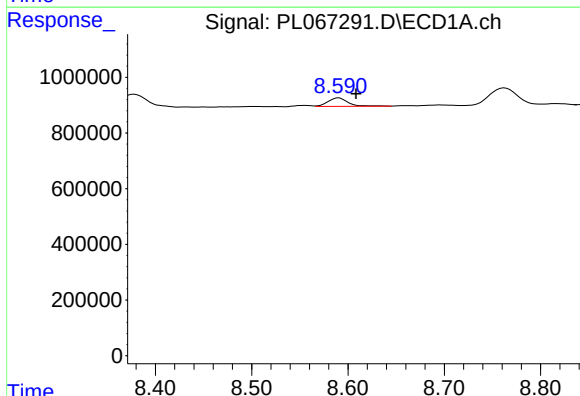


#19 Endosulfan Sulfate

R.T.: 8.591 min
Delta R.T.: -0.018 min
Response: 436980
Conc: 0.69 ng/ml

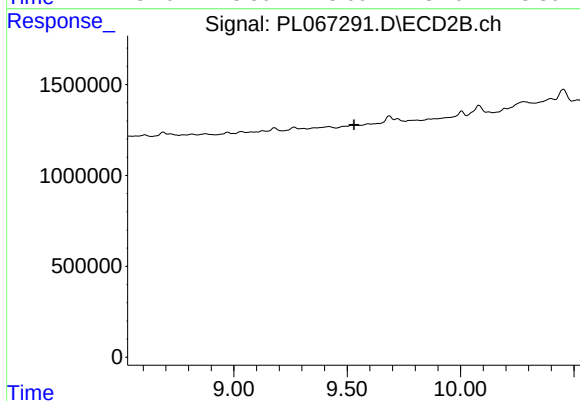

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

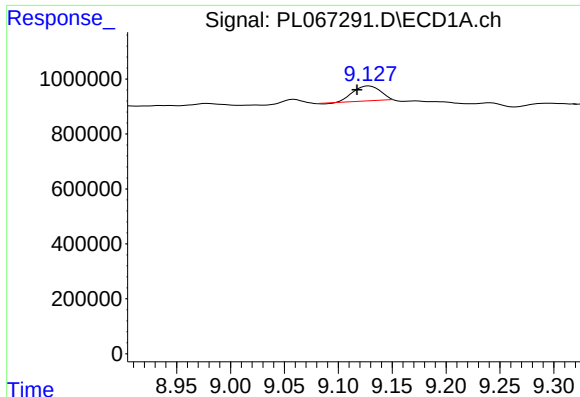

#21 Endrin ketone


R.T.: 9.129 min
Delta R.T.: 0.011 min
Response: 952733
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

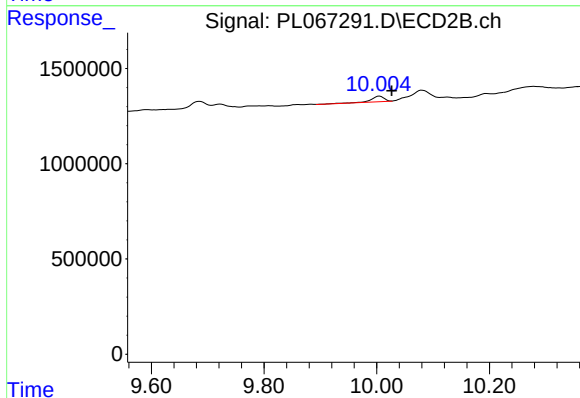


#21 Endrin ketone

R.T.: 10.005 min
Delta R.T.: -0.022 min
Response: 439227
Conc: 0.48 ng/ml

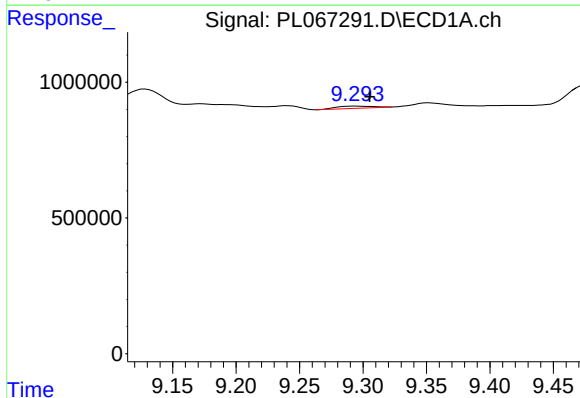


#22 Mirex

R.T.: 9.295 min
Delta R.T.: -0.010 min
Response: 162632
Conc: 0.26 ng/ml

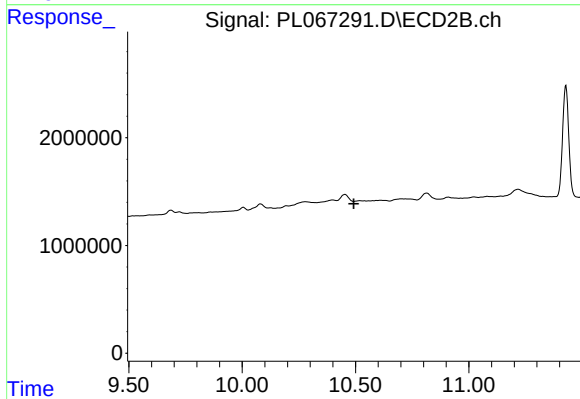

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.492 min
Response: 0
Conc: N.D.

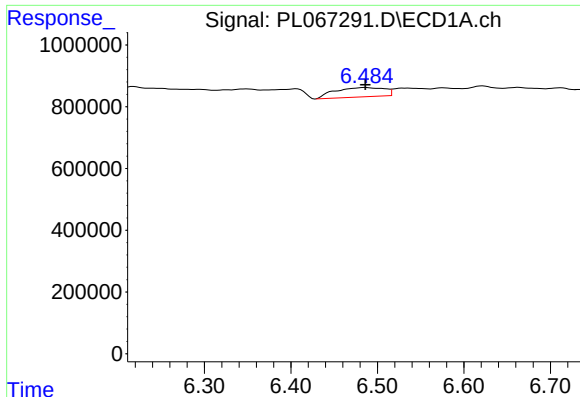

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 1204966
Conc: 45.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

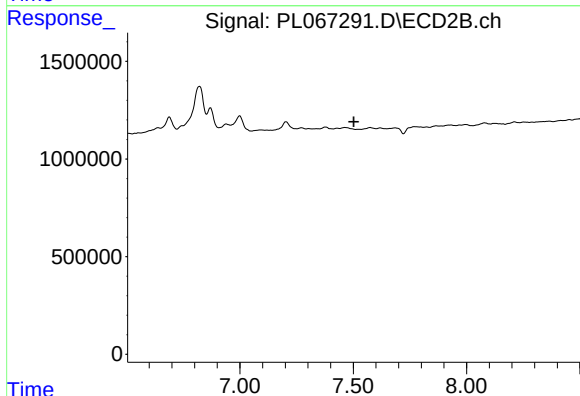


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

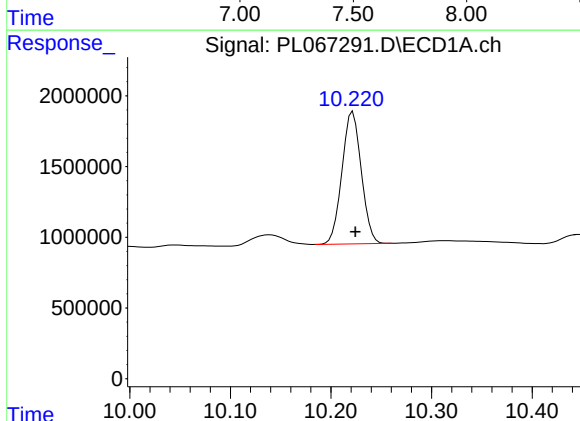

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.003 min
Response: 12458877
Conc: 17.58 ng/ml

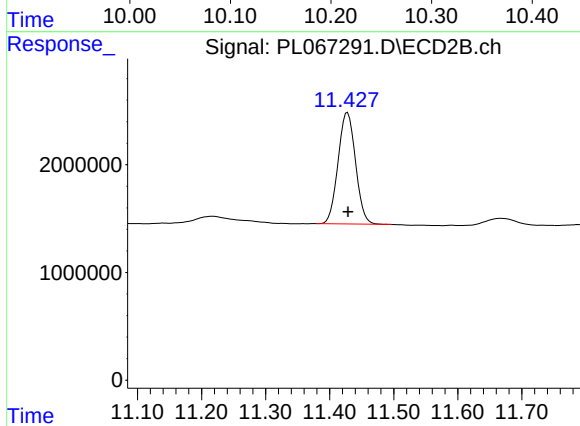

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 19585207
Conc: 19.66 ng/ml