

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
 Data File : PL067292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 15:14
 Operator : AR\AJ
 Sample : M2625-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:29:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.530	11398496	18777942	20.733	19.919
28)	SA Decachlor...	10.222	11.428	13005142	20181112	18.351	20.261
Target Compounds							
2)	A alpha-BHC	5.203f	0.000	167997	0	0.228	N.D. #
8)	B Heptachlo...	0.000	7.995	0	1446623	N.D.	1.444 #
15)	B Endosulfa...	8.177	9.181f	495982	845668	0.805	1.061 #
18)	B Endrin al...	8.378	0.000	507145	0	1.002	N.D. #
20)	A Methoxychlor	8.884f	9.860	1719003	1770183	4.836	4.553
21)	B Endrin ke...	9.126	10.041	461145	1669981	0.606	1.842 #
24)	Chlordane-2	6.470f	0.000	1944758	0	72.625	N.D. #
27)	Chlordane-5	8.177	0.000	495982	0	22.669	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
Data File : PL067292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 15:14
Operator : AR\AJ
Sample : M2625-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:29:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

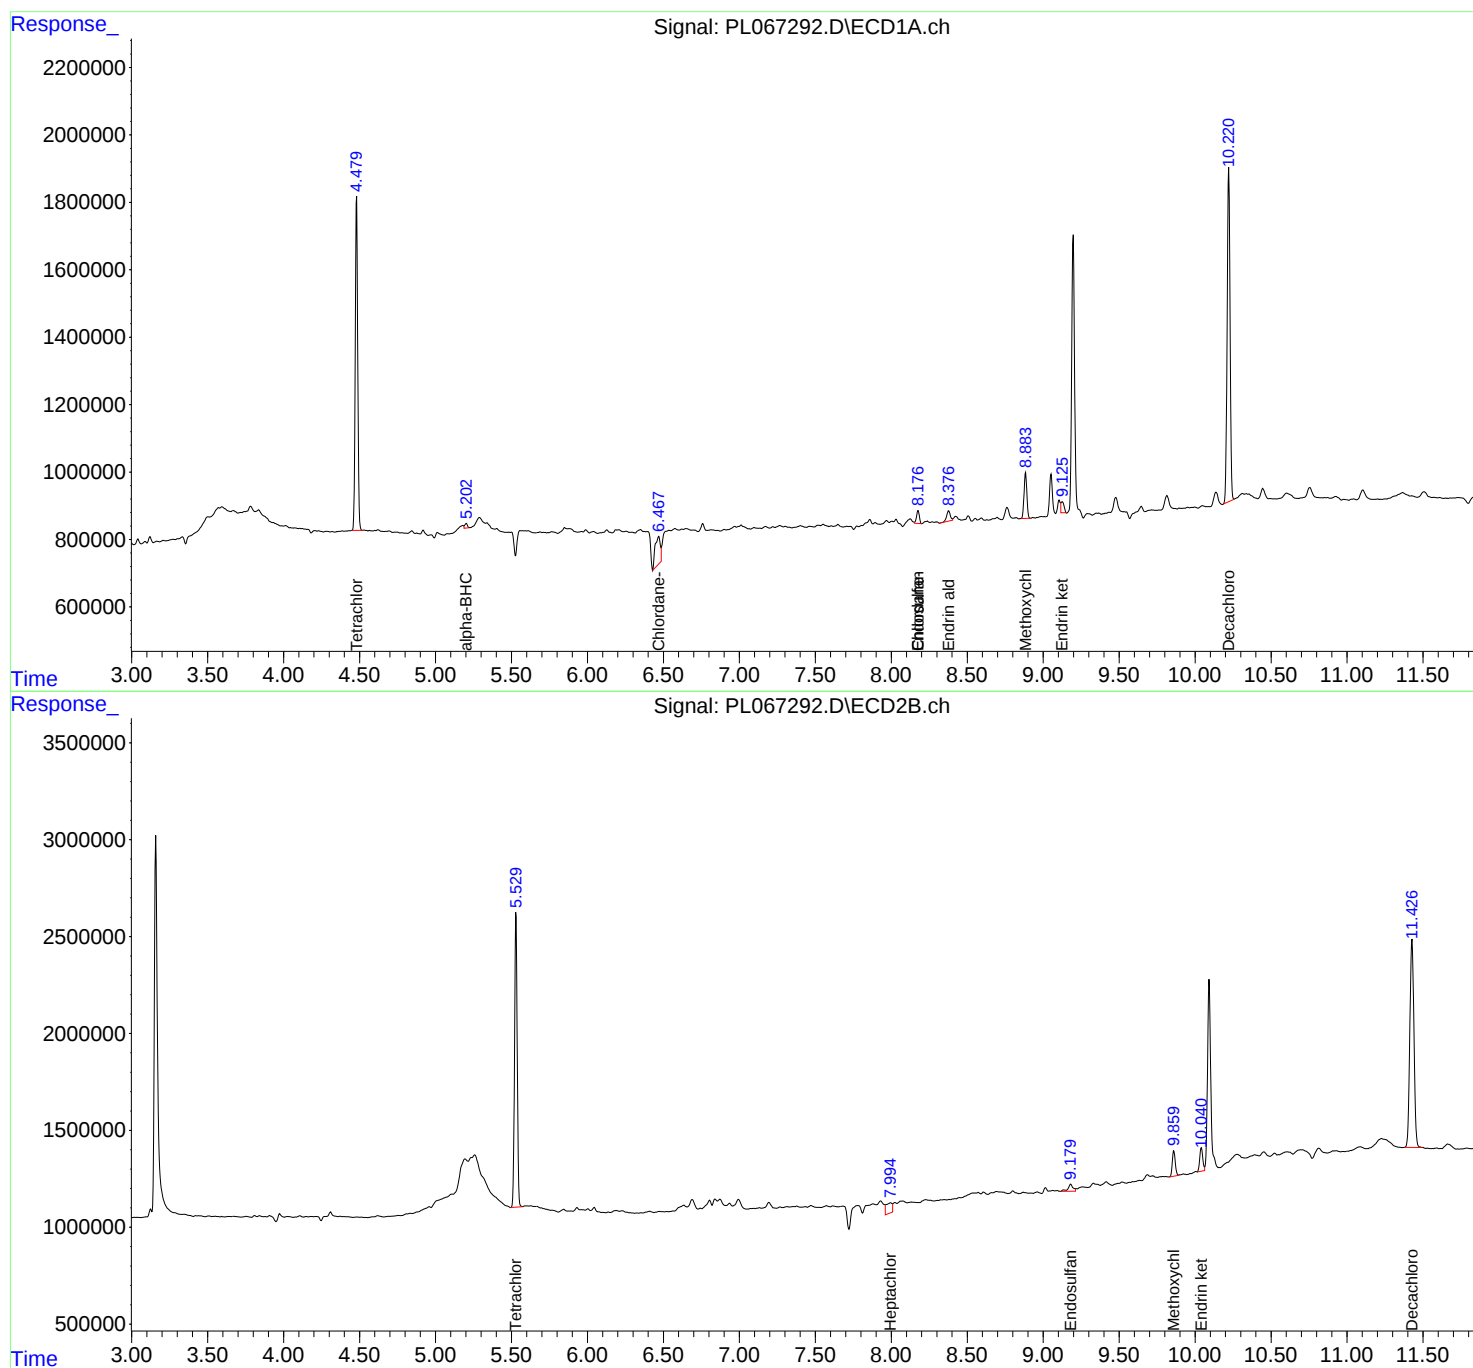


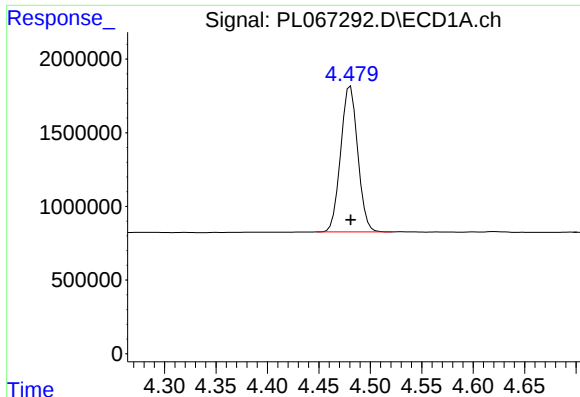

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 11398496
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

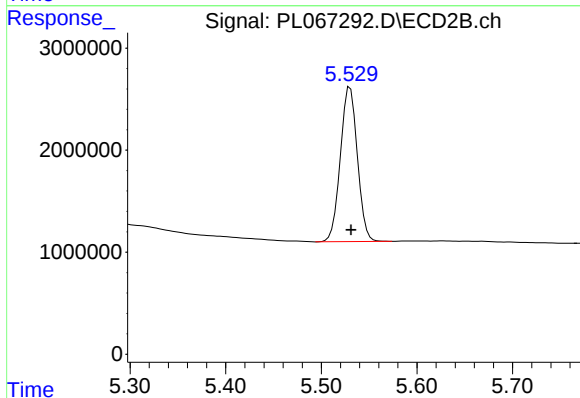


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 18777942
Conc: 19.92 ng/ml

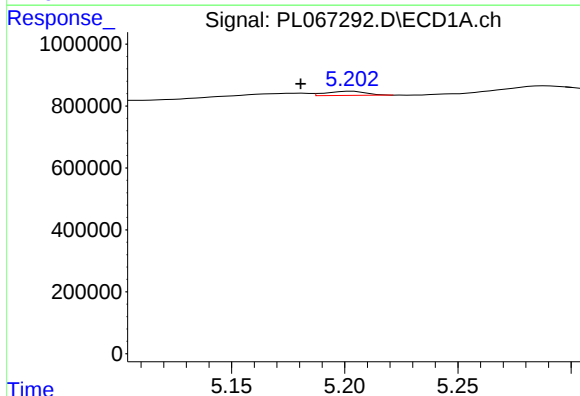


#2 alpha-BHC

R.T.: 5.203 min
Delta R.T.: 0.023 min
Response: 167997
Conc: 0.23 ng/ml

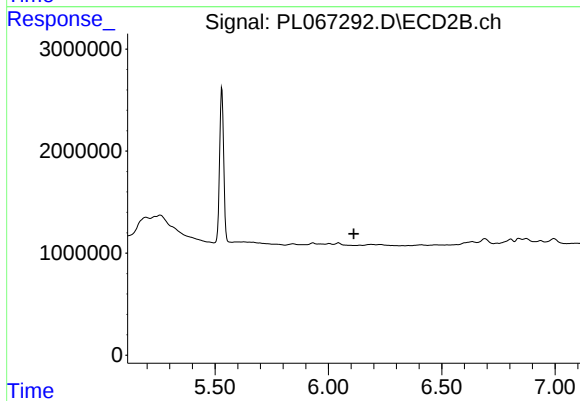

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

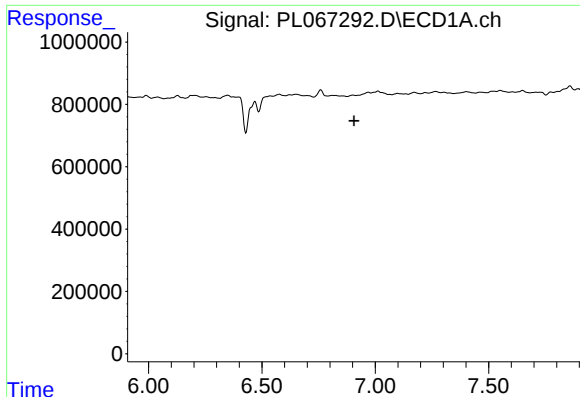

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

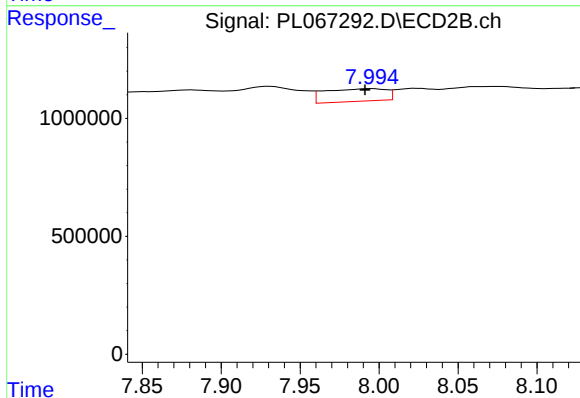


#8 Heptachlor epoxide

R.T.: 7.995 min
Delta R.T.: 0.004 min
Response: 1446623
Conc: 1.44 ng/ml

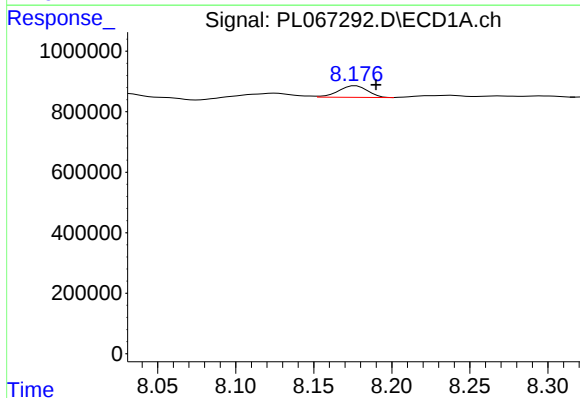


#15 Endosulfan II

R.T.: 8.177 min
Delta R.T.: -0.013 min
Response: 495982
Conc: 0.81 ng/ml

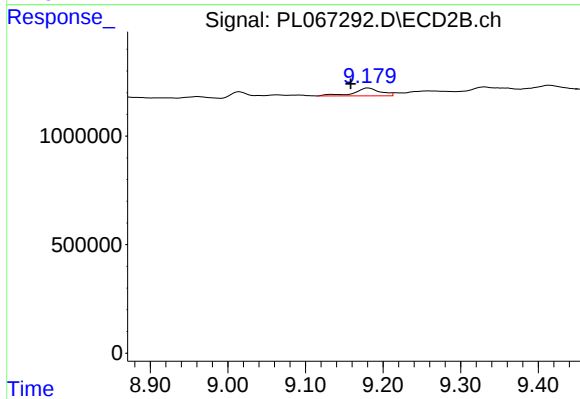

#15 Endosulfan II


R.T.: 9.181 min
Delta R.T.: 0.023 min
Response: 845668
Conc: 1.06 ng/ml

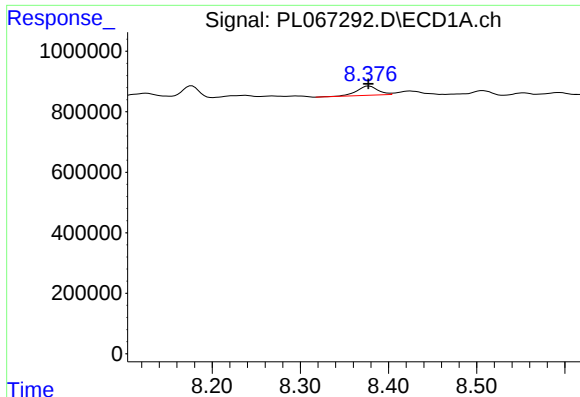

#18 Endrin aldehyde


R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 507145
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

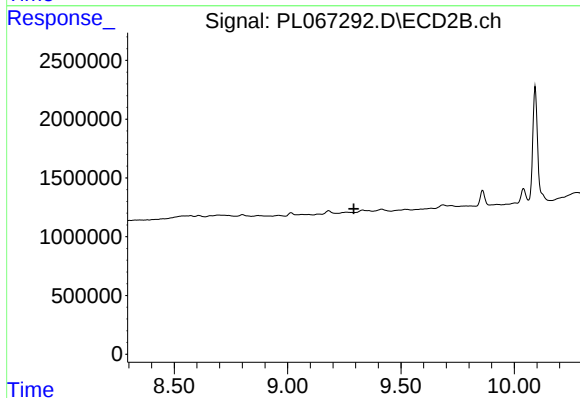


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

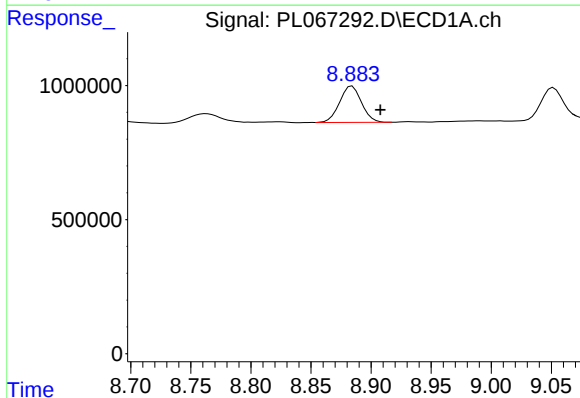


#20 Methoxychlor

R.T.: 8.884 min
Delta R.T.: -0.023 min
Response: 1719003
Conc: 4.84 ng/ml

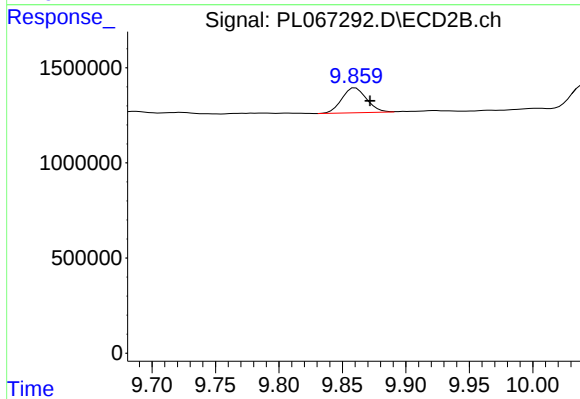

#20 Methoxychlor


R.T.: 9.860 min
Delta R.T.: -0.012 min
Response: 1770183
Conc: 4.55 ng/ml

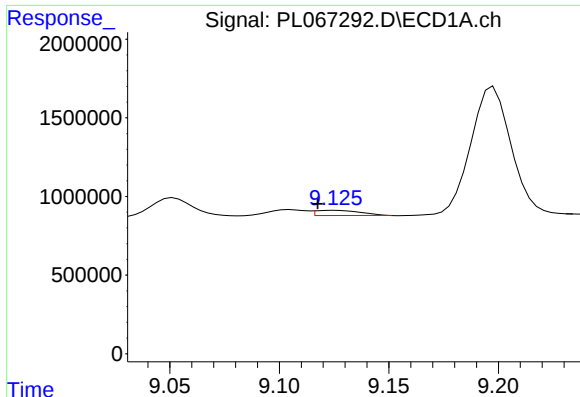

#21 Endrin ketone


R.T.: 9.126 min
Delta R.T.: 0.008 min
Response: 461145
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

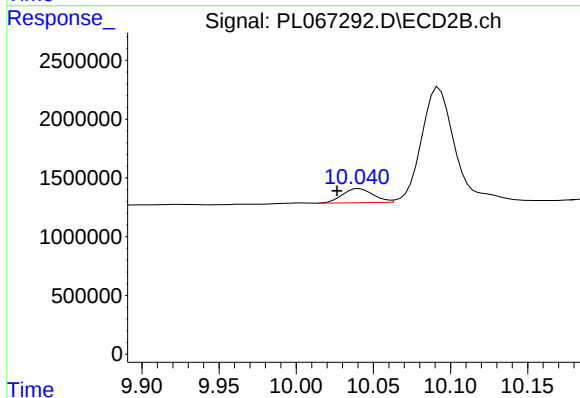


#21 Endrin ketone

R.T.: 10.041 min
Delta R.T.: 0.014 min
Response: 1669981
Conc: 1.84 ng/ml

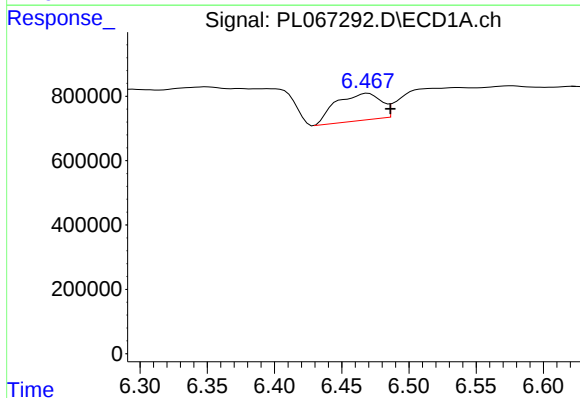


#24 Chlordane-2

R.T.: 6.470 min
Delta R.T.: -0.017 min
Response: 1944758
Conc: 72.62 ng/ml

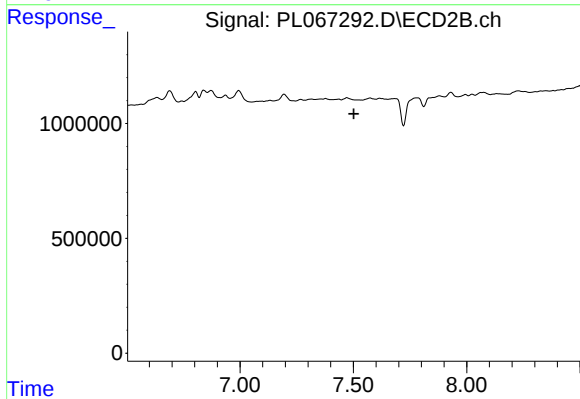

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

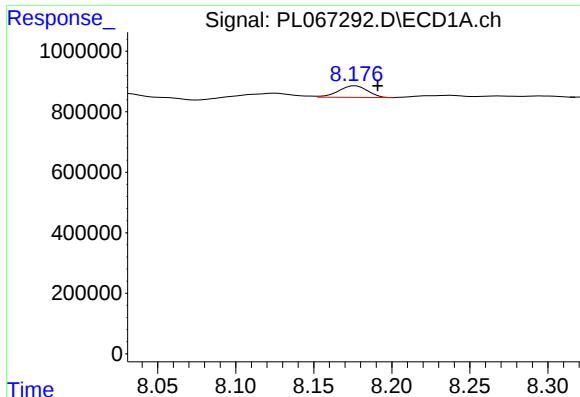

#27 Chlordane-5


R.T.: 8.177 min
Delta R.T.: -0.014 min
Response: 495982
Conc: 22.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

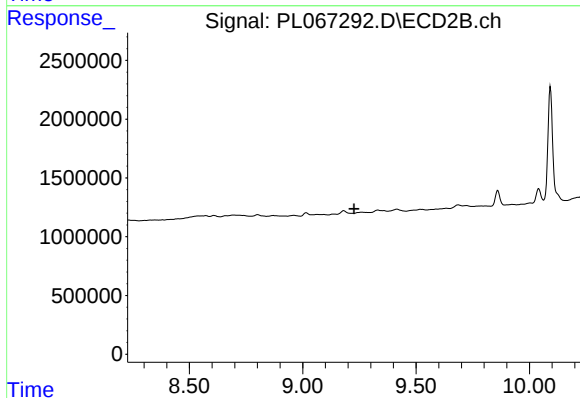


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

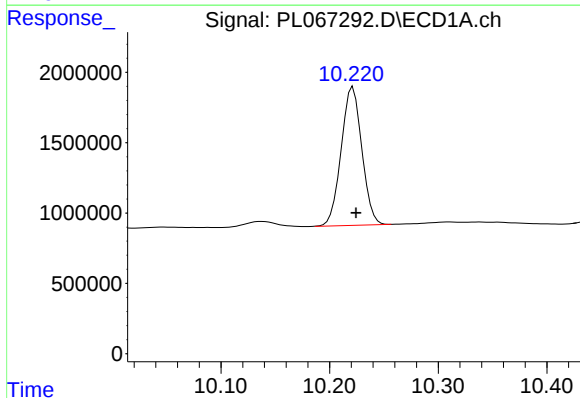

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.003 min
Response: 13005142
Conc: 18.35 ng/ml

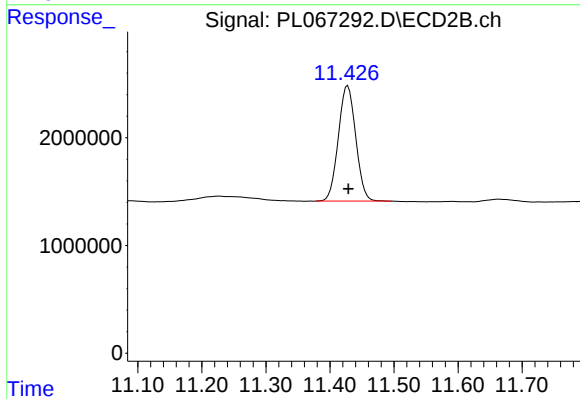

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 20181112
Conc: 20.26 ng/ml