

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
 Data File : PL067294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 15:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:29:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	10883806	18006680	19.796	19.100
28)	SA Decachlor...	10.222	11.428	12941062	20181265	18.261	20.261
Target Compounds							
4)	MA Heptachlor	5.990f	0.000	450840	0	0.598	N.D. #
6)	B beta-BHC	5.990	0.000	450840	0	1.260	N.D. #
7)	B delta-BHC	0.000	7.002f	0	1830651	N.D.	1.557 #
8)	B Heptachlo...	0.000	7.997	0	2090069	N.D.	2.086 #
14)	MA Endrin	7.896f	0.000	275726	0	0.421	N.D. #
18)	B Endrin al...	8.379	0.000	435569	0	0.860	N.D. #
21)	B Endrin ke...	9.125	0.000	118520	0	0.156	N.D. #
24)	Chlordane-2	6.488	0.000	1783196	0	66.591	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
Data File : PL067294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 15:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:29:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

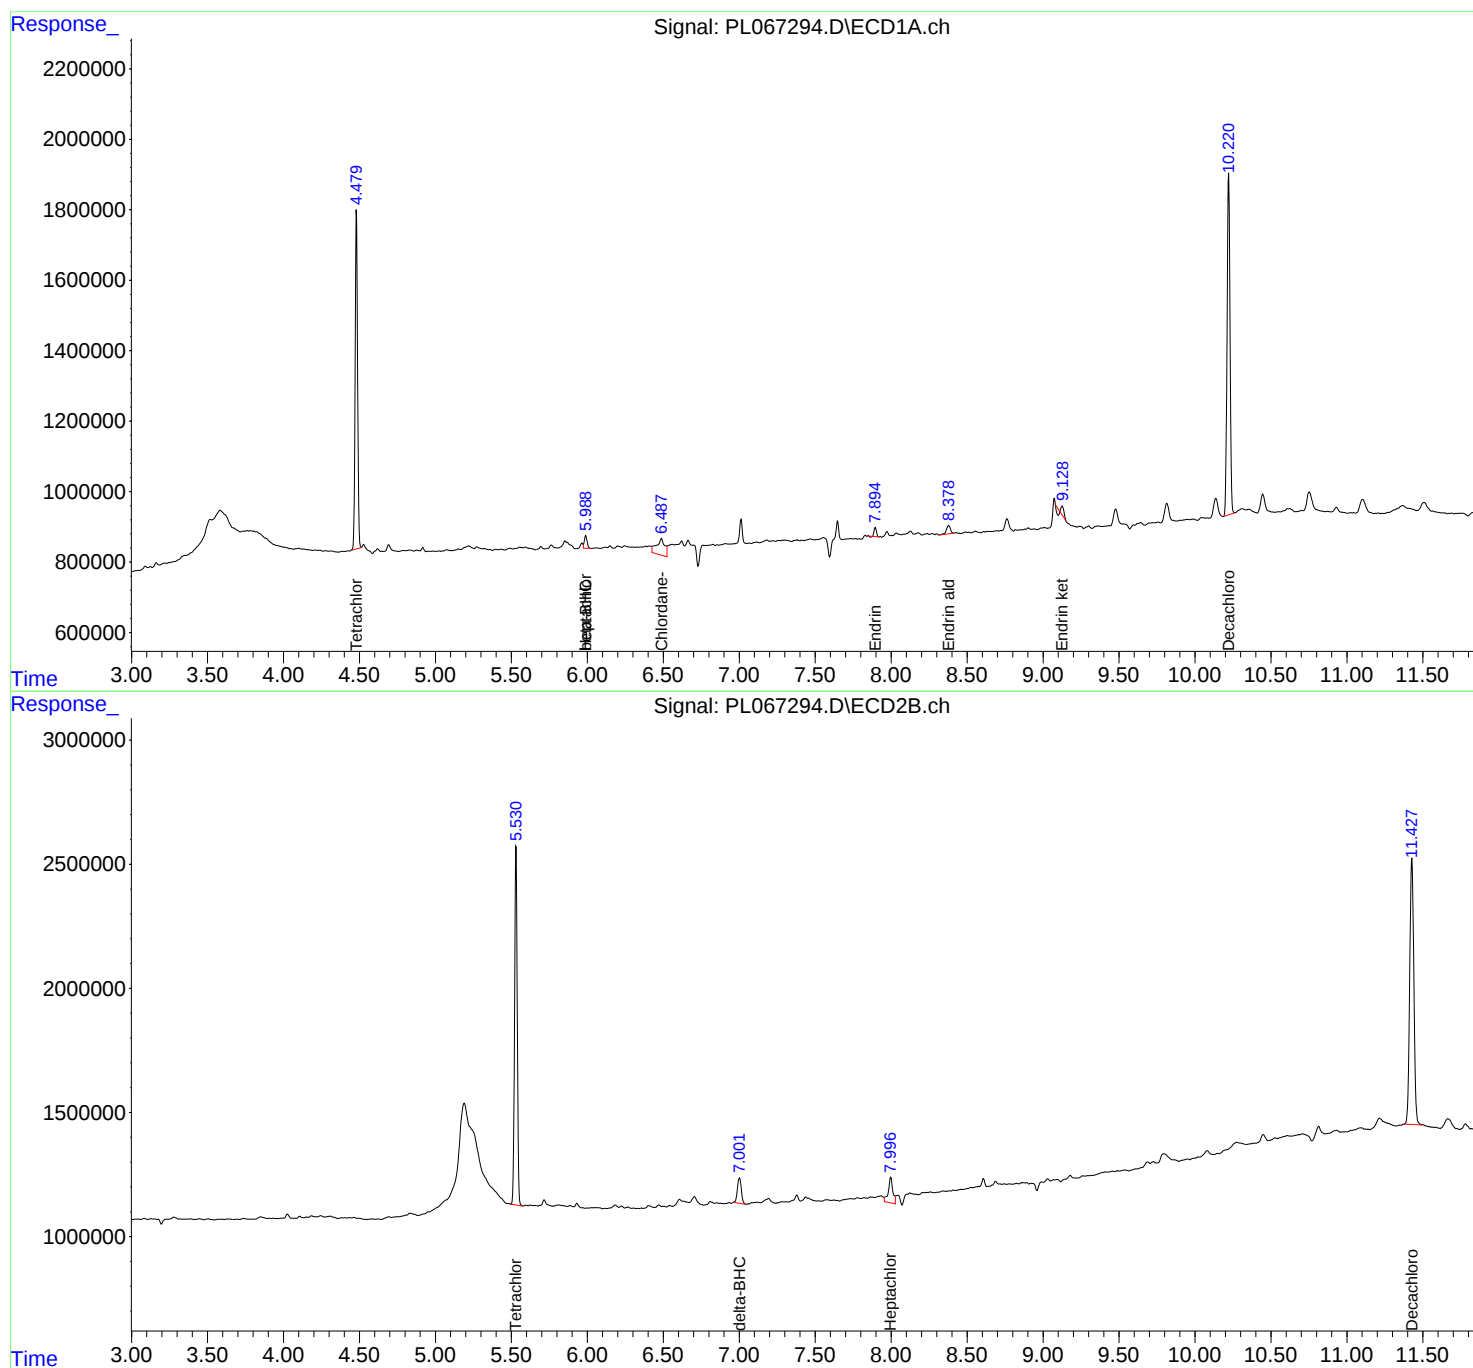


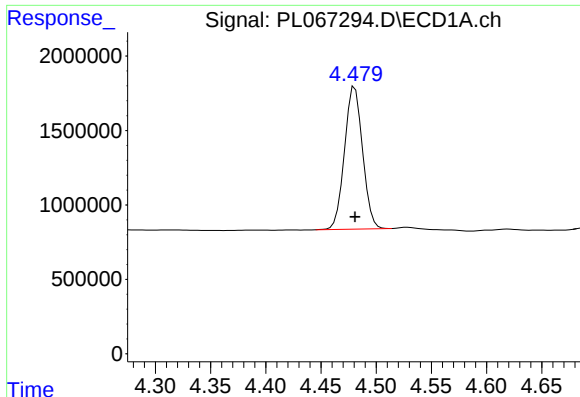

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10883806
Conc: 19.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

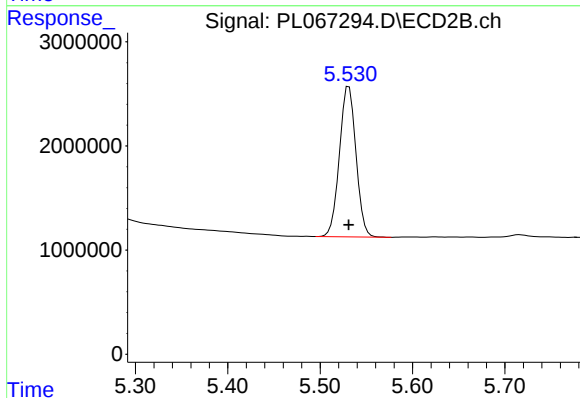


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 18006680
Conc: 19.10 ng/ml

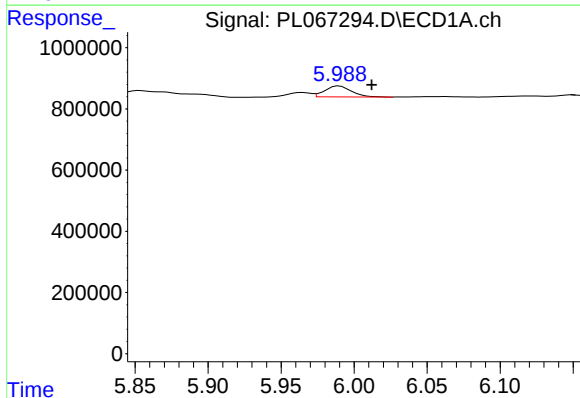


#4 Heptachlor

R.T.: 5.990 min
Delta R.T.: -0.022 min
Response: 450840
Conc: 0.60 ng/ml

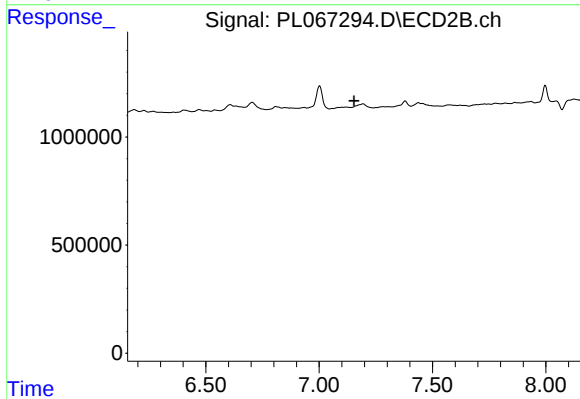

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

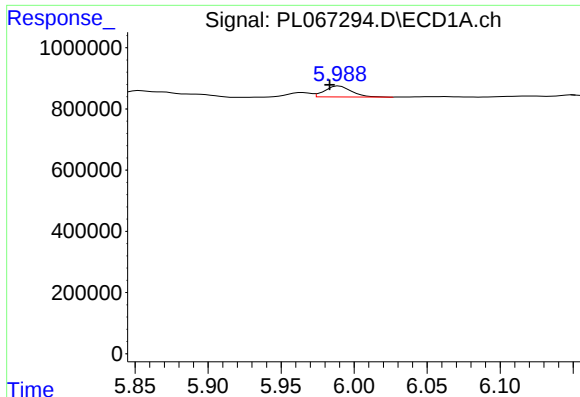

#6 beta-BHC


R.T.: 5.990 min
Delta R.T.: 0.006 min
Response: 450840
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

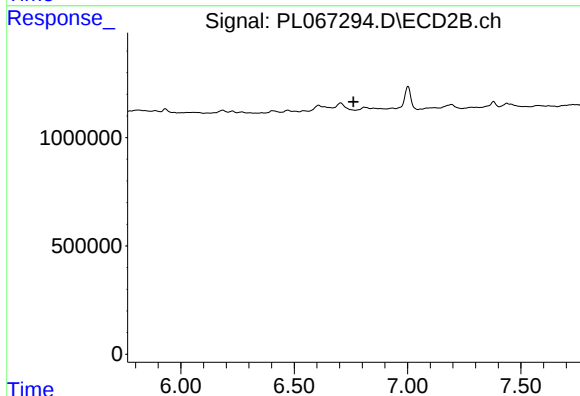


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

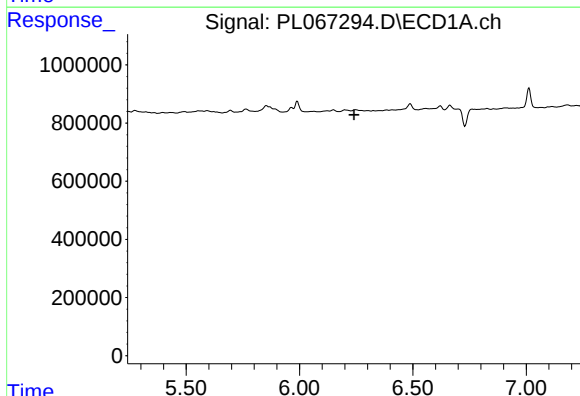


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

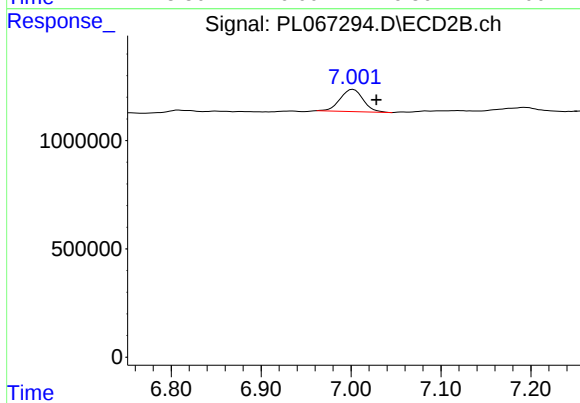

#7 delta-BHC


R.T.: 7.002 min
Delta R.T.: -0.026 min
Response: 1830651
Conc: 1.56 ng/ml

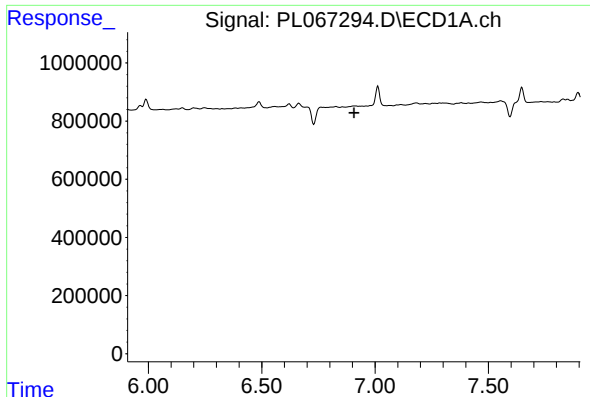

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

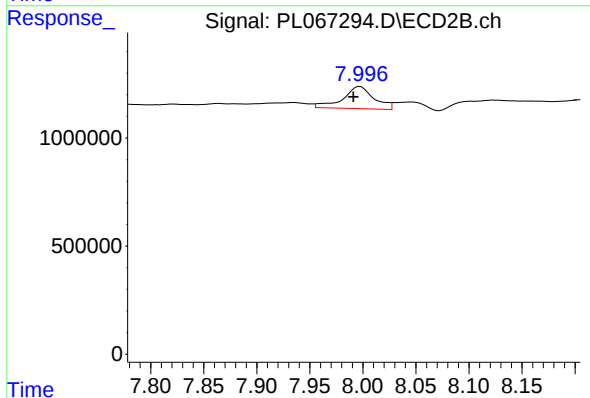


#8 Heptachlor epoxide

R.T.: 7.997 min
Delta R.T.: 0.006 min
Response: 2090069
Conc: 2.09 ng/ml

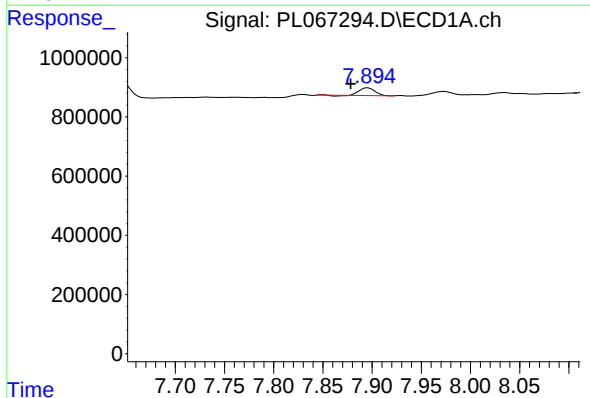


#14 Endrin

R.T.: 7.896 min
Delta R.T.: 0.017 min
Response: 275726
Conc: 0.42 ng/ml

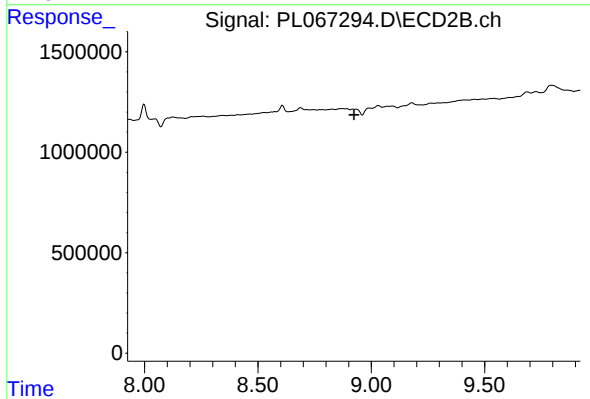

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.924 min
Response: 0
Conc: N.D.

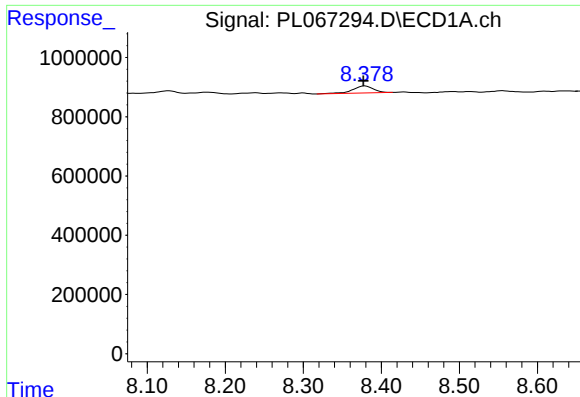

#18 Endrin aldehyde


R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 435569
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

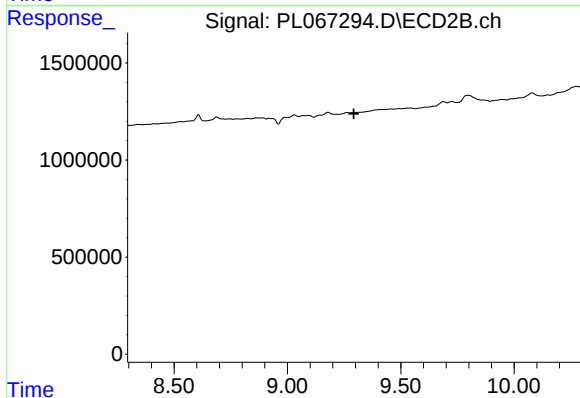


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

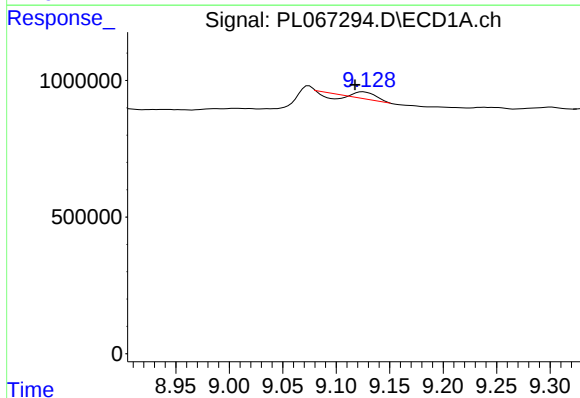


#21 Endrin ketone

R.T.: 9.125 min
Delta R.T.: 0.008 min
Response: 118520
Conc: 0.16 ng/ml

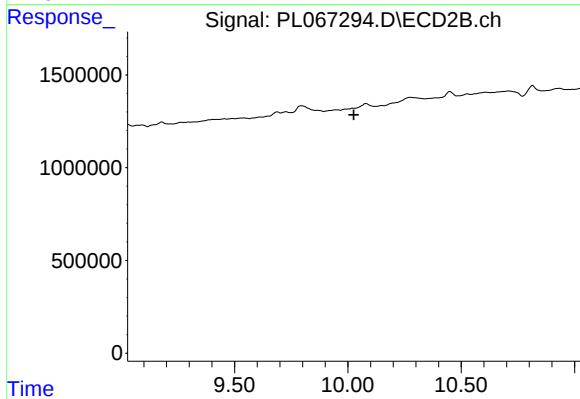

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

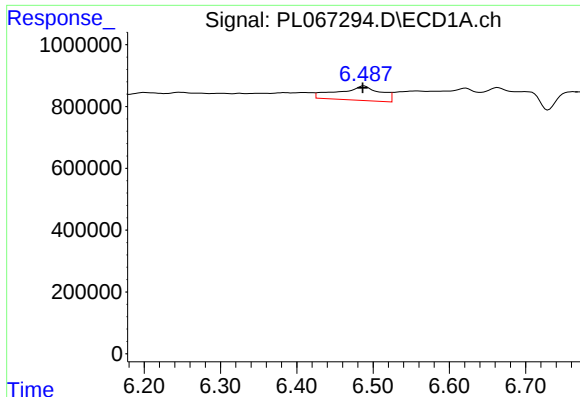

#24 Chlordane-2


R.T.: 6.488 min
Delta R.T.: 0.002 min
Response: 1783196
Conc: 66.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

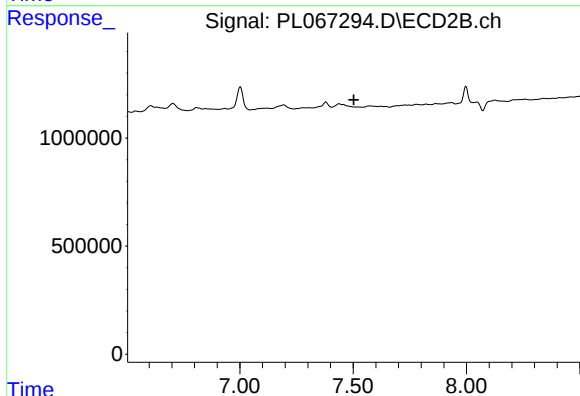


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

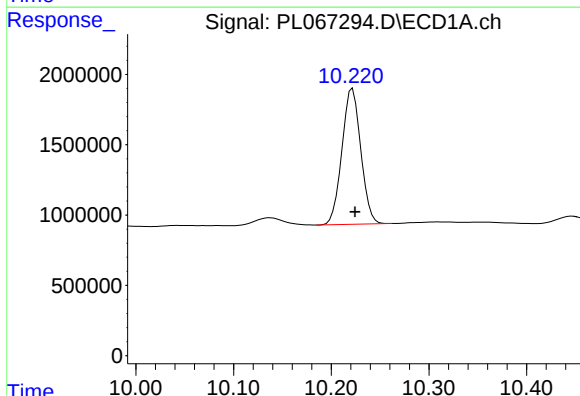

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.003 min
Response: 12941062
Conc: 18.26 ng/ml

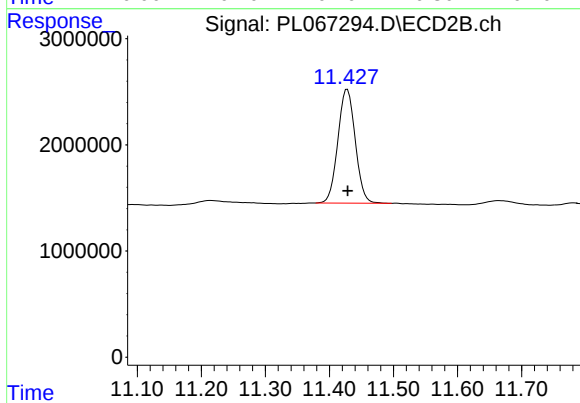

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 20181265
Conc: 20.26 ng/ml