

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
 Data File : PL067296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 16:43
 Operator : AR\AJ
 Sample : M2625-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:30:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	6300405	10534191	11.460	11.174
28)	SA Decachlor...	10.221	11.426	6454029	9562966	9.107	9.601
Target Compounds							
2)	A alpha-BHC	5.161f	0.000	243027	0	0.330	N.D. #
6)	B beta-BHC	5.962f	0.000	223724	0	0.625	N.D. #
7)	B delta-BHC	0.000	7.002f	0	1084975	N.D.	0.923 #
8)	B Heptachlo...	0.000	7.966f	0	70521	N.D.	0.070 #
14)	MA Endrin	7.896f	0.000	262402	0	0.400	N.D. #
18)	B Endrin al...	8.380	0.000	1163023	0	2.297	N.D. #
21)	B Endrin ke...	9.127	0.000	676116	0	0.888	N.D. #
22)	Mirex	9.299	0.000	256986	0	0.408	N.D. #
24)	Chlordane-2	6.476	0.000	892341	0	33.323	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
Data File : PL067296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 16:43
Operator : AR\AJ
Sample : M2625-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:30:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

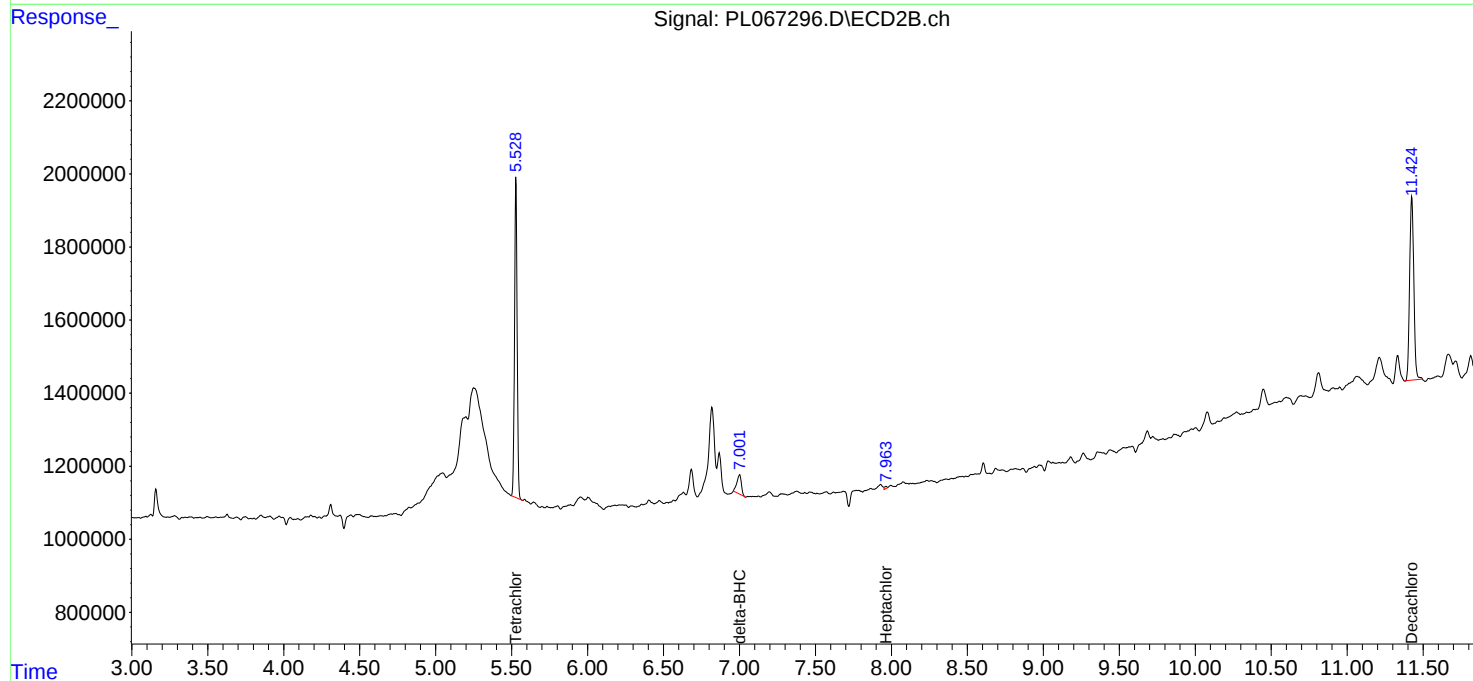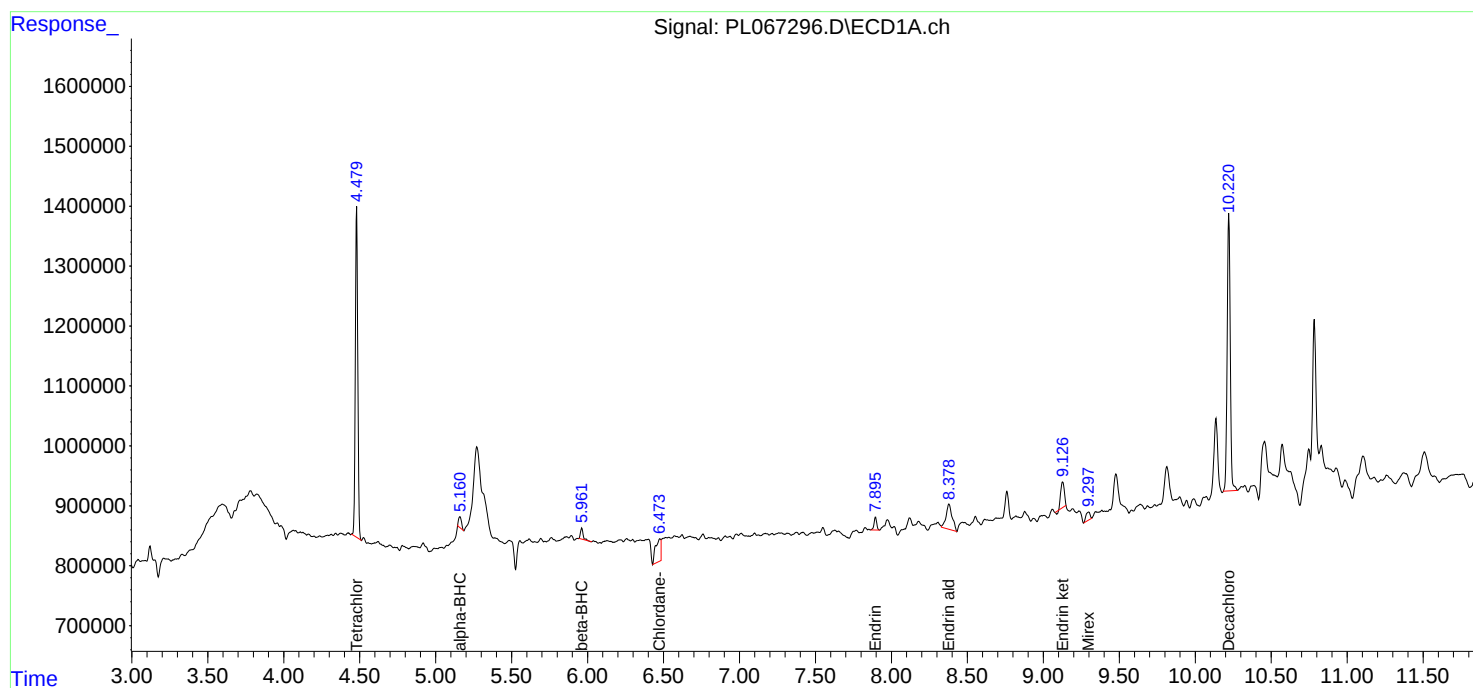


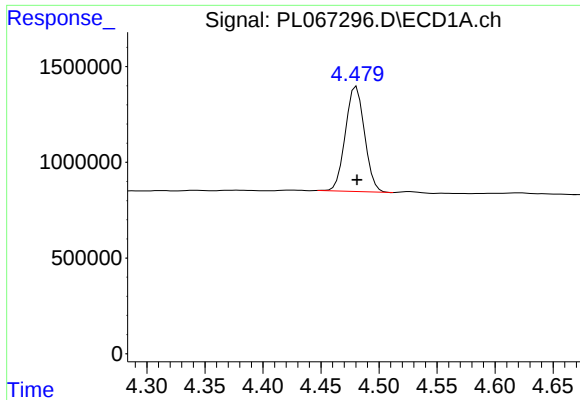

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 6300405
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

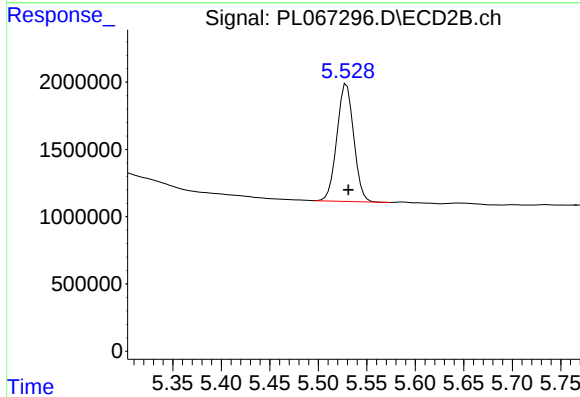


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 10534191
Conc: 11.17 ng/ml

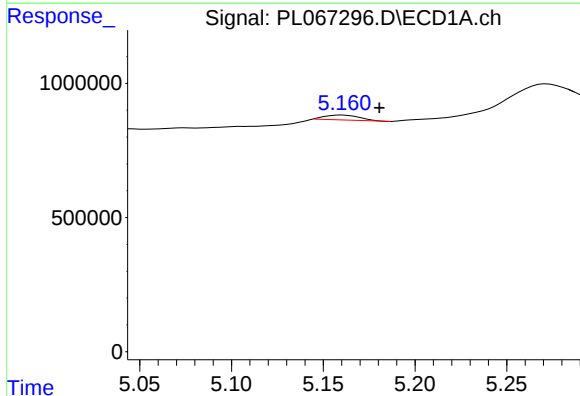


#2 alpha-BHC

R.T.: 5.161 min
Delta R.T.: -0.020 min
Response: 243027
Conc: 0.33 ng/ml

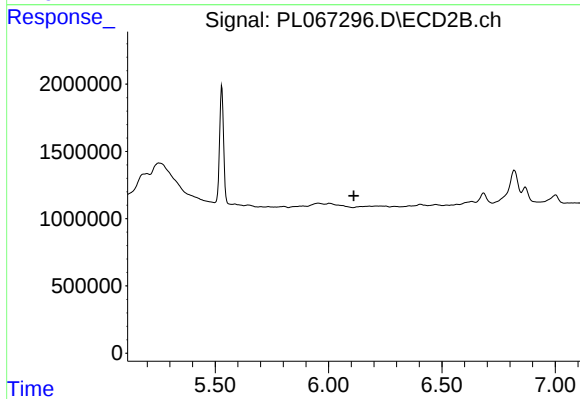

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

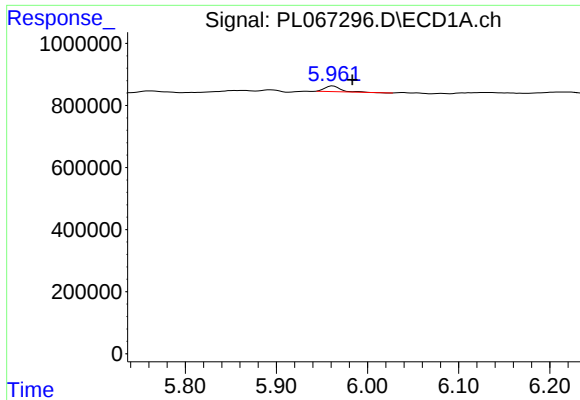

#6 beta-BHC


R.T.: 5.962 min
Delta R.T.: -0.021 min
Response: 223724
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

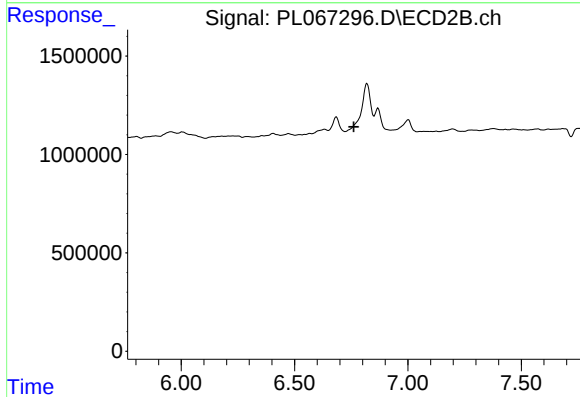


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

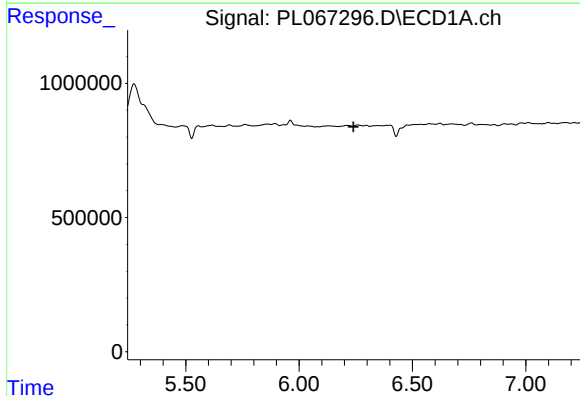


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

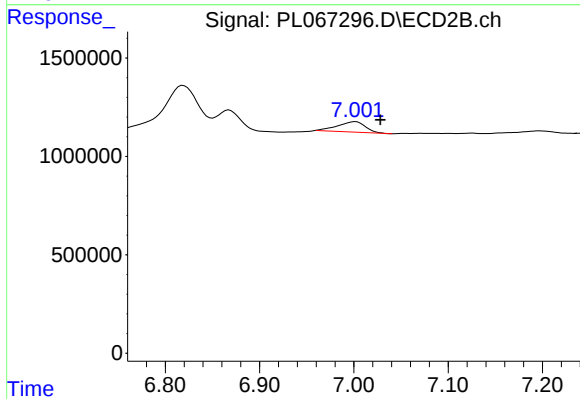

#7 delta-BHC


R.T.: 7.002 min
Delta R.T.: -0.026 min
Response: 1084975
Conc: 0.92 ng/ml

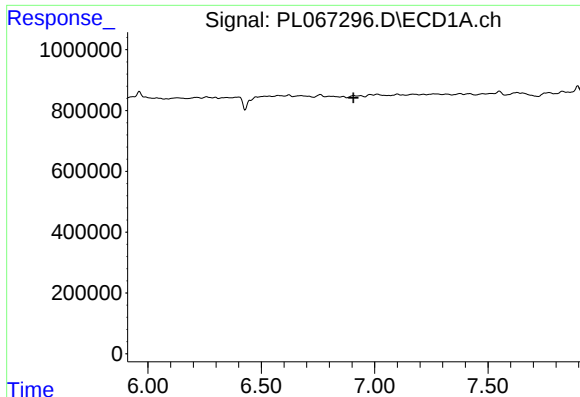

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

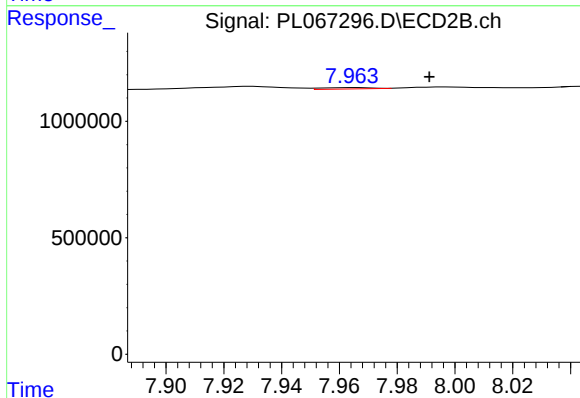


#8 Heptachlor epoxide

R.T.: 7.966 min
Delta R.T.: -0.026 min
Response: 70521
Conc: 0.07 ng/ml

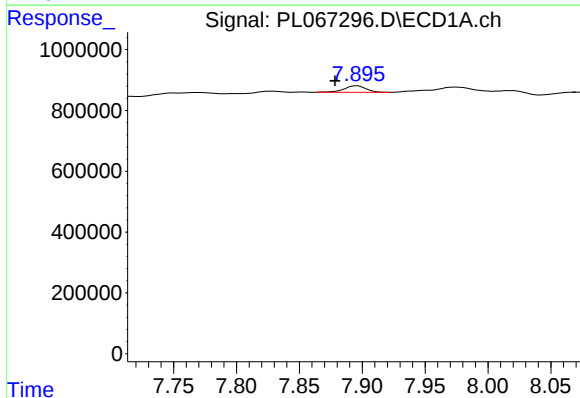


#14 Endrin

R.T.: 7.896 min
Delta R.T.: 0.018 min
Response: 262402
Conc: 0.40 ng/ml

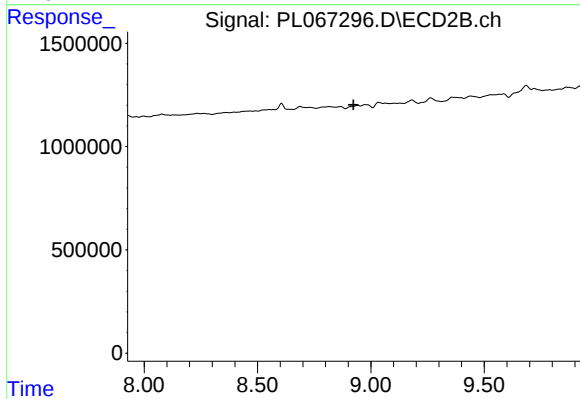

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.924 min
Response: 0
Conc: N.D.

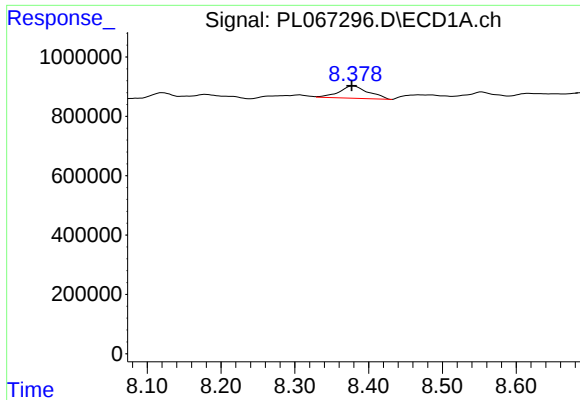

#18 Endrin aldehyde


R.T.: 8.380 min
Delta R.T.: 0.002 min
Response: 1163023
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

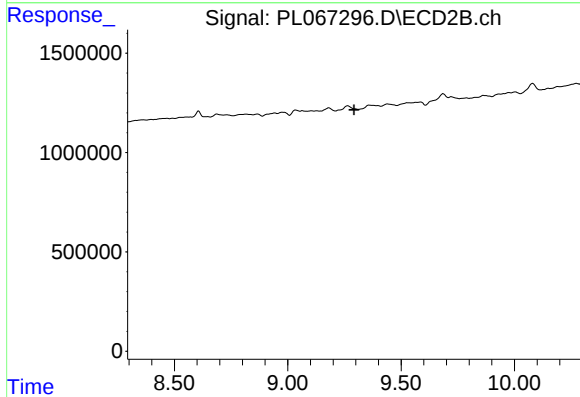


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

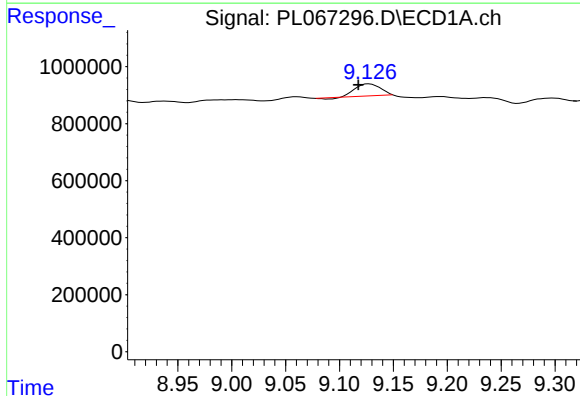


#21 Endrin ketone

R.T.: 9.127 min
Delta R.T.: 0.010 min
Response: 676116
Conc: 0.89 ng/ml

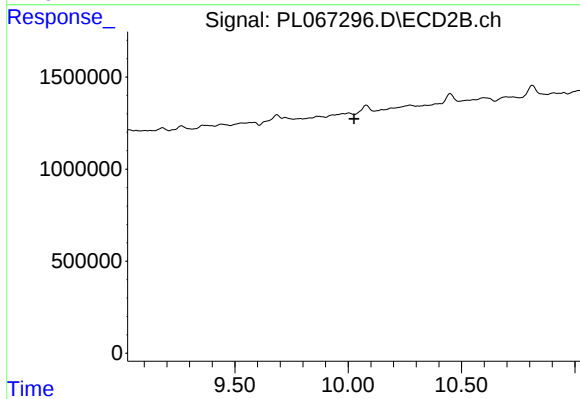

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

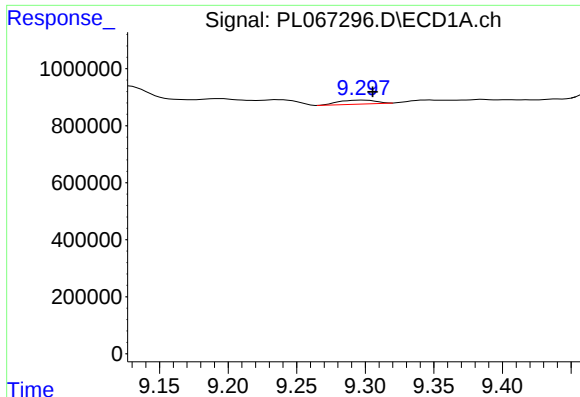

#22 Mirex


R.T.: 9.299 min
Delta R.T.: -0.007 min
Response: 256986
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

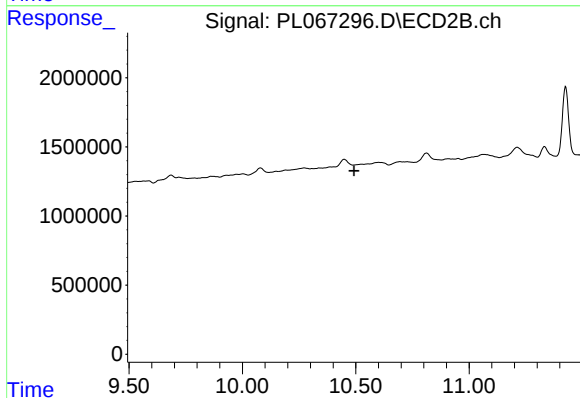


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

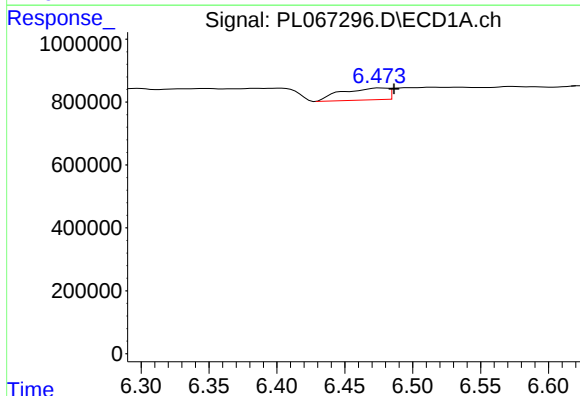


#24 Chlordane-2

R.T.: 6.476 min
Delta R.T.: -0.010 min
Response: 892341
Conc: 33.32 ng/ml

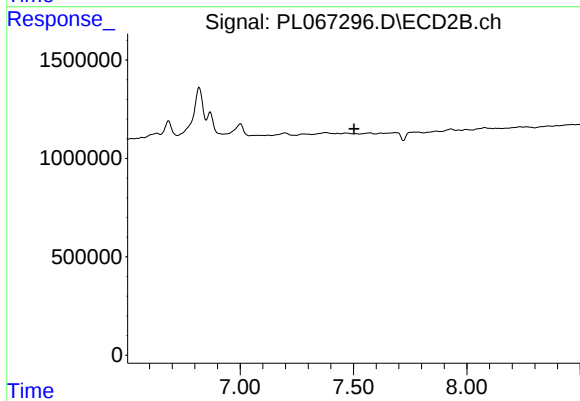

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

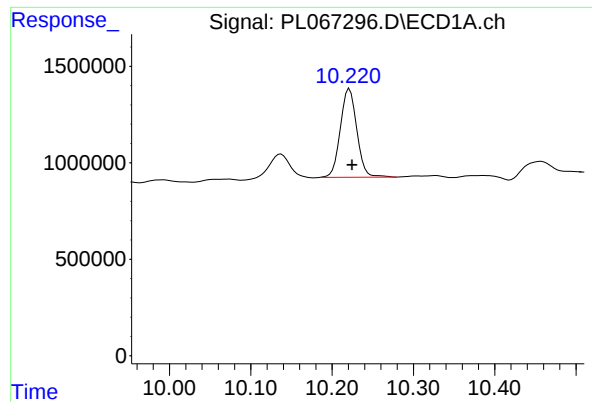

#28 Decachlorobiphenyl


R.T.: 10.221 min

Delta R.T.: -0.003 min

Response: 6454029

Conc: 9.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

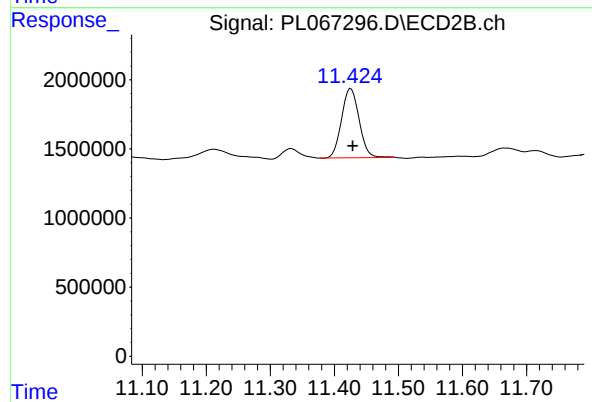

#28 Decachlorobiphenyl

R.T.: 11.426 min

Delta R.T.: -0.003 min

Response: 9562966

Conc: 9.60 ng/ml