

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
 Data File : PL067310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 21:42
 Operator : AR\AJ
 Sample : M2625-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:33:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	11908948	20110016	21.661	21.332
28)	SA Decachlor...	10.222	11.427	13649688	20615000	19.261	20.697
Target Compounds							
2)	A alpha-BHC	5.166	0.000	283351	0	0.385	N.D. #
7)	B delta-BHC	0.000	7.000f	0	871723	N.D.	0.742 #
11)	B alpha-Chl...	7.255	0.000	735667	0	1.005	N.D. #
15)	B Endosulfa...	8.176	0.000	674487	0	1.095	N.D. #
18)	B Endrin al...	8.379	0.000	579395	0	1.144	N.D. #
21)	B Endrin ke...	9.128	0.000	581640	0	0.764	N.D. #
22)	Mirex	9.300	0.000	181595	0	0.288	N.D. #
26)	Chlordane-4	7.255	0.000	735667	0	10.067	N.D. #
27)	Chlordane-5	8.176f	0.000	674487	0	30.828	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061121\
Data File : PL067310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 21:42
Operator : AR\AJ
Sample : M2625-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:33:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

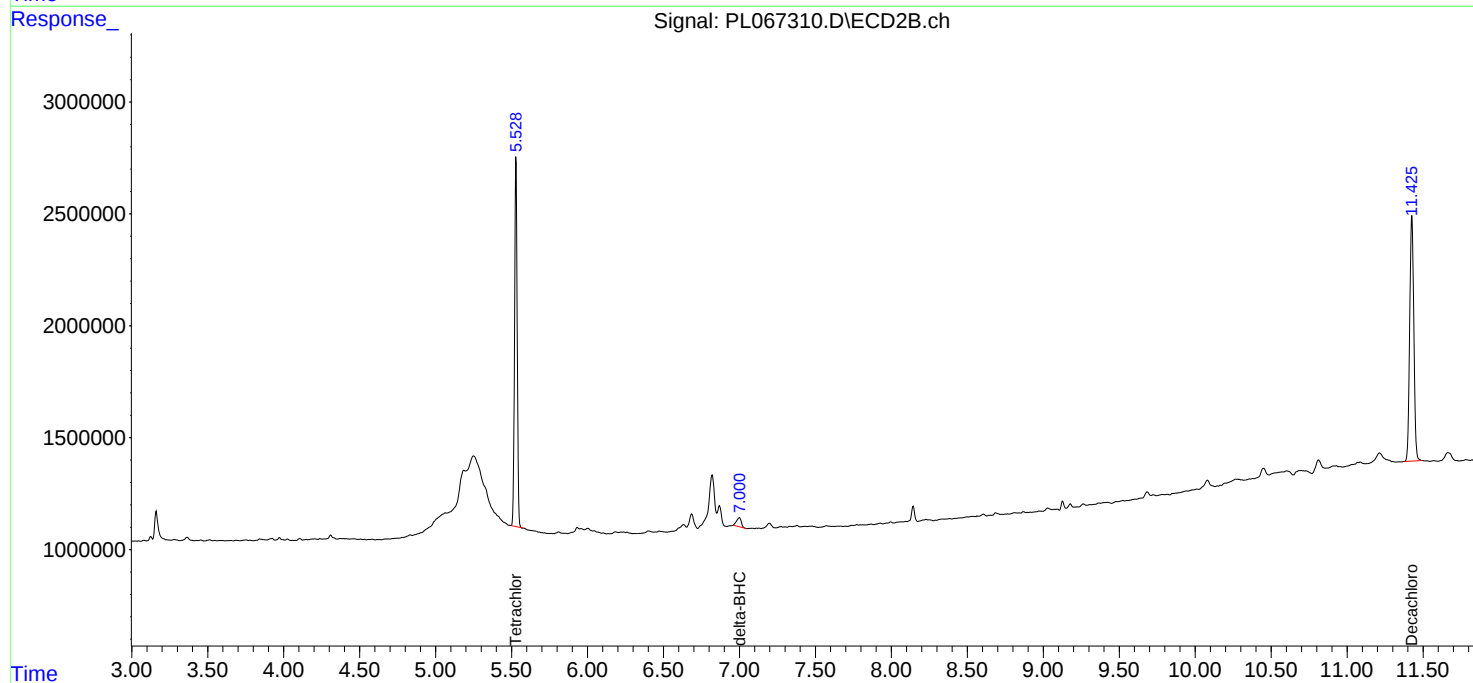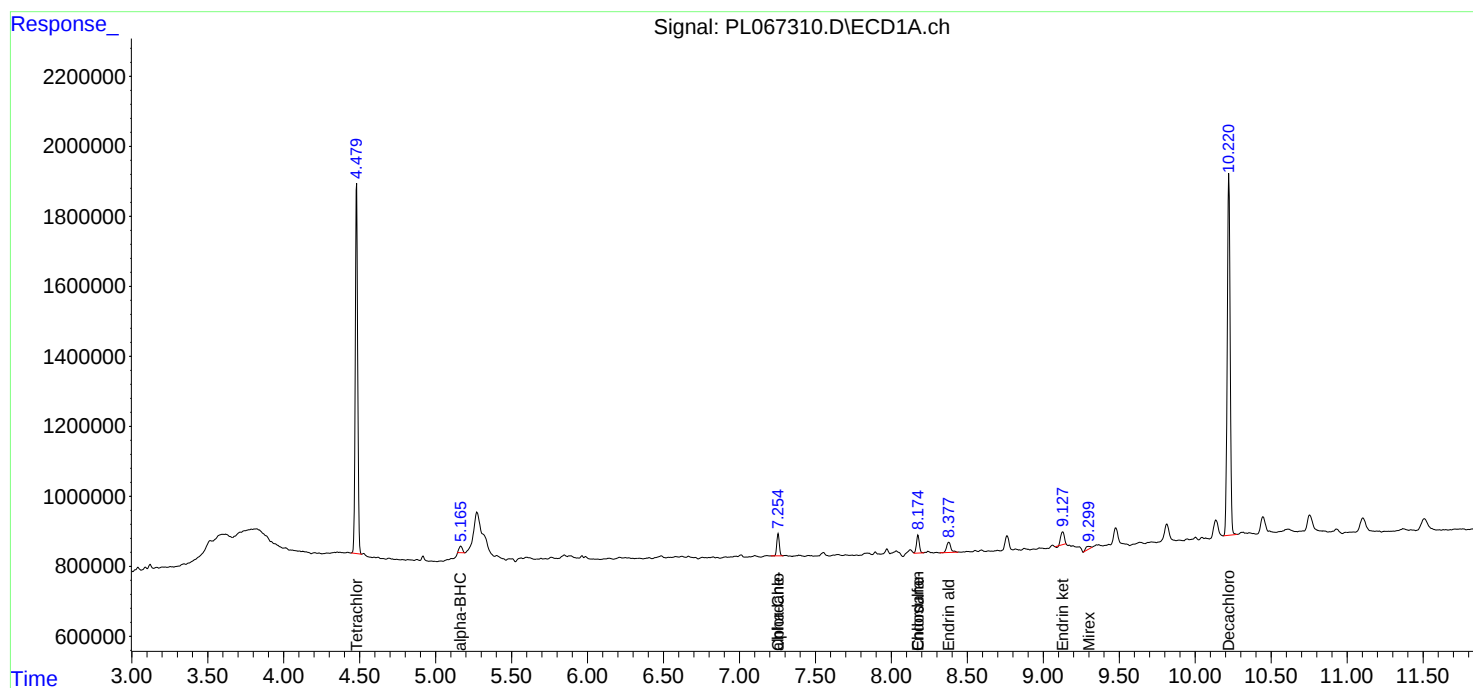


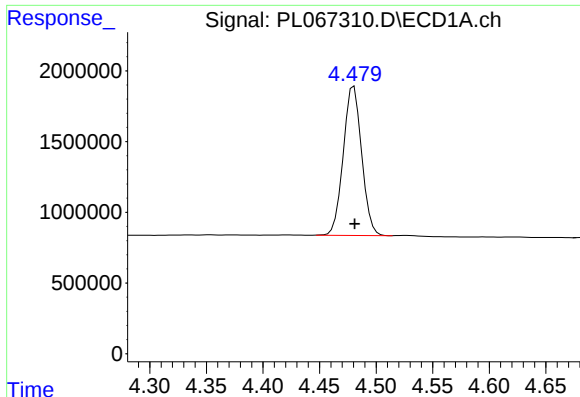

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 11908948
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

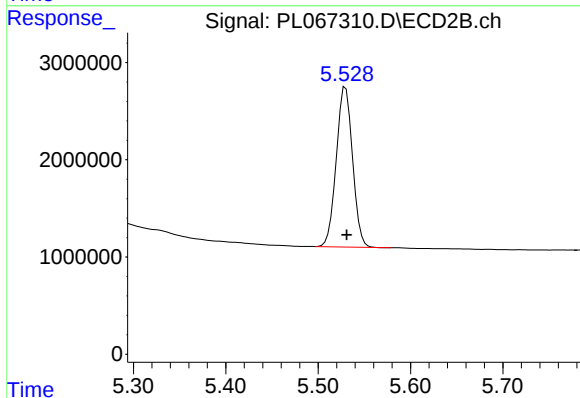


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 20110016
Conc: 21.33 ng/ml

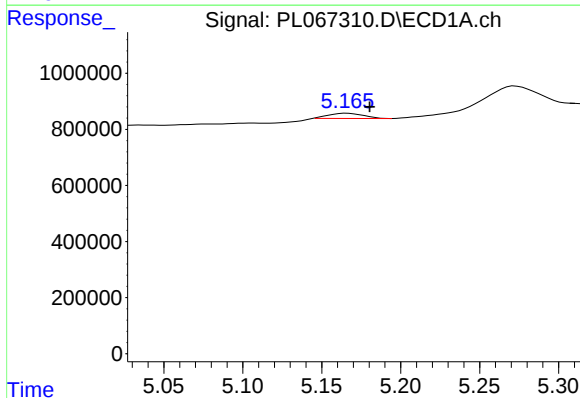


#2 alpha-BHC

R.T.: 5.166 min
Delta R.T.: -0.015 min
Response: 283351
Conc: 0.39 ng/ml

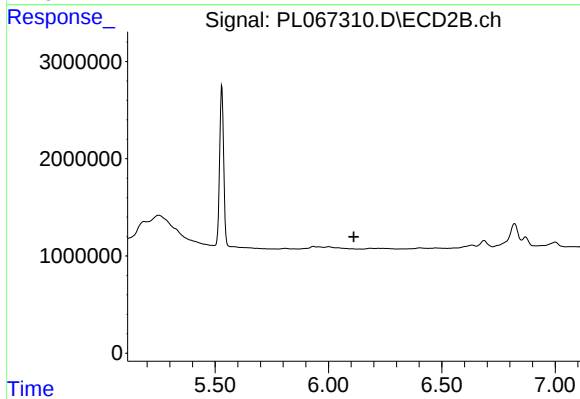

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

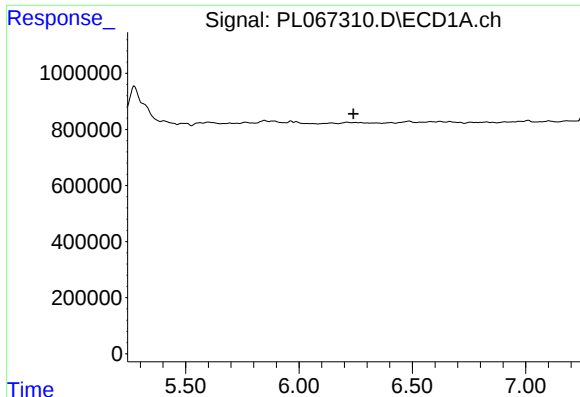

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

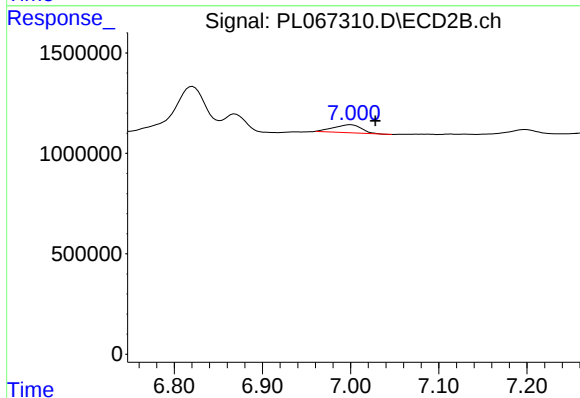


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 871723
Conc: 0.74 ng/ml

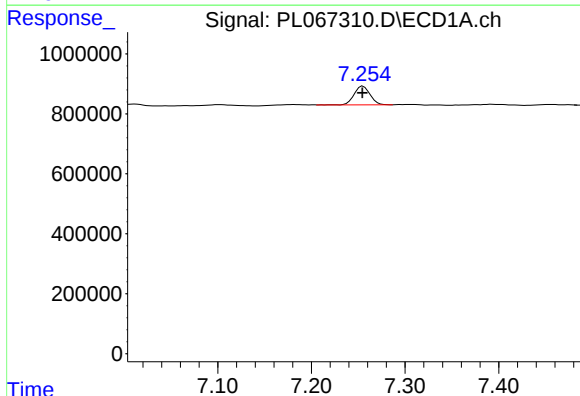


#11 alpha-Chlordane

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 735667
Conc: 1.00 ng/ml

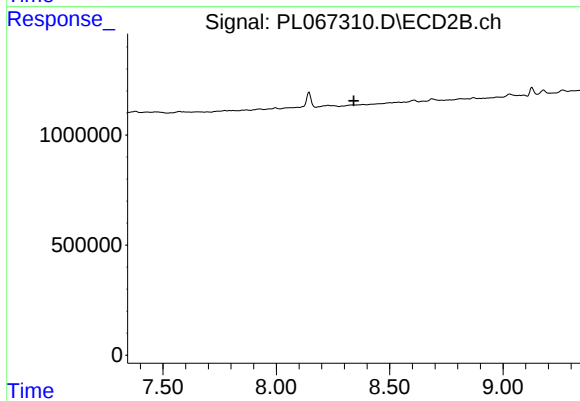

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

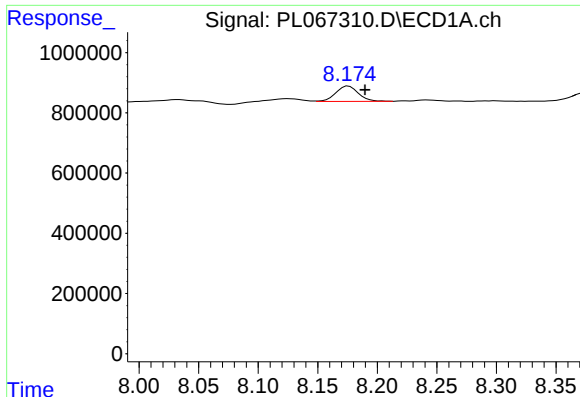

#15 Endosulfan II


R.T.: 8.176 min
Delta R.T.: -0.014 min
Response: 674487
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

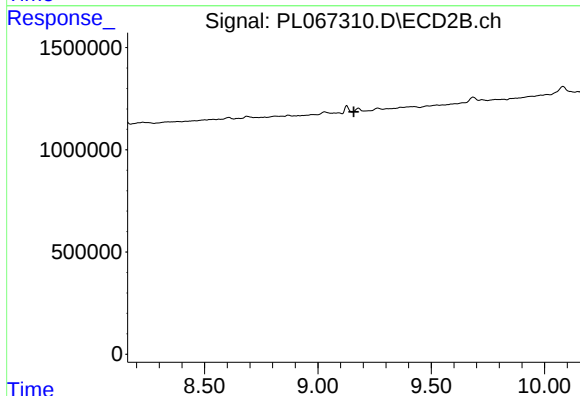


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

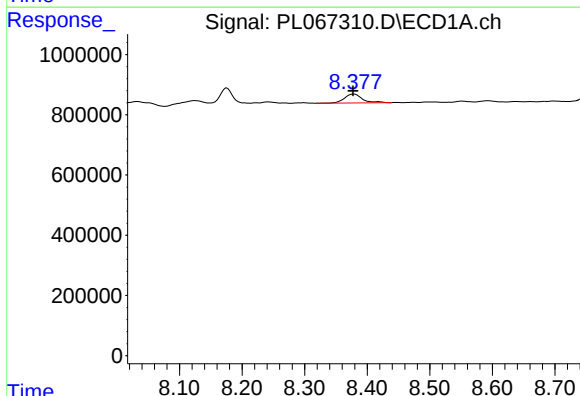


#18 Endrin aldehyde

R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 579395
Conc: 1.14 ng/ml

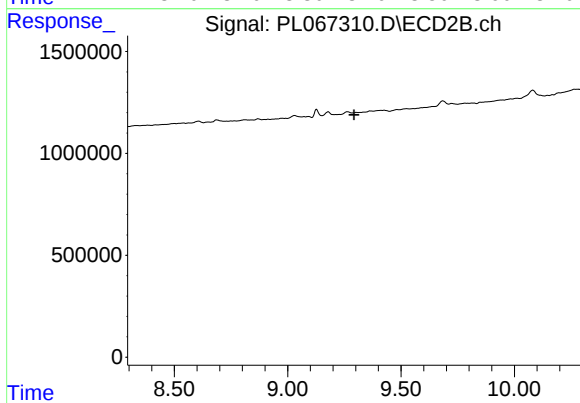

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

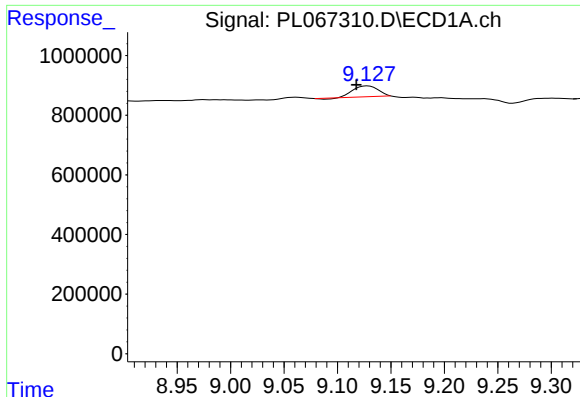

#21 Endrin ketone


R.T.: 9.128 min
Delta R.T.: 0.011 min
Response: 581640
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

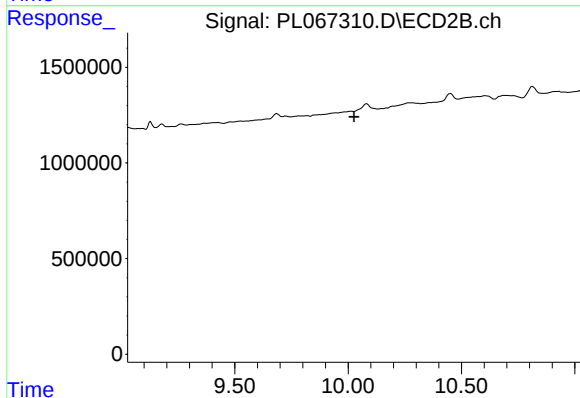


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

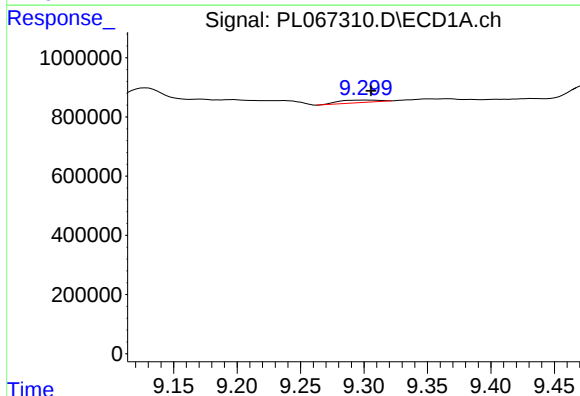


#22 Mirex

R.T.: 9.300 min
Delta R.T.: -0.006 min
Response: 181595
Conc: 0.29 ng/ml

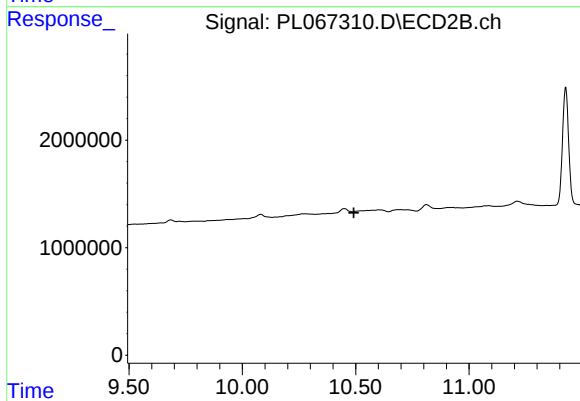

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

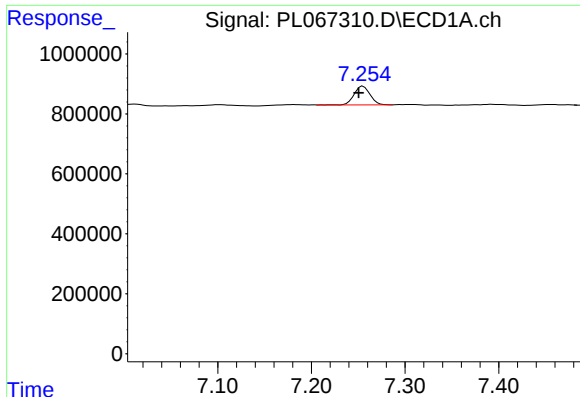

#26 Chlordane-4


R.T.: 7.255 min
Delta R.T.: 0.005 min
Response: 735667
Conc: 10.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

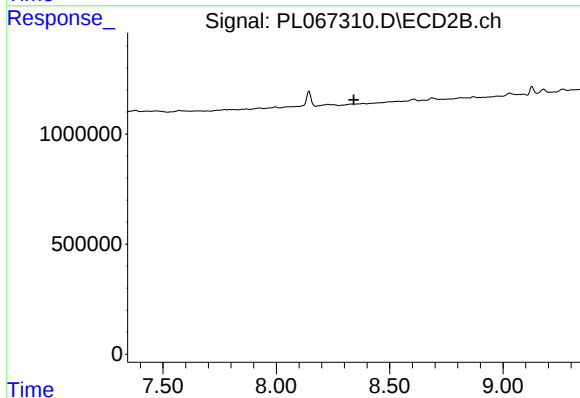


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

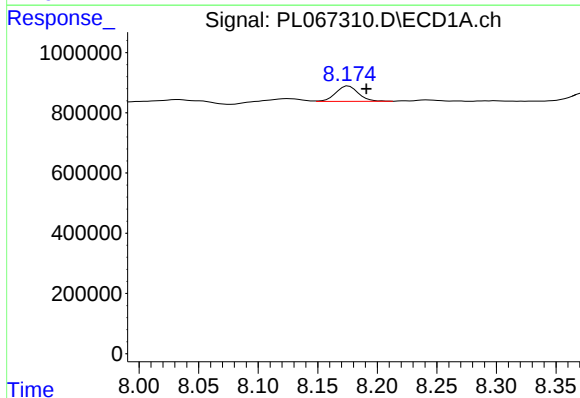


#27 Chlordane-5

R.T.: 8.176 min
Delta R.T.: -0.015 min
Response: 674487
Conc: 30.83 ng/ml

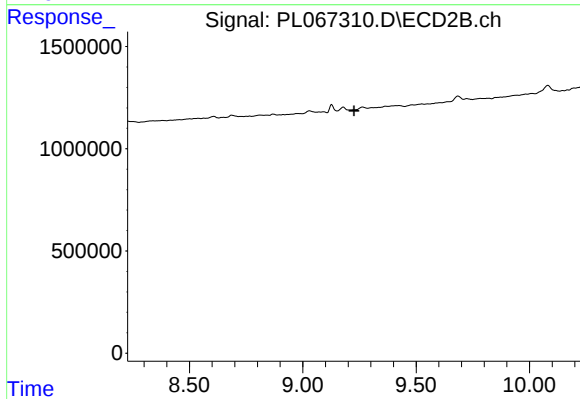

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

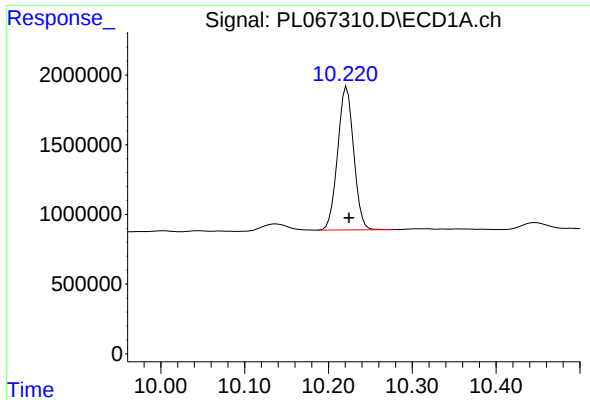

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.002 min
Response: 13649688
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

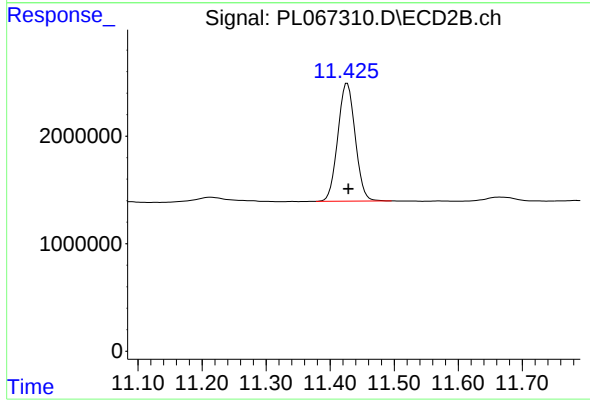

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 20615000
Conc: 20.70 ng/ml