

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061720\
 Data File : PL059303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2020 13:58
 Operator : AJ\MA
 Sample : L3024-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-17

Manual Integrations
 APPROVED

mohammad
 6/18/2020 2:51:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:20:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.070	39559774	59970700	22.909	23.049
28)	SA Decachlor...	8.285	9.176	31813930	43212721	19.347m	18.229m
Target Compounds							
15)	B Endosulfa...	6.359	7.011	3606890	5279635	2.334	2.027
17)	MA 4,4'-DDT	6.450	7.215	951155	1420853	0.754	0.624

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061720\
Data File : PL059303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2020 13:58
Operator : AJ\MA
Sample : L3024-19
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-17


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:20:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

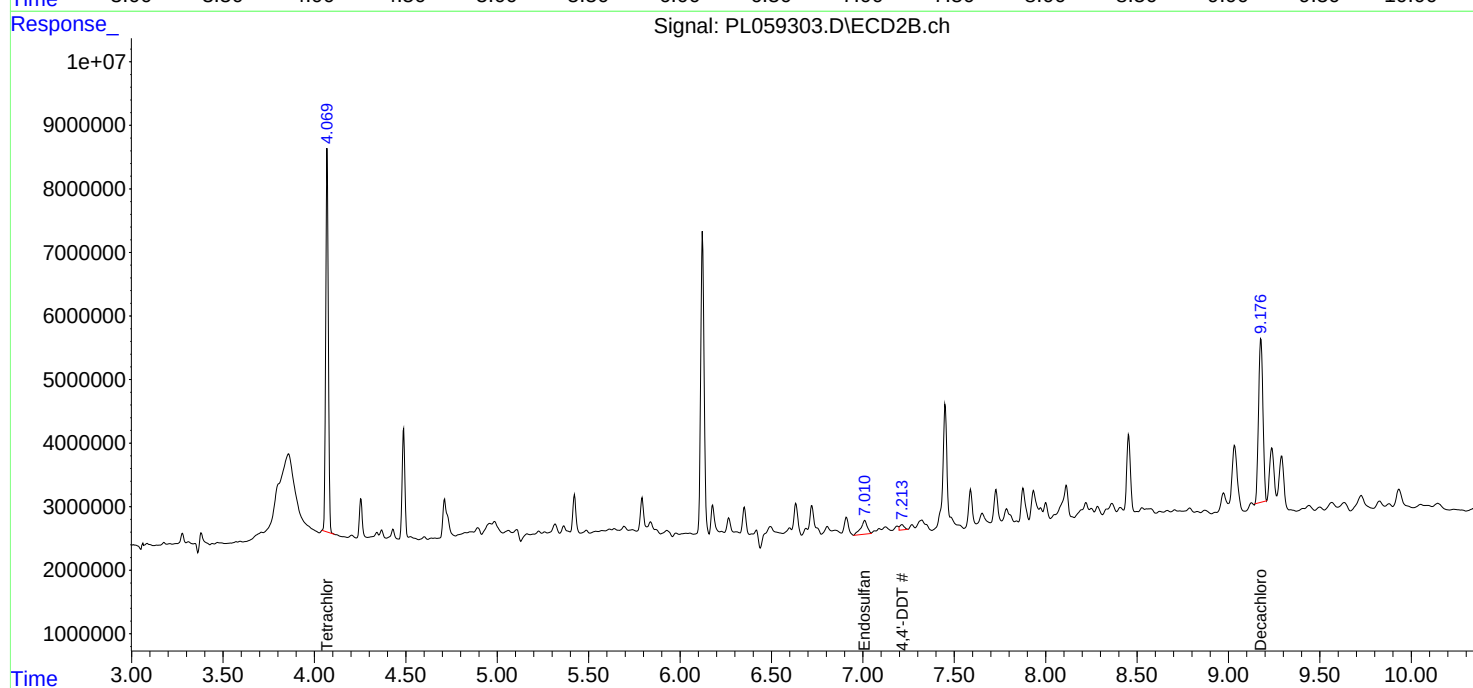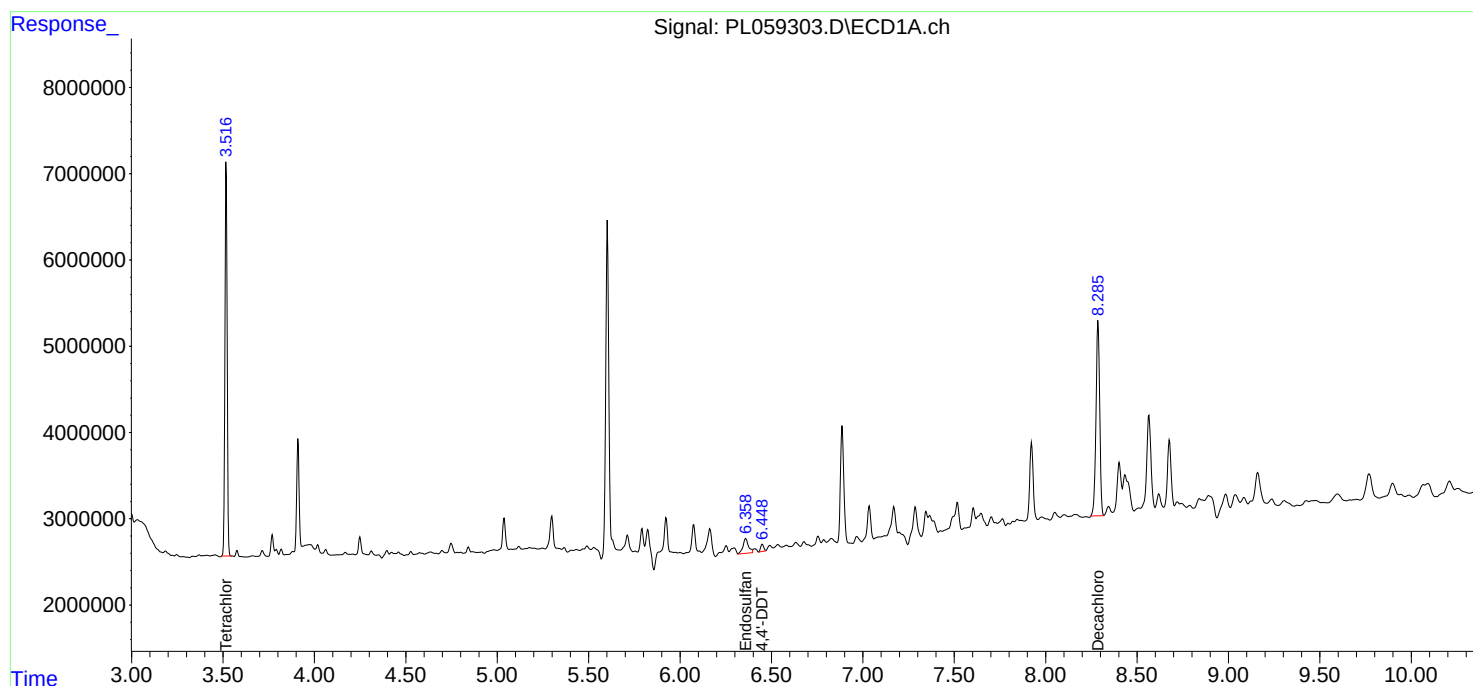

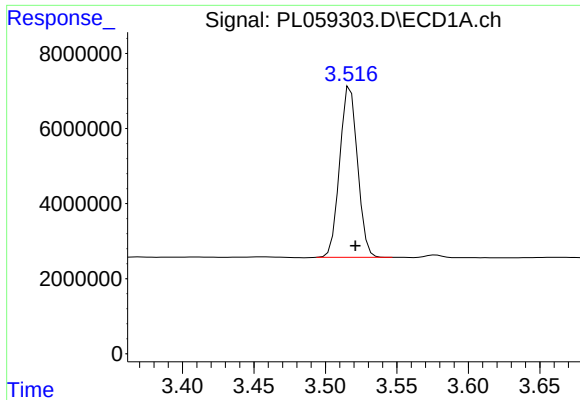


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.004 min
Response: 39559774
Conc: 22.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-17


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:26 PM

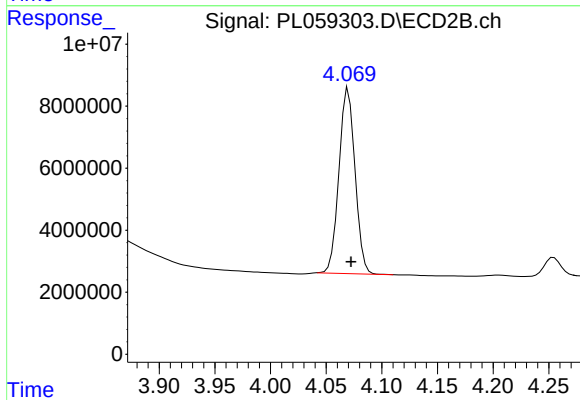


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.002 min
Response: 59970700
Conc: 23.05 ng/ml

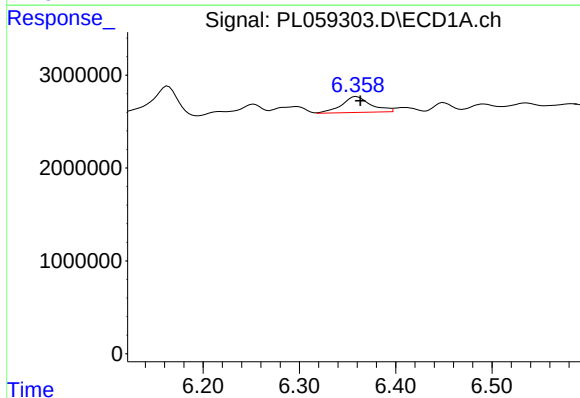


#15 Endosulfan II

R.T.: 6.359 min
Delta R.T.: -0.004 min
Response: 3606890
Conc: 2.33 ng/ml

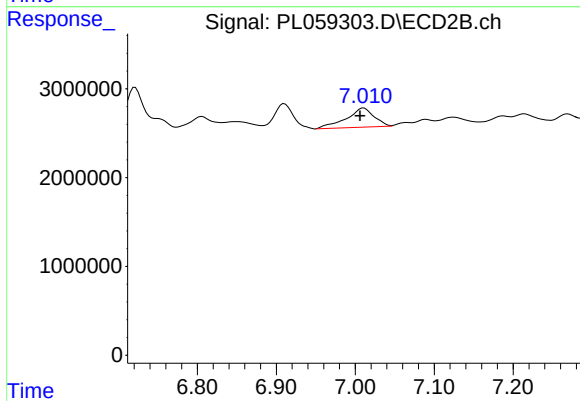

#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.005 min
Response: 5279635
Conc: 2.03 ng/ml

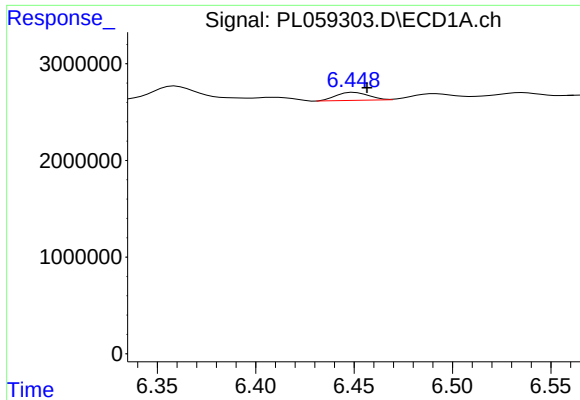


#17 4,4'-DDT

R.T.: 6.450 min
Delta R.T.: -0.007 min
Response: 951155
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-17


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:26 PM

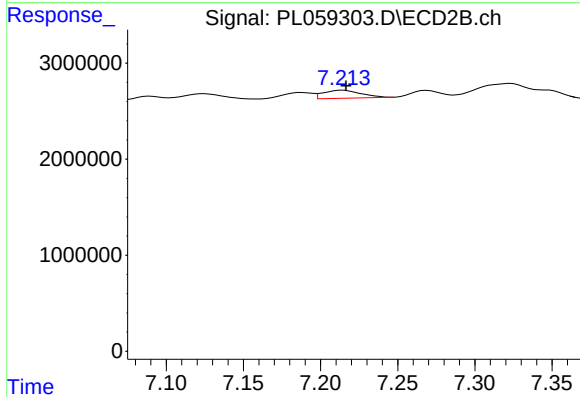


#17 4,4'-DDT

R.T.: 7.215 min
Delta R.T.: -0.002 min
Response: 1420853
Conc: 0.62 ng/ml

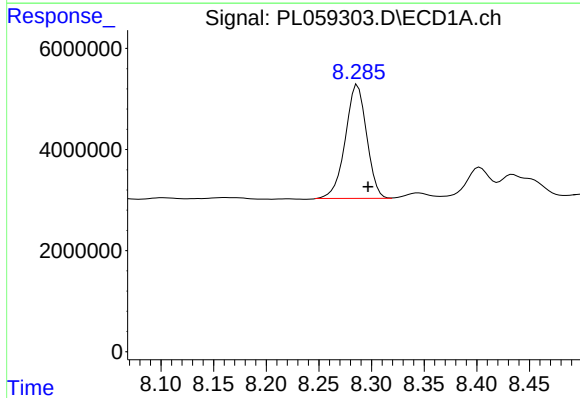

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.011 min
Response: 31813930
Conc: 19.35 ng/ml m

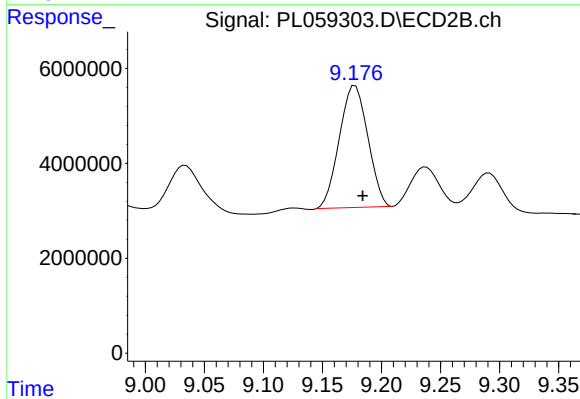

#28 Decachlorobiphenyl

R.T.: 9.176 min
Delta R.T.: -0.008 min
Response: 43212721
Conc: 18.23 ng/ml m