

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061720\
 Data File : PL059311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2020 15:51
 Operator : AJ\MA
 Sample : L3024-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-7

Manual Integrations
 APPROVED

mohammad
 6/18/2020 2:51:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 17:29:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.071	23037785	35470143	13.341	13.632
28)	SA Decachlor...	8.288	9.179	23745336	33906045	14.440m	14.303
Target Compounds							
12)	B 4,4'-DDE	5.693	6.422	3747727	8560802	2.464	3.075
17)	MA 4,4'-DDT	6.449	7.213	4002246	3658880	3.173	1.607 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061720\
Data File : PL059311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2020 15:51
Operator : AJ\MA
Sample : L3024-10
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-7


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 17:29:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

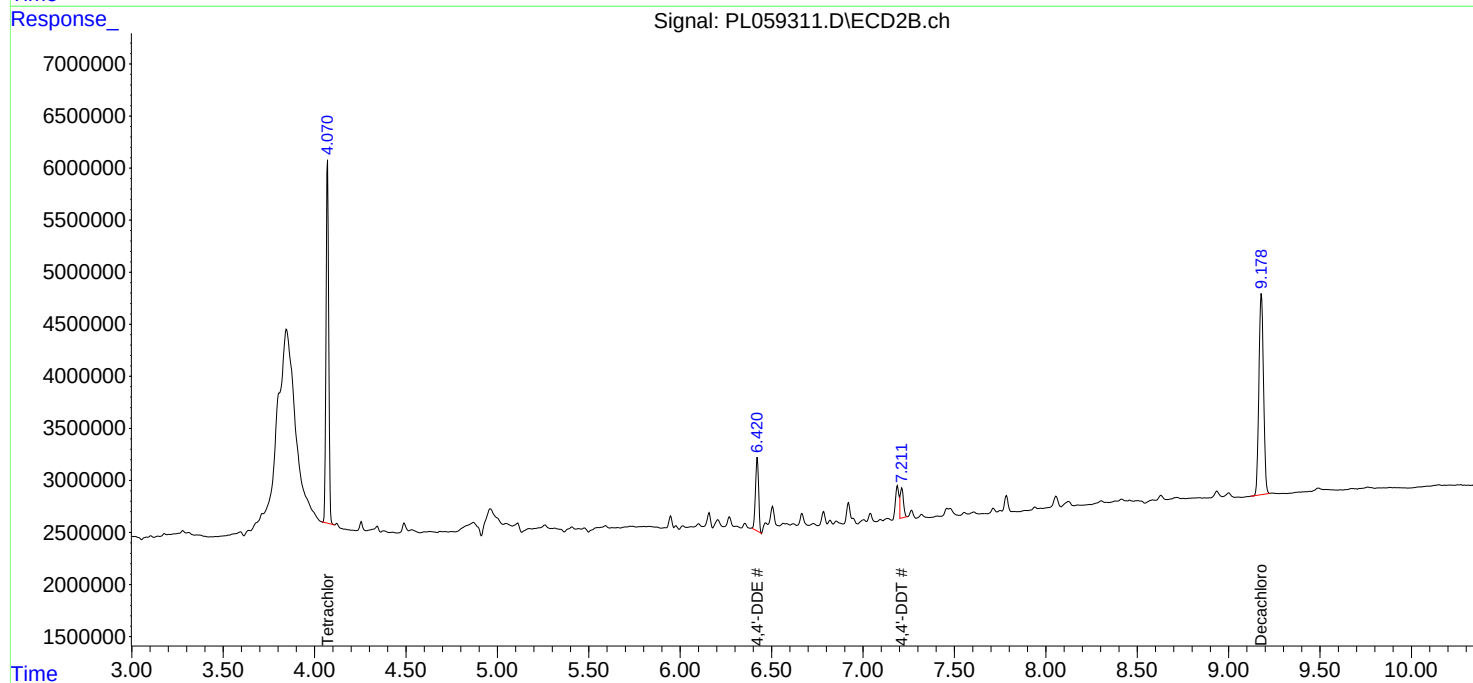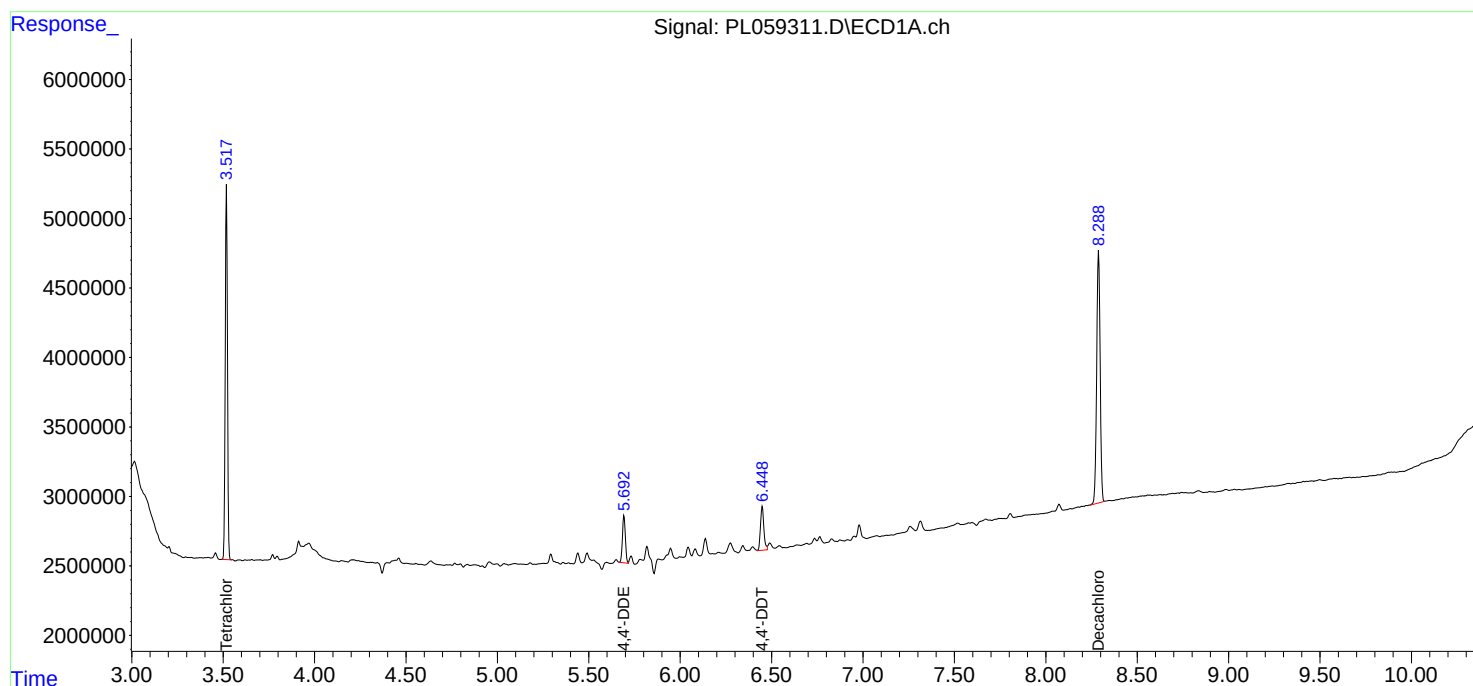

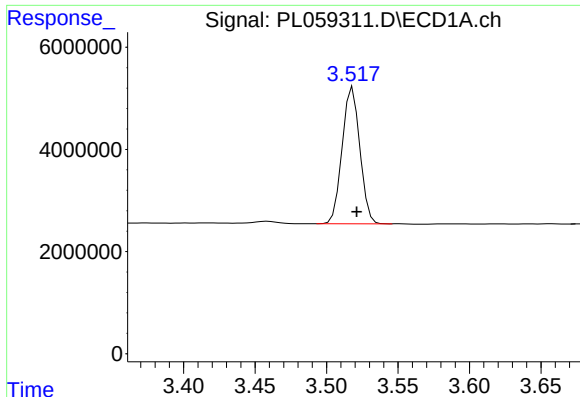


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: -0.003 min
Response: 23037785
Conc: 13.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-7


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:50 PM

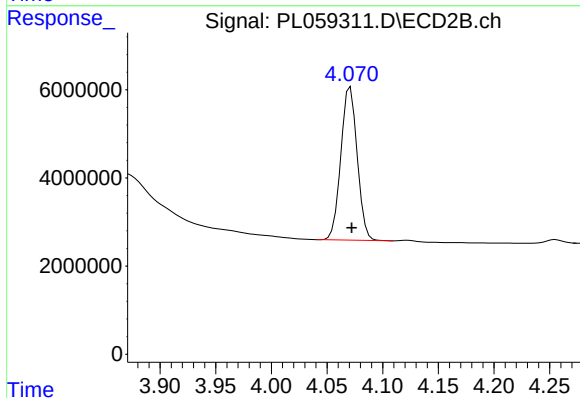


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.001 min
Response: 35470143
Conc: 13.63 ng/ml

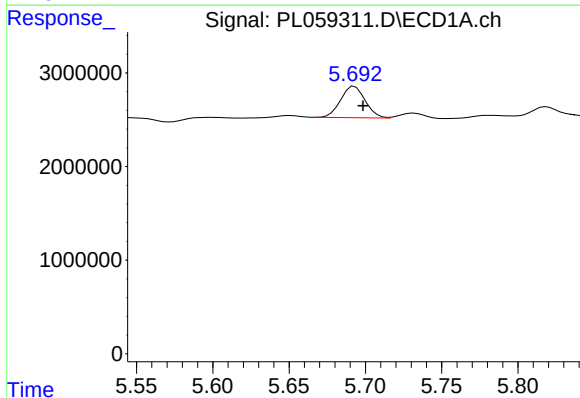


#12 4,4'-DDE

R.T.: 5.693 min
Delta R.T.: -0.006 min
Response: 3747727
Conc: 2.46 ng/ml

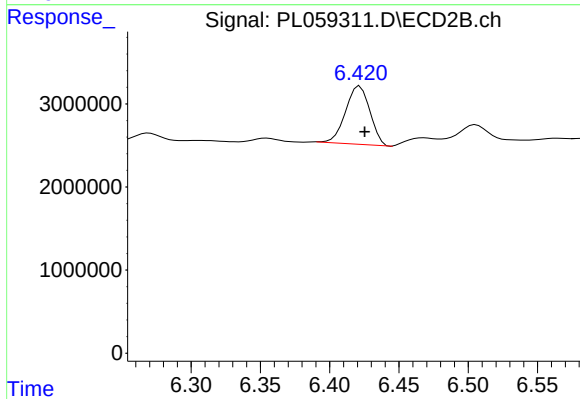

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.004 min
Response: 8560802
Conc: 3.08 ng/ml

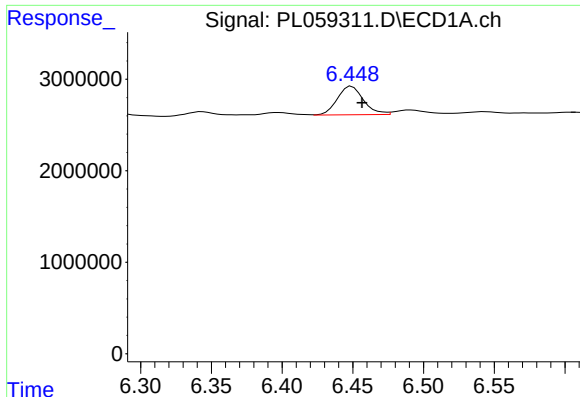


#17 4,4'-DDT

R.T.: 6.449 min
Delta R.T.: -0.007 min
Response: 4002246
Conc: 3.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-7


Manual Integrations
APPROVED

mohammad
6/18/2020 2:51:50 PM

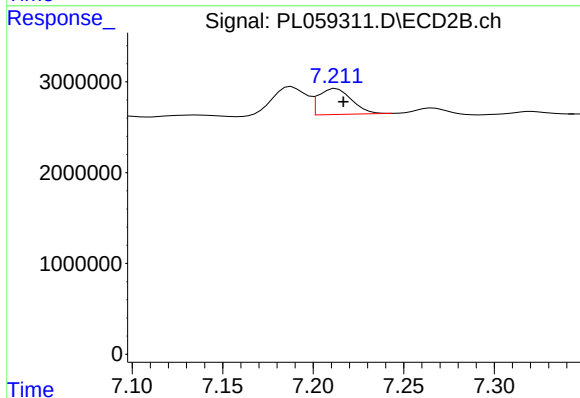


#17 4,4'-DDT

R.T.: 7.213 min
Delta R.T.: -0.004 min
Response: 3658880
Conc: 1.61 ng/ml

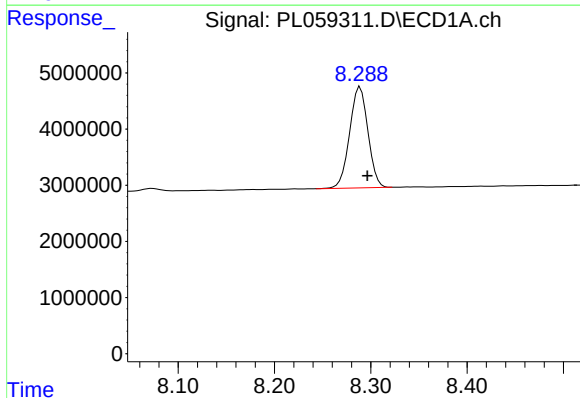

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: -0.009 min
Response: 23745336
Conc: 14.44 ng/ml m

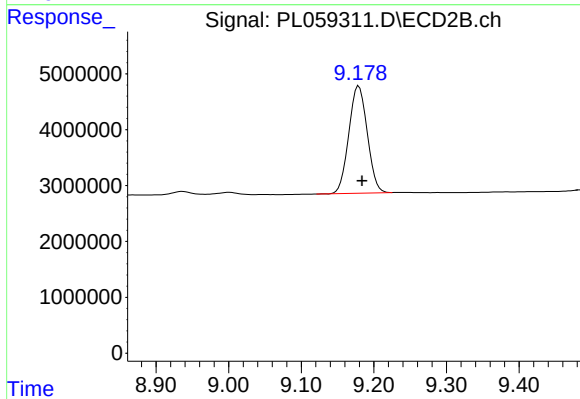

#28 Decachlorobiphenyl

R.T.: 9.179 min
Delta R.T.: -0.005 min
Response: 33906045
Conc: 14.30 ng/ml