

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 15:40
 Operator : UA\AJ
 Sample : J3249-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:57:36 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	85189327	25794564	10.769	9.323
28)	SA Decachlor...	8.021	8.950	52279567	18822178	8.664	9.487
Target Compounds							
2)	A alpha-BHC	3.781	0.000	6123871	0	0.500	N.D. #
5)	MB Aldrin	4.576	0.000	11111946	0	1.092	N.D. #
6)	B beta-BHC	4.257f	4.784f	41172751	-3288321	9.027	N.D. #
10)	B gamma-Chl...	5.166f	0.000	21891159	0	2.337	N.D. #
16)	A 4,4'-DDD	5.964	0.000	7132978	0	1.086	N.D. #
23)	Chlordane-1	4.187	0.000	2702811	0	8.802	N.D. #
24)	Chlordane-2	4.658	0.000	1570466	0	4.411	N.D. #
25)	Chlordane-3	5.166	0.000	21891159	0	20.595	N.D. #
27)	Chlordane-5	5.964	0.000	7132978	0	54.505	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 15:40
Operator : UA\AJ
Sample : J3249-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:57:36 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

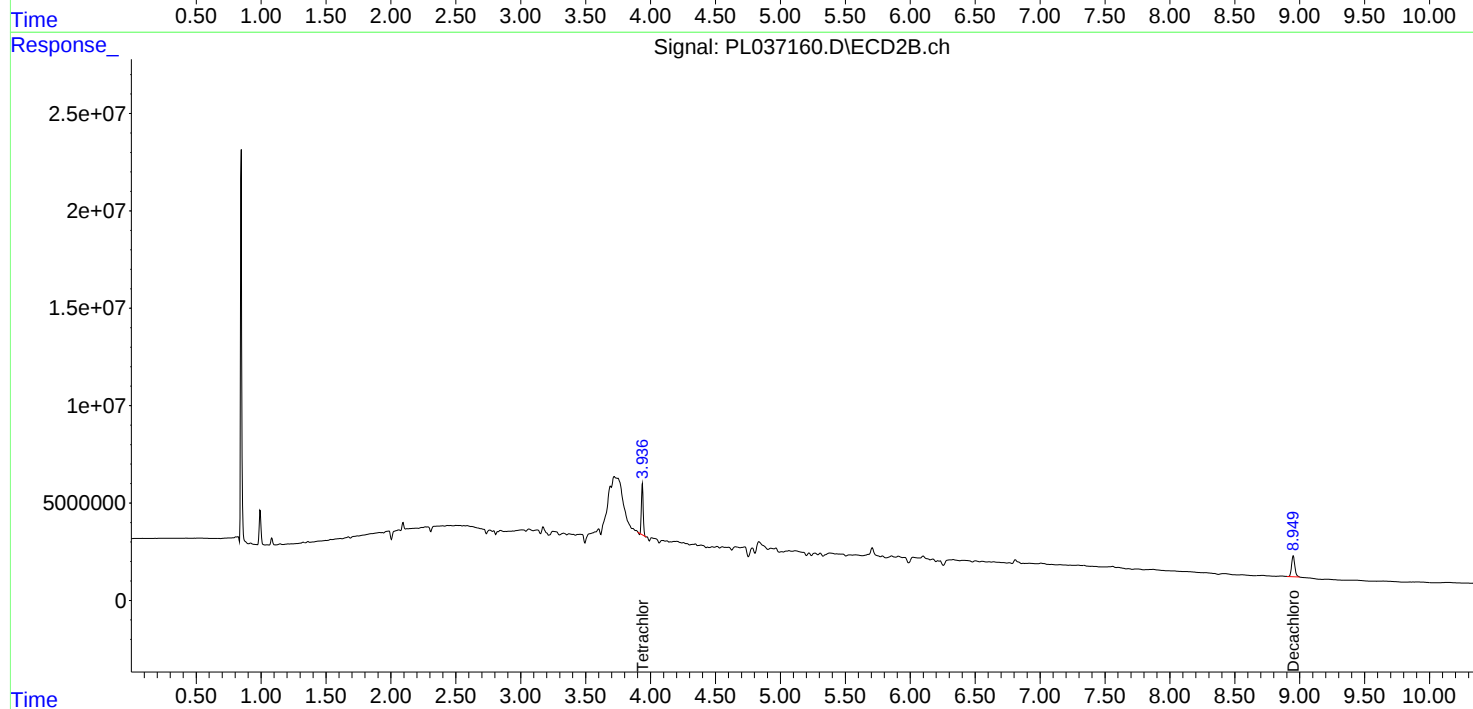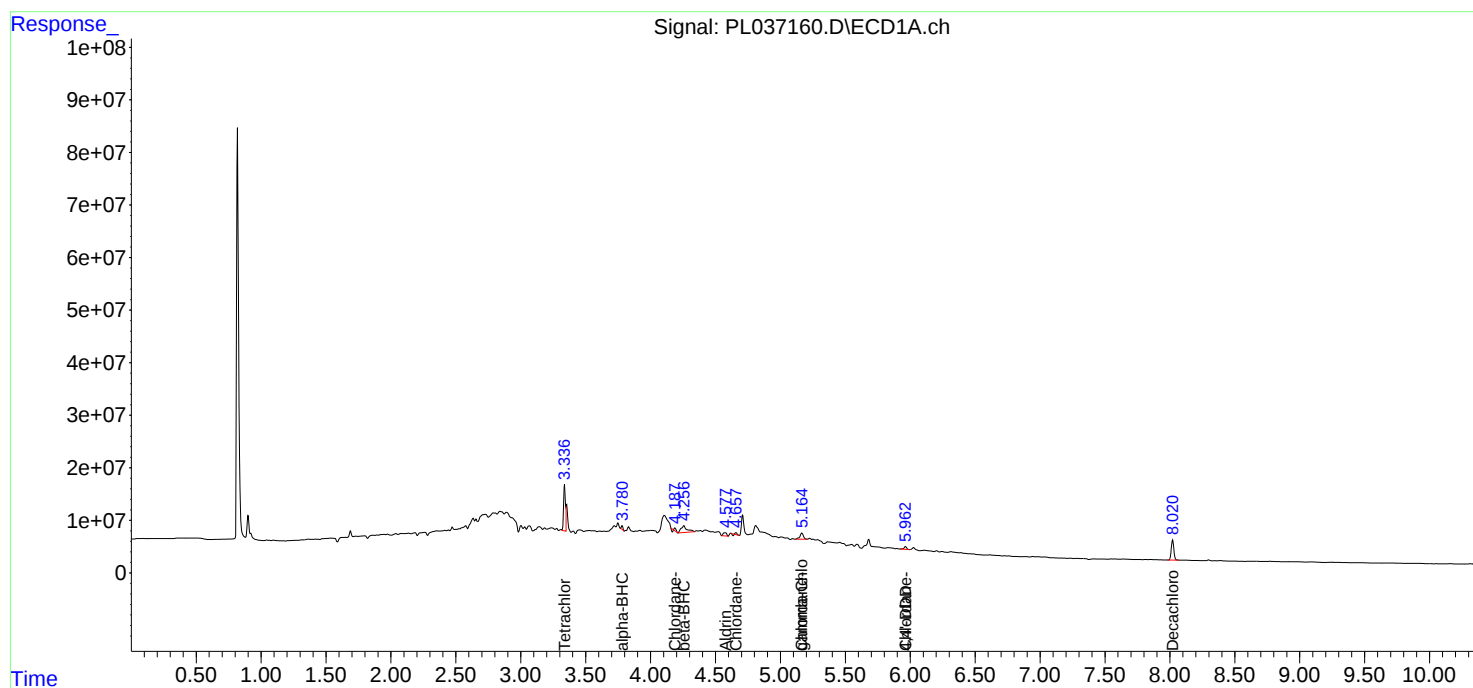


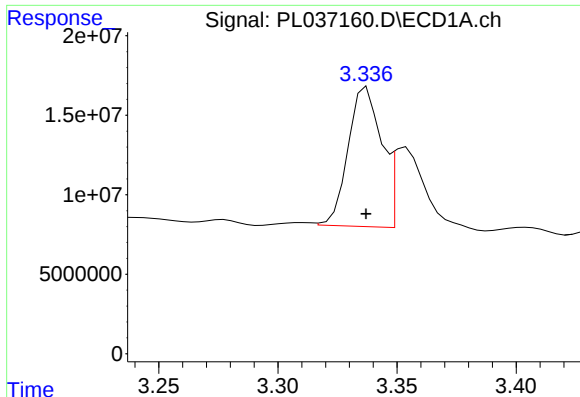

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 85189327
Conc: 10.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

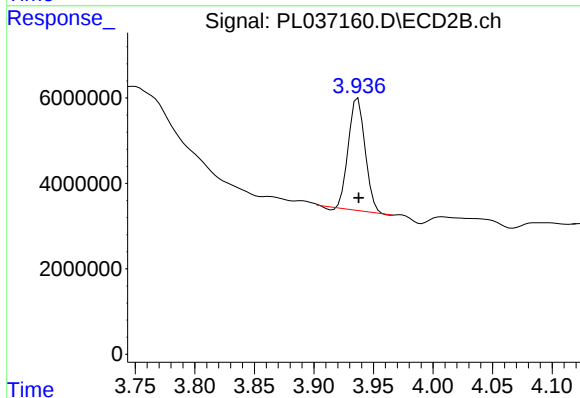


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 25794564
Conc: 9.32 ng/ml

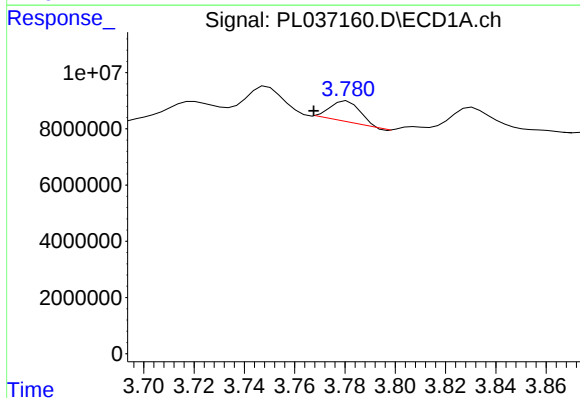


#2 alpha-BHC

R.T.: 3.781 min
Delta R.T.: 0.013 min
Response: 6123871
Conc: 0.50 ng/ml

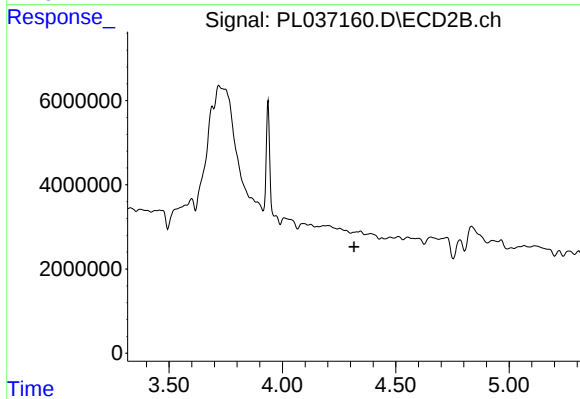

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

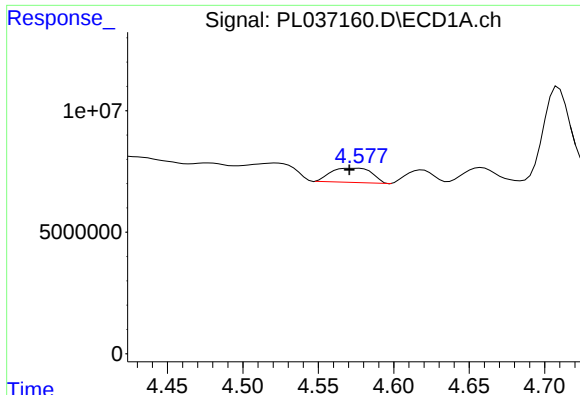

#5 Aldrin

R.T.: 4.576 min
Delta R.T.: 0.006 min
Response: 11111946
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

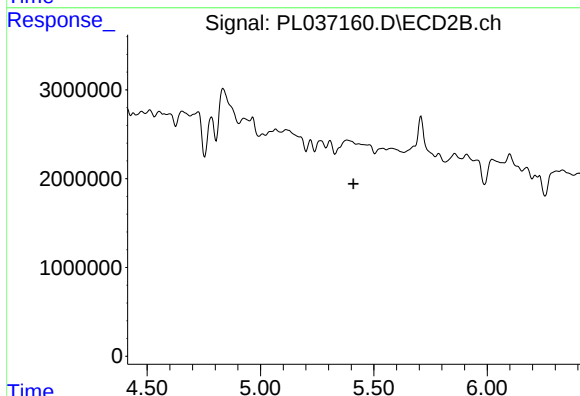


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.


#6 beta-BHC

R.T.: 4.257 min
Delta R.T.: -0.042 min
Response: 41172751
Conc: 9.03 ng/ml

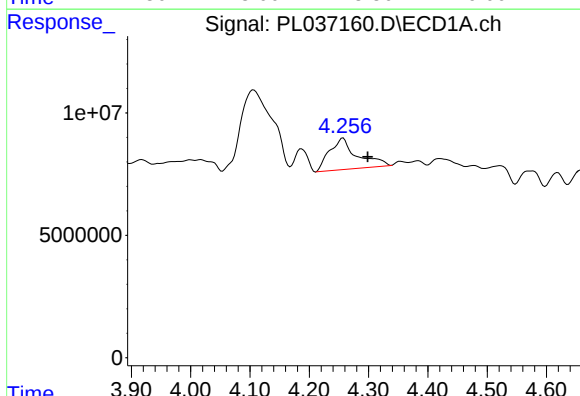

#6 beta-BHC


R.T.: 4.784 min
Delta R.T.: 0.026 min
Response: -3288321
Conc: N.D.

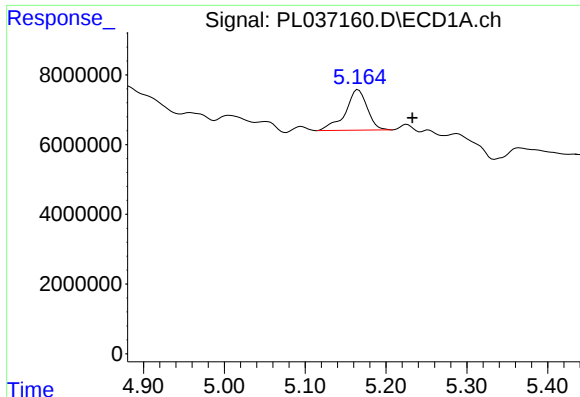

#10 gamma-Chlordane


R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 21891159
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

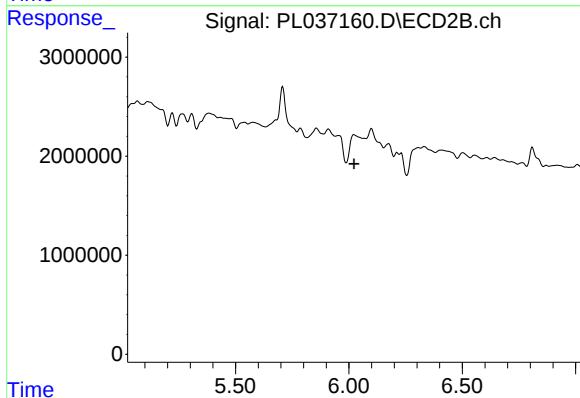


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

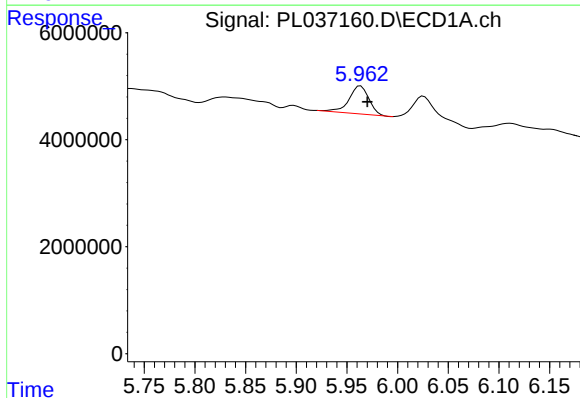


#16 4,4'-DDD

R.T.: 5.964 min
Delta R.T.: -0.007 min
Response: 7132978
Conc: 1.09 ng/ml

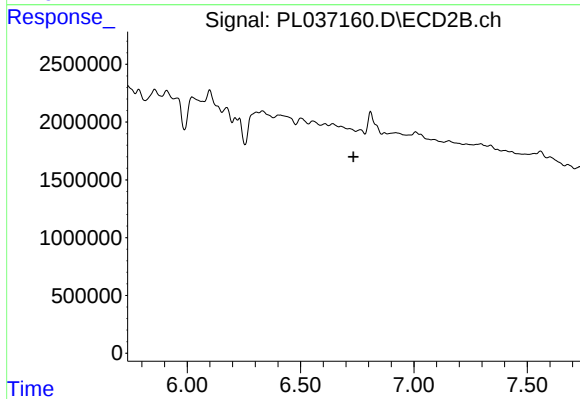

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

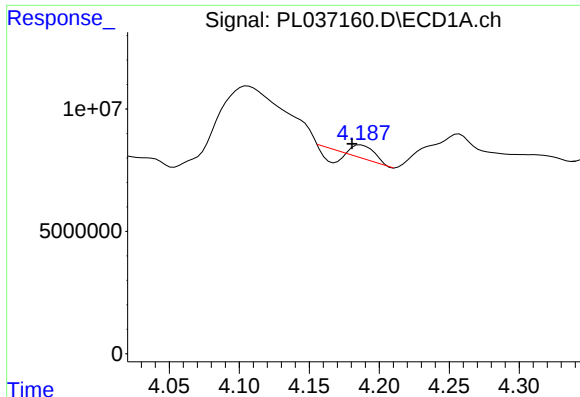

#23 Chlordane-1


R.T.: 4.187 min
Delta R.T.: 0.006 min
Response: 2702811
Conc: 8.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

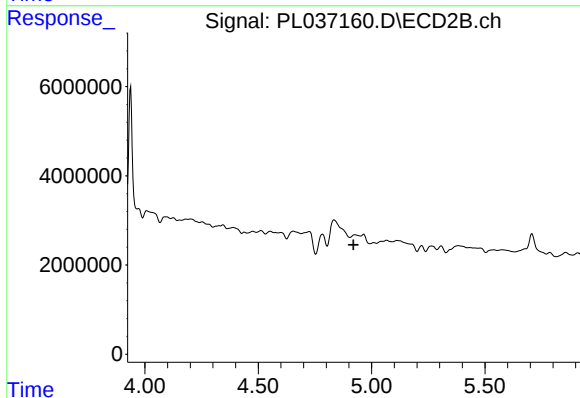


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

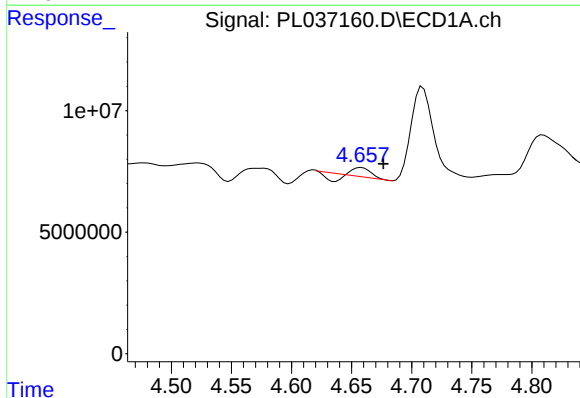


#24 Chlordane-2

R.T.: 4.658 min
Delta R.T.: -0.018 min
Response: 1570466
Conc: 4.41 ng/ml

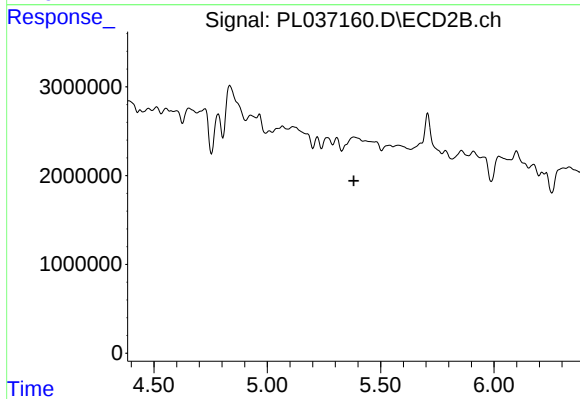

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

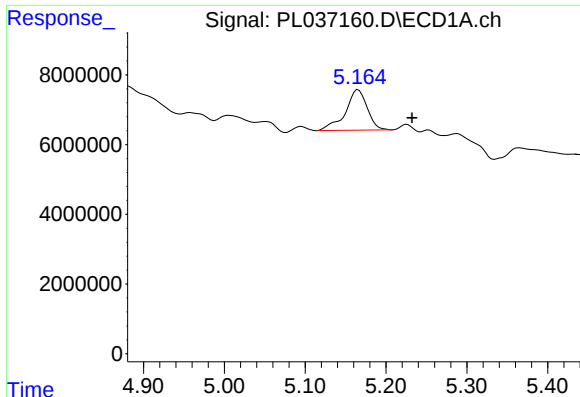

#25 Chlordane-3


R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 21891159
Conc: 20.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

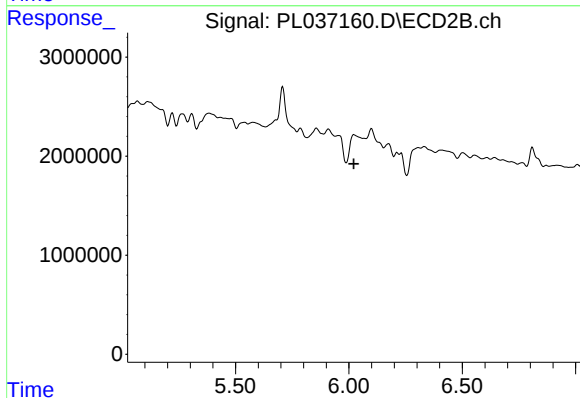


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

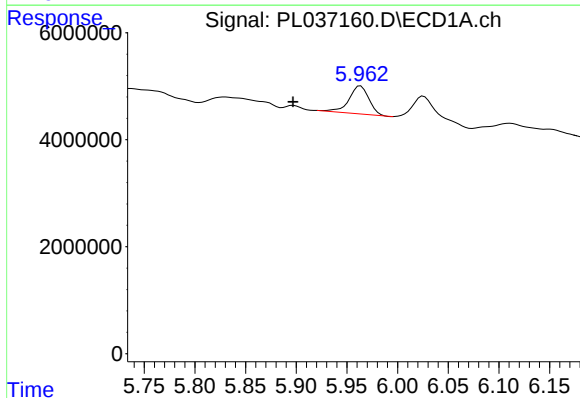


#27 Chlordane-5

R.T.: 5.964 min
Delta R.T.: 0.067 min
Response: 7132978
Conc: 54.51 ng/ml

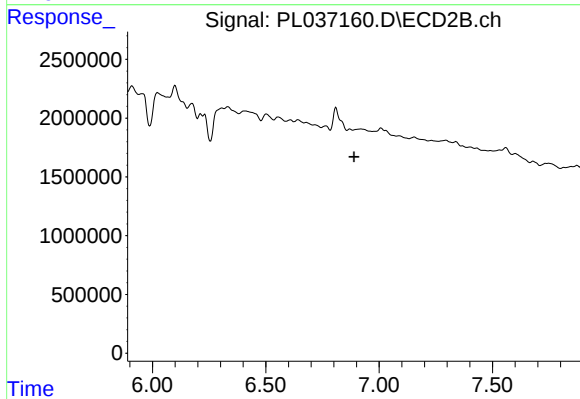

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

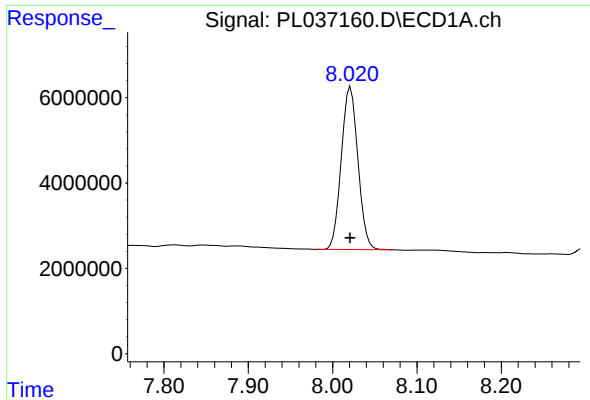

#28 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: 0.000 min
Response: 52279567
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

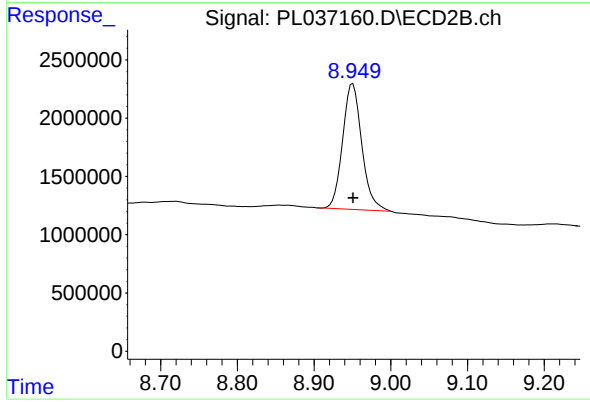

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 18822178
Conc: 9.49 ng/ml