

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 18:16
 Operator : UA\AJ
 Sample : J3570-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:59:37 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	49724157	17351526	6.286	6.271
28)	SA Decachlor...	8.021	8.950	36508086	12533376	6.050	6.317
Target Compounds							
2)	A alpha-BHC	3.722f	0.000	36333763	0	2.968	N.D. #
6)	B beta-BHC	4.256f	0.000	12033780	0	2.638	N.D. #
8)	B Heptachlo...	5.066f	0.000	7216622	0	0.770	N.D. #
10)	B gamma-Chl...	5.210	0.000	4794831	0	0.512	N.D. #
12)	B 4,4'-DDE	5.458	6.251	14000174	4978152	1.585	1.956
14)	MA Endrin	5.896f	0.000	7061600	0	0.896	N.D. #
17)	MA 4,4'-DDT	6.200	0.000	7740717	0	1.199	N.D. #
25)	Chlordane-3	5.210	0.000	4794831	0	4.511	N.D. #
27)	Chlordane-5	5.896	0.000	7061600	0	53.960	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 18:16
Operator : UA\AJ
Sample : J3570-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:59:37 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

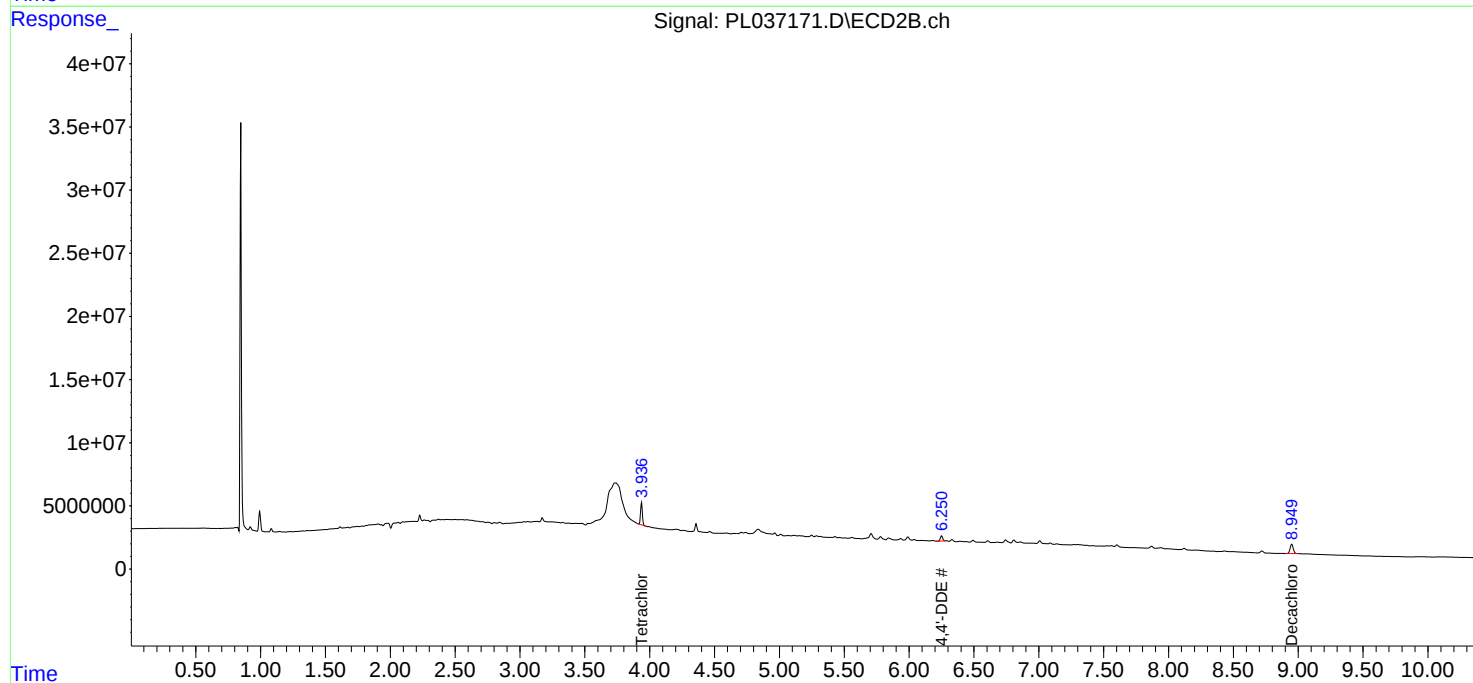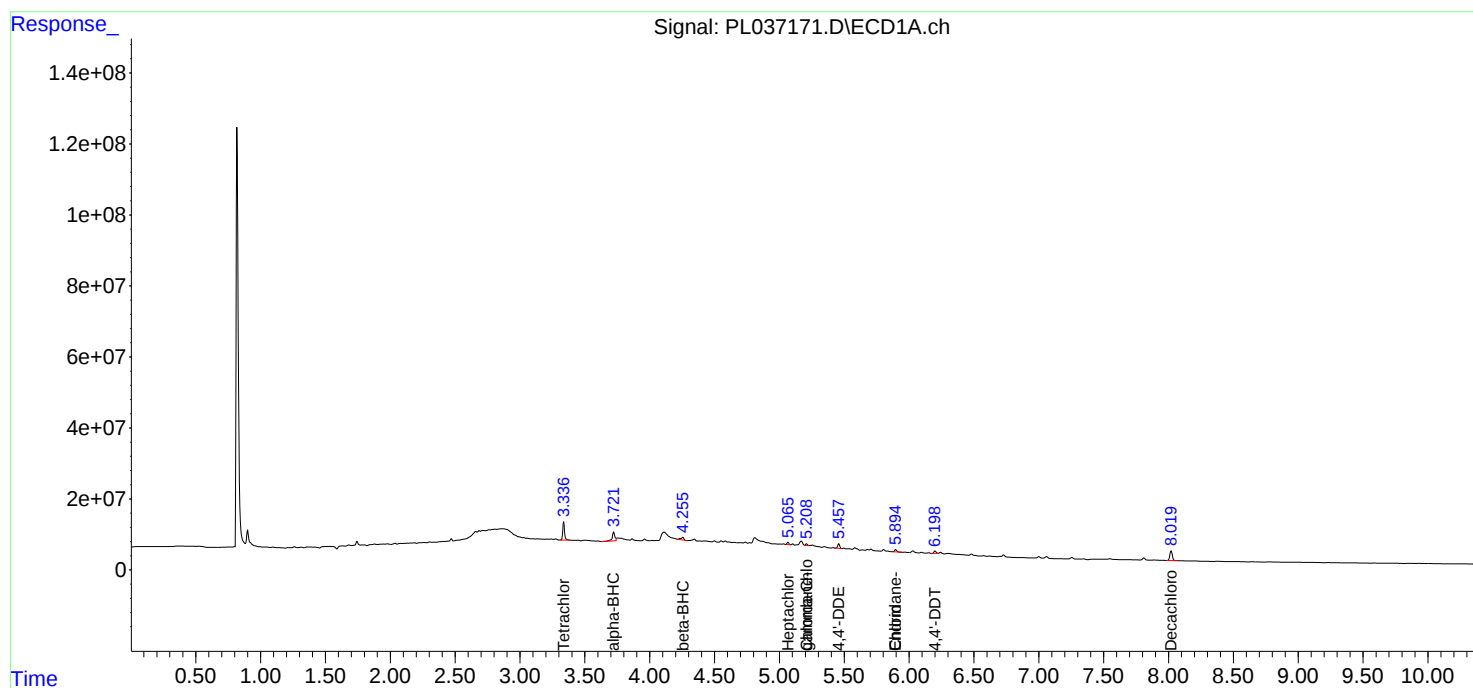


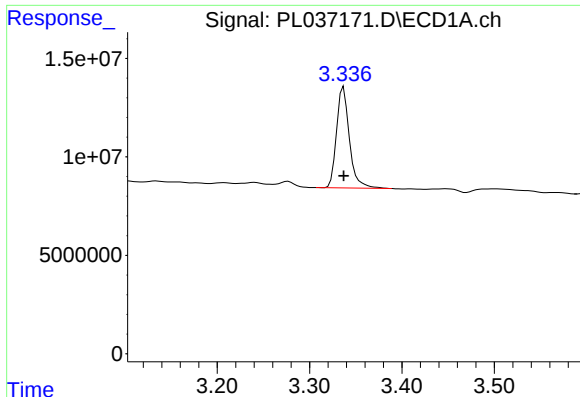

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 49724157
Conc: 6.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

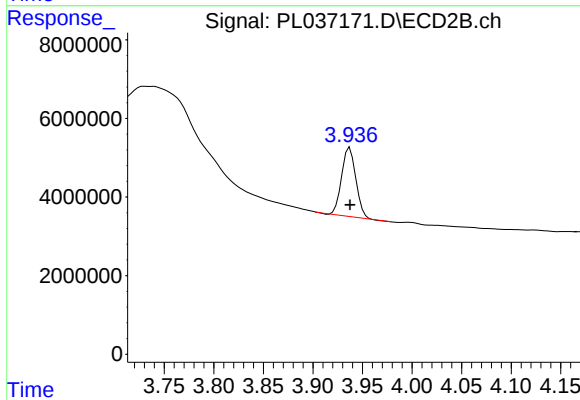


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 17351526
Conc: 6.27 ng/ml

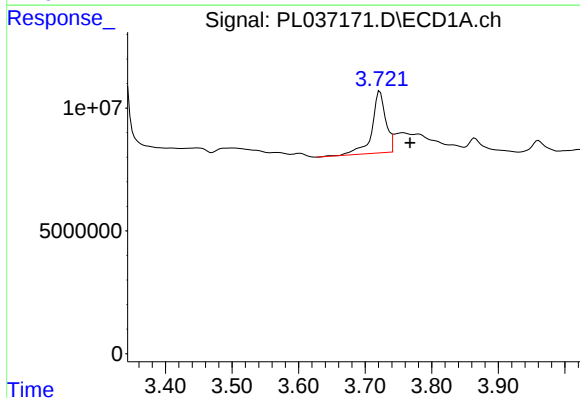


#2 alpha-BHC

R.T.: 3.722 min
Delta R.T.: -0.045 min
Response: 36333763
Conc: 2.97 ng/ml

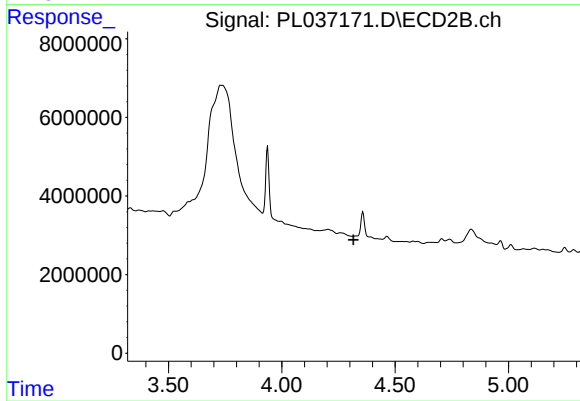

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

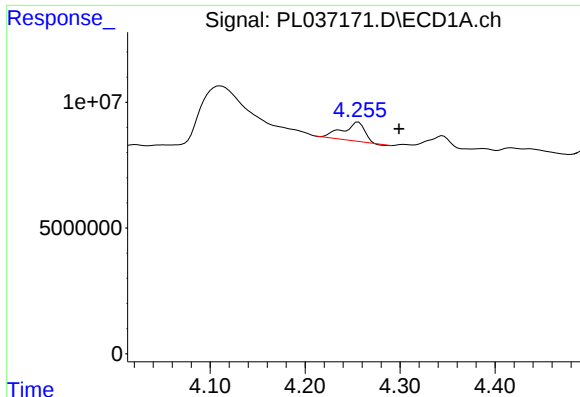

#6 beta-BHC


R.T.: 4.256 min
Delta R.T.: -0.043 min
Response: 12033780
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

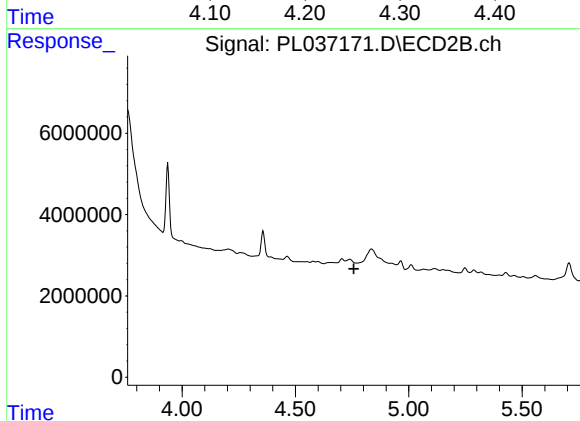


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

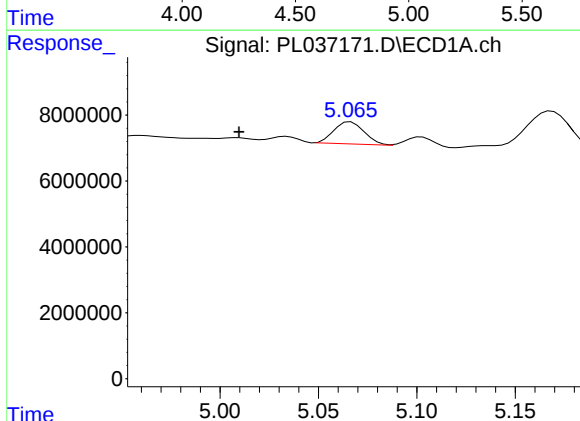


#8 Heptachlor epoxide

R.T.: 5.066 min
Delta R.T.: 0.057 min
Response: 7216622
Conc: 0.77 ng/ml

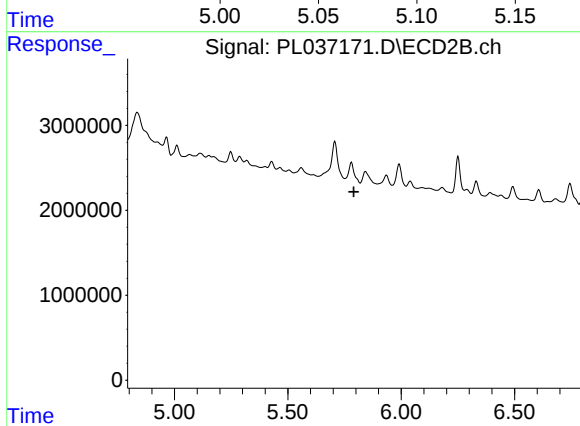

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

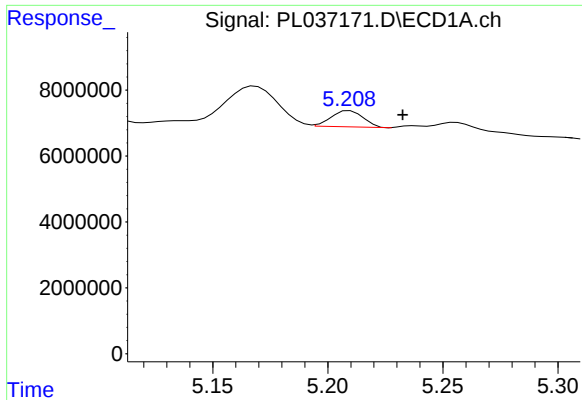

#10 gamma-Chlordane


R.T.: 5.210 min
Delta R.T.: -0.023 min
Response: 4794831
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

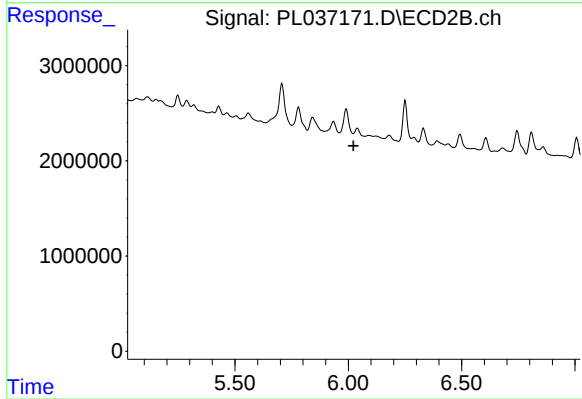


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

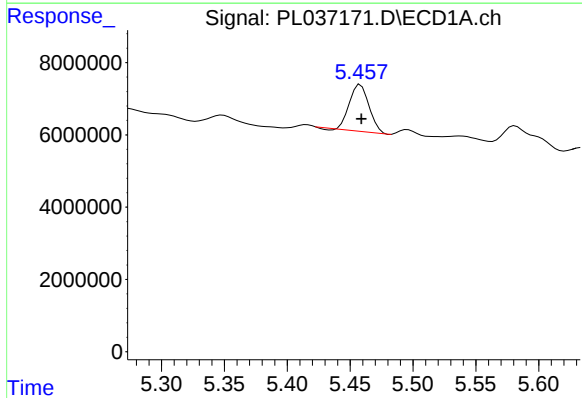


#12 4,4'-DDE

R.T.: 5.458 min
Delta R.T.: 0.000 min
Response: 14000174
Conc: 1.59 ng/ml

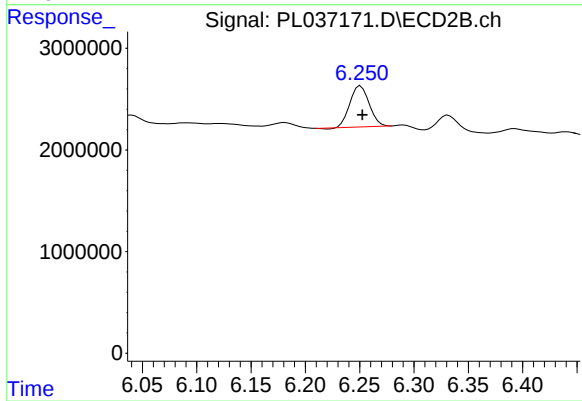

#12 4,4'-DDE


R.T.: 6.251 min
Delta R.T.: -0.002 min
Response: 4978152
Conc: 1.96 ng/ml

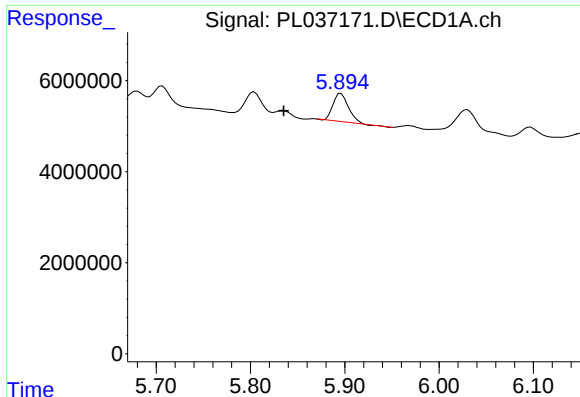

#14 Endrin


R.T.: 5.896 min
Delta R.T.: 0.061 min
Response: 7061600
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

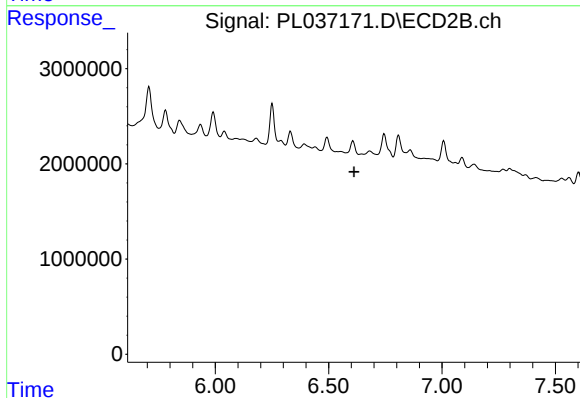


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

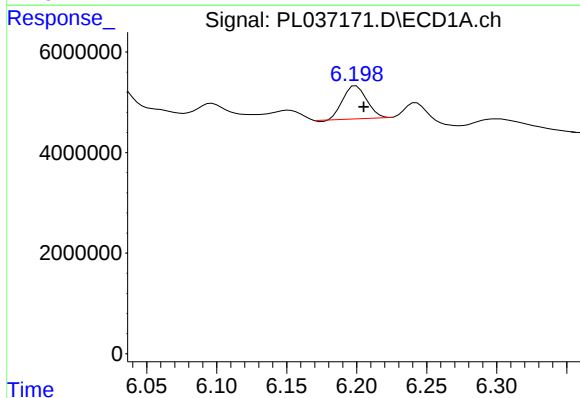


#17 4,4'-DDT

R.T.: 6.200 min
Delta R.T.: -0.005 min
Response: 7740717
Conc: 1.20 ng/ml

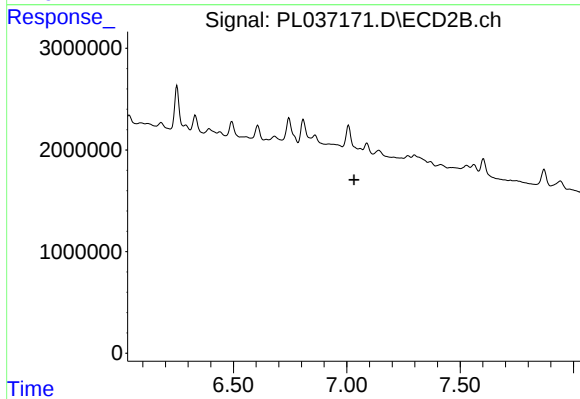

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

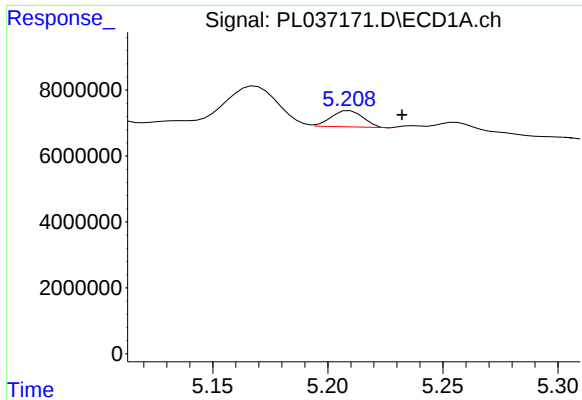

#25 Chlordane-3


R.T.: 5.210 min
Delta R.T.: -0.023 min
Response: 4794831
Conc: 4.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

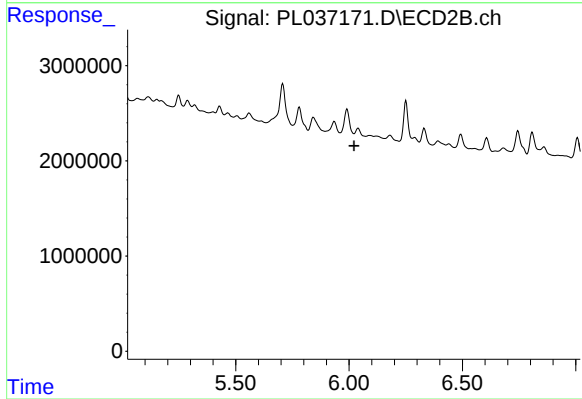


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

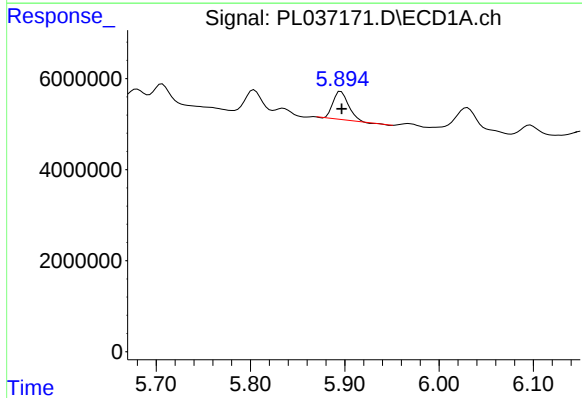


#27 Chlordane-5

R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 7061600
Conc: 53.96 ng/ml

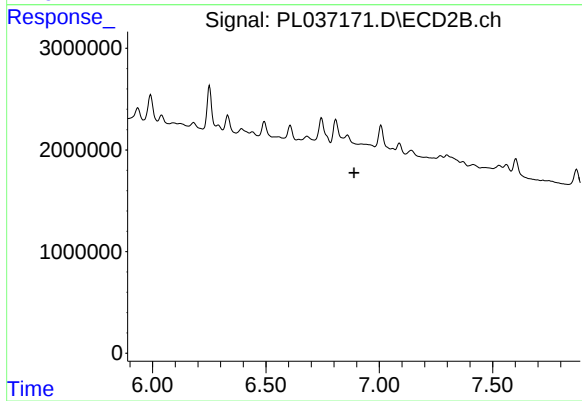

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

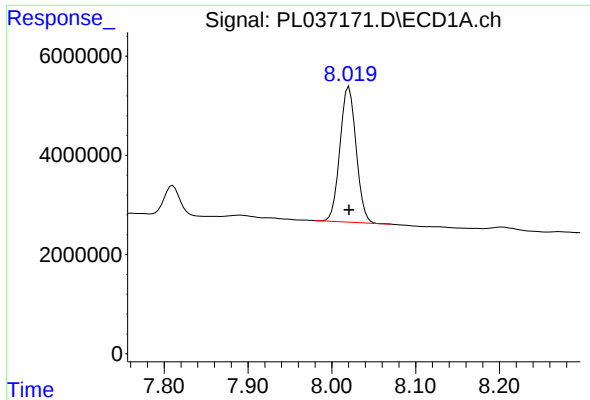

#28 Decachlorobiphenyl


R.T.: 8.021 min

Delta R.T.: 0.000 min

Response: 36508086

Conc: 6.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

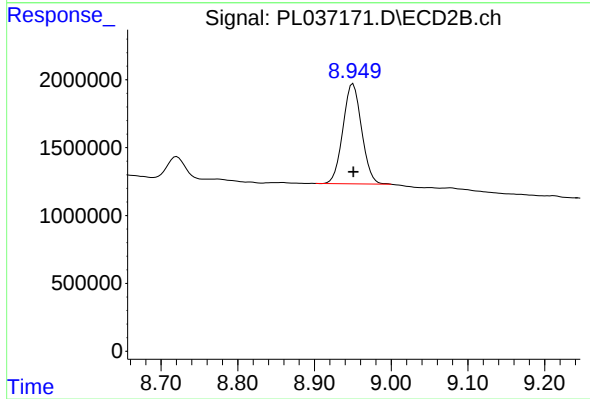

#28 Decachlorobiphenyl

R.T.: 8.950 min

Delta R.T.: 0.000 min

Response: 12533376

Conc: 6.32 ng/ml