

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 02:10
 Operator : UA\AJ
 Sample : J3575-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 04:25:48 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.342	3.937	140.7E6	50996508	17.789	18.432
28)	SA Decachlor...	8.027	8.953	117.4E6	36576562	19.463	18.436
Target Compounds							
4)	MA Heptachlor	4.262f	0.000	11091384	0	1.083	N.D. #
6)	B beta-BHC	4.262f	0.000	11091384	0	2.432	N.D. #
10)	B gamma-Chl...	5.168f	0.000	16847432	0	1.799	N.D. #
23)	Chlordane-1	4.114	0.000	19899101	0	64.807	N.D. #
25)	Chlordane-3	5.168	0.000	16847432	0	15.850	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 02:10
Operator : UA\AJ
Sample : J3575-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 04:25:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

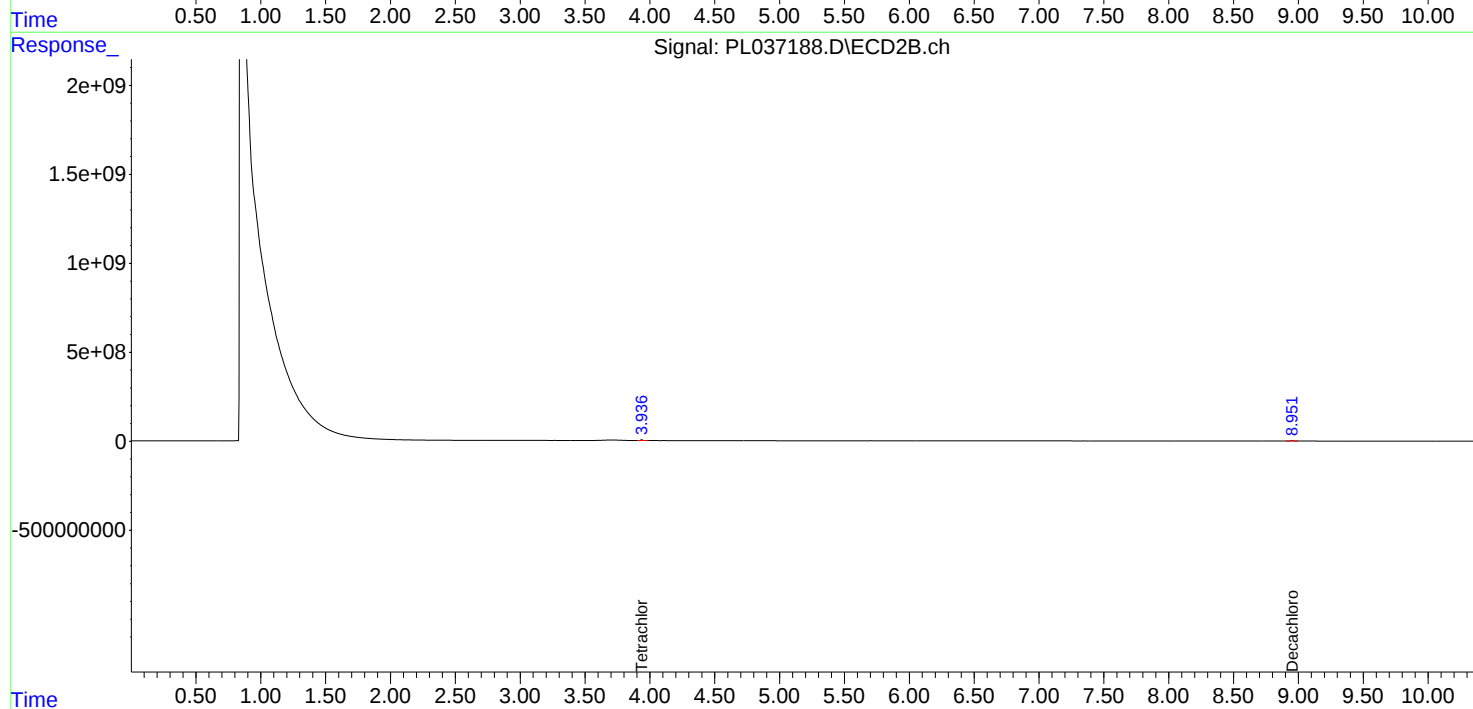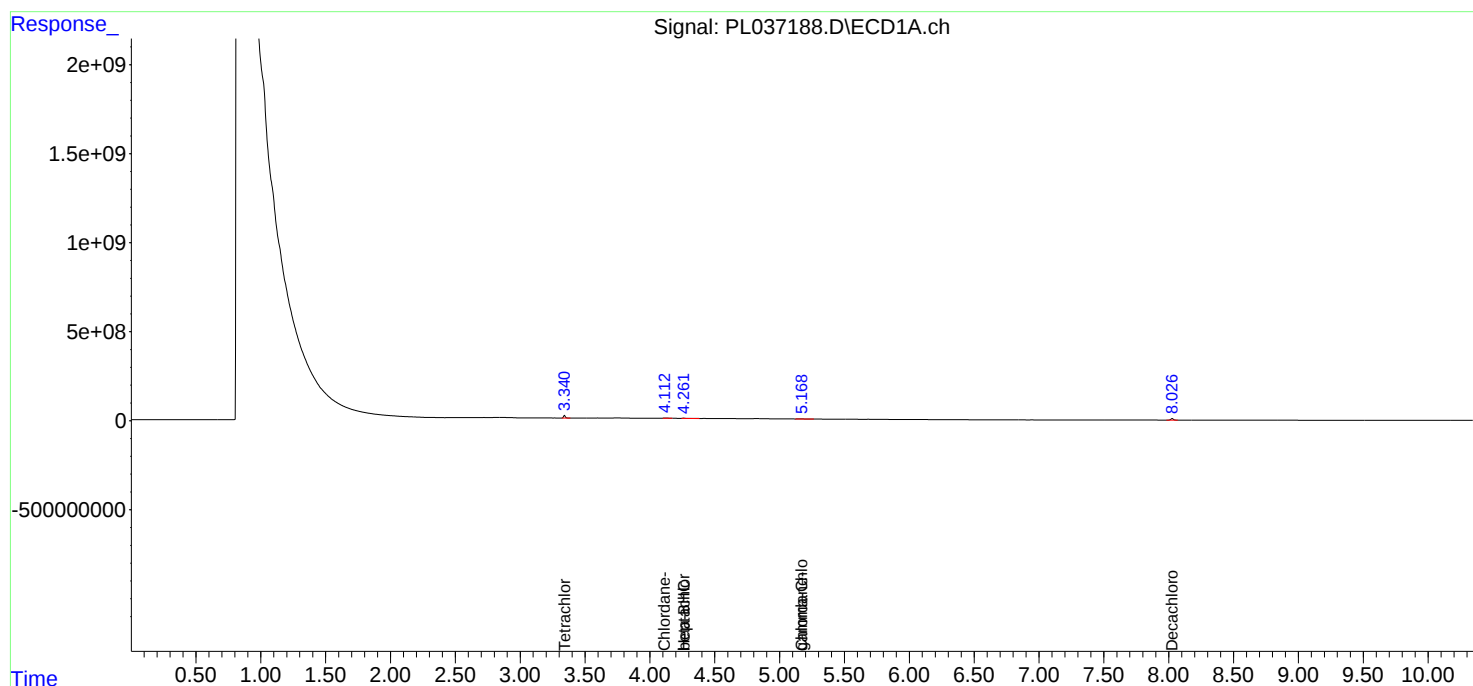


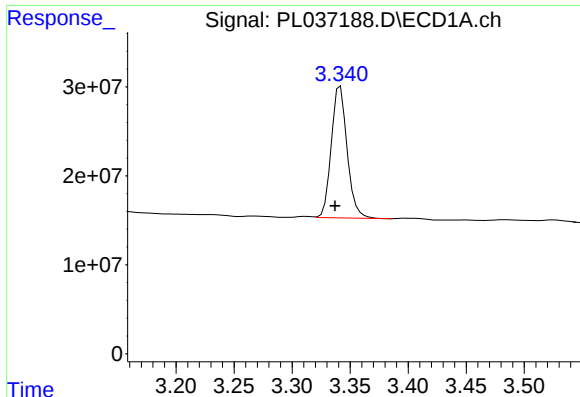

#1 Tetrachloro-m-xylene


R.T.: 3.342 min
Delta R.T.: 0.005 min
Response: 140717857
Conc: 17.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

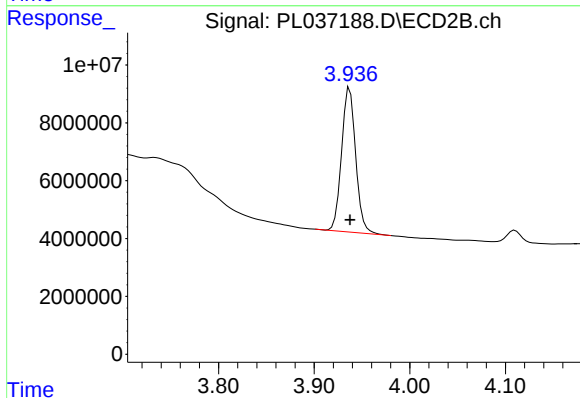


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 50996508
Conc: 18.43 ng/ml

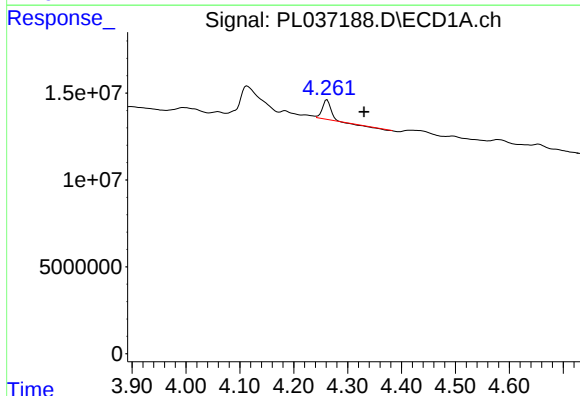


#4 Heptachlor

R.T.: 4.262 min
Delta R.T.: -0.069 min
Response: 11091384
Conc: 1.08 ng/ml

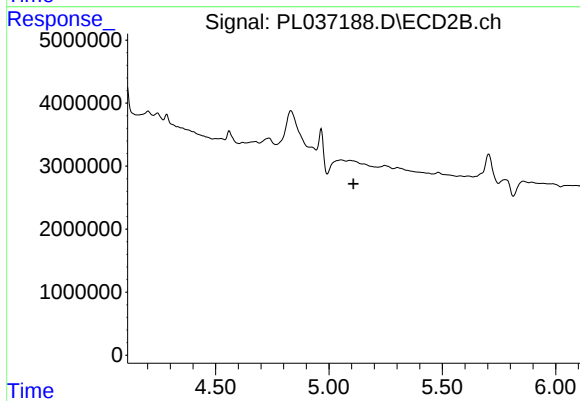

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

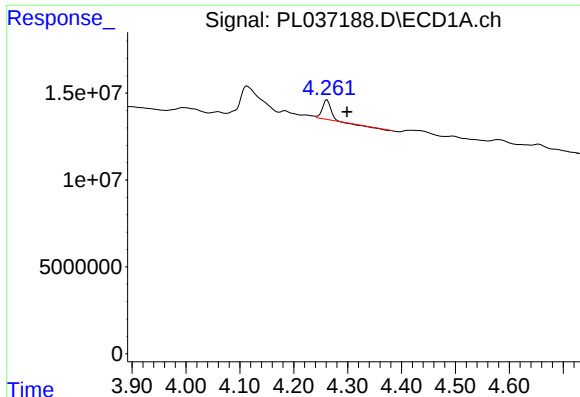

#6 beta-BHC


R.T.: 4.262 min
Delta R.T.: -0.037 min
Response: 11091384
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

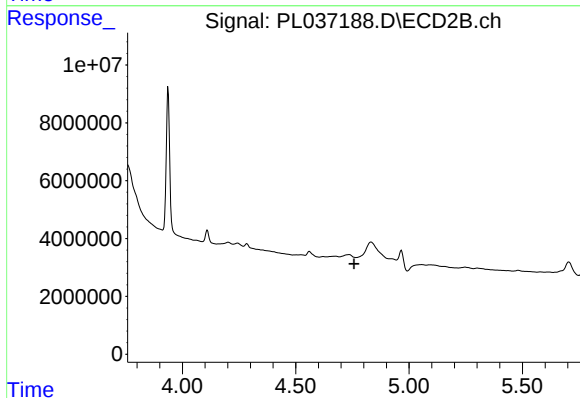


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

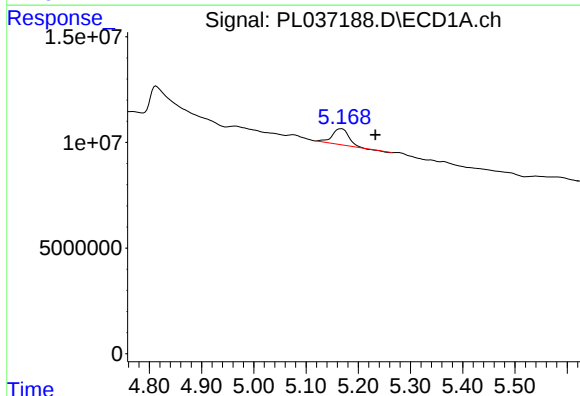


#10 gamma-Chlordane

R.T.: 5.168 min
Delta R.T.: -0.064 min
Response: 16847432
Conc: 1.80 ng/ml

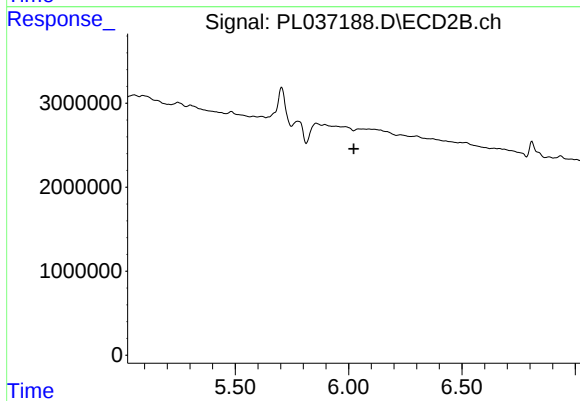

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

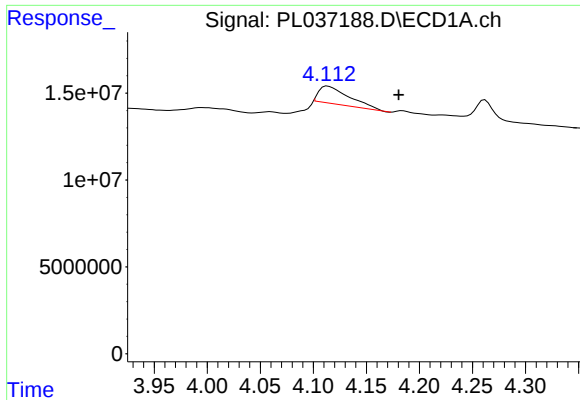

#23 Chlordane-1


R.T.: 4.114 min
Delta R.T.: -0.067 min
Response: 19899101
Conc: 64.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

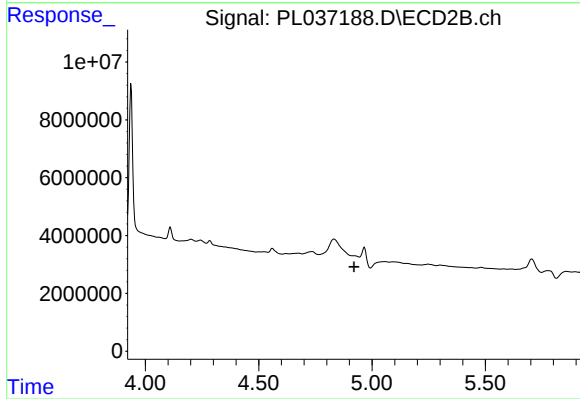


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

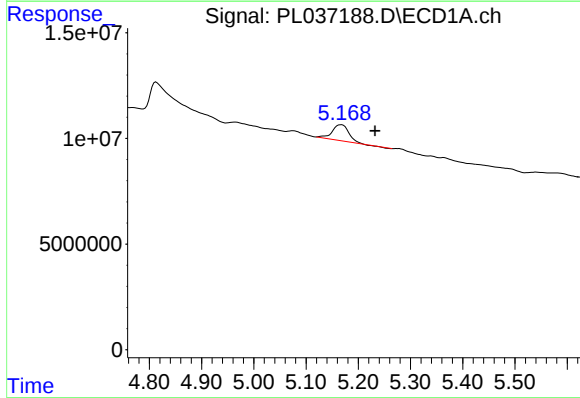


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: -0.064 min
Response: 16847432
Conc: 15.85 ng/ml

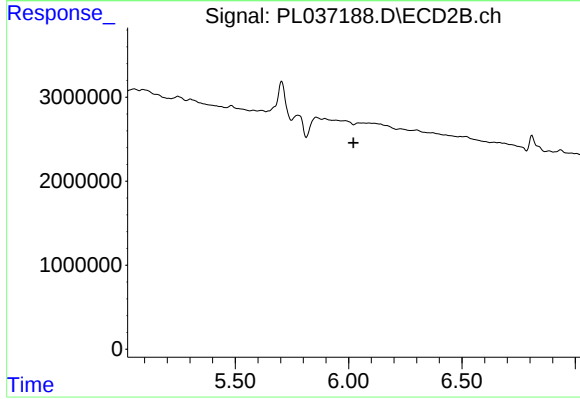

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

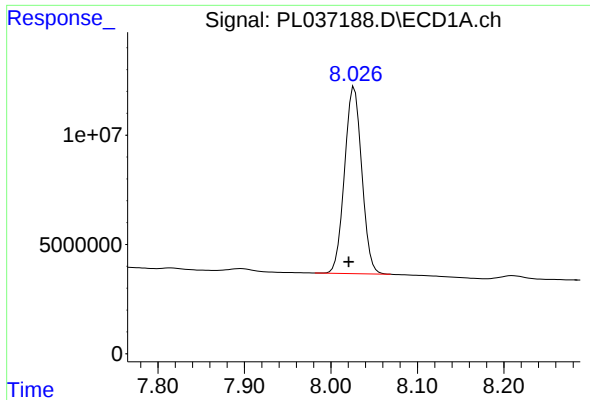

#28 Decachlorobiphenyl


R.T.: 8.027 min

Delta R.T.: 0.006 min

Response: 117442841

Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

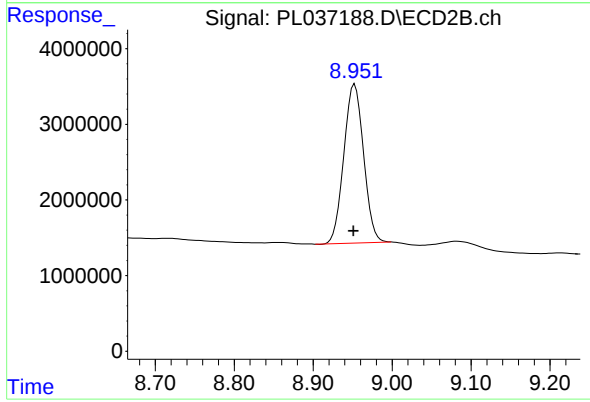

#28 Decachlorobiphenyl

R.T.: 8.953 min

Delta R.T.: 0.002 min

Response: 36576562

Conc: 18.44 ng/ml