

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 03:34
 Operator : UA\AJ
 Sample : J3575-19
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 04:27:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.938	140.5E6	51964626	17.766	18.782
28)	SA Decachlor...	8.022	8.951	120.5E6	38643874	19.977	19.478
Target Compounds							
2)	A alpha-BHC	3.767	0.000	9751192	0	0.796	N.D. #
6)	B beta-BHC	4.257f	0.000	15149155	0	3.322	N.D. #
7)	B delta-BHC	0.000	4.966	0	8303094	N.D.	2.944 #
10)	B gamma-Chl...	5.167f	0.000	21945959	0	2.343	N.D. #
23)	Chlordane-1	4.117	4.966	15206080	8303094	49.523	69.100 #
25)	Chlordane-3	5.167	0.000	21945959	0	20.647	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 03:34
Operator : UA\AJ
Sample : J3575-19
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 04:27:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

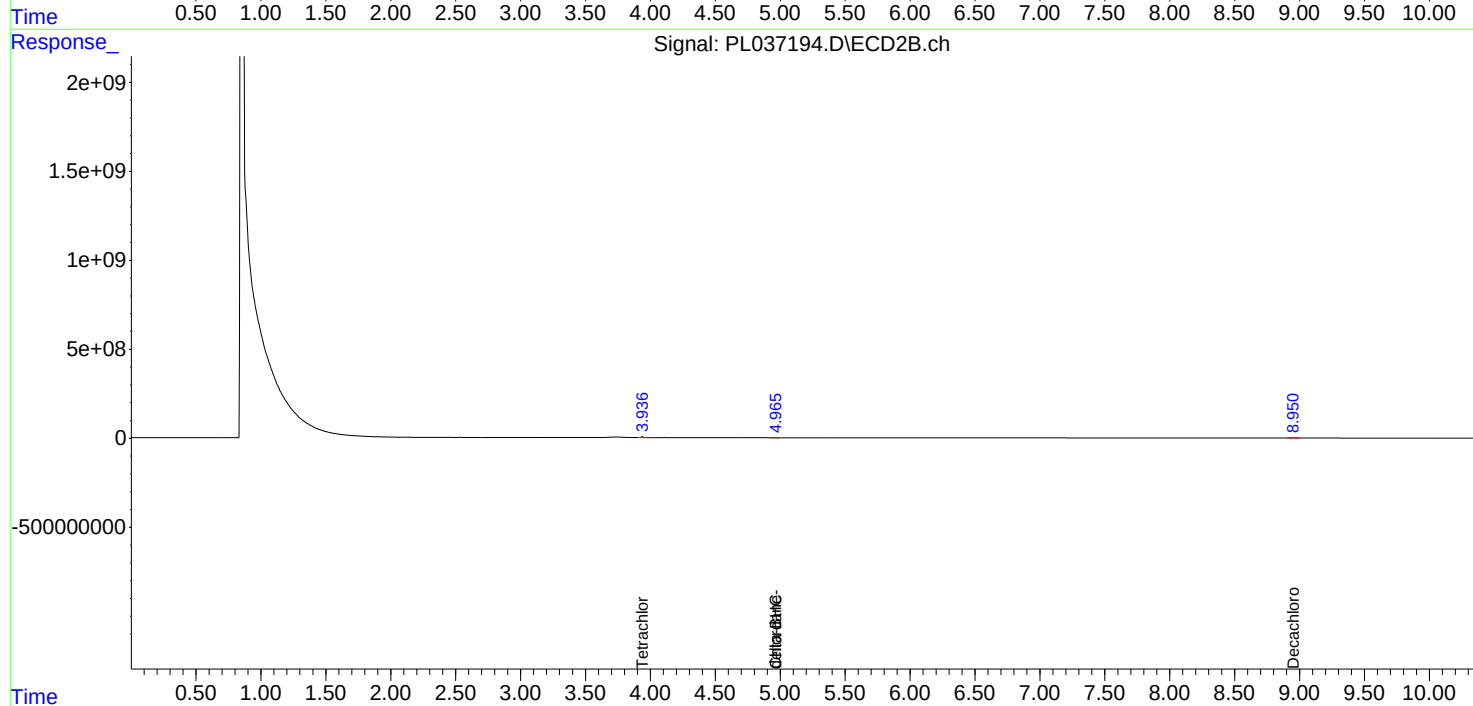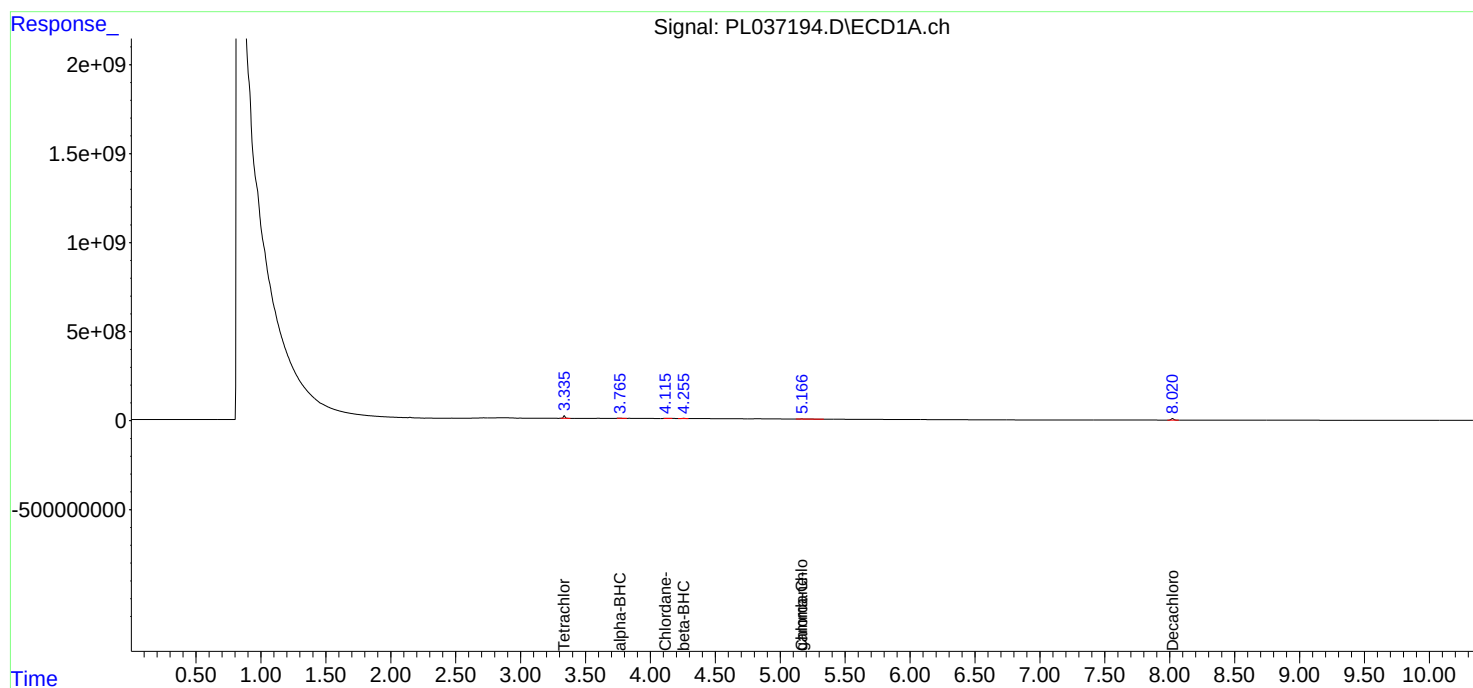


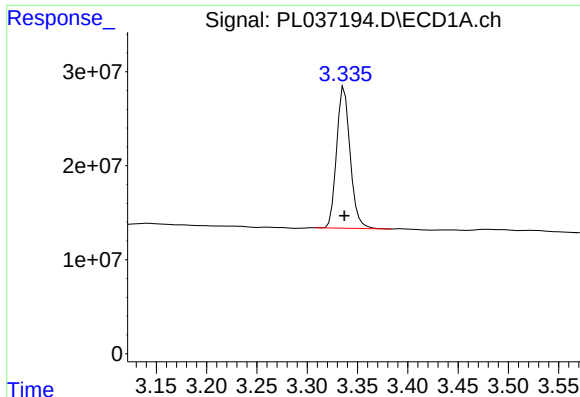

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 140537386
Conc: 17.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

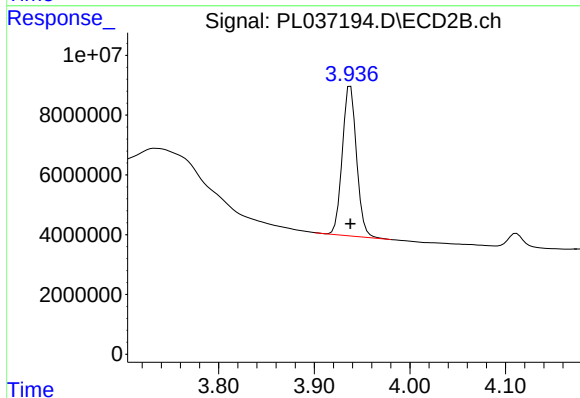


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 51964626
Conc: 18.78 ng/ml

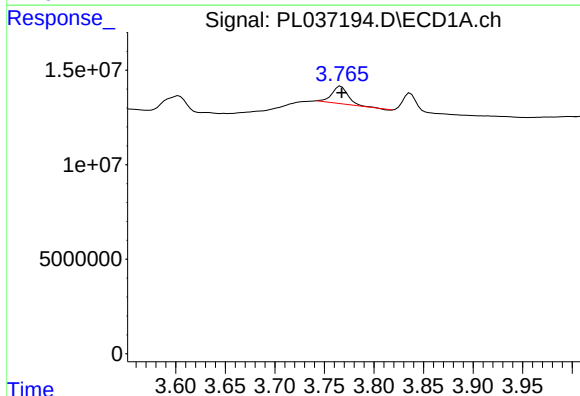


#2 alpha-BHC

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 9751192
Conc: 0.80 ng/ml

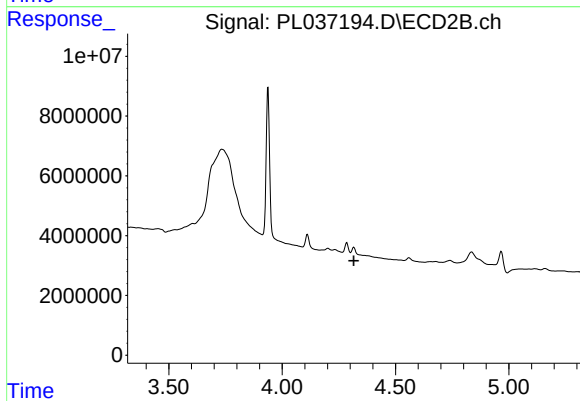

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

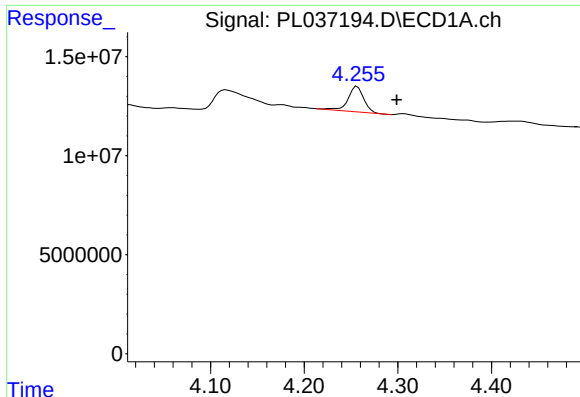

#6 beta-BHC


R.T.: 4.257 min
Delta R.T.: -0.042 min
Response: 15149155
Conc: 3.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

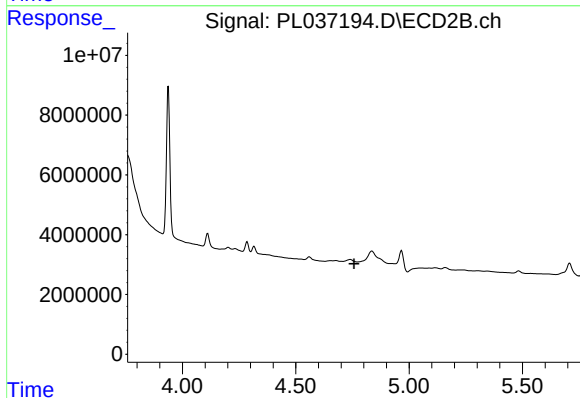


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

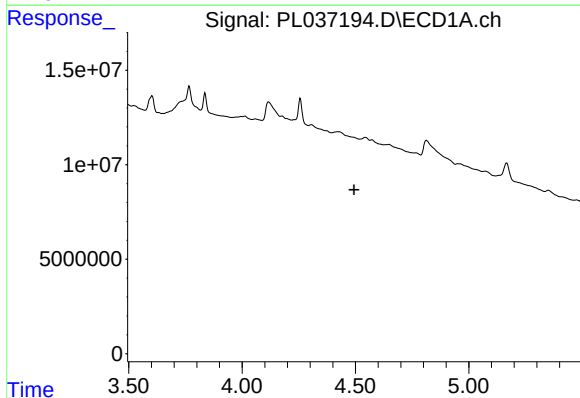


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

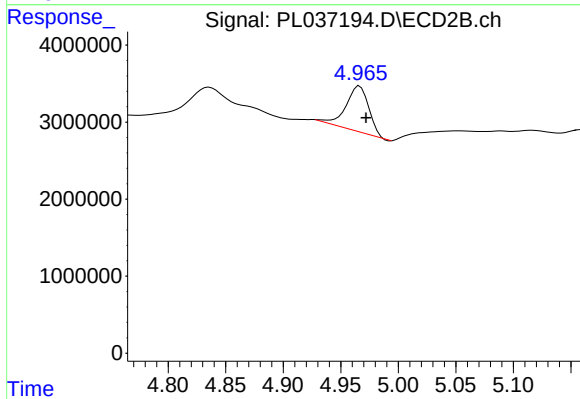

#7 delta-BHC


R.T.: 4.966 min
Delta R.T.: -0.005 min
Response: 8303094
Conc: 2.94 ng/ml

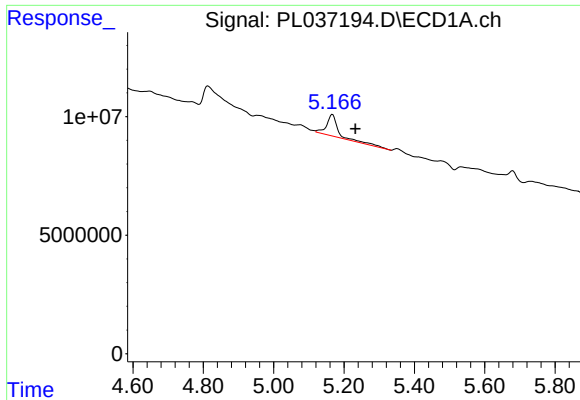

#10 gamma-Chlordane


R.T.: 5.167 min
Delta R.T.: -0.065 min
Response: 21945959
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

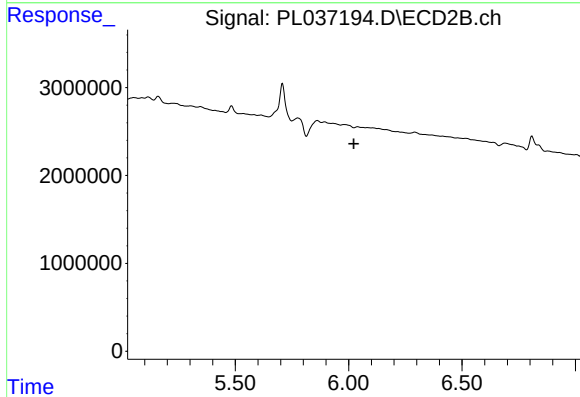


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

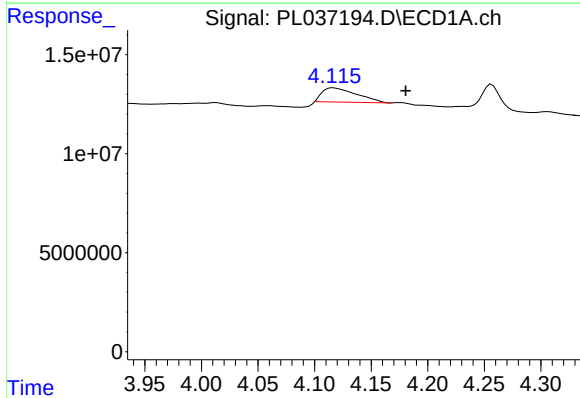


#23 Chlordane-1

R.T.: 4.117 min
Delta R.T.: -0.064 min
Response: 15206080
Conc: 49.52 ng/ml

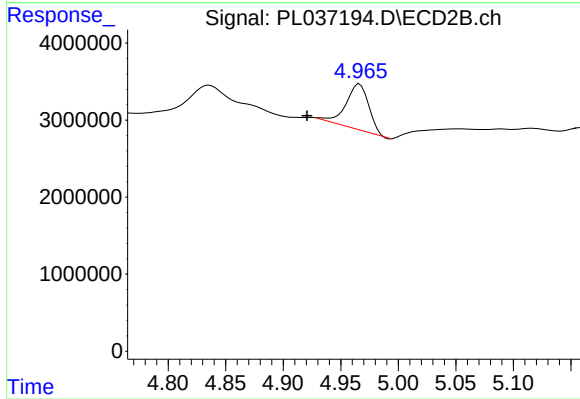

#23 Chlordane-1


R.T.: 4.966 min
Delta R.T.: 0.046 min
Response: 8303094
Conc: 69.10 ng/ml

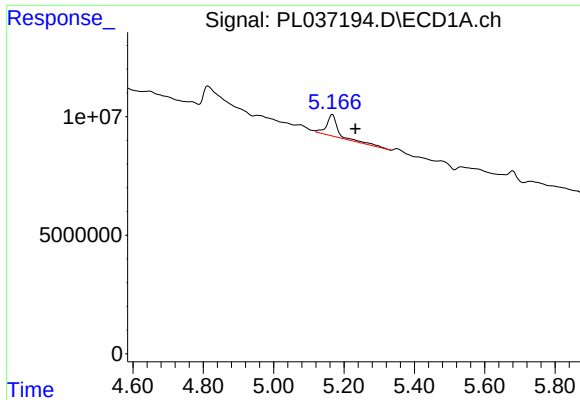

#25 Chlordane-3


R.T.: 5.167 min
Delta R.T.: -0.065 min
Response: 21945959
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

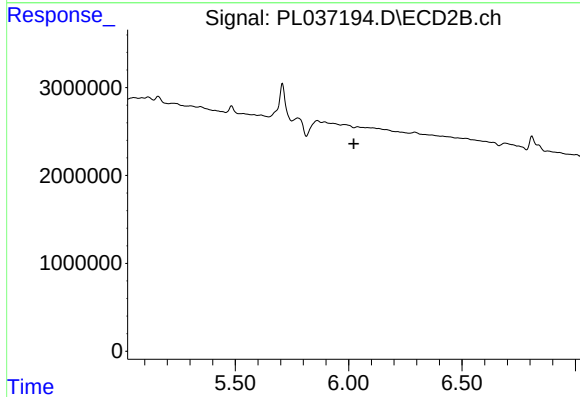


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

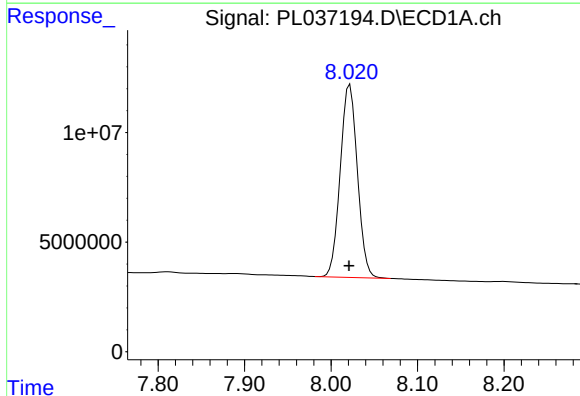

#28 Decachlorobiphenyl

R.T.: 8.022 min
Delta R.T.: 0.001 min
Response: 120541019
Conc: 19.98 ng/ml

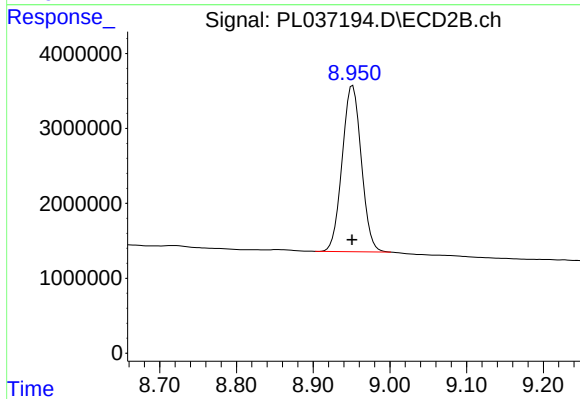

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 38643874
Conc: 19.48 ng/ml