

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 12:08
 Operator : UA\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 13:29:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 13:28:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.938	789.4E6	270.9E6	96.022	97.863
28)	SA Decachlor...	8.021	8.950	556.2E6	181.3E6	94.534	92.699
Target Compounds							
23)	Chlordane-1	4.183	4.922	315.3E6	119.3E6	991.033	996.736
24)	Chlordane-2	4.676	5.384	332.5E6	119.7E6	944.224	949.203
25)	Chlordane-3	5.233	6.024	1058.3E6	396.8E6	974.302	996.383
26)	Chlordane-4	5.289	6.100	966.3E6	474.9E6	980.672	981.470
27)	Chlordane-5	5.898	6.892	137.7E6	88279265	1044.986	980.097



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 12:08
Operator : UA\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:29:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 13:28:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

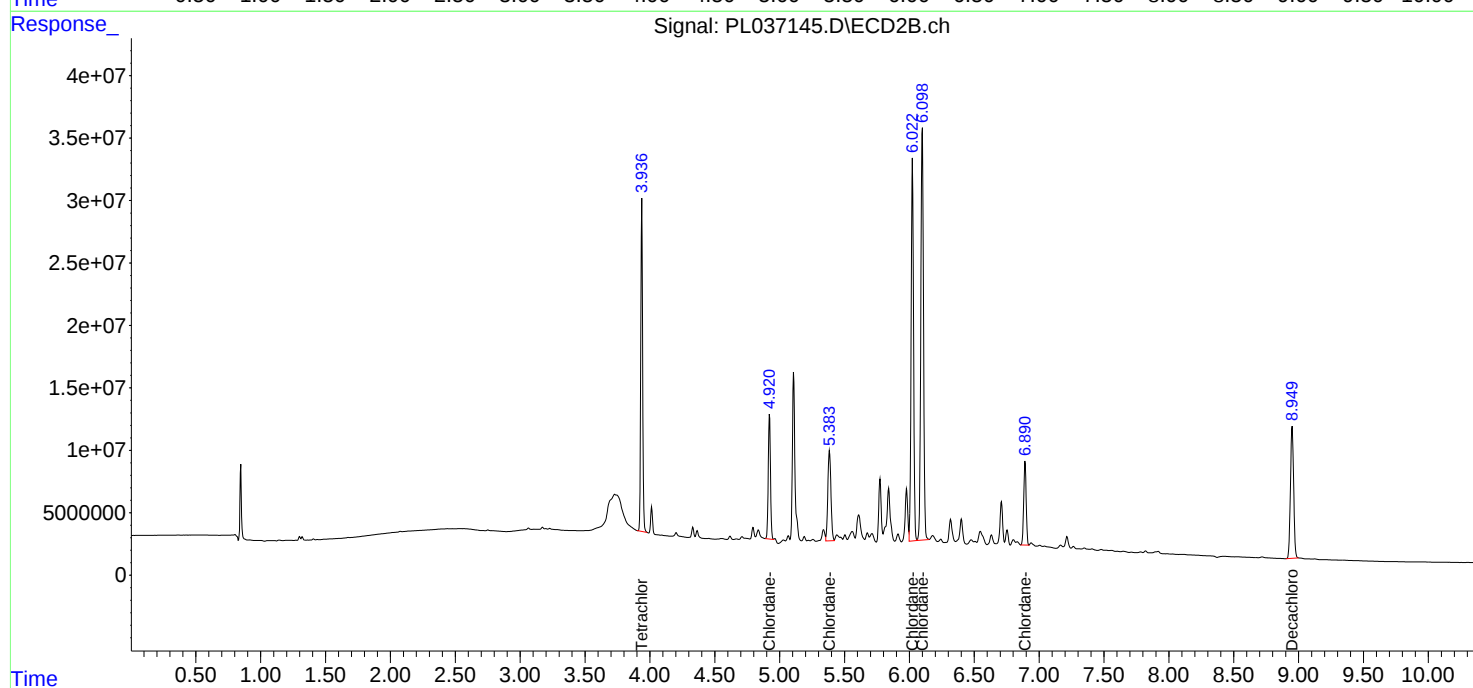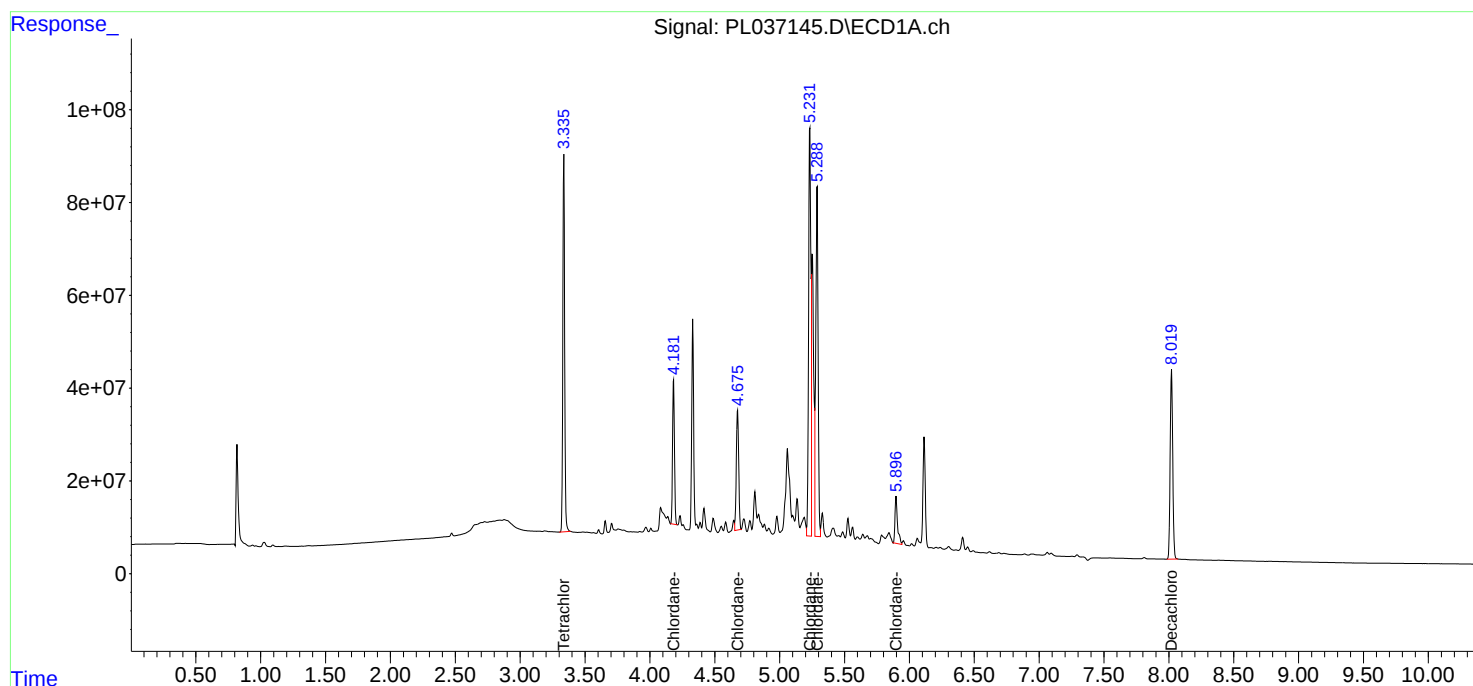


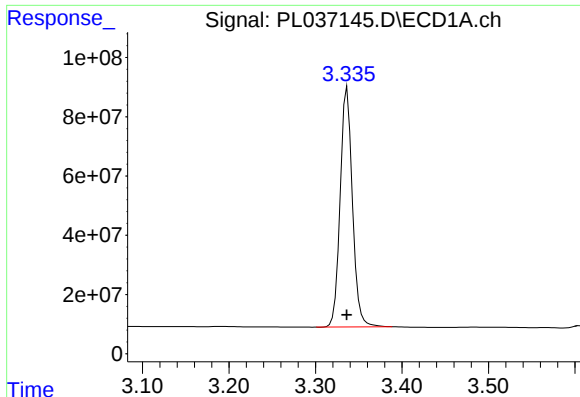

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 789403335
Conc: 96.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

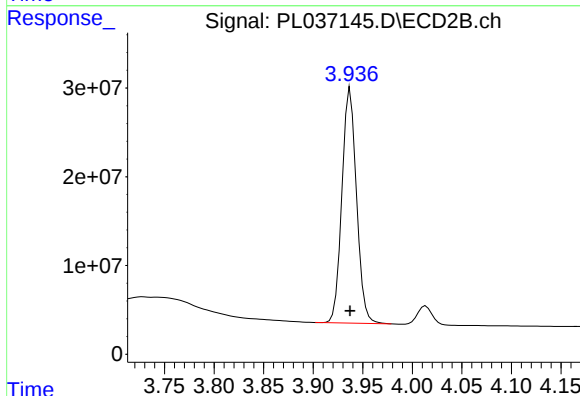


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 270912444
Conc: 97.86 ng/ml

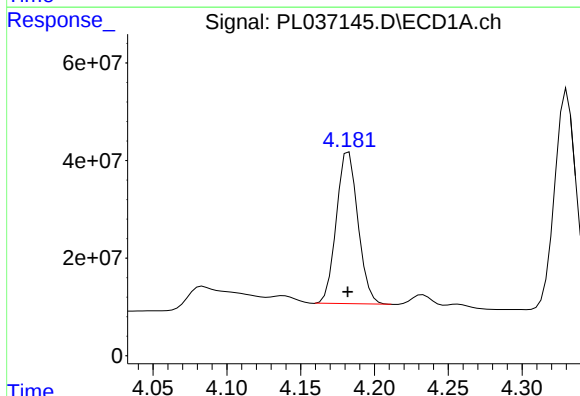


#23 Chlordane-1

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 315281688
Conc: 991.03 ng/ml

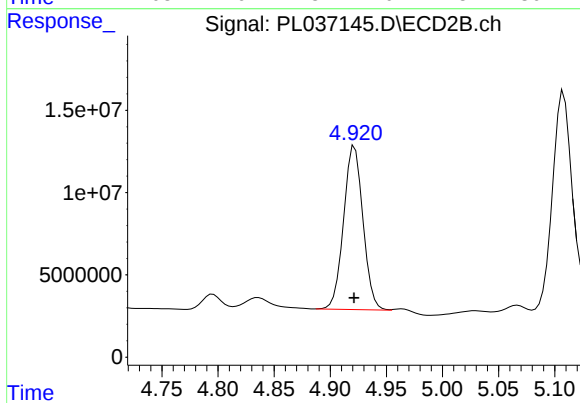

#23 Chlordane-1


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 119340972
Conc: 996.74 ng/ml

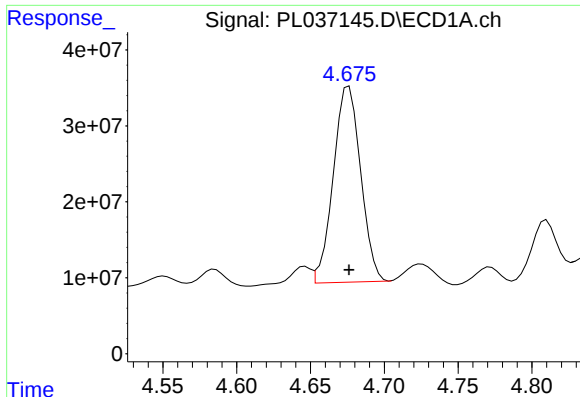

#24 Chlordane-2


R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 332529006
Conc: 944.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

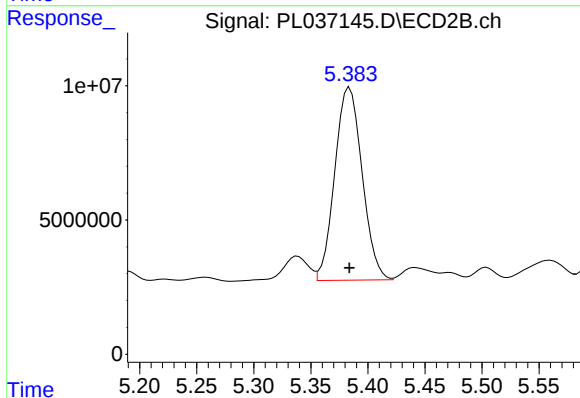


#24 Chlordane-2

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 119655191
Conc: 949.20 ng/ml

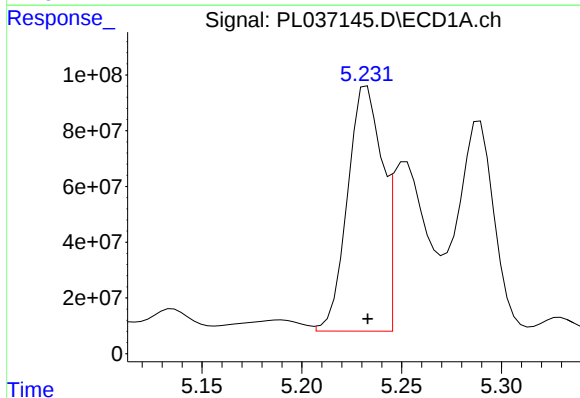


#25 Chlordane-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 1058281028
Conc: 974.30 ng/ml

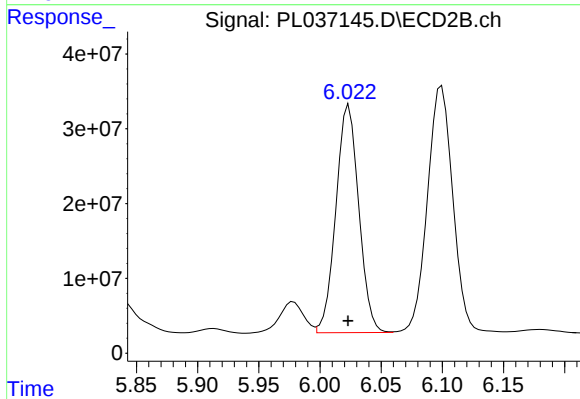

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 396756305
Conc: 996.38 ng/ml

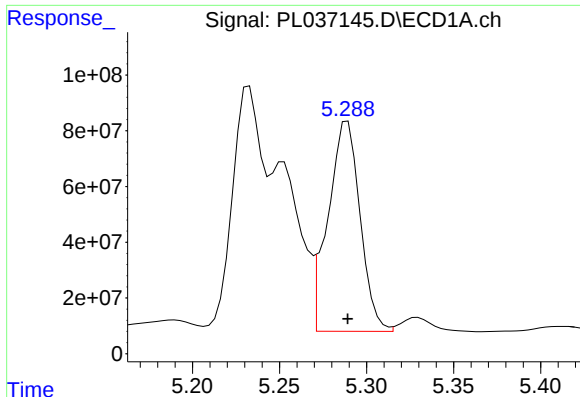

#26 Chlordane-4


R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 966310059
Conc: 980.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

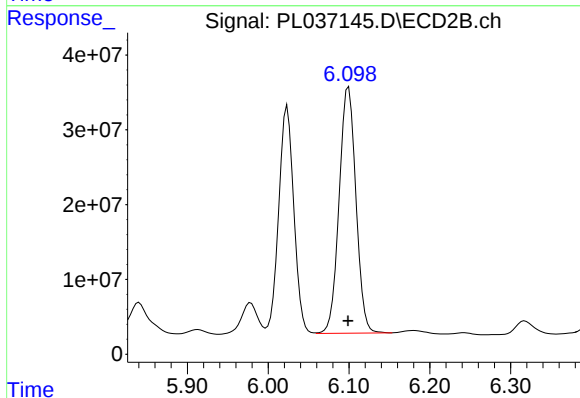


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 474858858
Conc: 981.47 ng/ml

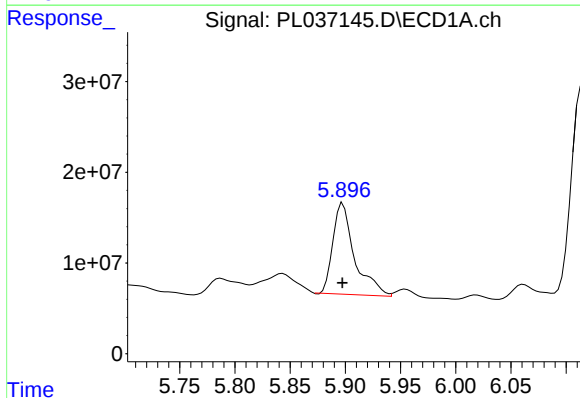


#27 Chlordane-5

R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 137747036
Conc: 1044.99 ng/ml

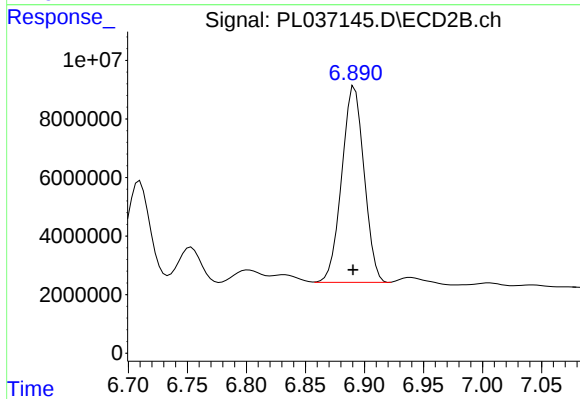

#27 Chlordane-5


R.T.: 6.892 min
Delta R.T.: 0.001 min
Response: 88279265
Conc: 980.10 ng/ml

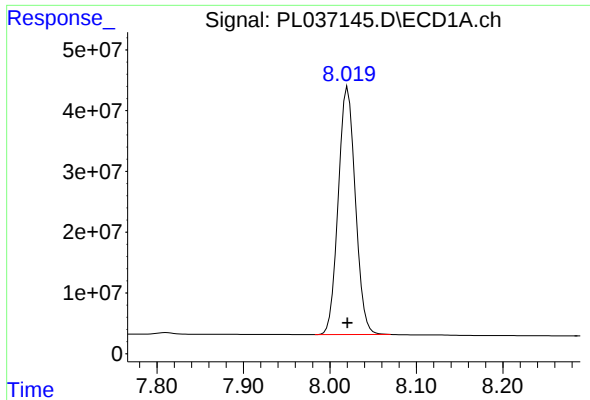

#28 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: 0.000 min
Response: 556198199
Conc: 94.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

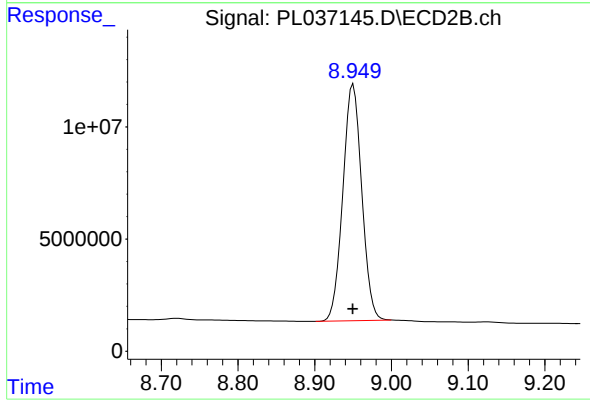

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 181281595
Conc: 92.70 ng/ml