

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 12:22
 Operator : UA\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 13:29:17 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 13:28:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	602.1E6	204.5E6	73.240	73.857
28)	SA Decachlor...	8.020	8.950	425.8E6	139.8E6	72.363	71.489
Target Compounds							
23)	Chlordane-1	4.183	4.921	237.6E6	89456191	746.918	747.138
24)	Chlordane-2	4.676	5.383	255.1E6	91257214	724.272	723.927
25)	Chlordane-3	5.233	6.023	811.4E6	296.3E6	747.040	744.152
26)	Chlordane-4	5.289	6.099	719.9E6	356.9E6	730.564	737.670
27)	Chlordane-5	5.898	6.891	97847744	66176152	742.299	734.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 12:22
Operator : UA\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:29:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 13:28:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

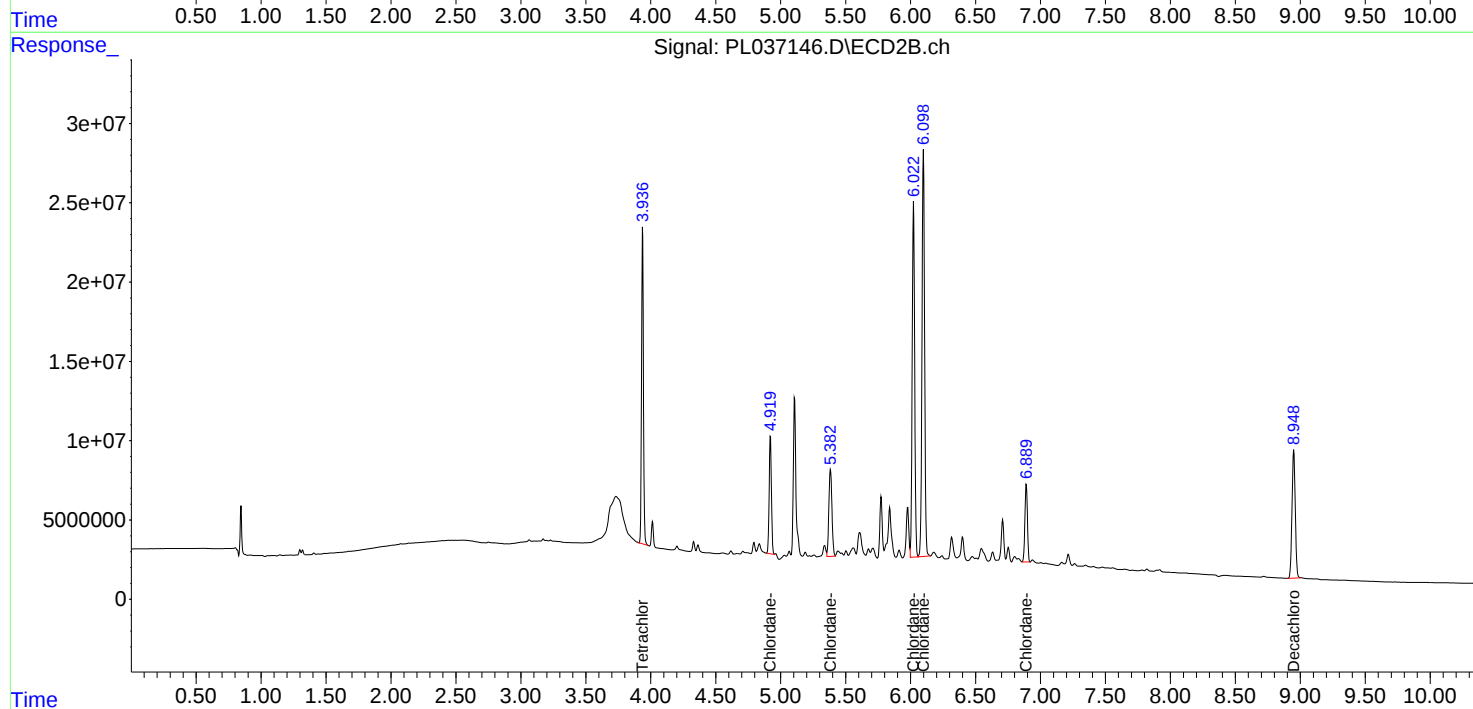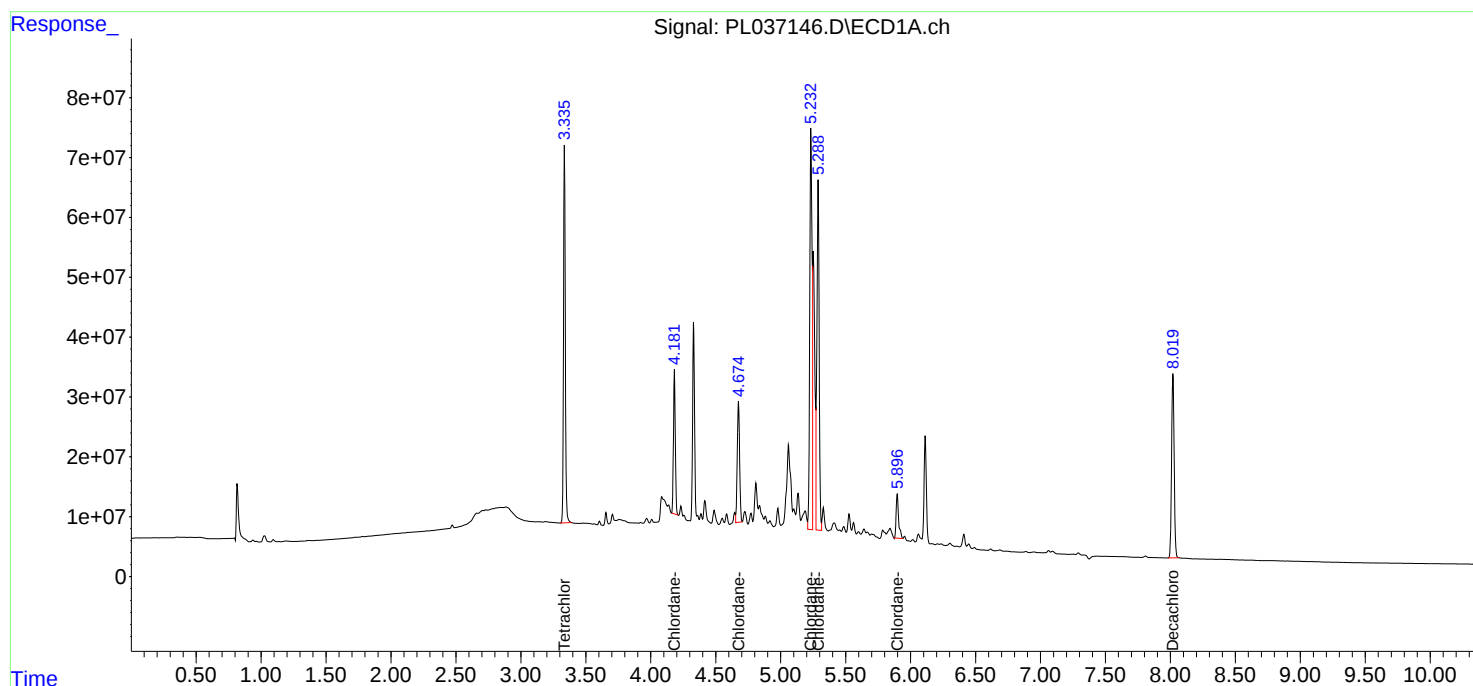


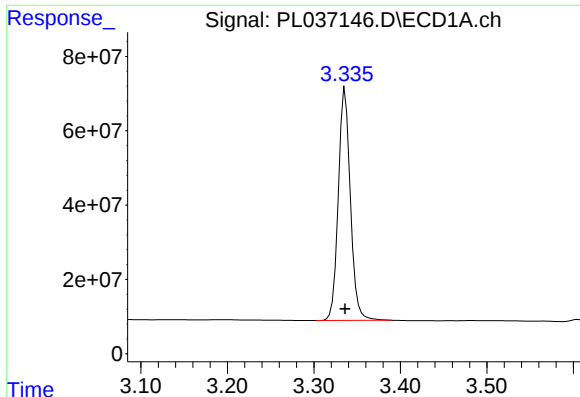

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 602116808
Conc: 73.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

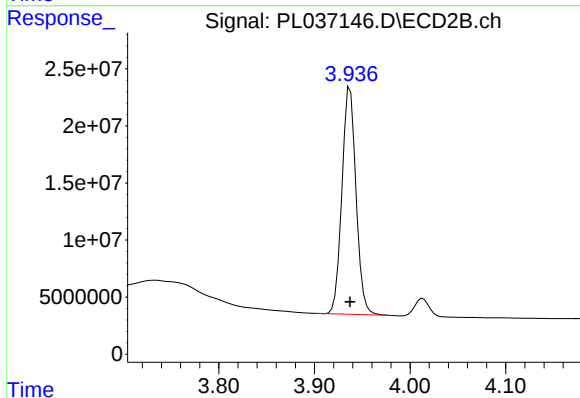


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 204456266
Conc: 73.86 ng/ml

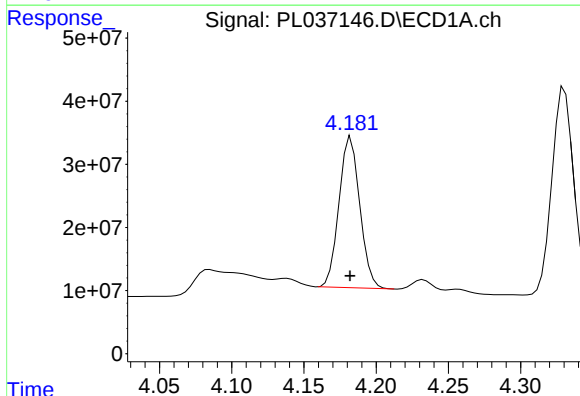


#23 Chlordane-1

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 237620402
Conc: 746.92 ng/ml

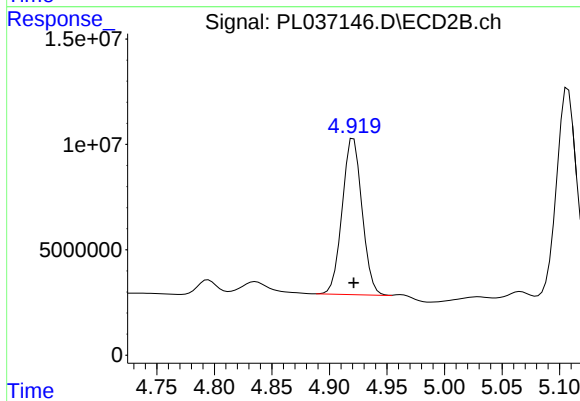

#23 Chlordane-1


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 89456191
Conc: 747.14 ng/ml

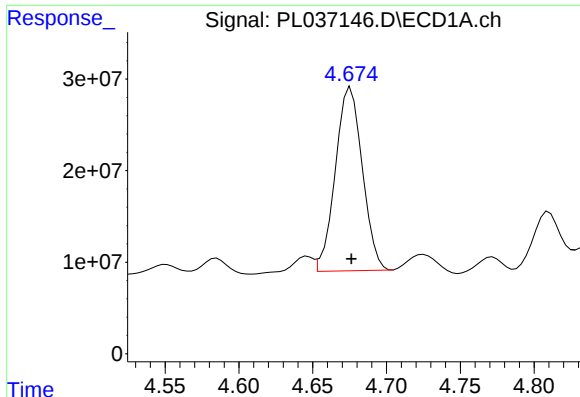

#24 Chlordane-2


R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 255068053
Conc: 724.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

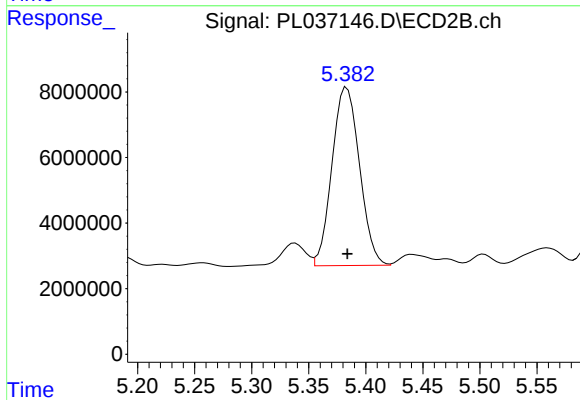


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 91257214
Conc: 723.93 ng/ml

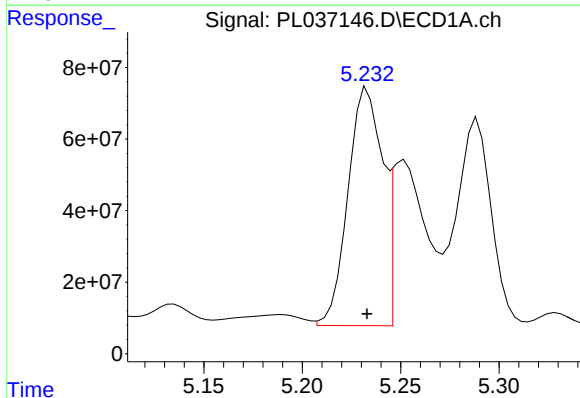


#25 Chlordane-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 811429708
Conc: 747.04 ng/ml

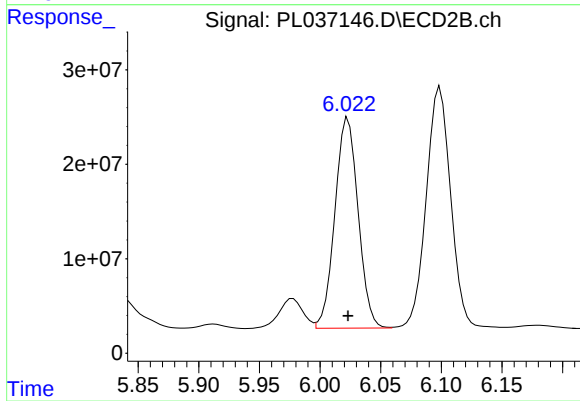

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 296318584
Conc: 744.15 ng/ml

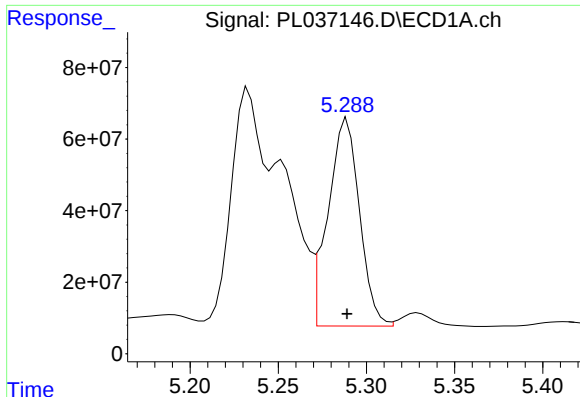

#26 Chlordane-4


R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 719865257
Conc: 730.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

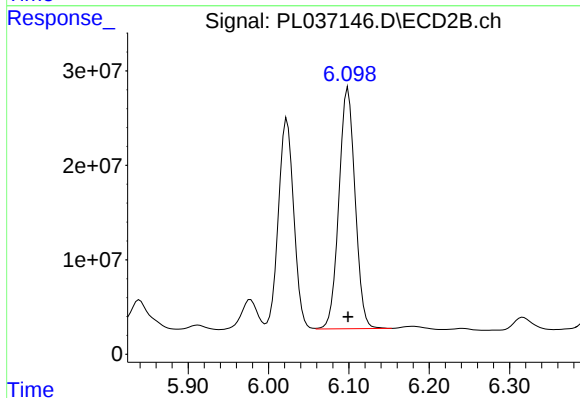


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 356902732
Conc: 737.67 ng/ml

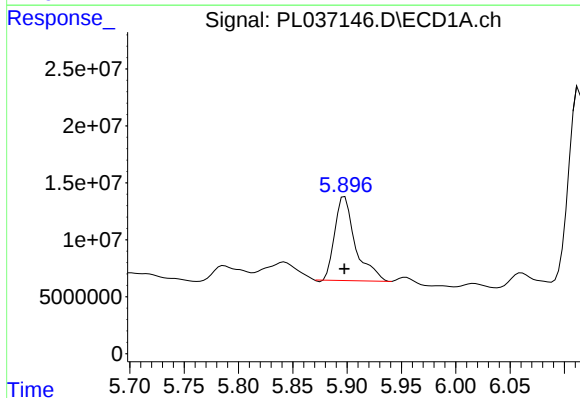


#27 Chlordane-5

R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 97847744
Conc: 742.30 ng/ml

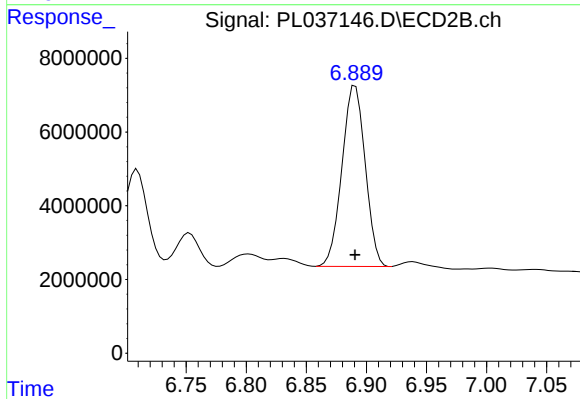

#27 Chlordane-5


R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 66176152
Conc: 734.70 ng/ml

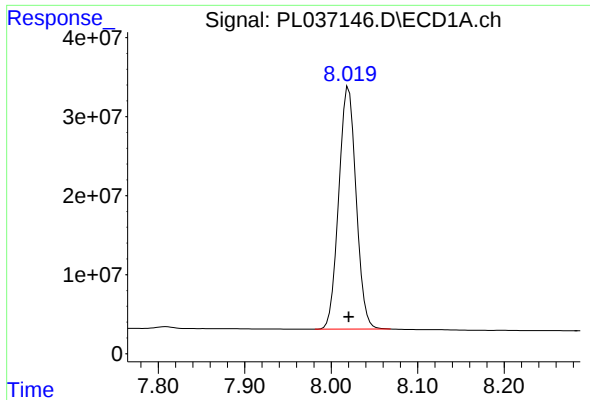

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 425753064
Conc: 72.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

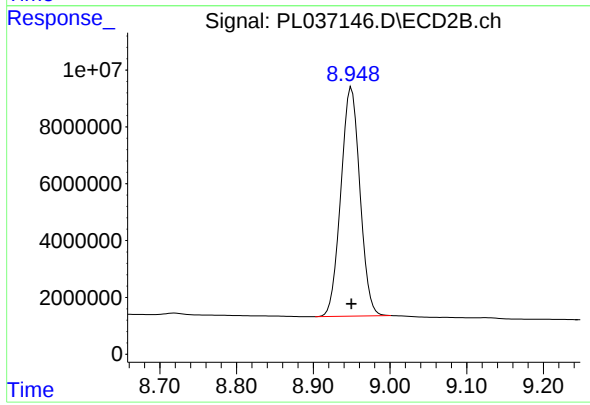

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 139804139
Conc: 71.49 ng/ml