

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 12:36
 Operator : UA\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 13:28:28 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 13:28:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	411.1E6	138.4E6	50.000	50.000
28)	SA Decachlor...	8.020	8.950	294.2E6	97779502	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.182	4.921	159.1E6	59865895	500.000	500.000
24)	Chlordane-2	4.676	5.384	176.1E6	63029314	500.000	500.000
25)	Chlordane-3	5.233	6.023	543.1E6	199.1E6	500.000	500.000
26)	Chlordane-4	5.289	6.099	492.7E6	241.9E6	500.000	500.000
27)	Chlordane-5	5.897	6.890	65908575	45035962	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 12:36
Operator : UA\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:28:28 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 13:28:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

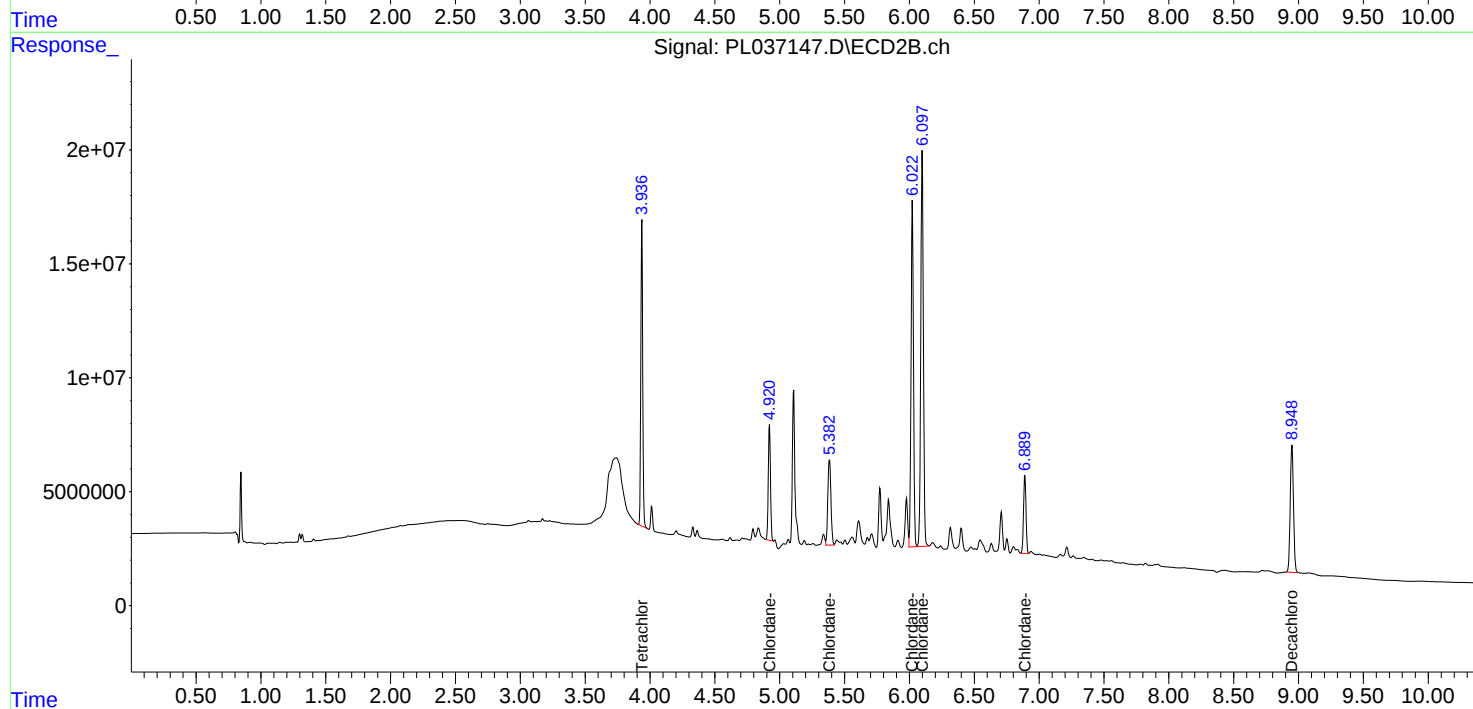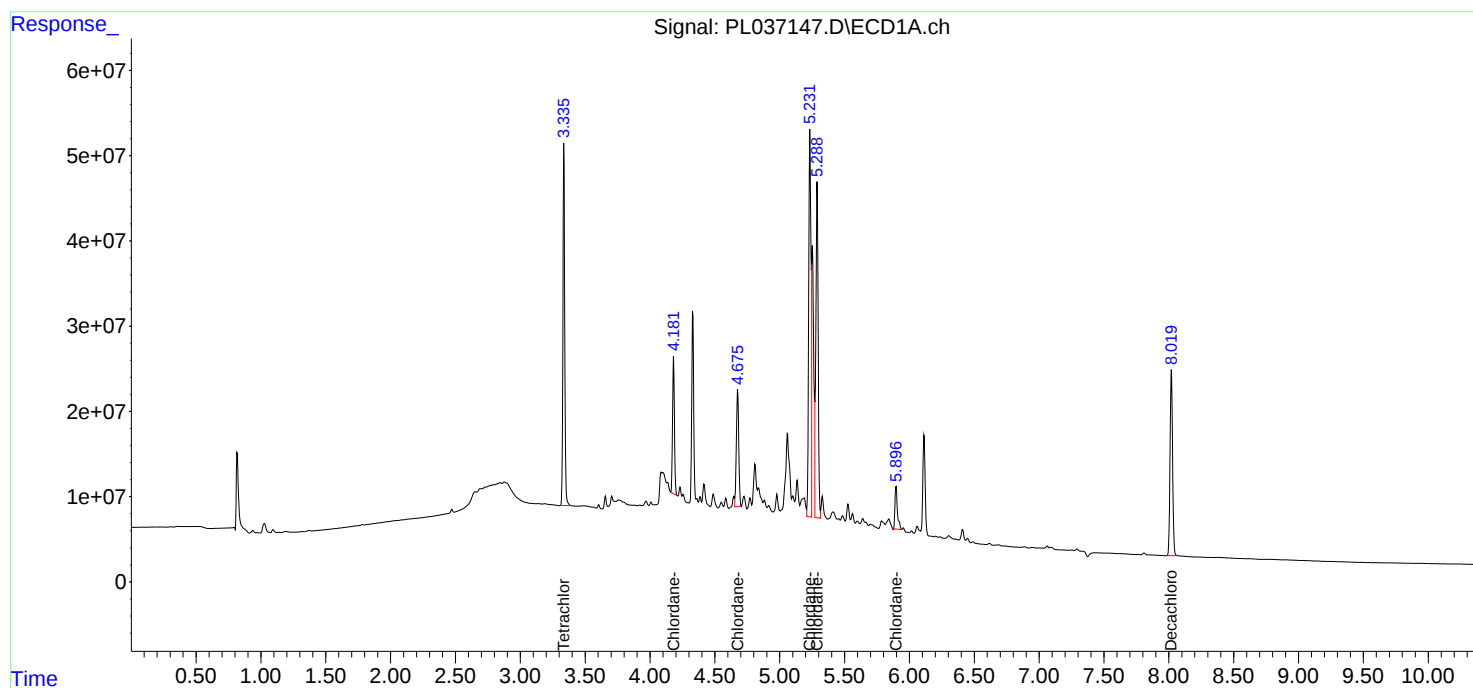


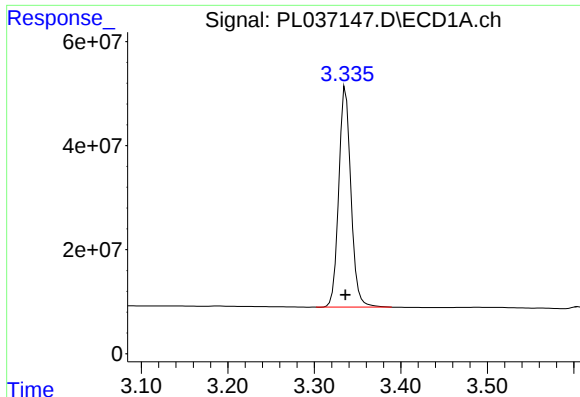

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 411054936
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

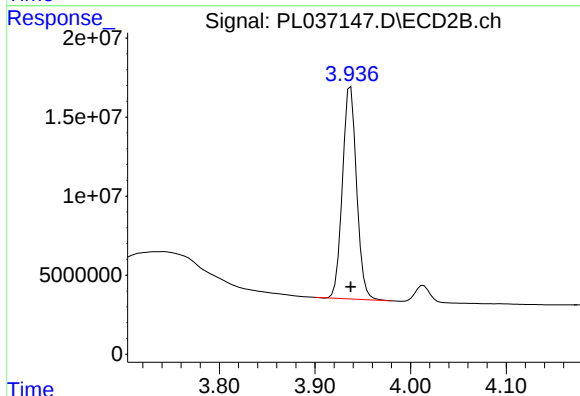


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 138413559
Conc: 50.00 ng/ml

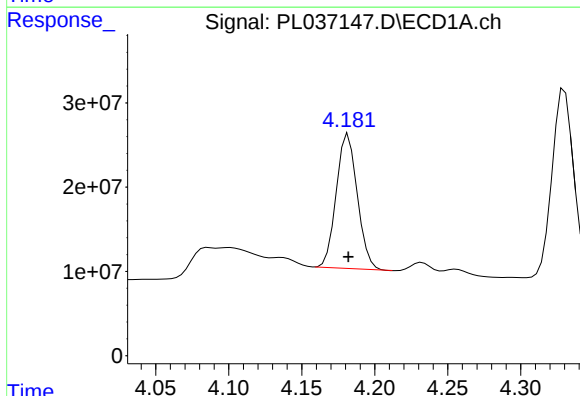


#23 Chlordane-1

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 159067188
Conc: 500.00 ng/ml

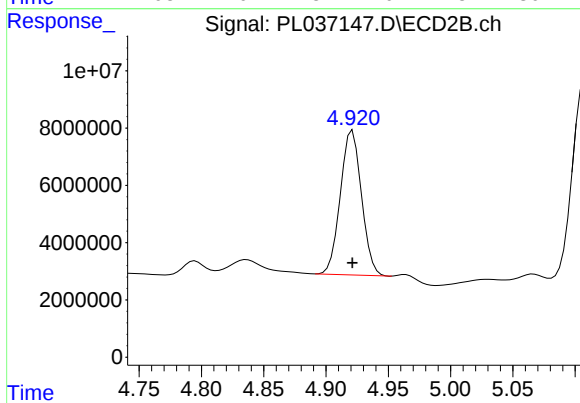

#23 Chlordane-1


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 59865895
Conc: 500.00 ng/ml

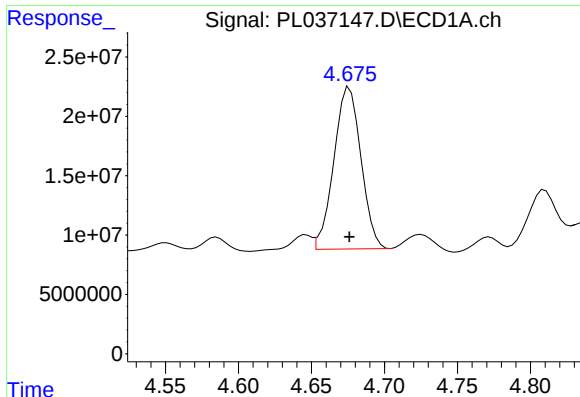

#24 Chlordane-2


R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 176085841
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

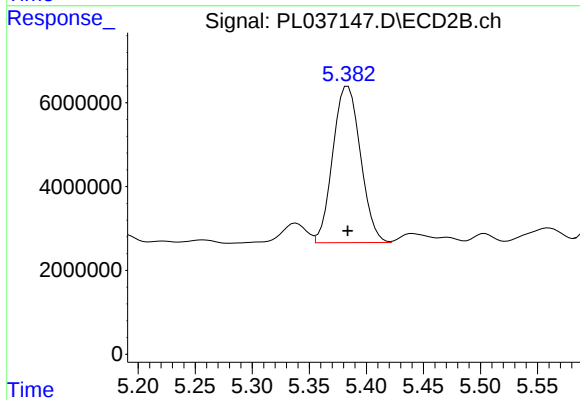


#24 Chlordane-2

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 63029314
Conc: 500.00 ng/ml

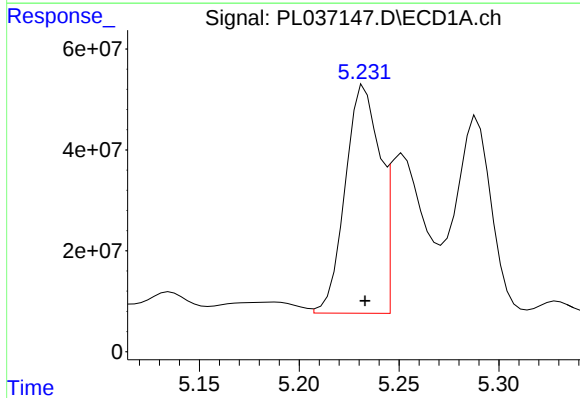


#25 Chlordane-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 543096896
Conc: 500.00 ng/ml

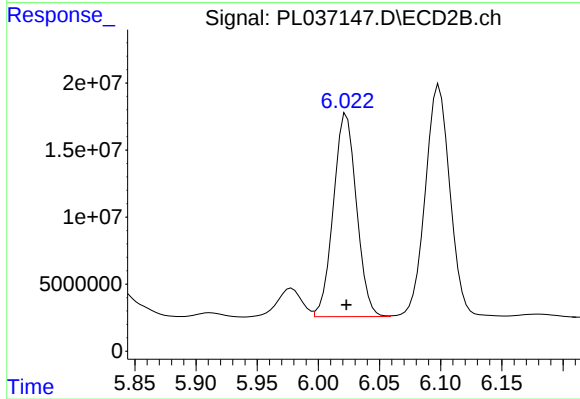

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 199098276
Conc: 500.00 ng/ml

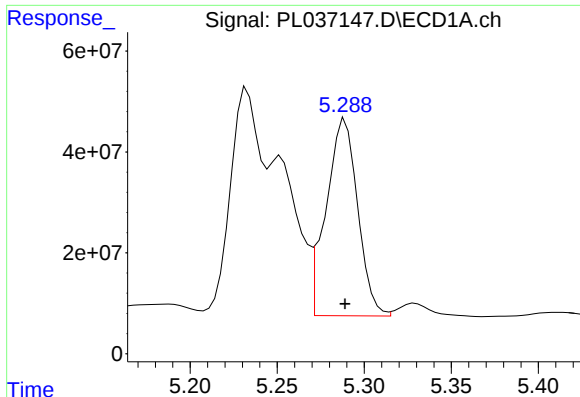

#26 Chlordane-4


R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 492677455
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

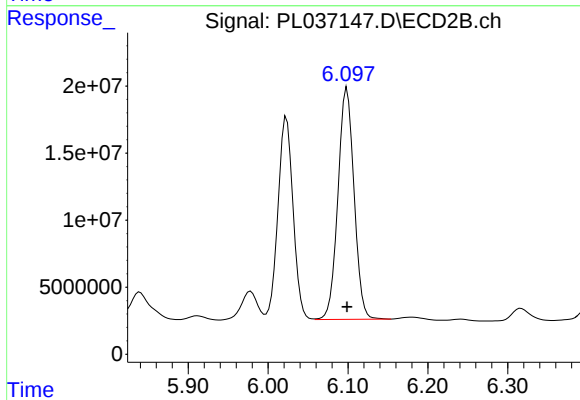


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 241912048
Conc: 500.00 ng/ml

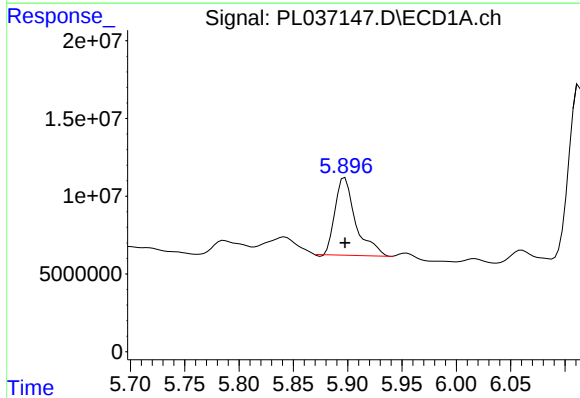


#27 Chlordane-5

R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 65908575
Conc: 500.00 ng/ml

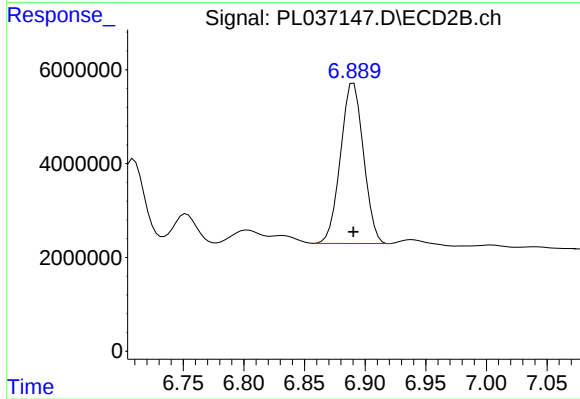

#27 Chlordane-5


R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 45035962
Conc: 500.00 ng/ml

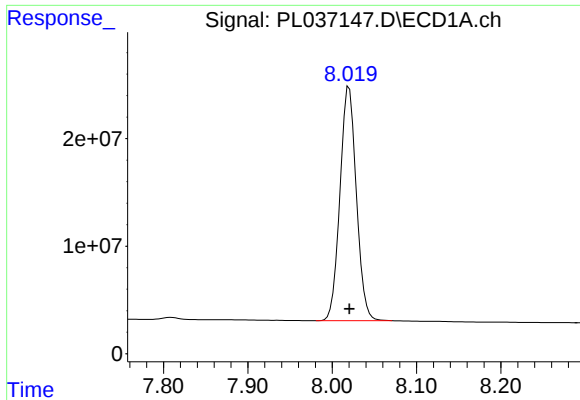

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 294179051
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

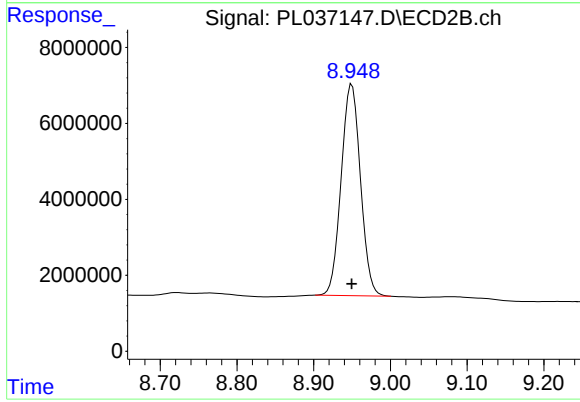

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 97779502
Conc: 50.00 ng/ml