

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 12:50
 Operator : UA\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 13:29:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 13:28:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	204.6E6	67727707	24.883	24.466
28)	SA Decachlor...	8.020	8.950	150.3E6	50654503	25.551	25.902
Target Compounds							
23)	Chlordane-1	4.182	4.921	75245339	29399717	236.521	245.546
24)	Chlordane-2	4.676	5.383	89179235	31577053	253.227	250.495
25)	Chlordane-3	5.233	6.023	262.9E6	95960606	241.998	240.988
26)	Chlordane-4	5.289	6.099	240.5E6	118.2E6	244.055	244.271
27)	Chlordane-5	5.898	6.891	31701344	22314362	240.495	247.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 12:50
Operator : UA\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:29:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 13:28:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

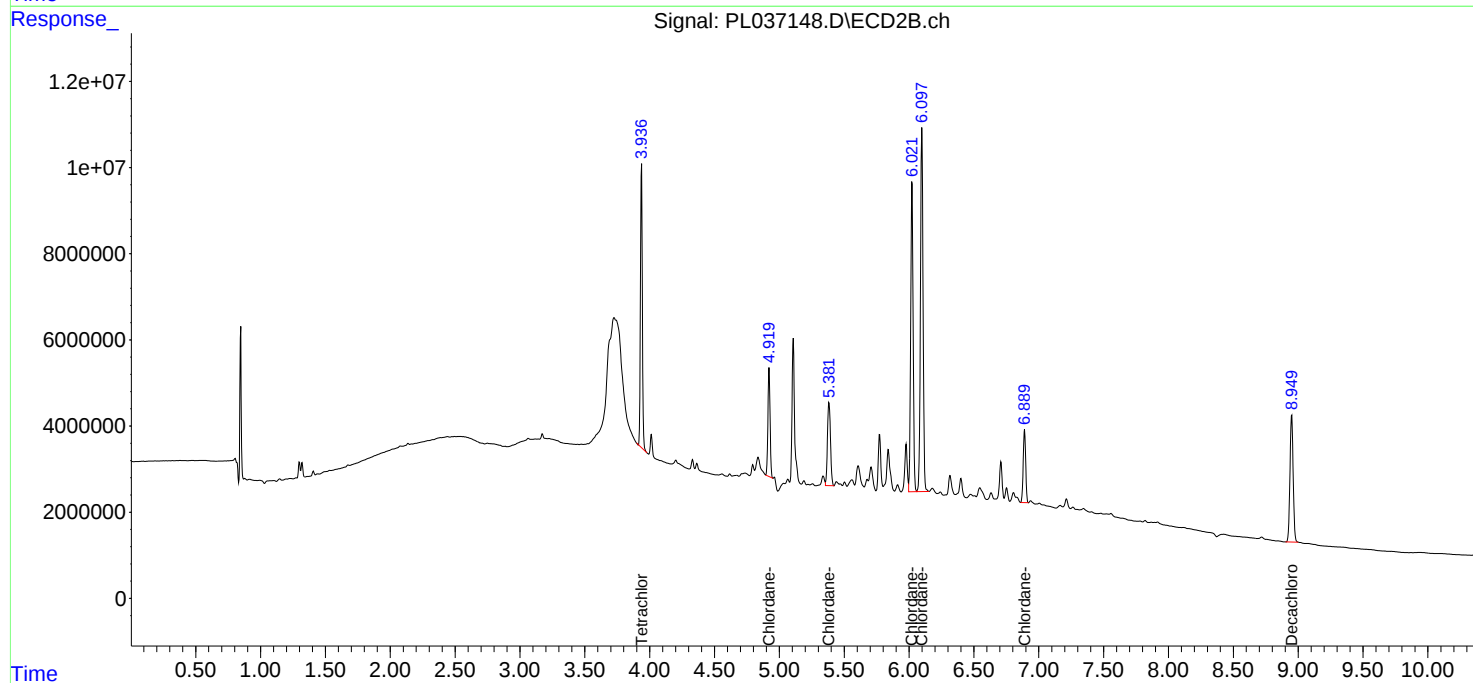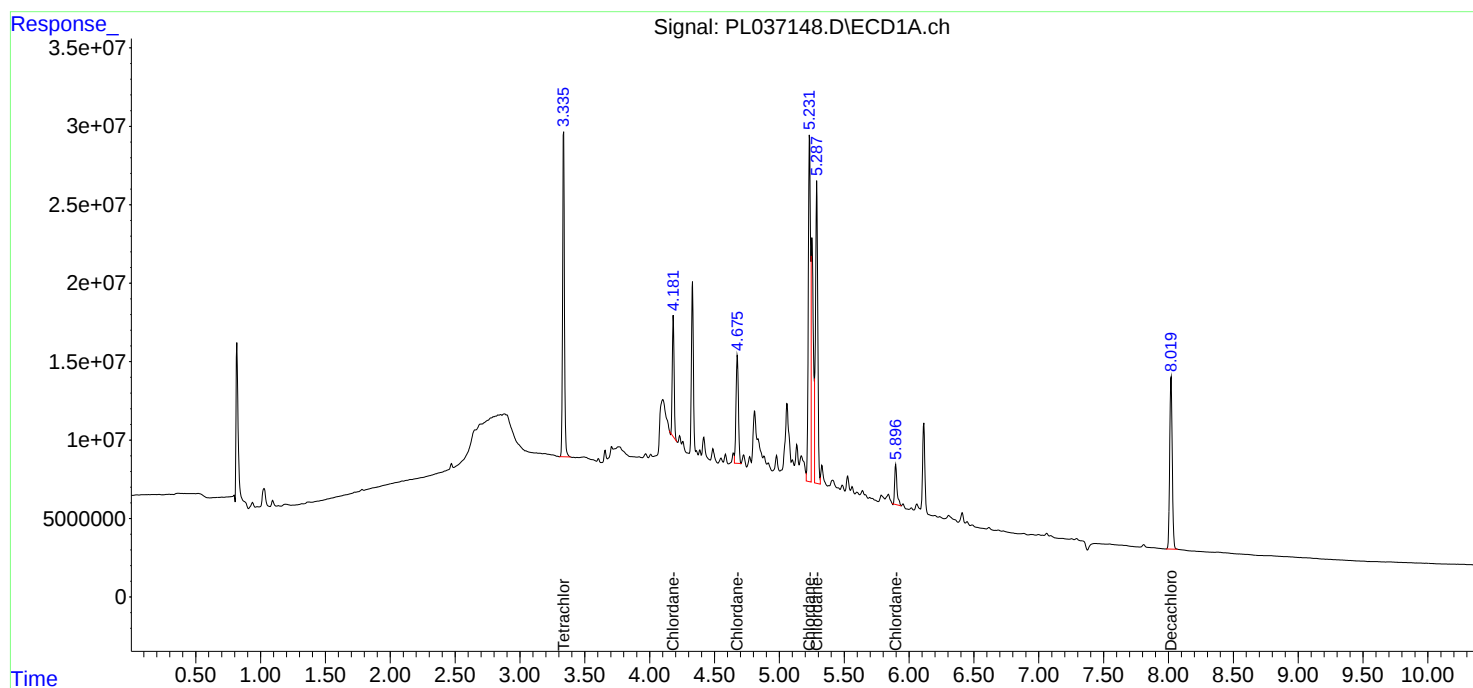


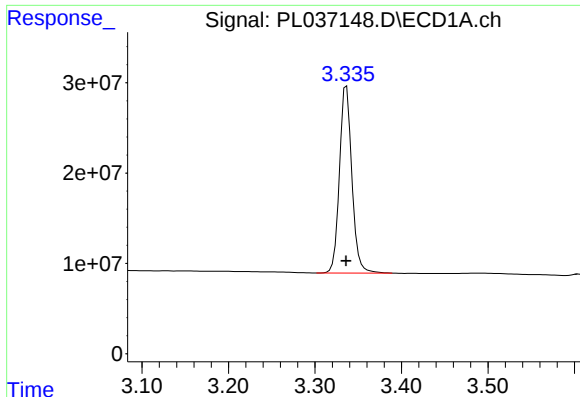

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 204568737
Conc: 24.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

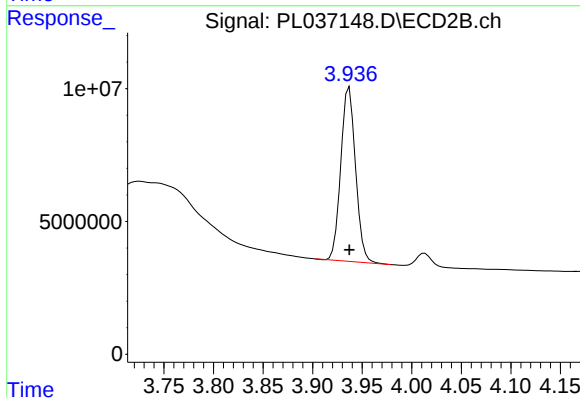


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 67727707
Conc: 24.47 ng/ml

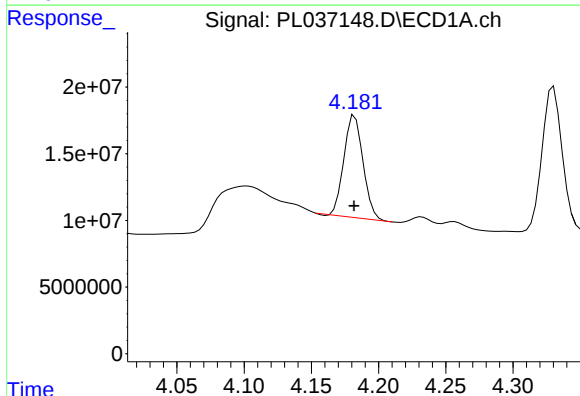


#23 Chlordane-1

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 75245339
Conc: 236.52 ng/ml

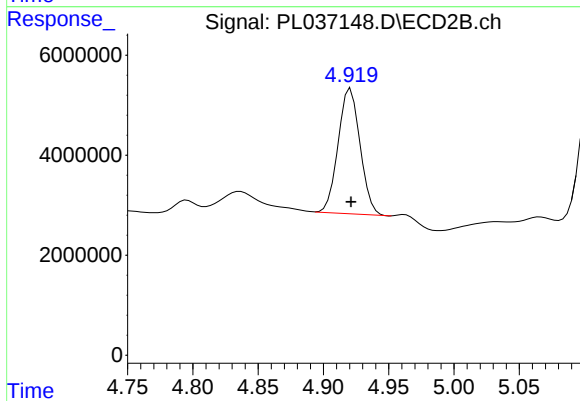

#23 Chlordane-1


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 29399717
Conc: 245.55 ng/ml

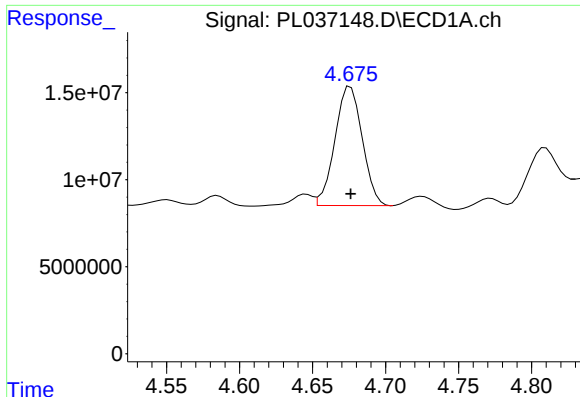

#24 Chlordane-2


R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 89179235
Conc: 253.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

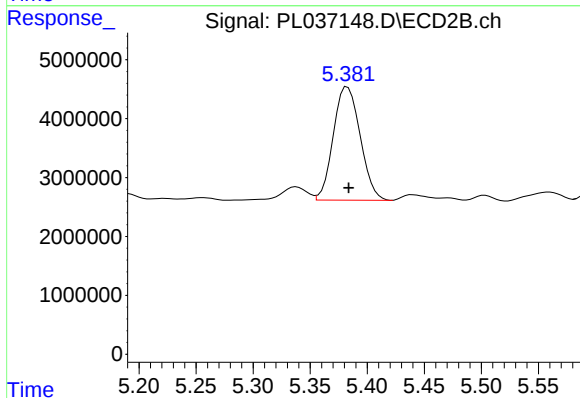


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: -0.001 min
Response: 31577053
Conc: 250.49 ng/ml

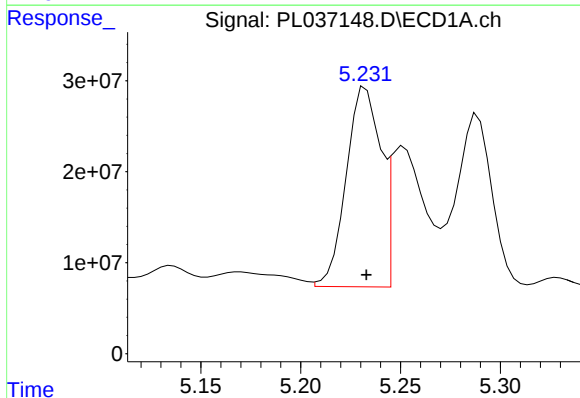


#25 Chlordane-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 262857150
Conc: 242.00 ng/ml

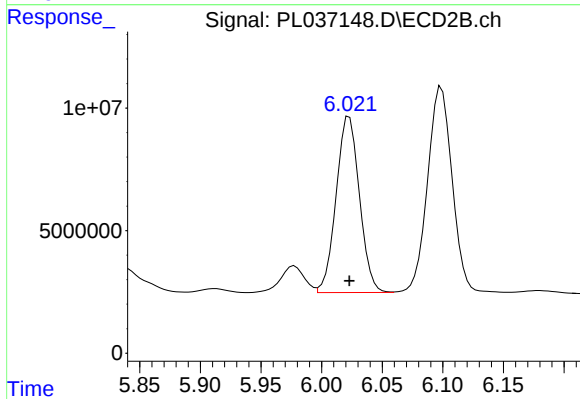

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 95960606
Conc: 240.99 ng/ml

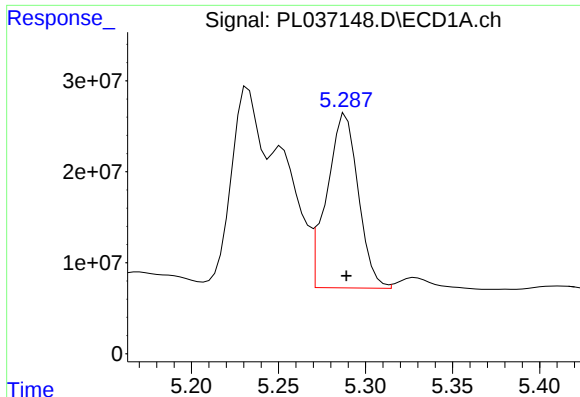

#26 Chlordane-4


R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 240480502
Conc: 244.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

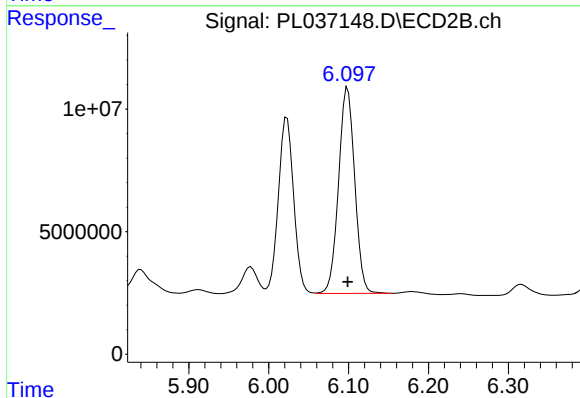


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 118184416
Conc: 244.27 ng/ml

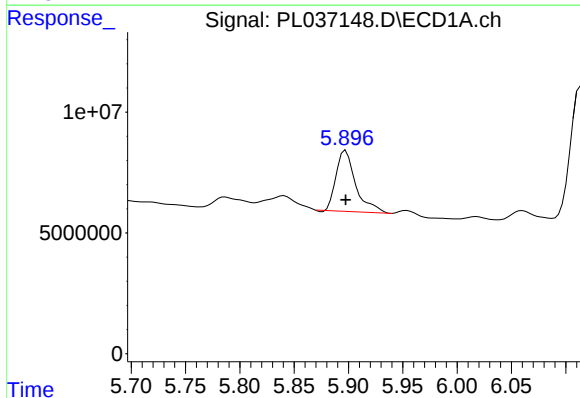


#27 Chlordane-5

R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 31701344
Conc: 240.49 ng/ml

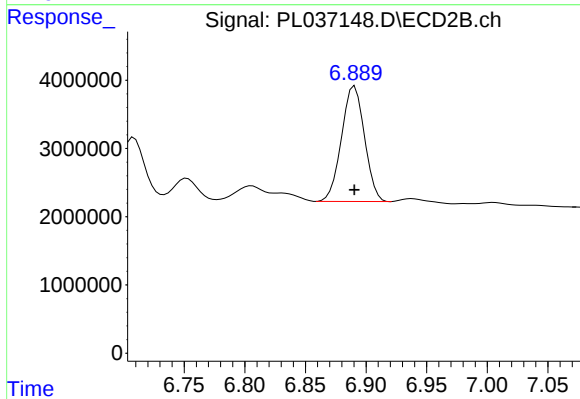

#27 Chlordane-5


R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 22314362
Conc: 247.74 ng/ml

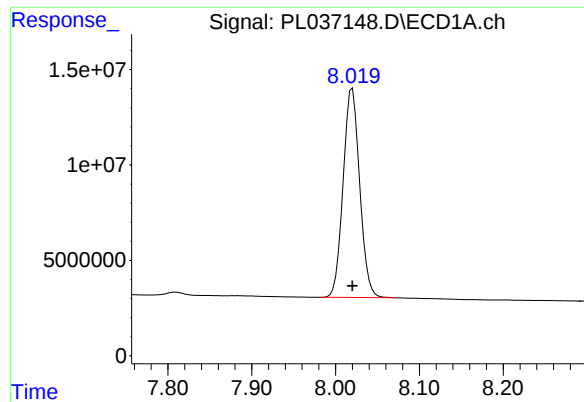

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 150330059
Conc: 25.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

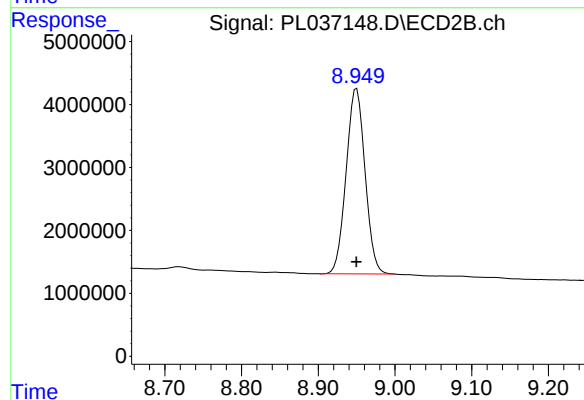

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 50654503
Conc: 25.90 ng/ml