

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 13:04
 Operator : UA\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Manual Integrations
 APPROVED

UGO
 6/21/2018 3:21:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 13:29:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 13:28:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	41720980	13541063	5.075	4.892
28)	SA Decachlor...	8.021	8.950	33677547	11275178	5.724	5.766
Target Compounds							
23)	Chlordane-1	4.181	4.921	14201751	6242911	44.641m	52.141
24)	Chlordane-2	4.676	5.382	19925065	6952768	56.578	55.155m
25)	Chlordane-3	5.232	6.022	51839411	19076865	47.726	47.908
26)	Chlordane-4	5.289	6.098	47206352	24433541	47.908	50.501
27)	Chlordane-5	5.897	6.889	6375397	4703590	48.365m	52.220m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 13:04
Operator : UA\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PCHLORICC050


Manual Integrations
APPROVED

UGO
6/21/2018 3:21:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:29:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 13:28:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

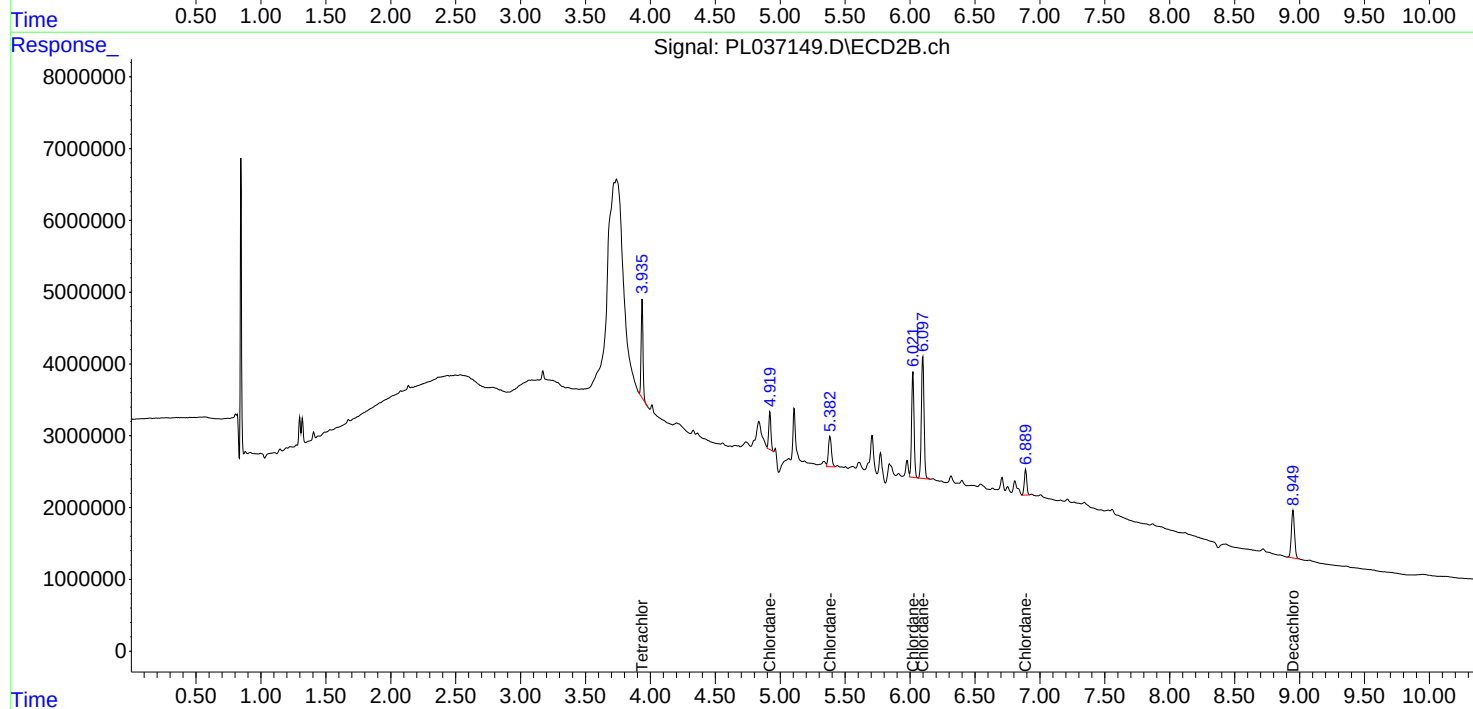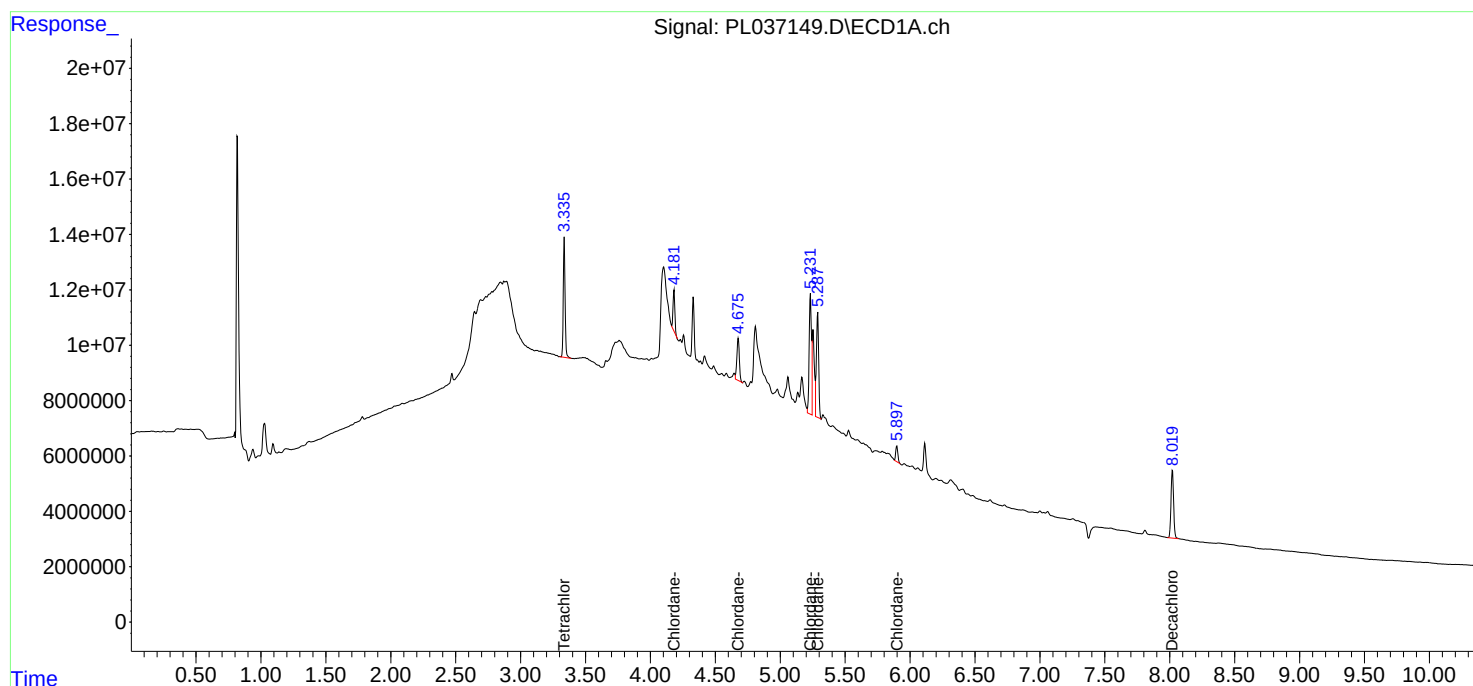

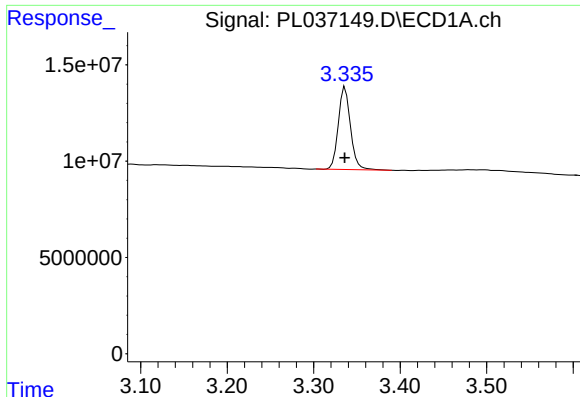


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 41720980
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

UGO
6/21/2018 3:21:36 PM

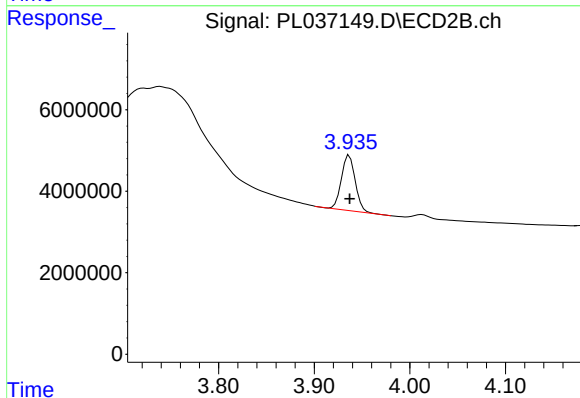


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 13541063
Conc: 4.89 ng/ml

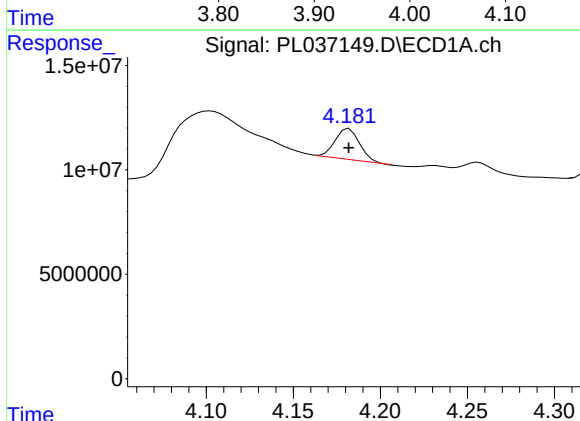


#23 Chlordane-1

R.T.: 4.181 min
Delta R.T.: -0.001 min
Response: 14201751
Conc: 44.64 ng/ml m

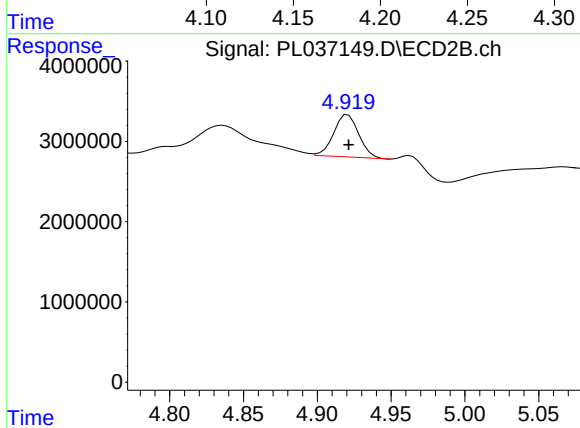

#23 Chlordane-1

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 6242911
Conc: 52.14 ng/ml

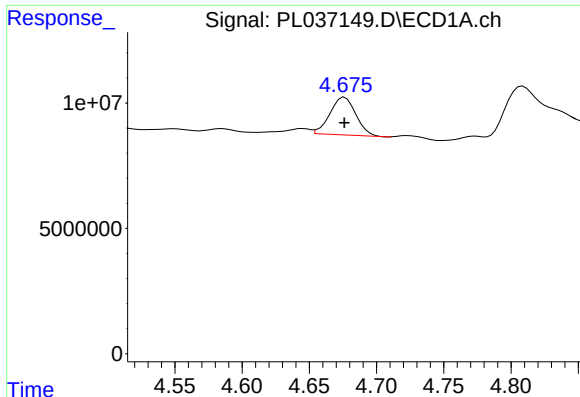


#24 Chlordane-2

R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 19925065
Conc: 56.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

UGO
6/21/2018 3:21:36 PM

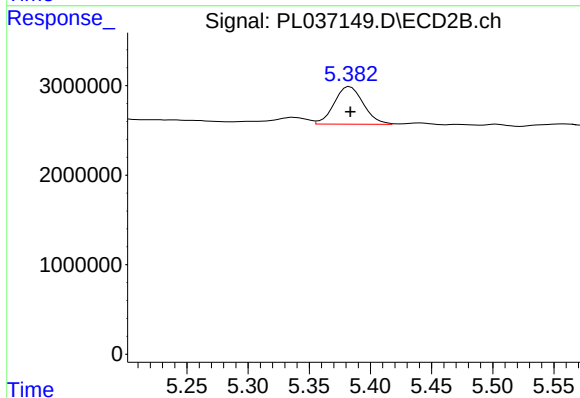


#24 Chlordane-2

R.T.: 5.382 min
Delta R.T.: -0.002 min
Response: 6952768
Conc: 55.16 ng/ml m

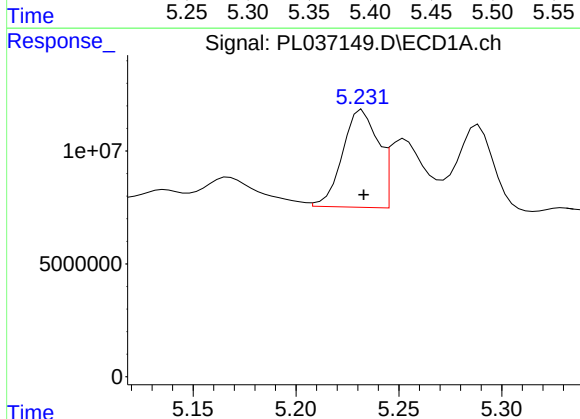


#25 Chlordane-3

R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 51839411
Conc: 47.73 ng/ml

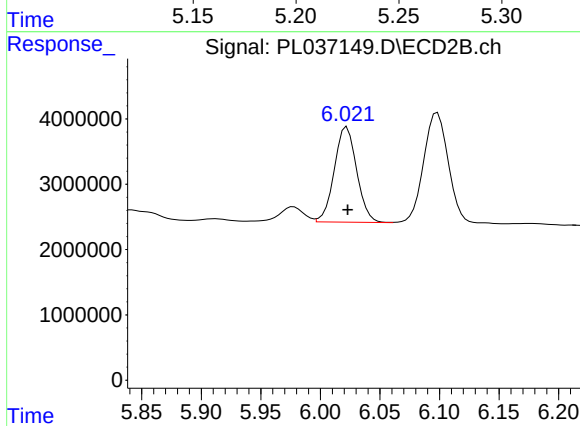

#25 Chlordane-3

R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 19076865
Conc: 47.91 ng/ml

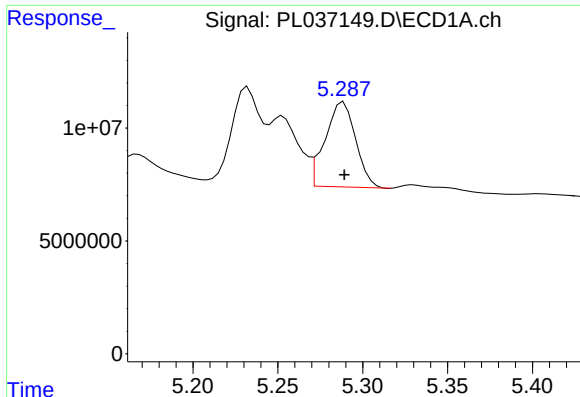


#26 Chlordane-4

R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 47206352
Conc: 47.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

UGO
6/21/2018 3:21:36 PM

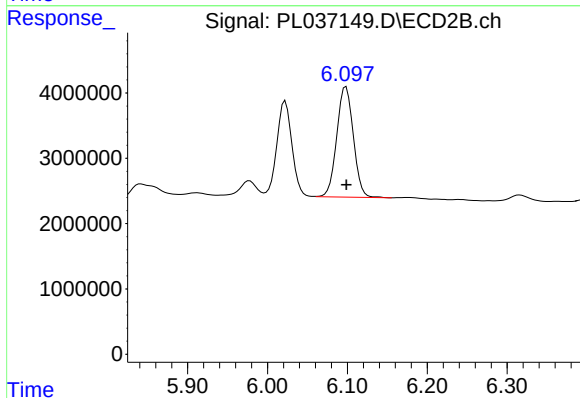


#26 Chlordane-4

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 24433541
Conc: 50.50 ng/ml

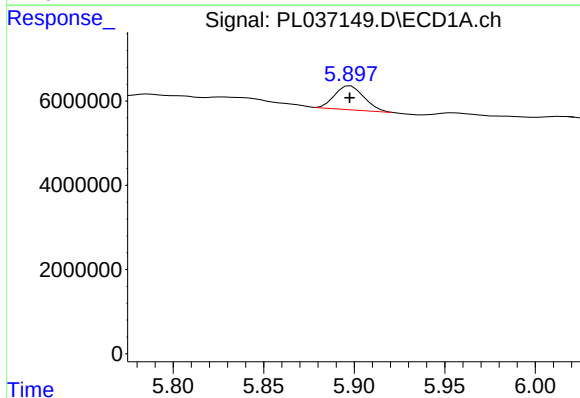


#27 Chlordane-5

R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 6375397
Conc: 48.37 ng/ml m

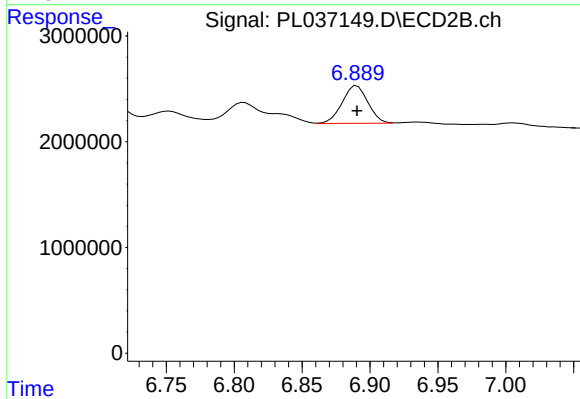

#27 Chlordane-5

R.T.: 6.889 min
Delta R.T.: -0.002 min
Response: 4703590
Conc: 52.22 ng/ml m

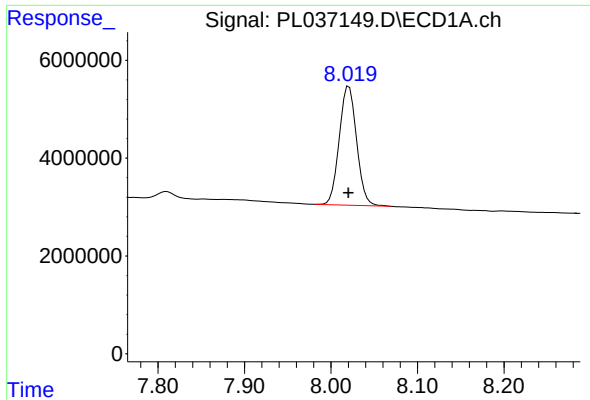


#28 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: 0.000 min
Response: 33677547
Conc: 5.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Manual Integrations
APPROVED

UGO
6/21/2018 3:21:36 PM

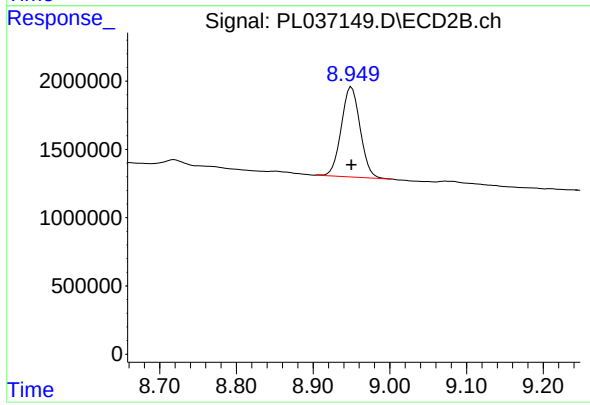

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 11275178
Conc: 5.77 ng/ml