

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 13:46
 Operator : UA\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL062018CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:28:42 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	405.6E6	139.5E6	51.278	50.405
28)	SA Decachlor...	8.020	8.950	296.6E6	98310613	49.151	49.553
Target Compounds							
23)	Chlordane-1	4.183	4.921	160.1E6	60061340	521.355	499.841
24)	Chlordane-2	4.676	5.384	175.7E6	63178386	493.420	499.234
25)	Chlordane-3	5.234	6.023	551.1E6	200.1E6	518.471	511.744
26)	Chlordane-4	5.289	6.099	497.5E6	242.3E6	516.354	505.610
27)	Chlordane-5	5.898	6.891	68081220	45329351	520.227	503.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 13:46
Operator : UA\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL062018CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:28:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

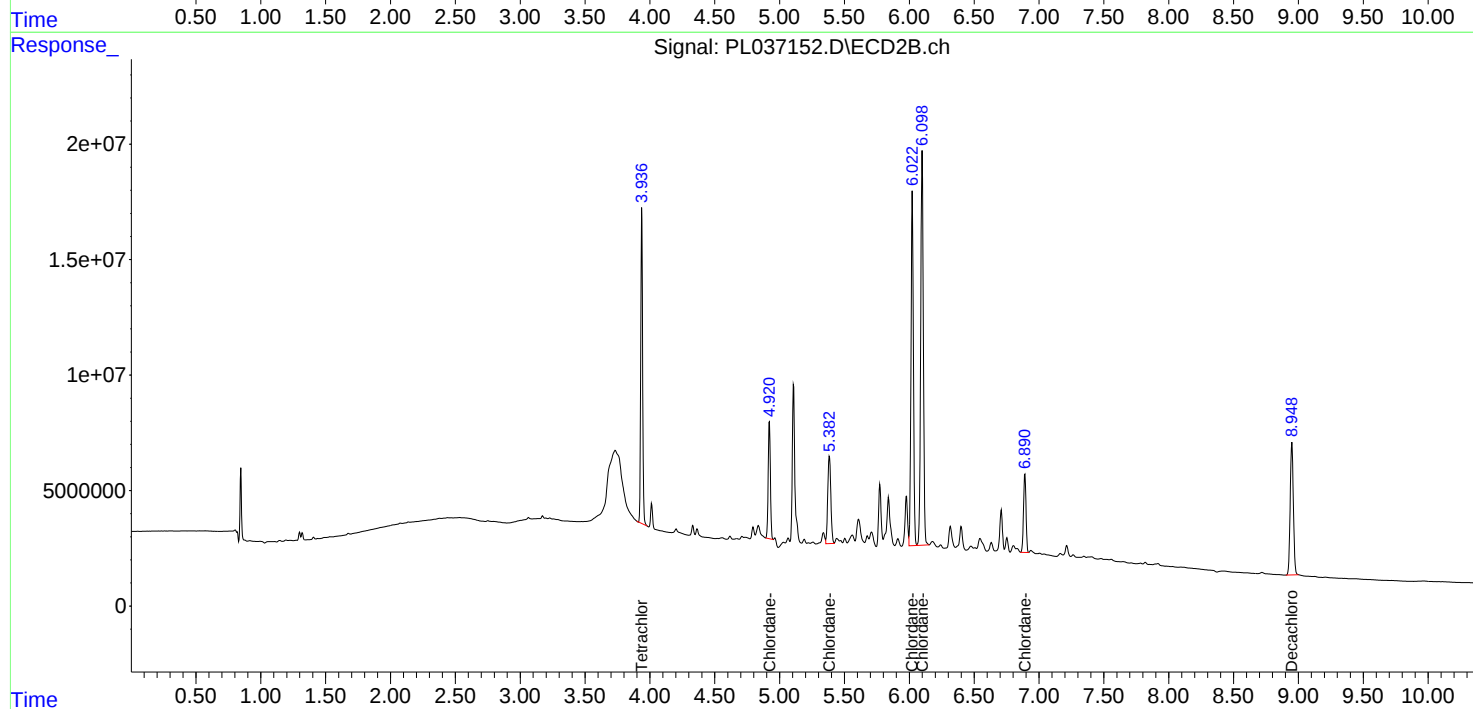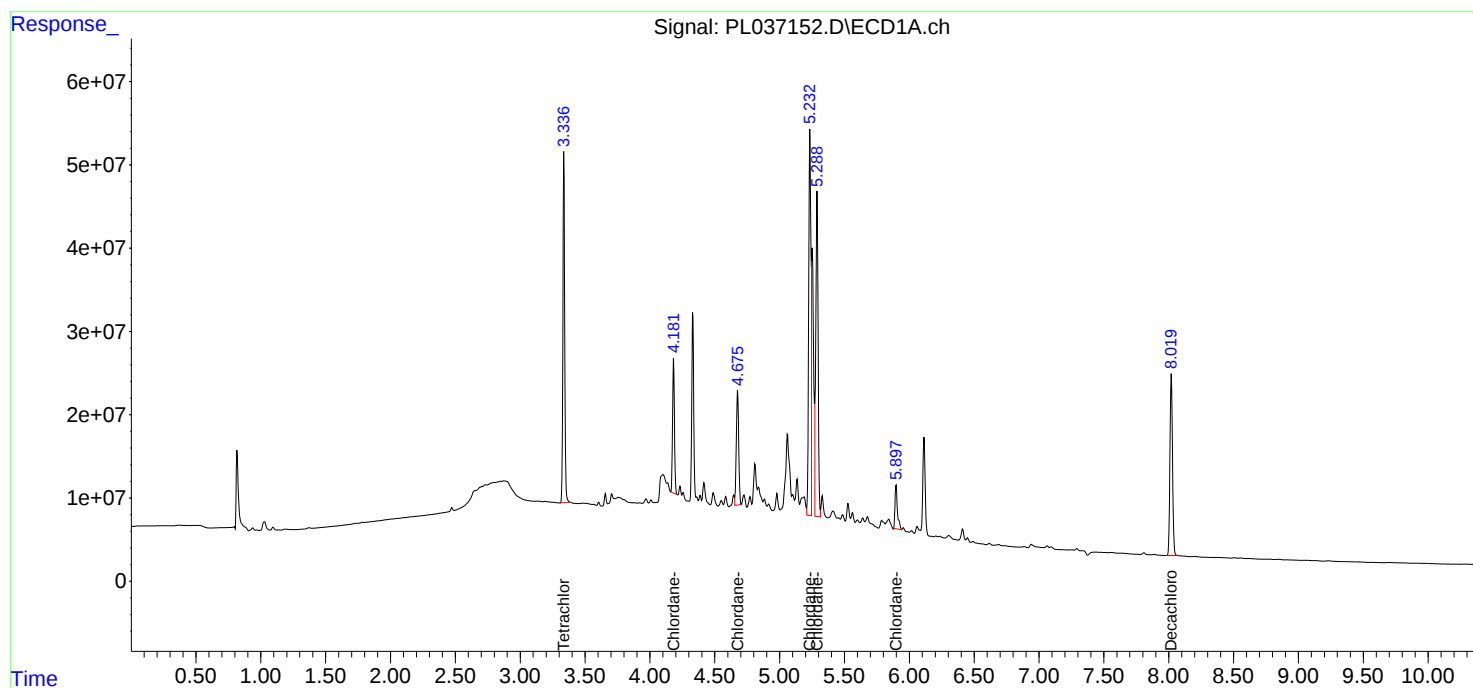


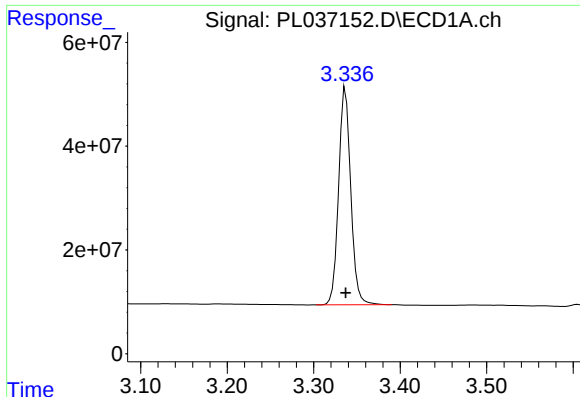

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 405622955
Conc: 51.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062018CHLOR

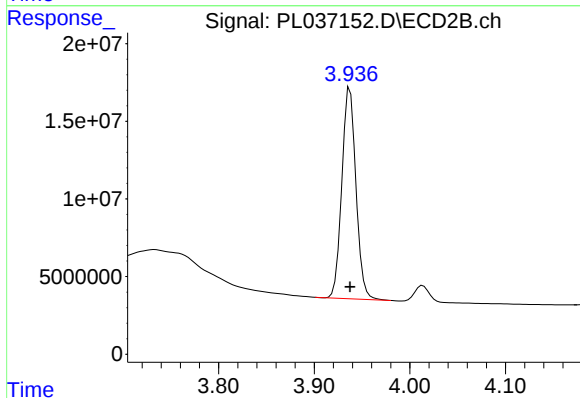


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 139457315
Conc: 50.41 ng/ml

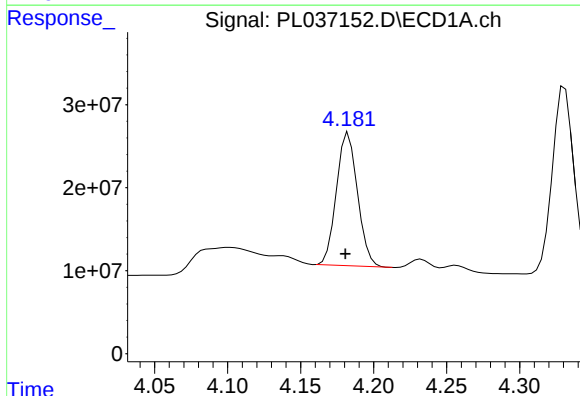


#23 Chlordane-1

R.T.: 4.183 min
Delta R.T.: 0.002 min
Response: 160082938
Conc: 521.35 ng/ml

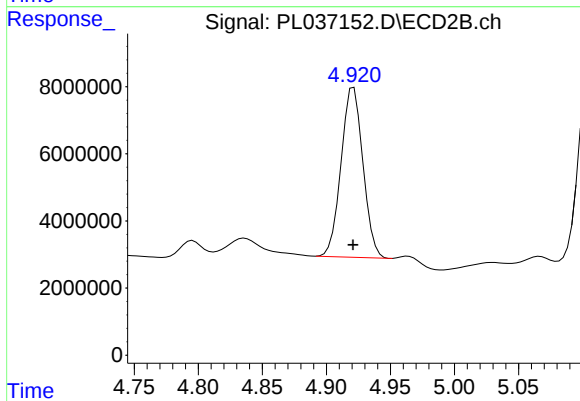

#23 Chlordane-1


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 60061340
Conc: 499.84 ng/ml

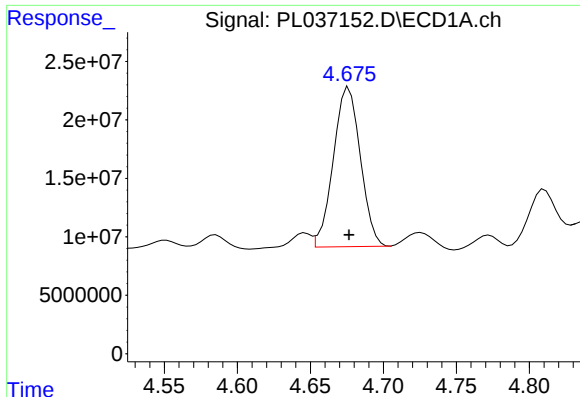

#24 Chlordane-2


R.T.: 4.676 min
Delta R.T.: 0.000 min
Response: 175658371
Conc: 493.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062018CHLOR

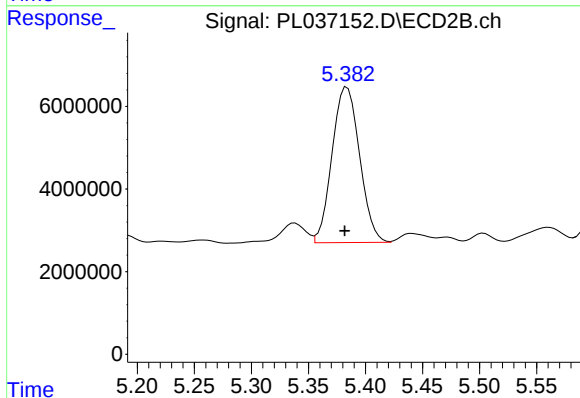


#24 Chlordane-2

R.T.: 5.384 min
Delta R.T.: 0.002 min
Response: 63178386
Conc: 499.23 ng/ml

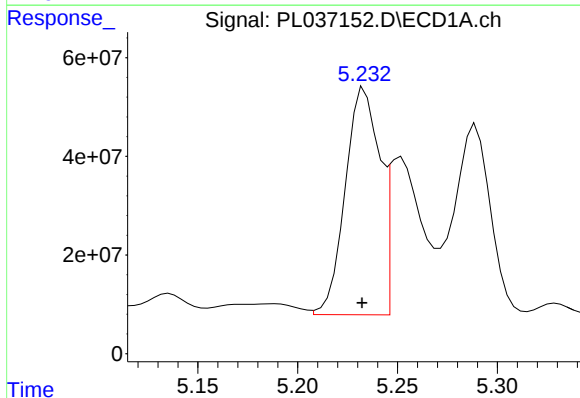


#25 Chlordane-3

R.T.: 5.234 min
Delta R.T.: 0.001 min
Response: 551093217
Conc: 518.47 ng/ml

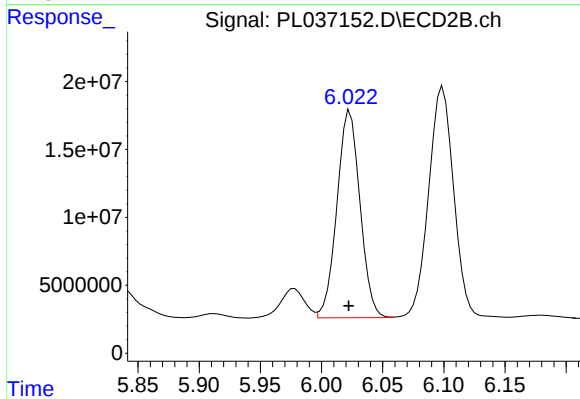

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: 0.001 min
Response: 200135310
Conc: 511.74 ng/ml

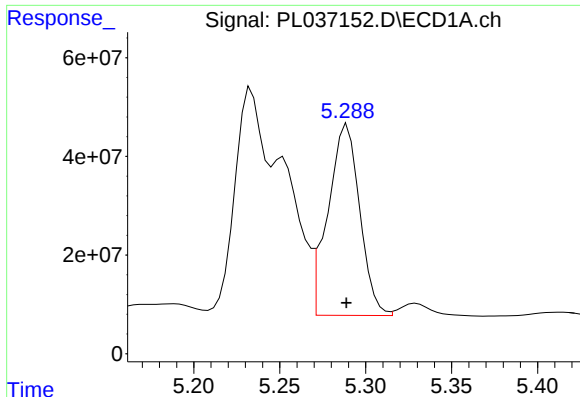

#26 Chlordane-4


R.T.: 5.289 min
Delta R.T.: 0.000 min
Response: 497511032
Conc: 516.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062018CHLOR

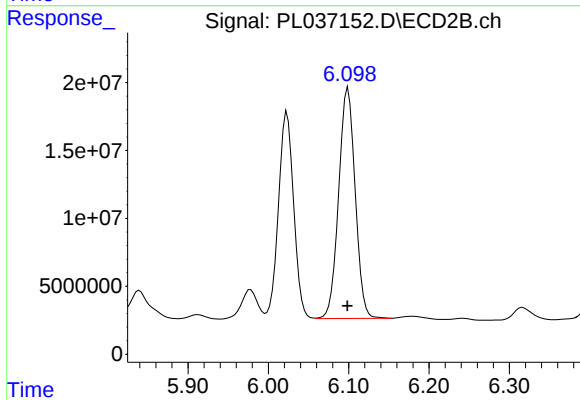


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 242284670
Conc: 505.61 ng/ml

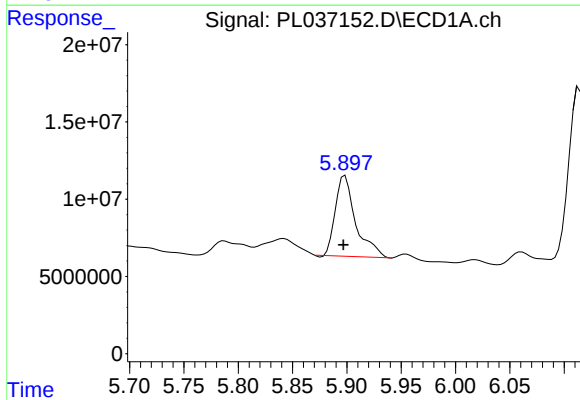


#27 Chlordane-5

R.T.: 5.898 min
Delta R.T.: 0.002 min
Response: 68081220
Conc: 520.23 ng/ml

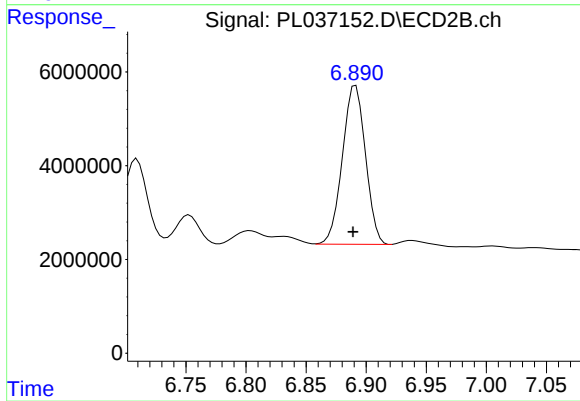

#27 Chlordane-5

R.T.: 6.891 min
Delta R.T.: 0.002 min
Response: 45329351
Conc: 503.75 ng/ml

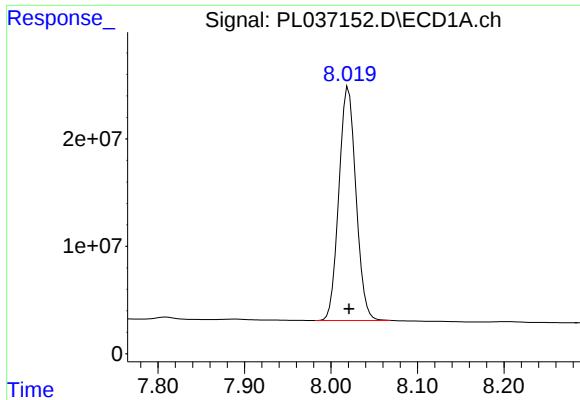

#28 Decachlorobiphenyl


R.T.: 8.020 min

Delta R.T.: 0.000 min

Response: 296576840

Conc: 49.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL062018CHLOR

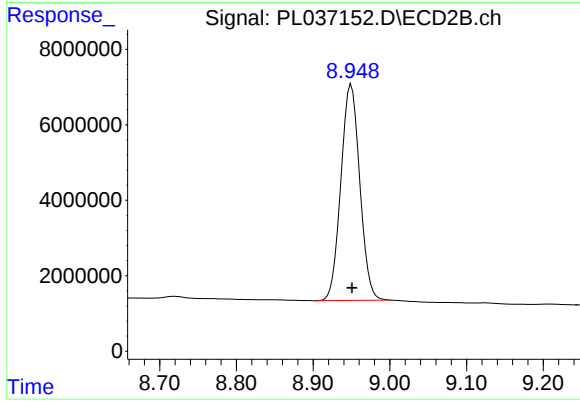

#28 Decachlorobiphenyl

R.T.: 8.950 min

Delta R.T.: -0.001 min

Response: 98310613

Conc: 49.55 ng/ml