

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 17:33
 Operator : UA\AJ
 Sample : J3570-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20180373-AMENDED-COMPOSITE-

Manual Integrations
 APPROVED

UGO
 6/21/2018 3:20:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:59:00 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	49367495	16917527	6.241	6.115
28)	SA Decachlor...	8.021	8.951	34875168	11743573	5.780	5.919
Target Compounds							
12)	B 4,4'-DDE	5.457	6.250	83948808	32449335	9.504m	12.752m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 17:33
Operator : UA\AJ
Sample : J3570-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20180373-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

UGO
6/21/2018 3:20:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:59:00 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

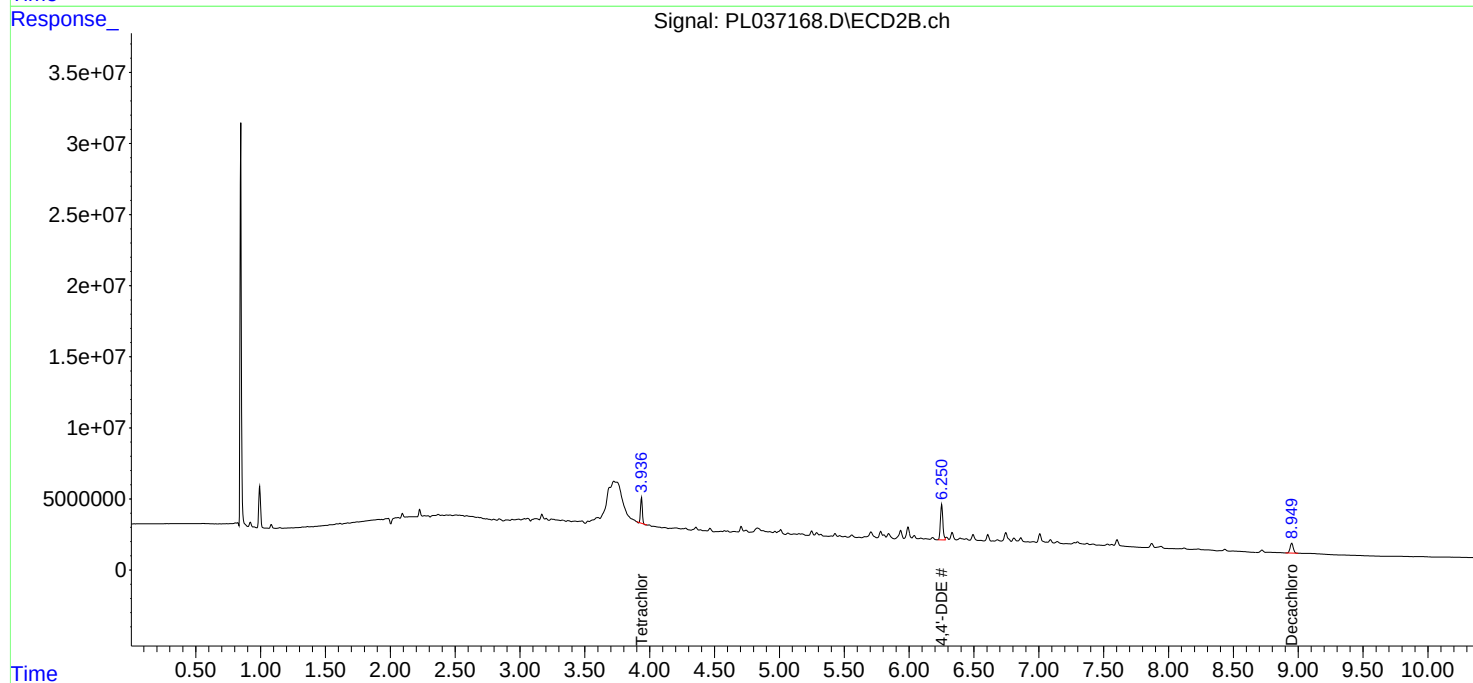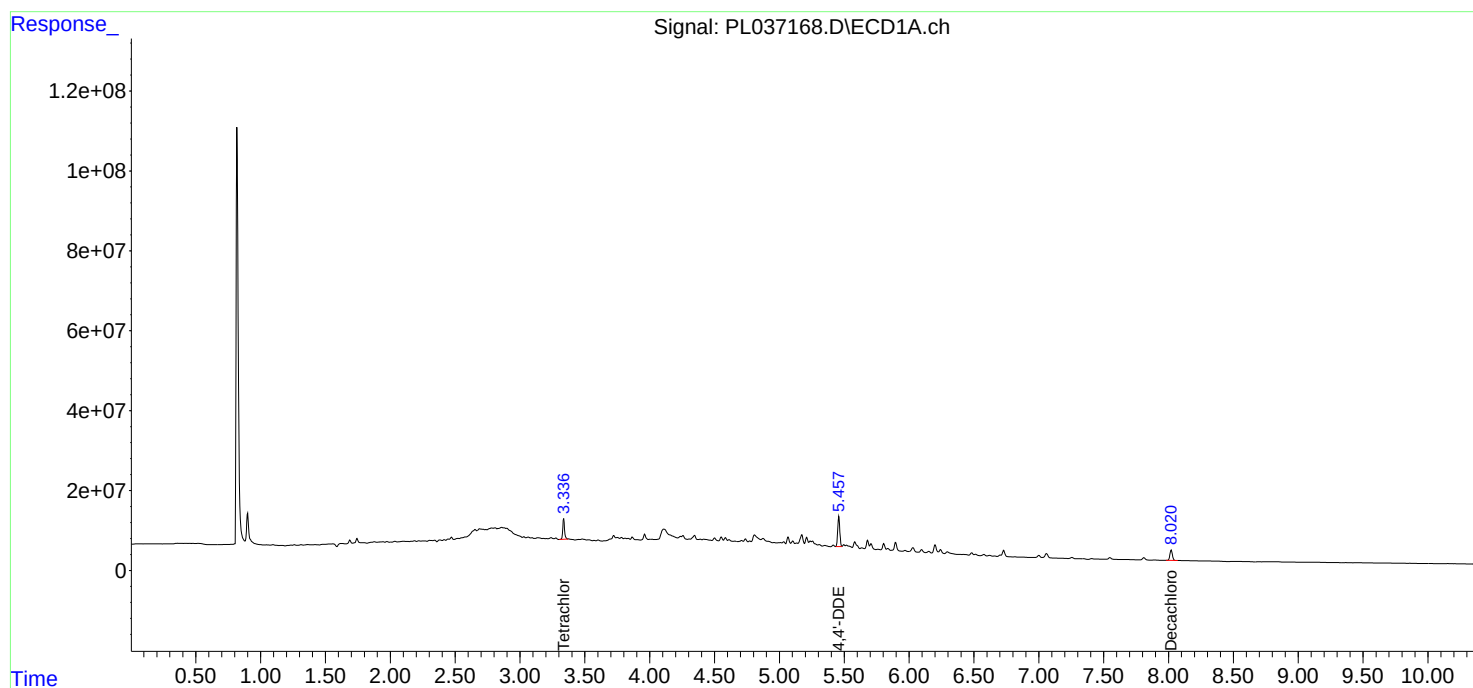

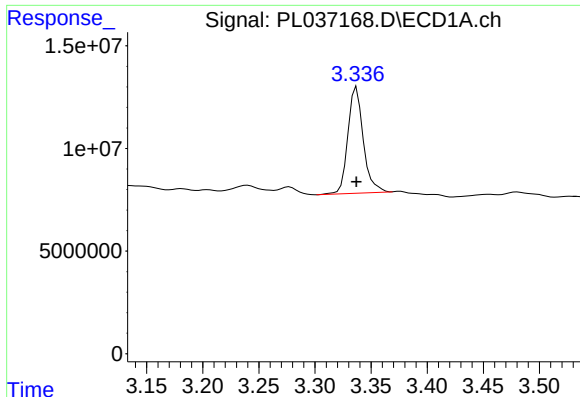


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 49367495
Conc: 6.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
20180373-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

UGO
6/21/2018 3:20:53 PM

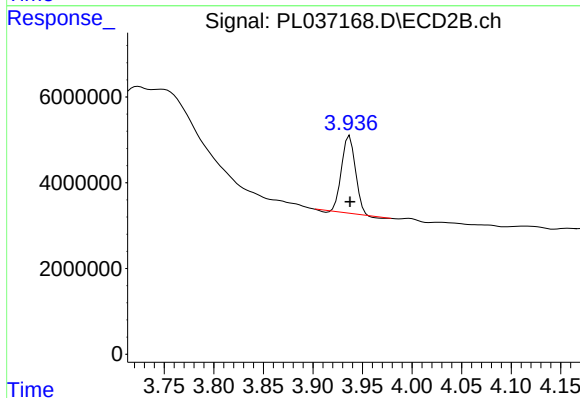


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 16917527
Conc: 6.11 ng/ml

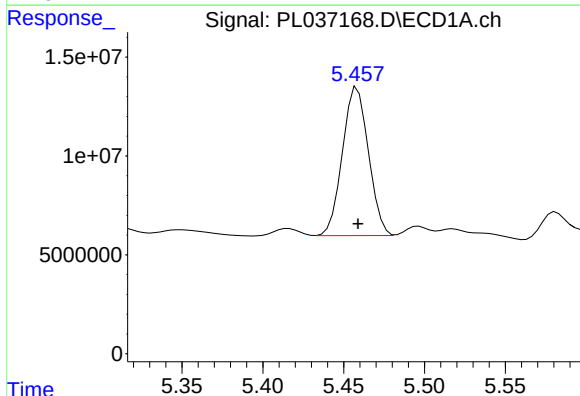


#12 4,4'-DDE

R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 83948808
Conc: 9.50 ng/ml m

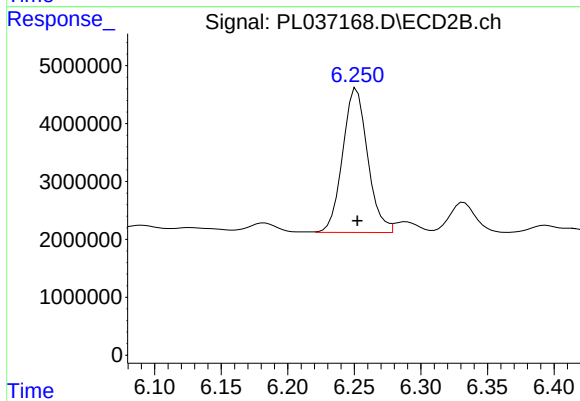

#12 4,4'-DDE

R.T.: 6.250 min
Delta R.T.: -0.002 min
Response: 32449335
Conc: 12.75 ng/ml m

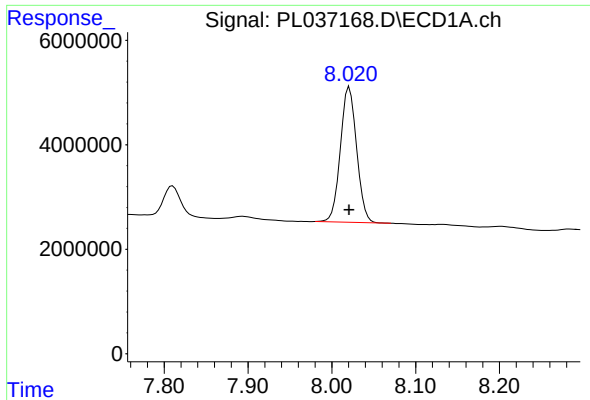

#28 Decachlorobiphenyl

R.T.: 8.021 min

Delta R.T.: 0.000 min


Response: 34875168

Conc: 5.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
20180373-AMENDED-COMPOSITE-

Manual Integrations
APPROVED

UGO
6/21/2018 3:20:53 PM

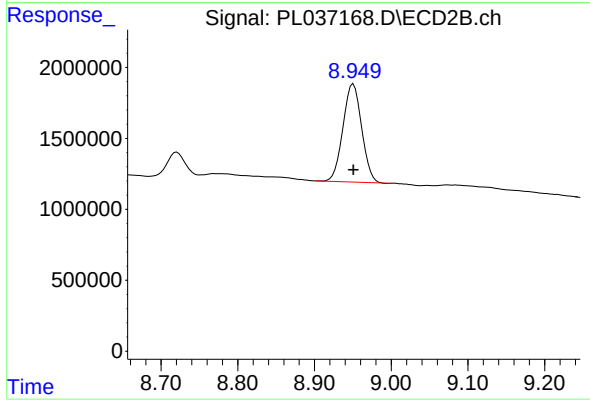

#28 Decachlorobiphenyl

R.T.: 8.951 min

Delta R.T.: 0.000 min

Response: 11743573

Conc: 5.92 ng/ml