

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
 Data File : PL037171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 18:16
 Operator : UA\AJ
 Sample : J3570-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20180374-AMENDED-COMPOSITE-

Manual Integrations
 APPROVED

UGO
 6/21/2018 3:20:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:59:37 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	49724157	17351526	6.286	6.271
28)	SA Decachlor...	8.021	8.950	36508086	12533376	6.050	6.317
Target Compounds							
12)	B 4,4'-DDE	5.457	6.250	14984938	5752664	1.697m	2.261m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062018\
Data File : PL037171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 18:16
Operator : UA\AJ
Sample : J3570-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20180374-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

UGO
6/21/2018 3:20:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:59:37 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

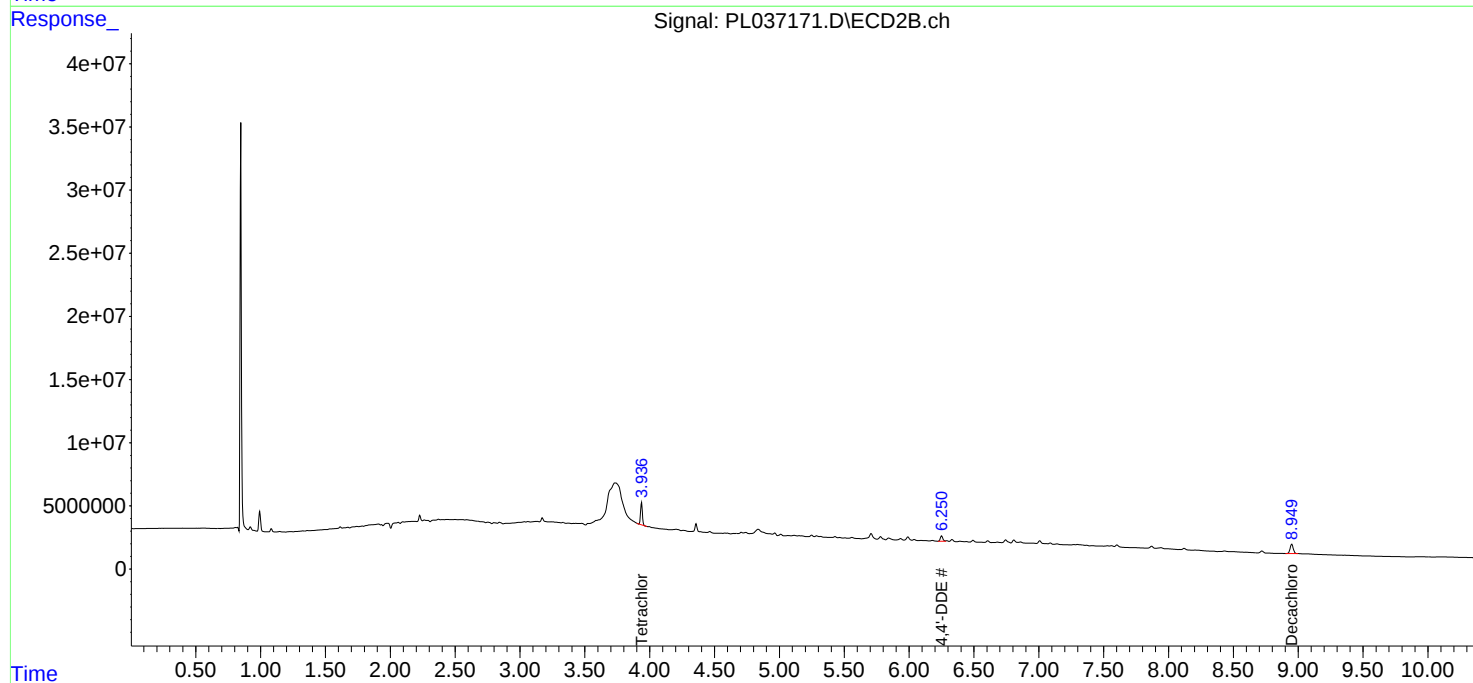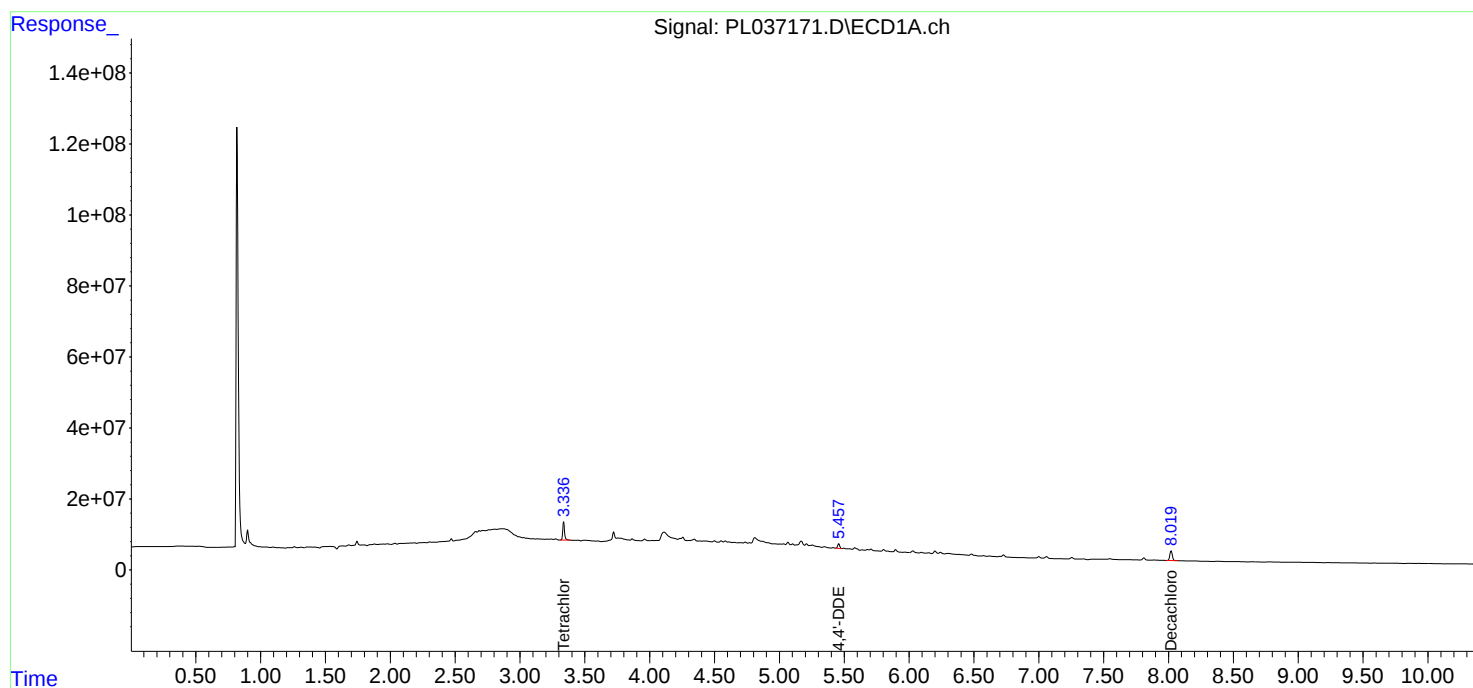

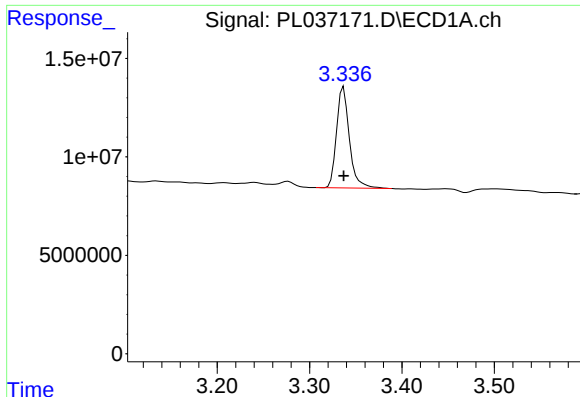


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 49724157
Conc: 6.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
20180374-AMENDED-COMPOSITE-


Manual Integrations
APPROVED

UGO
6/21/2018 3:20:49 PM

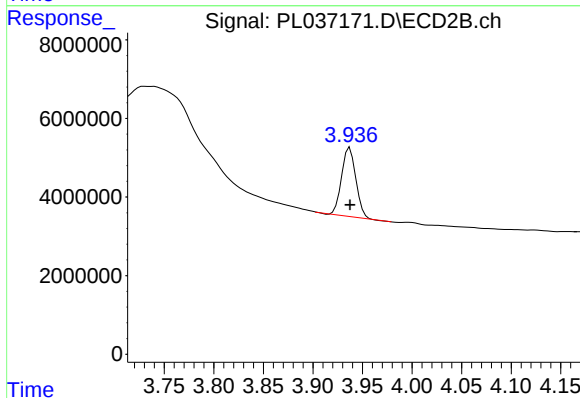


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 17351526
Conc: 6.27 ng/ml

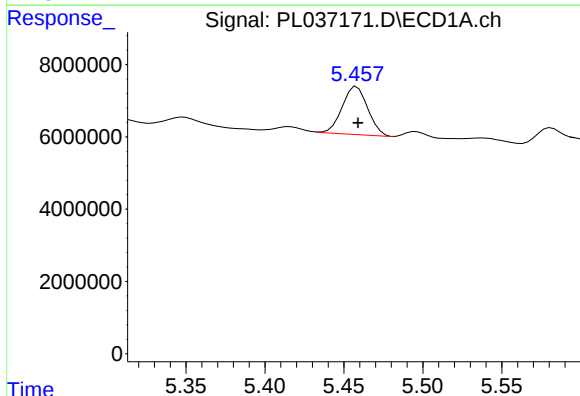


#12 4,4'-DDE

R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 14984938
Conc: 1.70 ng/ml m

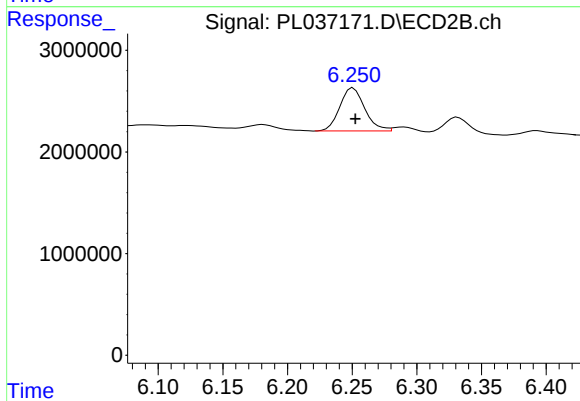

#12 4,4'-DDE

R.T.: 6.250 min
Delta R.T.: -0.003 min
Response: 5752664
Conc: 2.26 ng/ml m

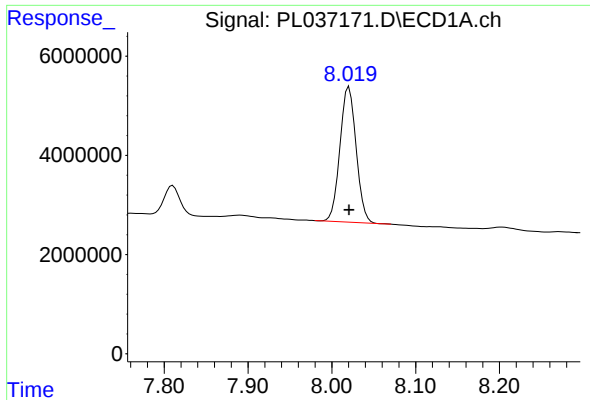

#28 Decachlorobiphenyl

R.T.: 8.021 min

Delta R.T.: 0.000 min


Response: 36508086

Conc: 6.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
20180374-AMENDED-COMPOSITE-

Manual Integrations
APPROVED

UGO
6/21/2018 3:20:49 PM

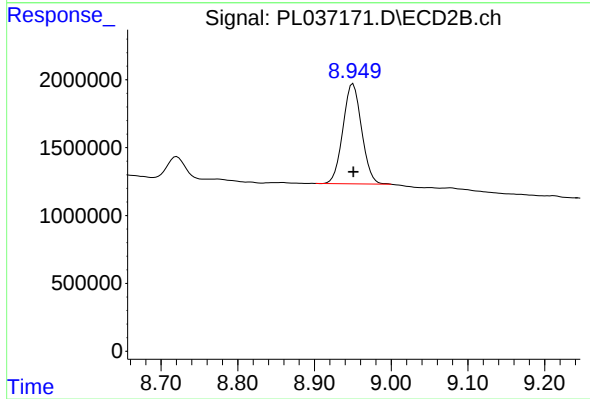

#28 Decachlorobiphenyl

R.T.: 8.950 min

Delta R.T.: 0.000 min

Response: 12533376

Conc: 6.32 ng/ml