

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 10:21
 Operator : UA\AJ
 Sample : J3575-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 13:14:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	103.2E6	38181138	13.045	13.800
28)	SA Decachlor...	8.020	8.950	76568896	26325200	12.689	13.269
Target Compounds							
7)	B delta-BHC	4.494	0.000	11085092	0	1.048	N.D. #
10)	B gamma-Chl...	5.168f	0.000	35166182	0	3.755	N.D. #
18)	B Endrin al...	6.279	0.000	5550850	0	0.979	N.D. #
19)	B Endosulfa...	6.489	0.000	10577973	0	1.584	N.D. #
23)	Chlordane-1	4.113	0.000	15526675	0	51.427	N.D. #
25)	Chlordane-3	5.168	0.000	35166182	0	33.085	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 10:21
Operator : UA\AJ
Sample : J3575-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 13:14:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

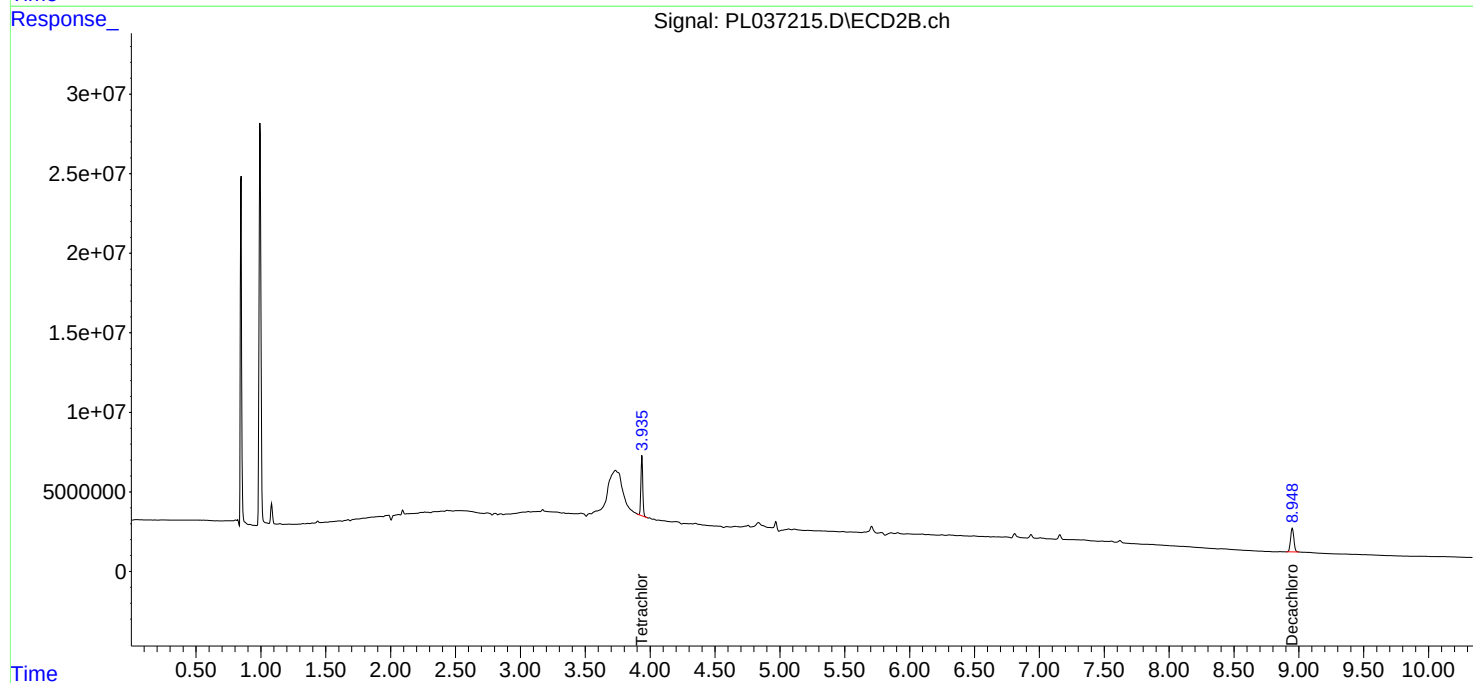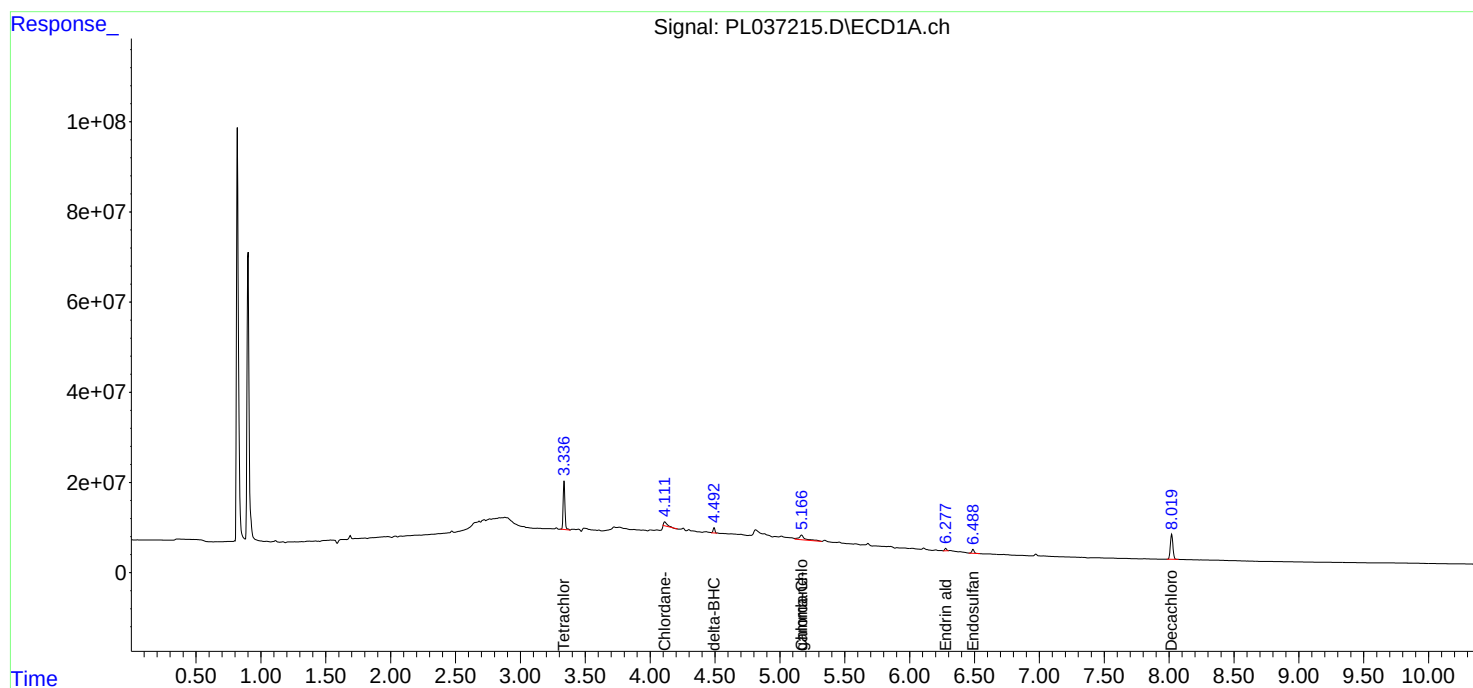


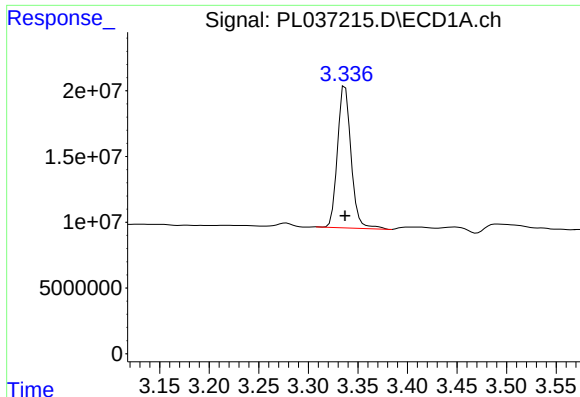

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 103187354
Conc: 13.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

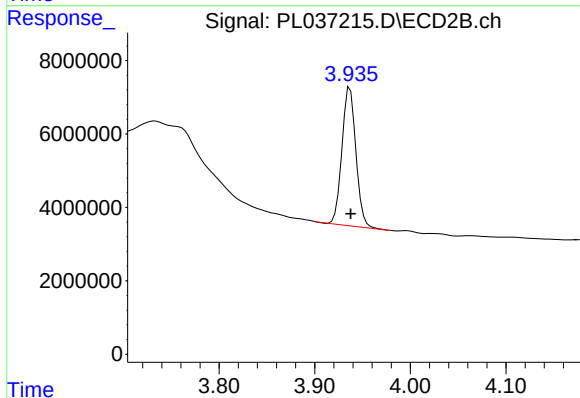


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 38181138
Conc: 13.80 ng/ml

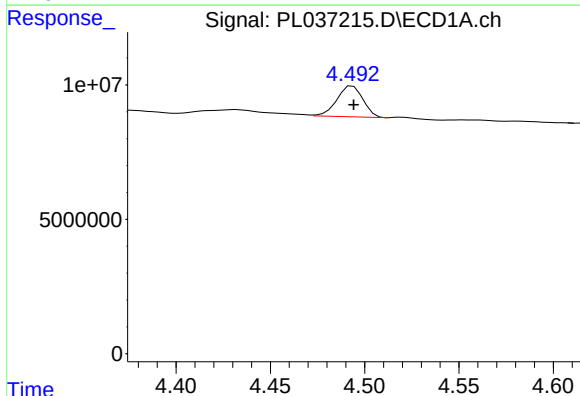


#7 delta-BHC

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 11085092
Conc: 1.05 ng/ml

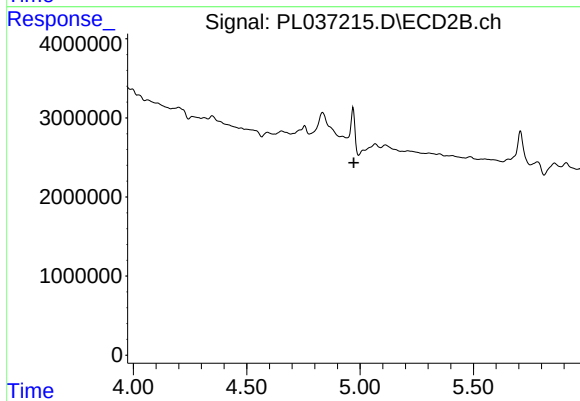

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

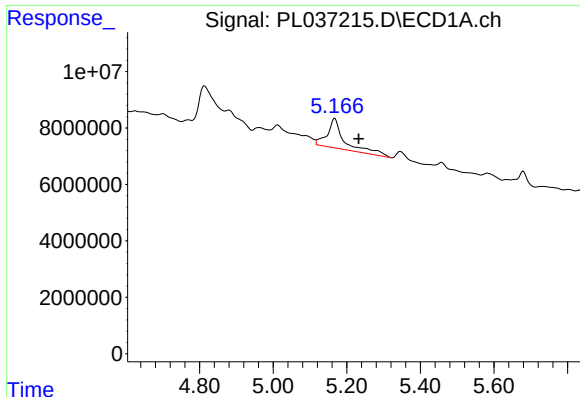

#10 gamma-Chlordane


R.T.: 5.168 min
Delta R.T.: -0.065 min
Response: 35166182
Conc: 3.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

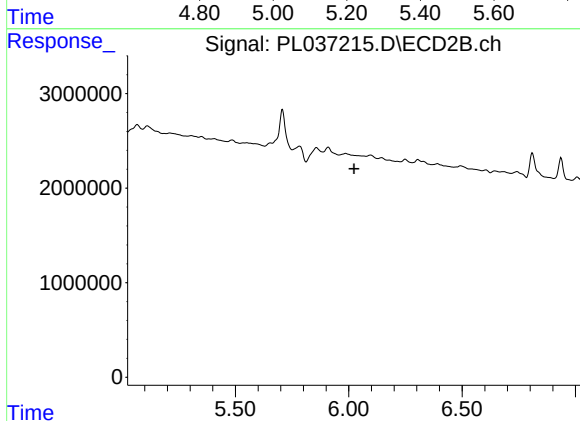


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

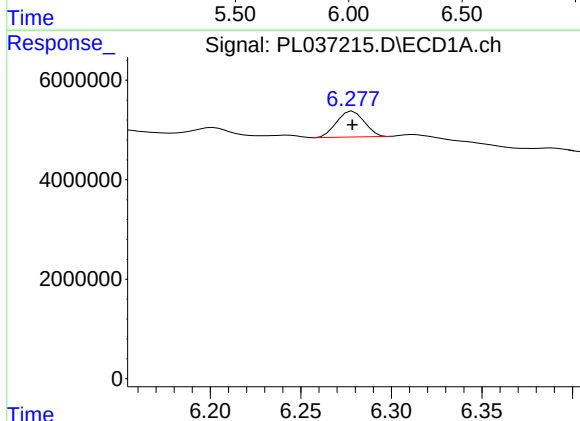


#18 Endrin aldehyde

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 5550850
Conc: 0.98 ng/ml

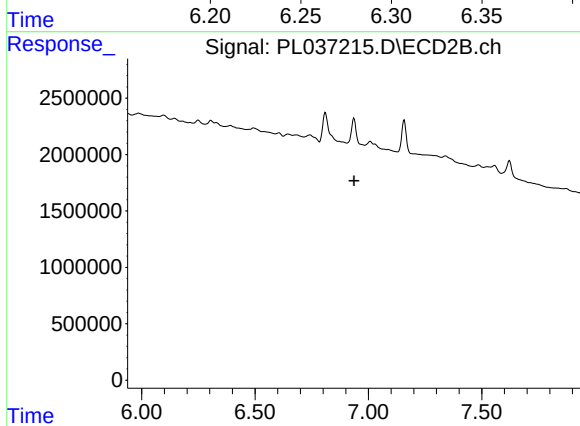

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.937 min
Response: 0
Conc: N.D.

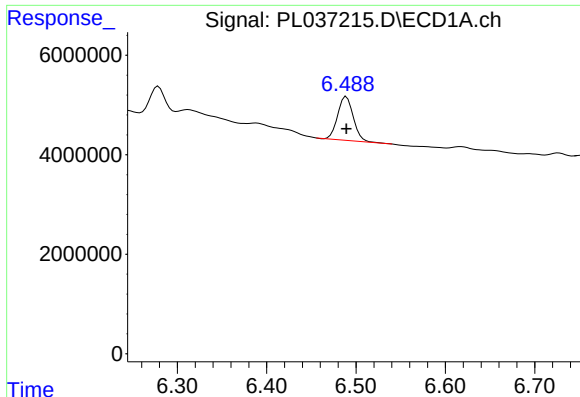

#19 Endosulfan Sulfate


R.T.: 6.489 min
Delta R.T.: 0.000 min
Response: 10577973
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

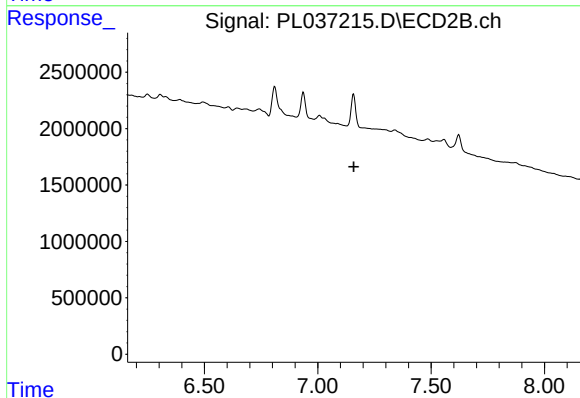


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.159 min
Response: 0
Conc: N.D.

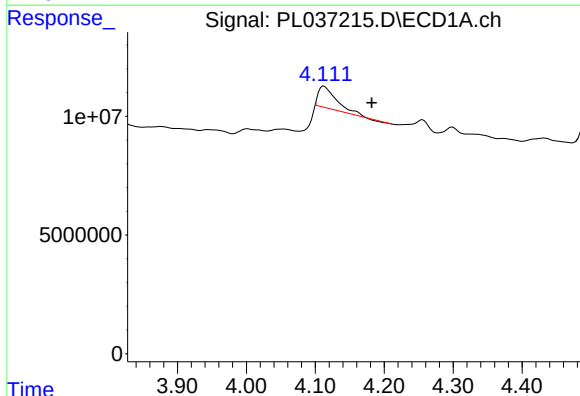


#23 Chlordane-1

R.T.: 4.113 min
Delta R.T.: -0.069 min
Response: 15526675
Conc: 51.43 ng/ml

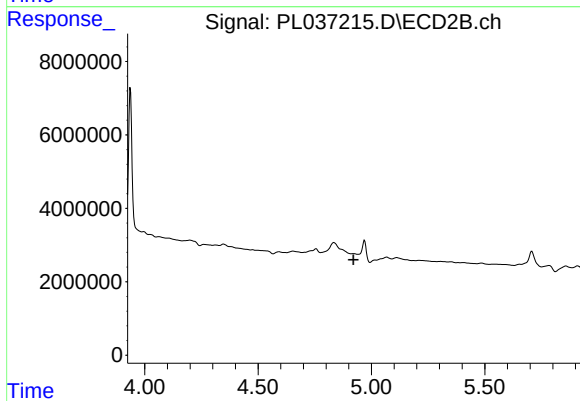

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

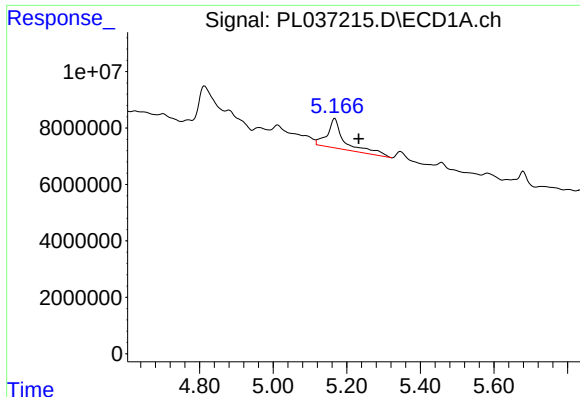

#25 Chlordane-3


R.T.: 5.168 min
Delta R.T.: -0.065 min
Response: 35166182
Conc: 33.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

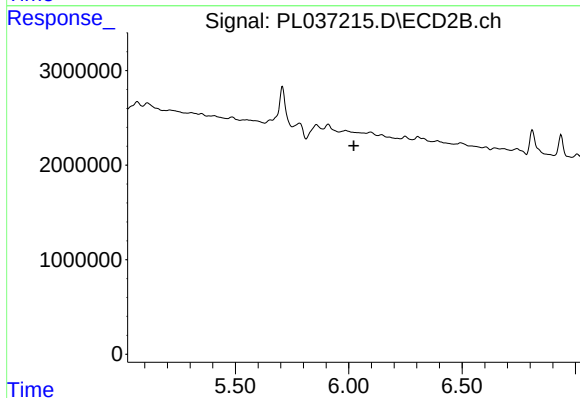


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

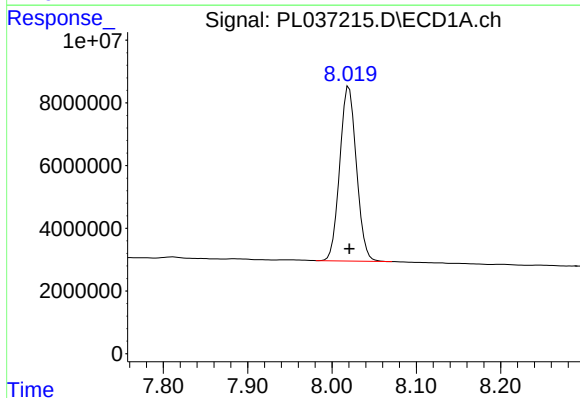

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 76568896
Conc: 12.69 ng/ml

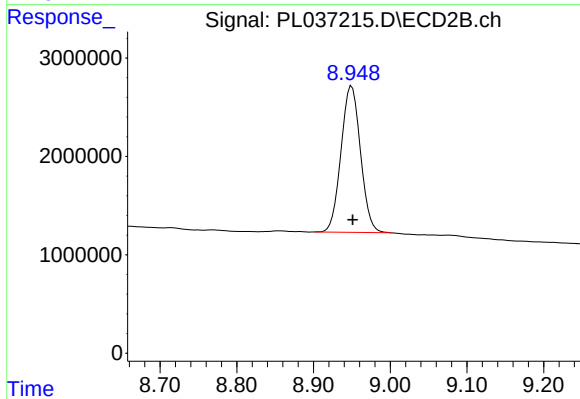

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: -0.001 min
Response: 26325200
Conc: 13.27 ng/ml