

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 12:42
 Operator : UA\AJ
 Sample : J3584-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 13:15:35 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	90633378	32441253	11.458	11.725
28)	SA Decachlor...	8.020	8.951	70666062	24583369	11.711	12.391
Target Compounds							
7)	B delta-BHC	4.494	0.000	8198899	0	0.775	N.D. #
10)	B gamma-Chl...	5.167f	0.000	18561695	0	1.982	N.D. #
23)	Chlordane-1	4.120	0.000	12355567	0	40.924	N.D. #
25)	Chlordane-3	5.167	0.000	18561695	0	17.463	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 12:42
Operator : UA\AJ
Sample : J3584-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 13:15:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

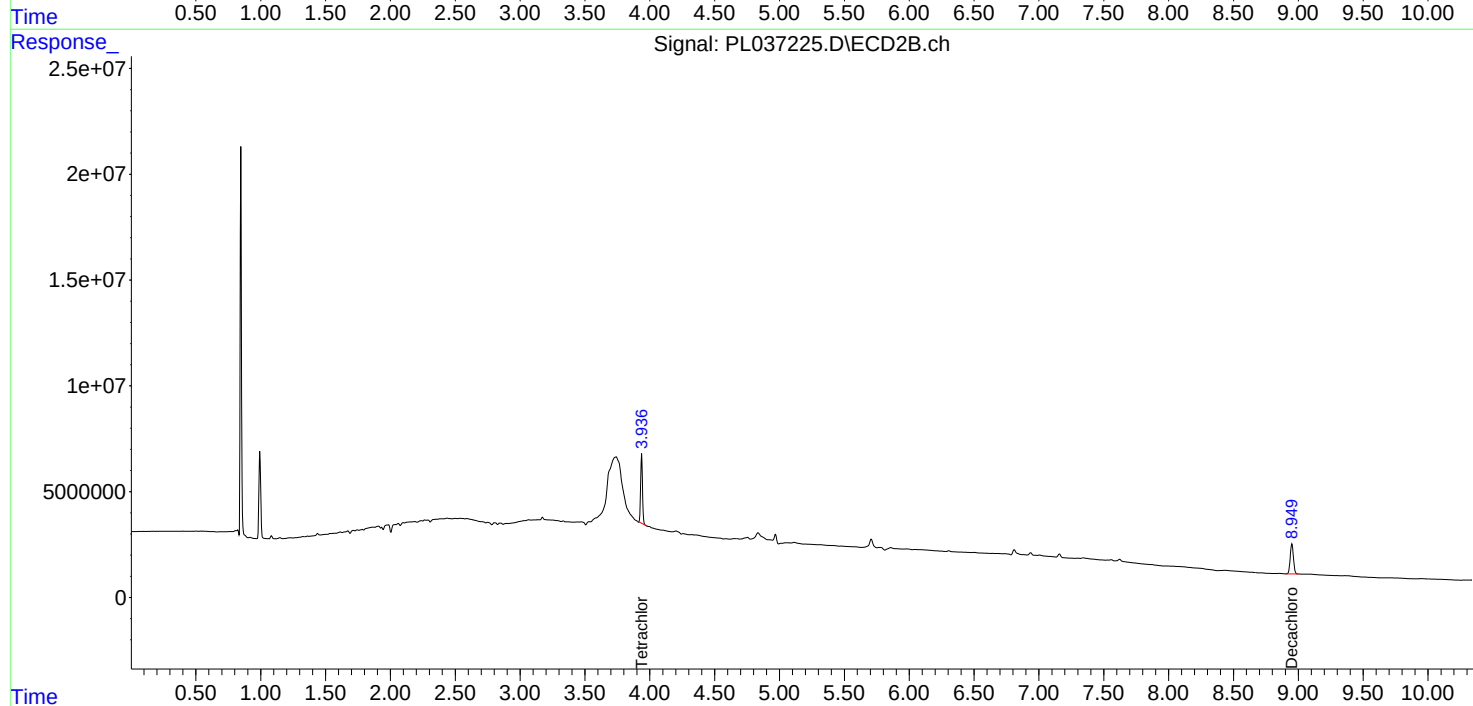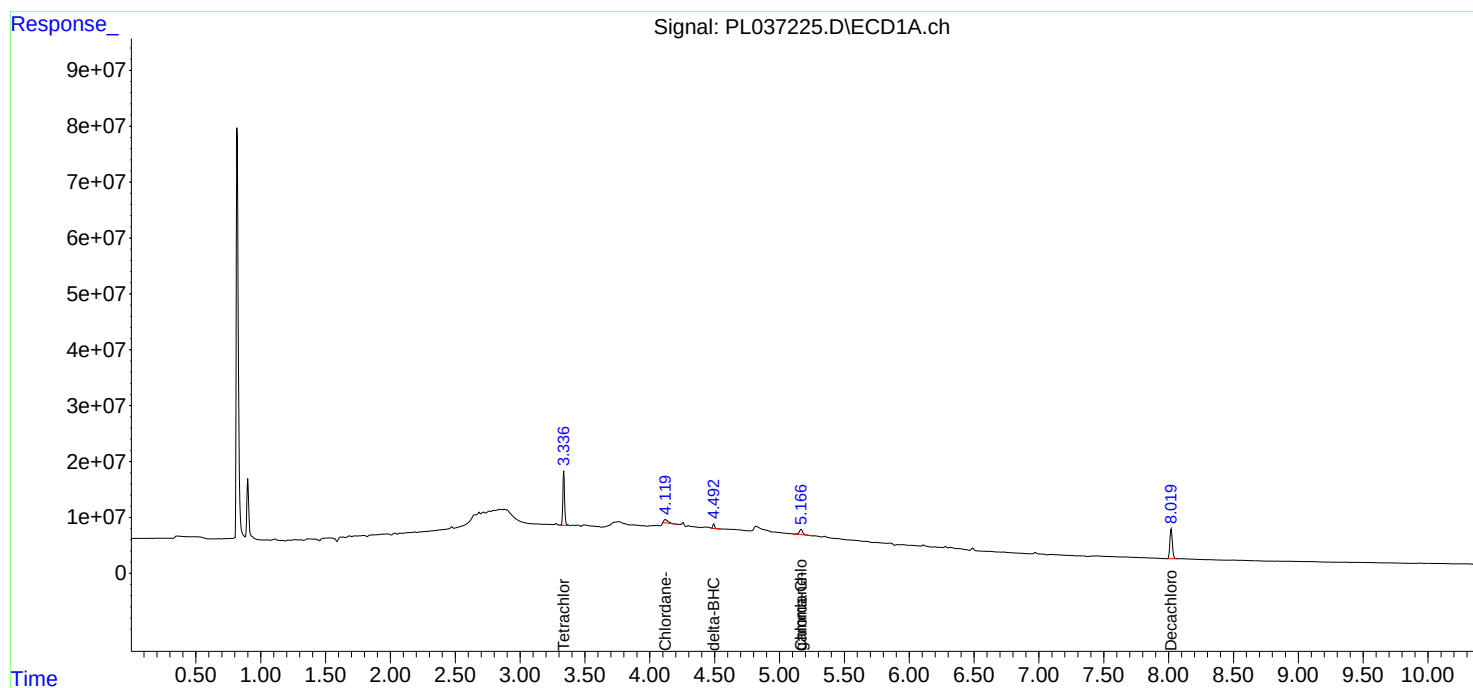


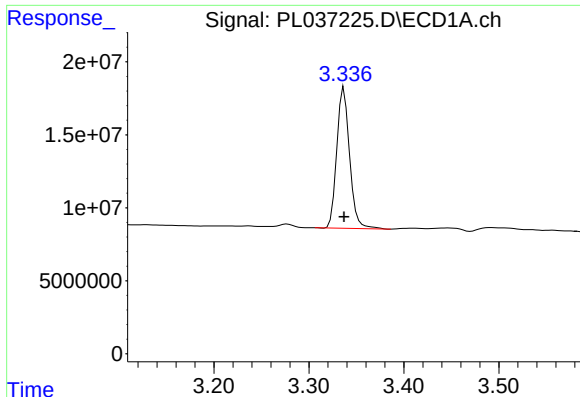

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 90633378
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

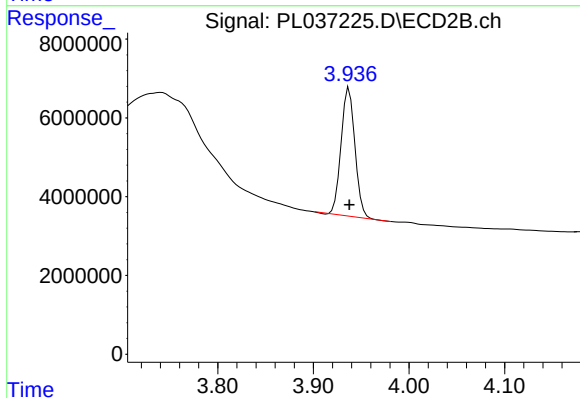


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 32441253
Conc: 11.73 ng/ml

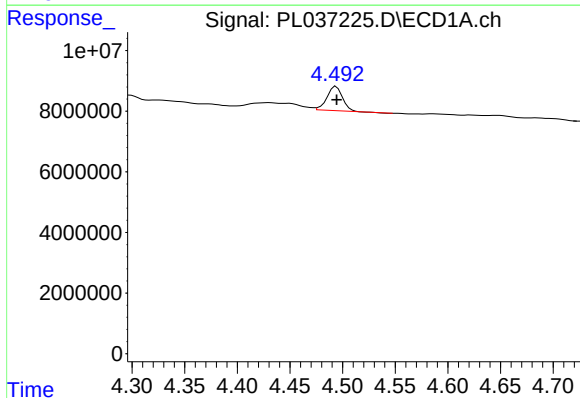


#7 delta-BHC

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 8198899
Conc: 0.78 ng/ml

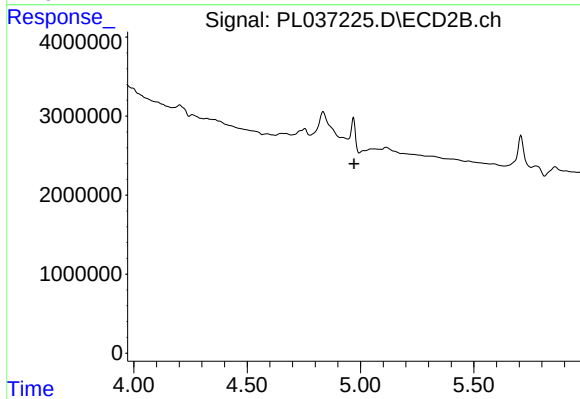

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

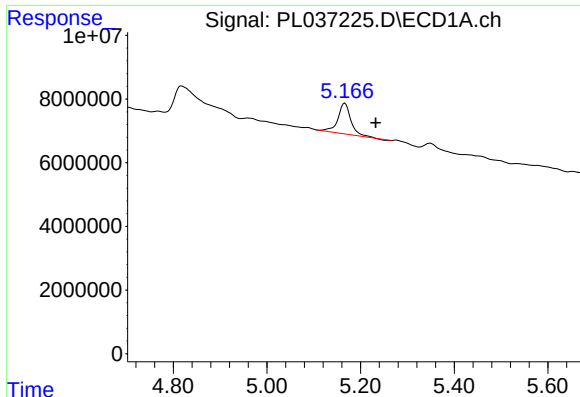

#10 gamma-Chlordane


R.T.: 5.167 min
Delta R.T.: -0.066 min
Response: 18561695
Conc: 1.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

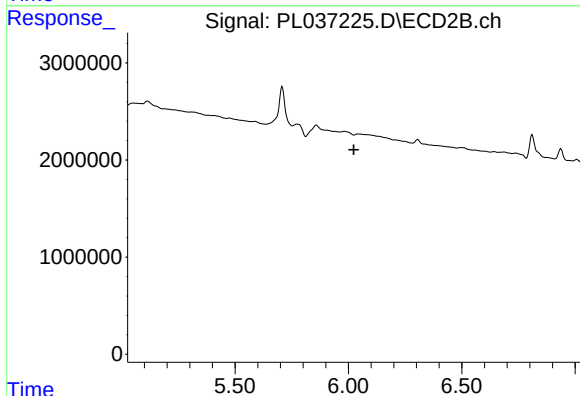


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

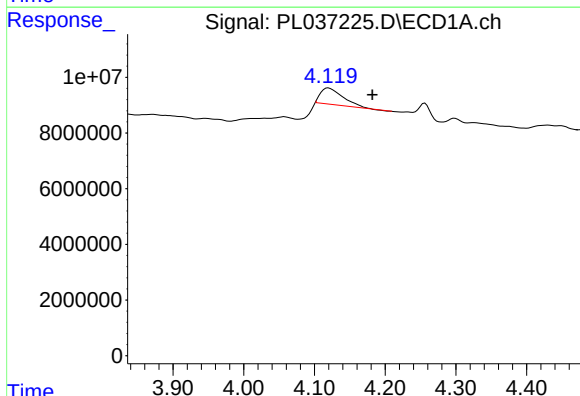


#23 Chlordane-1

R.T.: 4.120 min
Delta R.T.: -0.062 min
Response: 12355567
Conc: 40.92 ng/ml

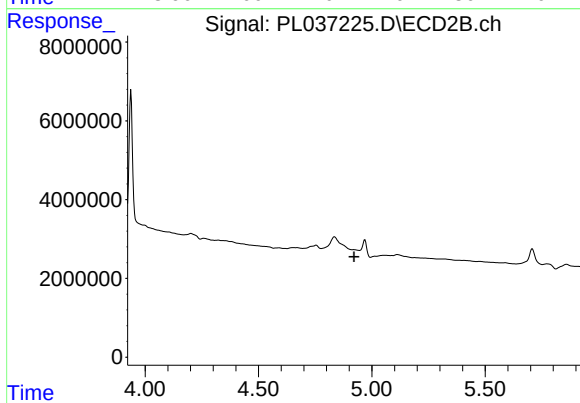

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

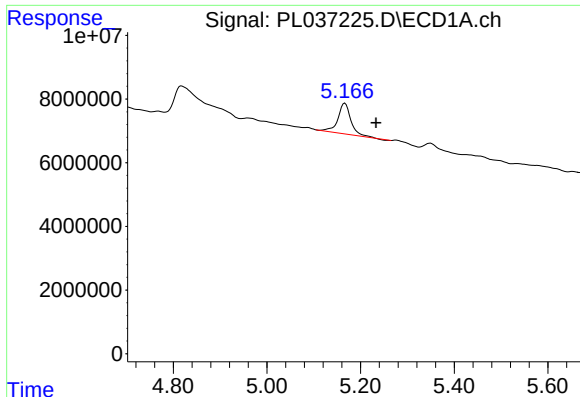

#25 Chlordane-3


R.T.: 5.167 min
Delta R.T.: -0.066 min
Response: 18561695
Conc: 17.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

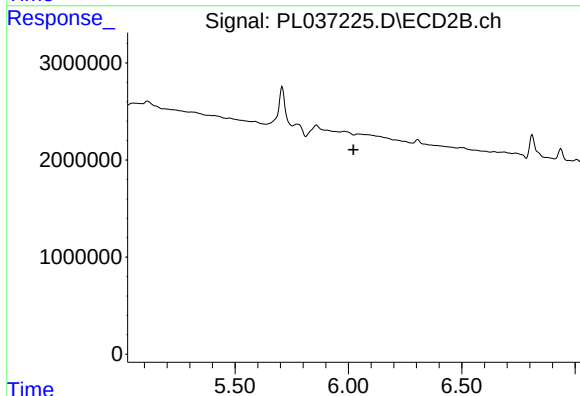


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

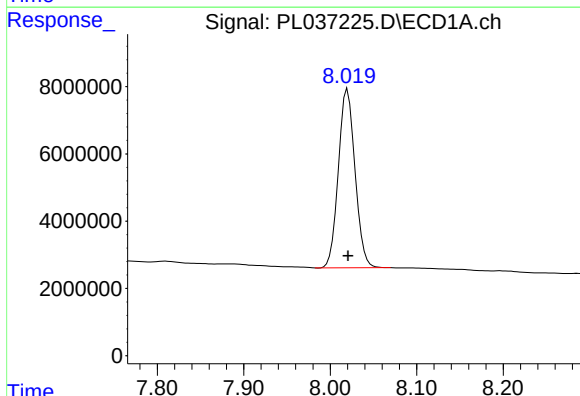

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 70666062
Conc: 11.71 ng/ml

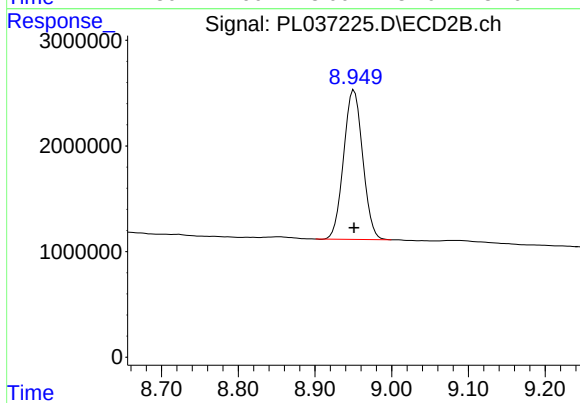

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 24583369
Conc: 12.39 ng/ml