

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 13:10
 Operator : UA\AJ
 Sample : J3584-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 13:52:24 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	85156930	30573388	10.765	11.050
28)	SA Decachlor...	8.019	8.950	67077964	23732620	11.117	11.962
Target Compounds							
7)	B delta-BHC	4.494	0.000	7678754	0	0.726	N.D. #
10)	B gamma-Chl...	5.166f	0.000	17468982	0	1.865	N.D. #
23)	Chlordane-1	4.120	0.000	12766921	0	42.286	N.D. #
25)	Chlordane-3	5.166	0.000	17468982	0	16.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 13:10
Operator : UA\AJ
Sample : J3584-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 13:52:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

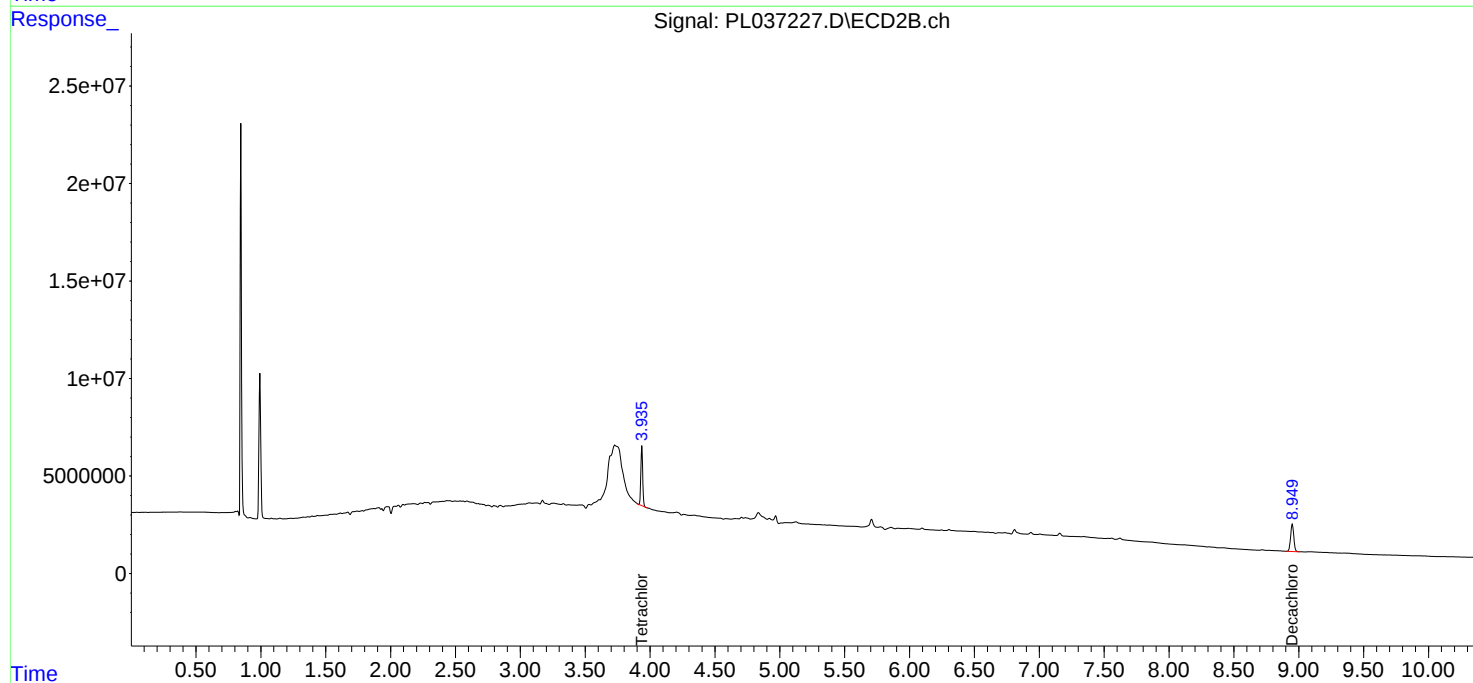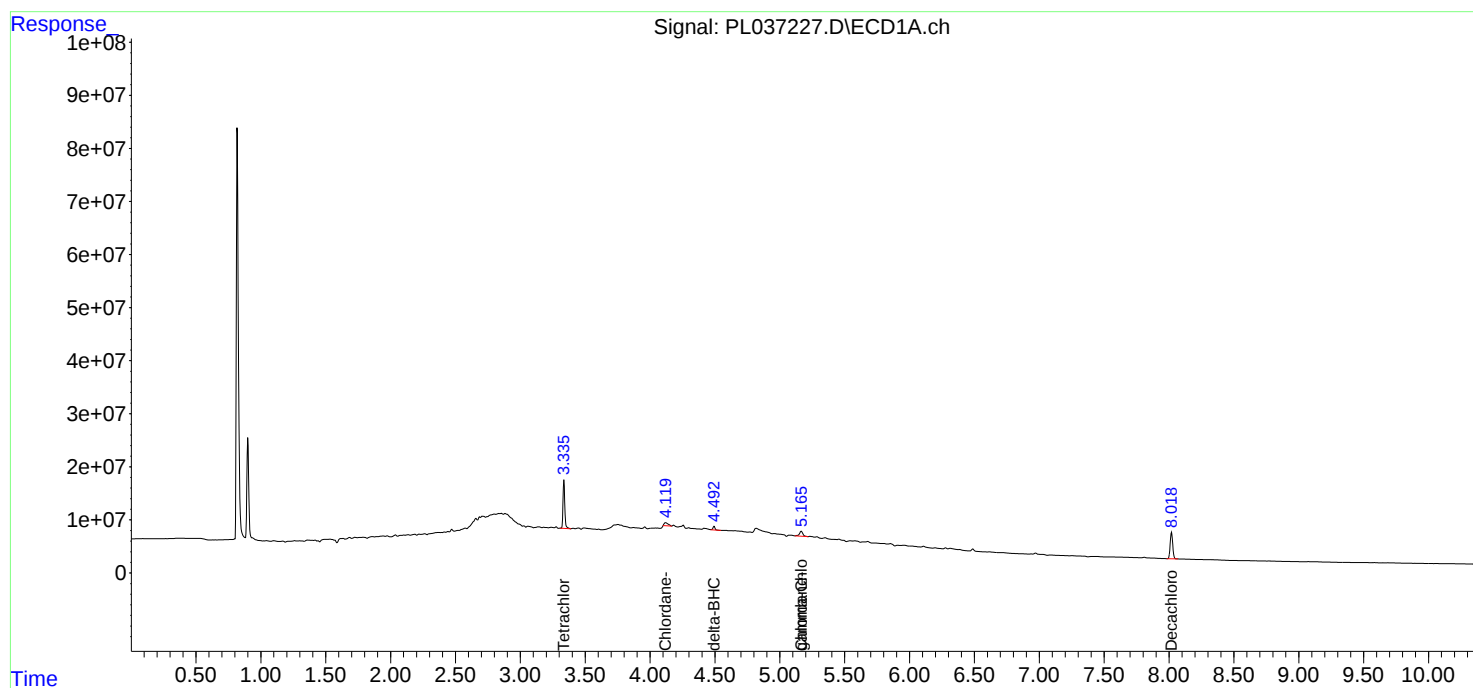


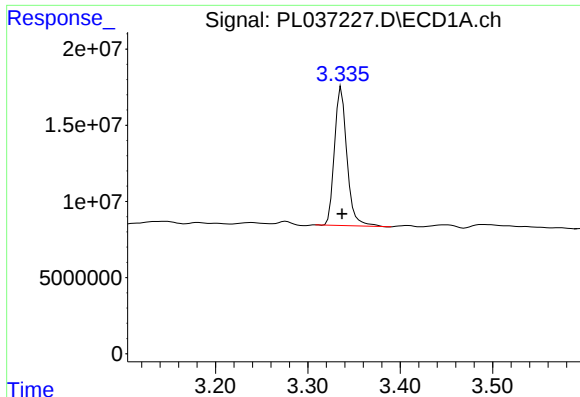

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 85156930
Conc: 10.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

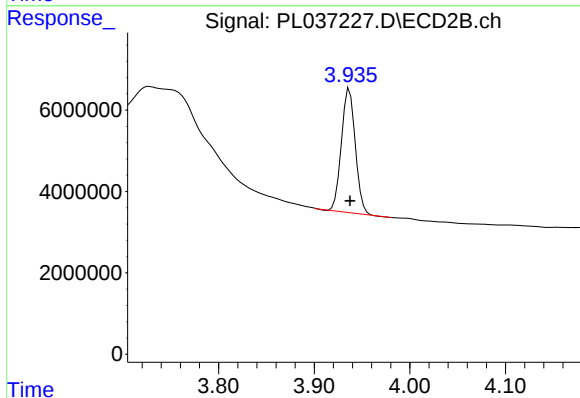


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 30573388
Conc: 11.05 ng/ml

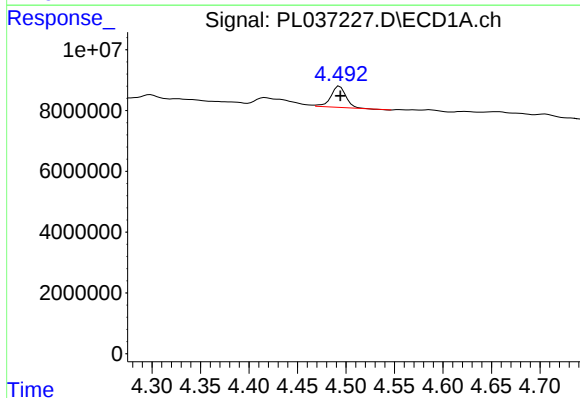


#7 delta-BHC

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 7678754
Conc: 0.73 ng/ml

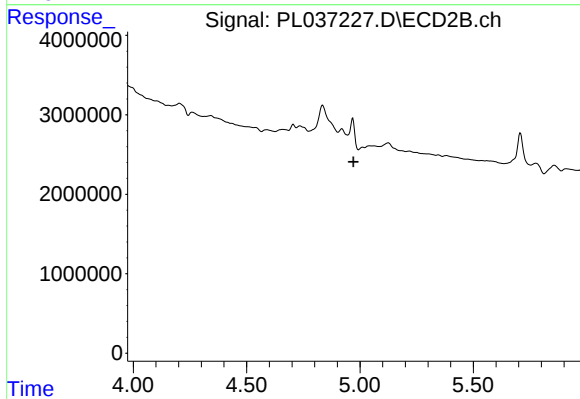

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

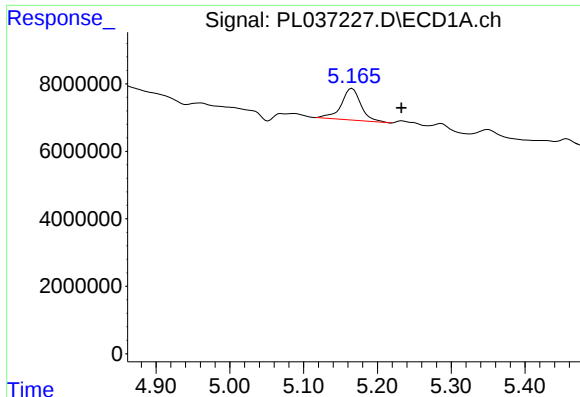

#10 gamma-Chlordane


R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 17468982
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

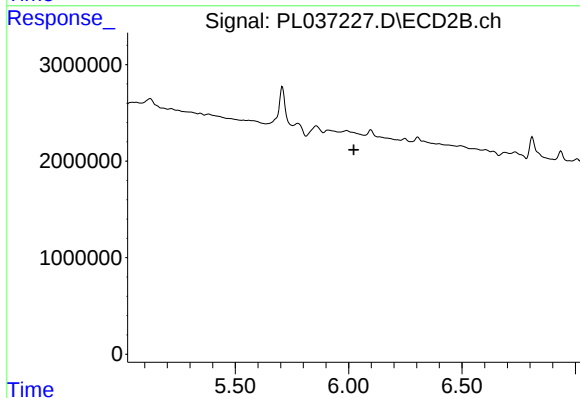


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

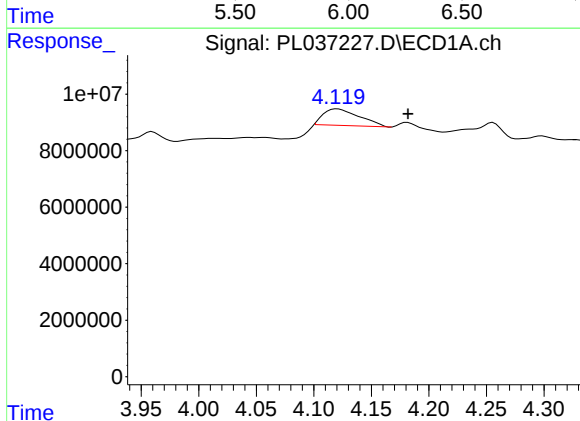


#23 Chlordane-1

R.T.: 4.120 min
Delta R.T.: -0.061 min
Response: 12766921
Conc: 42.29 ng/ml

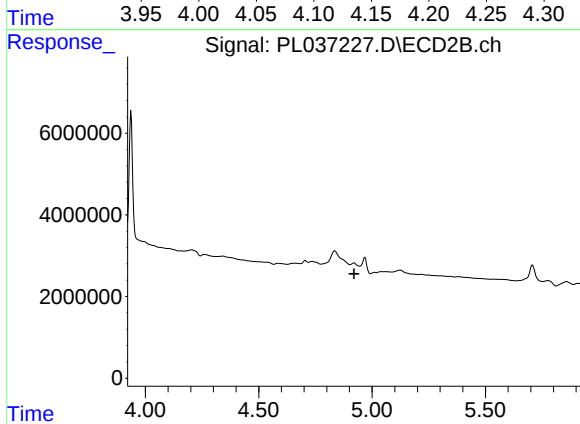

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

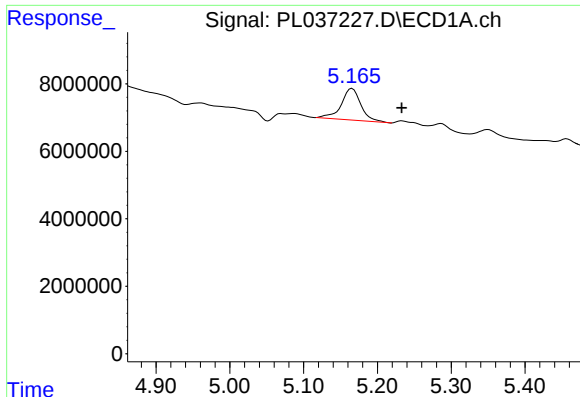

#25 Chlordane-3


R.T.: 5.166 min
Delta R.T.: -0.067 min
Response: 17468982
Conc: 16.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

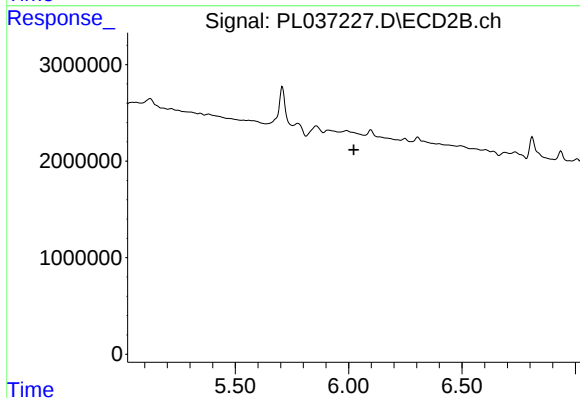


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

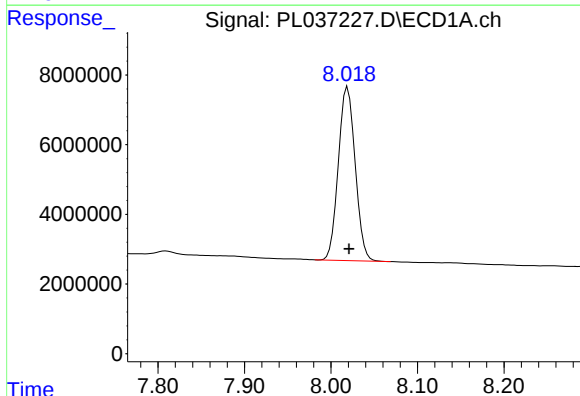

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.001 min
Response: 67077964
Conc: 11.12 ng/ml

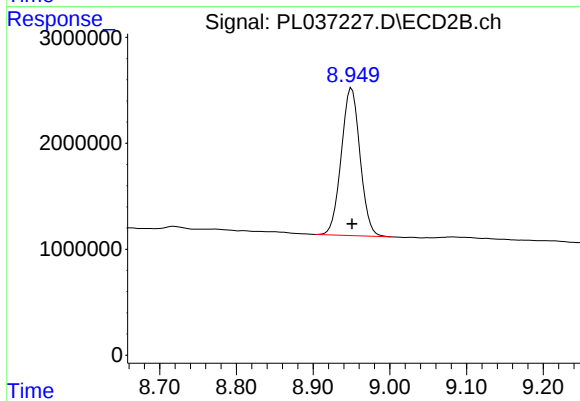

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 23732620
Conc: 11.96 ng/ml