

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 04:56
 Operator : UA\AJ
 Sample : J3246-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:47:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	139.2E6	31675755	17.600	11.449 #
28)	SA Decachlor...	8.019	8.949	75098287	30423001	12.446	15.335
Target Compounds							
2)	A alpha-BHC	3.781	0.000	5880628	0	0.480	N.D. #
6)	B beta-BHC	4.256f	0.000	21170385	0	4.642	N.D. #
9)	A Endosulfan I	5.287f	6.100f	15189805	11904599	1.795	4.642 #
10)	B gamma-Chl...	5.251	0.000	34152254	0	3.646	N.D. #
11)	B alpha-Chl...	5.287	6.100	15189805	11904599	1.673	4.136 #
12)	B 4,4'-DDE	5.457	0.000	24634133	0	2.789	N.D. #
17)	MA 4,4'-DDT	6.204	0.000	12381725	0	1.918	N.D. #
23)	Chlordane-1	4.186	0.000	12376148	0	40.306	N.D. #
25)	Chlordane-3	5.251	0.000	34152254	0	32.131	N.D. #
26)	Chlordane-4	5.287	6.100	15189805	11904599	15.765	24.843 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 04:56
Operator : UA\AJ
Sample : J3246-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:47:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

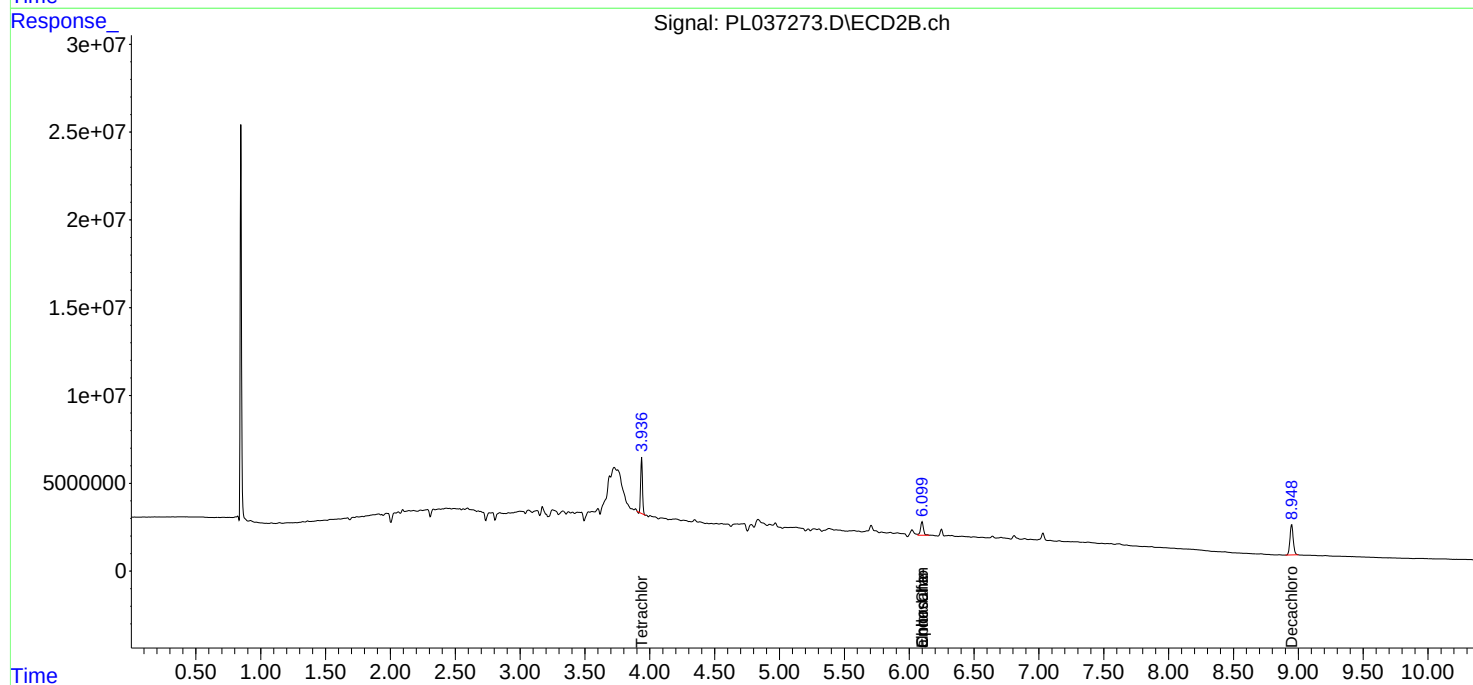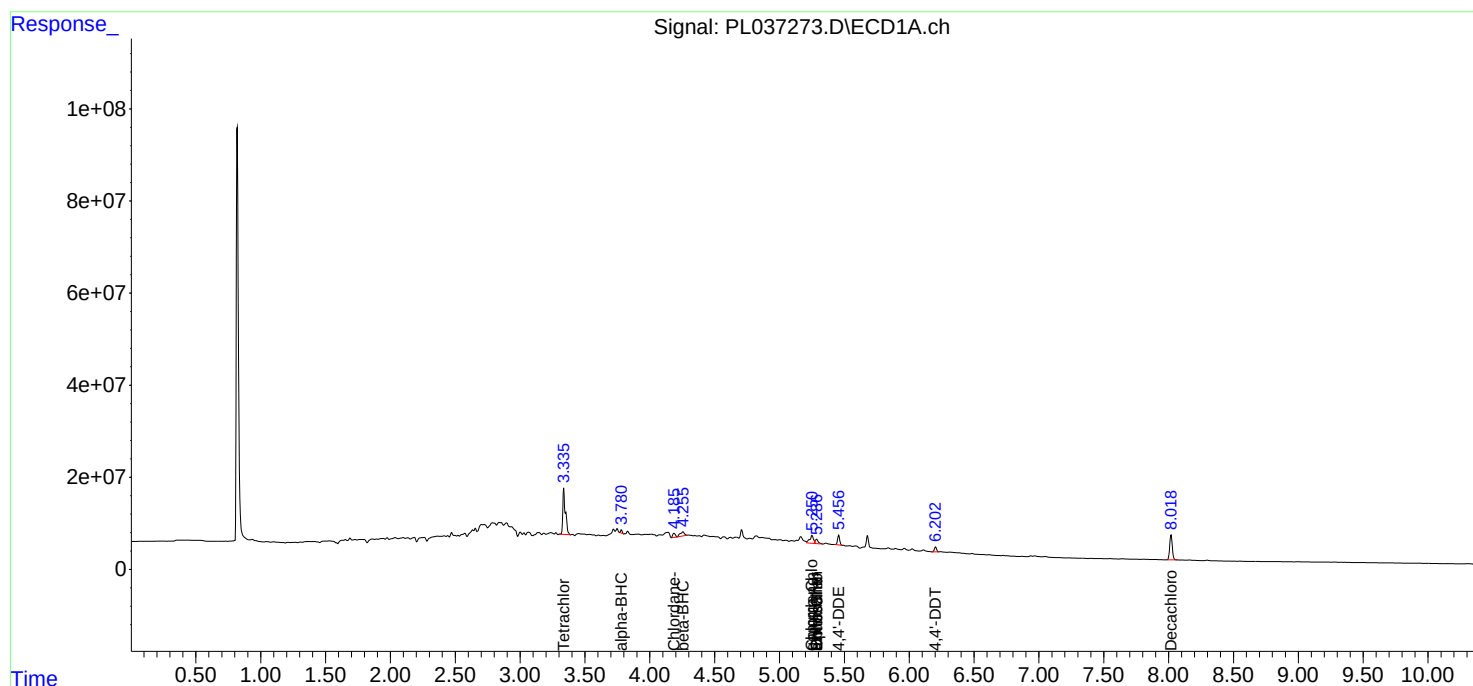


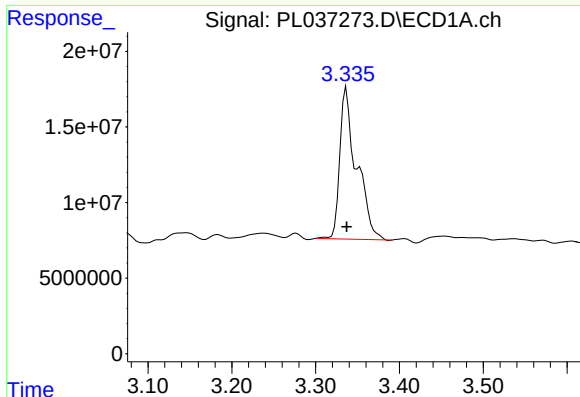

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 139218671
Conc: 17.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

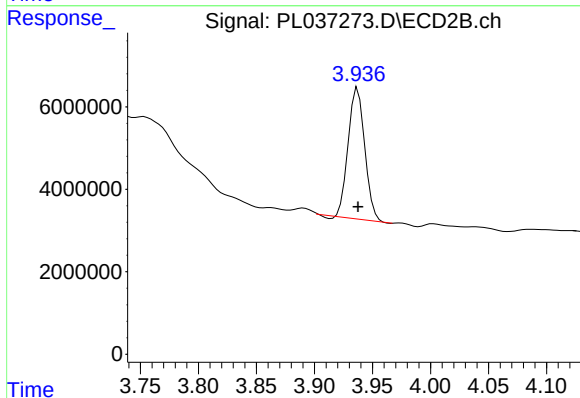


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 31675755
Conc: 11.45 ng/ml

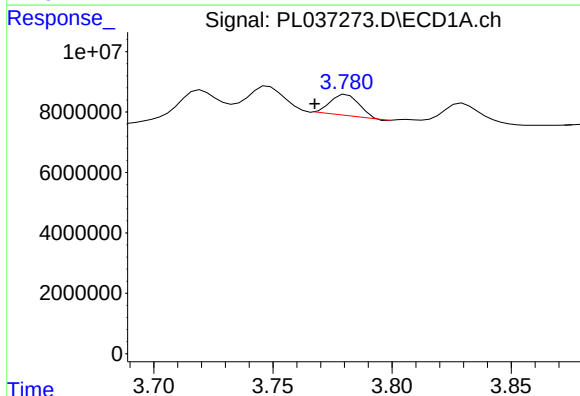


#2 alpha-BHC

R.T.: 3.781 min
Delta R.T.: 0.014 min
Response: 5880628
Conc: 0.48 ng/ml

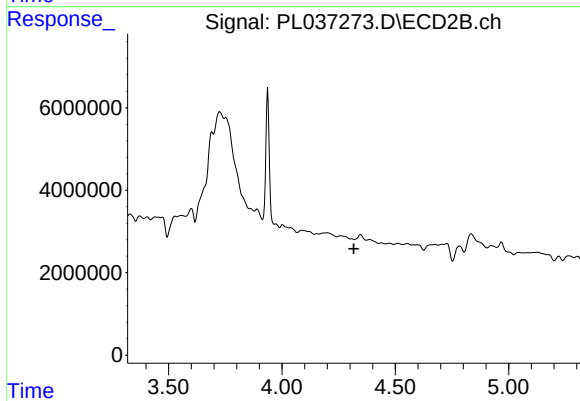

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

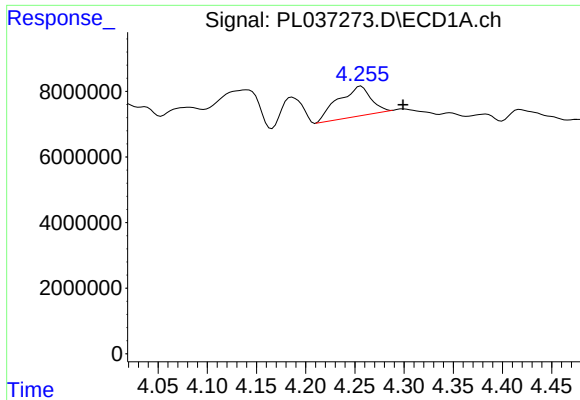

#6 beta-BHC


R.T.: 4.256 min
Delta R.T.: -0.043 min
Response: 21170385
Conc: 4.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

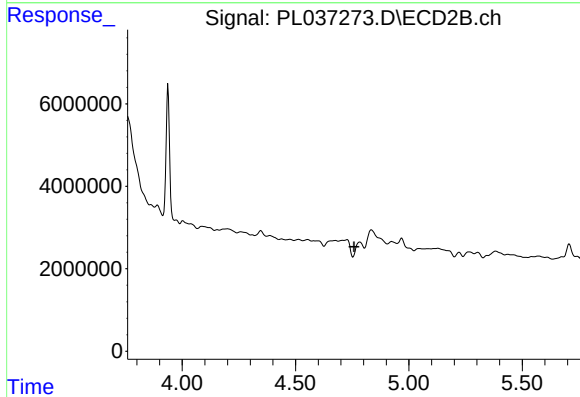


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

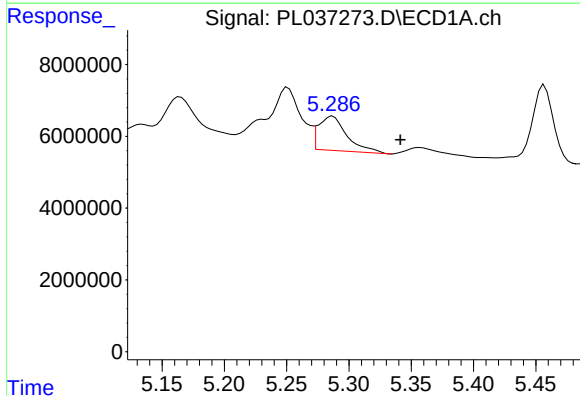


#9 Endosulfan I

R.T.: 5.287 min
Delta R.T.: -0.054 min
Response: 15189805
Conc: 1.80 ng/ml

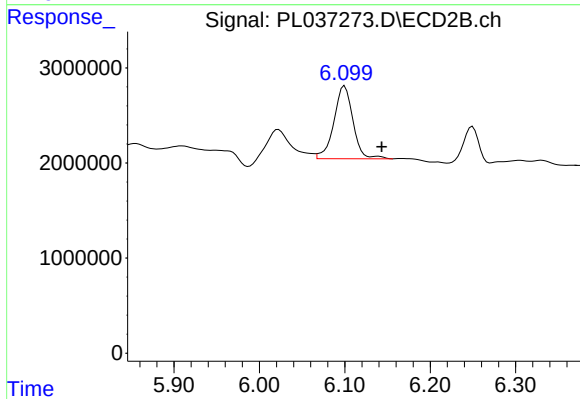

#9 Endosulfan I


R.T.: 6.100 min
Delta R.T.: -0.044 min
Response: 11904599
Conc: 4.64 ng/ml

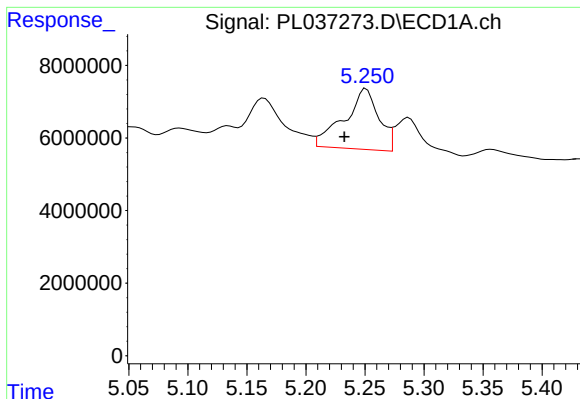

#10 gamma-Chlordane


R.T.: 5.251 min
Delta R.T.: 0.019 min
Response: 34152254
Conc: 3.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

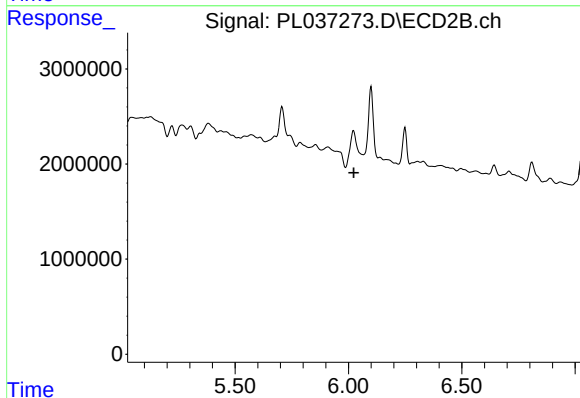


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

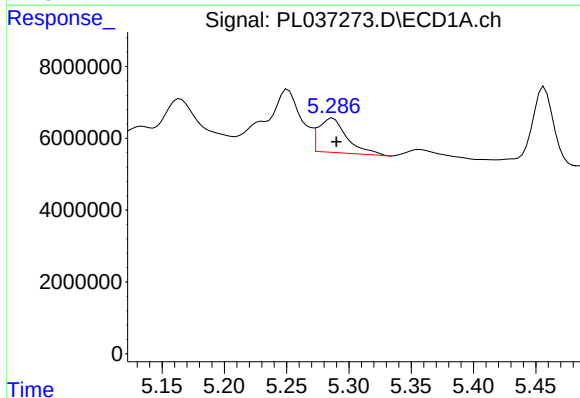


#11 alpha-Chlordane

R.T.: 5.287 min
Delta R.T.: -0.003 min
Response: 15189805
Conc: 1.67 ng/ml

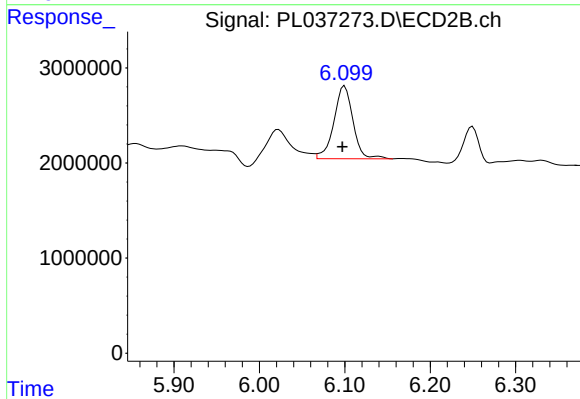

#11 alpha-Chlordane


R.T.: 6.100 min
Delta R.T.: 0.003 min
Response: 11904599
Conc: 4.14 ng/ml

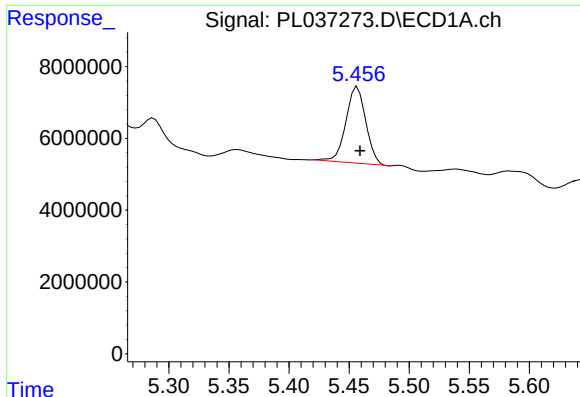

#12 4,4'-DDE


R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 24634133
Conc: 2.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

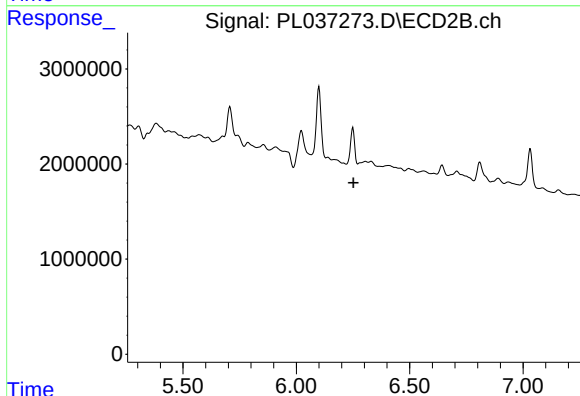


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

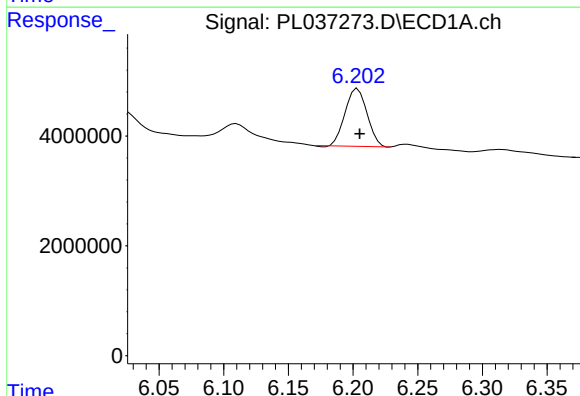


#17 4,4'-DDT

R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 12381725
Conc: 1.92 ng/ml

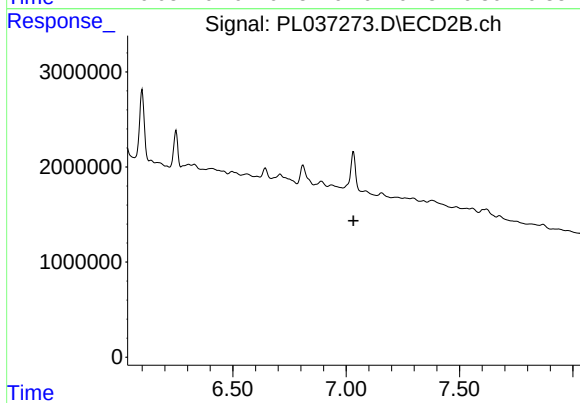

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

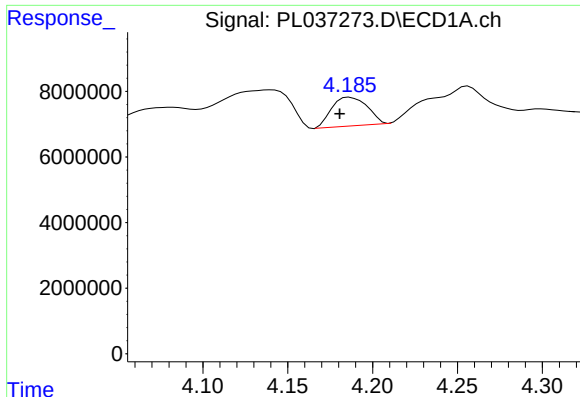

#23 Chlordane-1


R.T.: 4.186 min
Delta R.T.: 0.006 min
Response: 12376148
Conc: 40.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

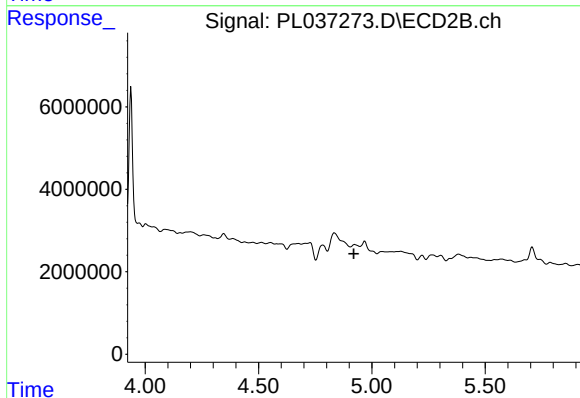


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

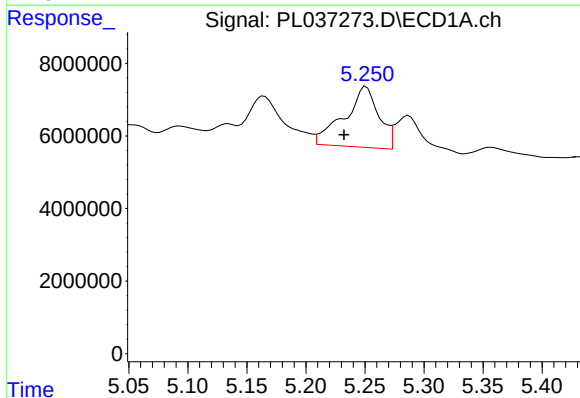


#25 Chlordane-3

R.T.: 5.251 min
Delta R.T.: 0.019 min
Response: 34152254
Conc: 32.13 ng/ml

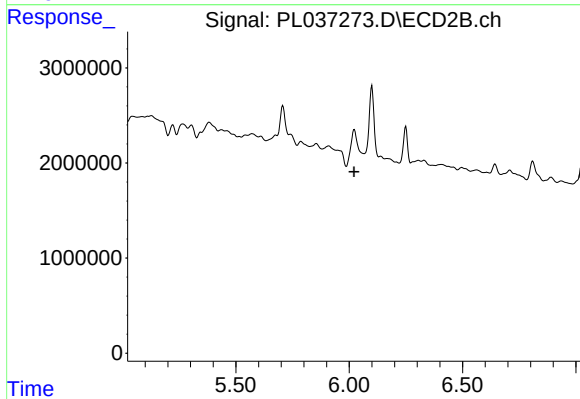

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

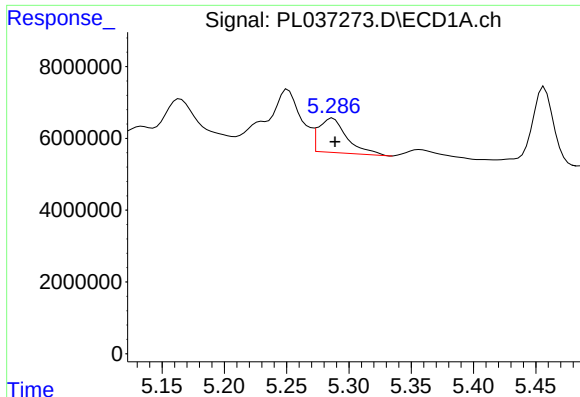

#26 Chlordane-4


R.T.: 5.287 min
Delta R.T.: -0.002 min
Response: 15189805
Conc: 15.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

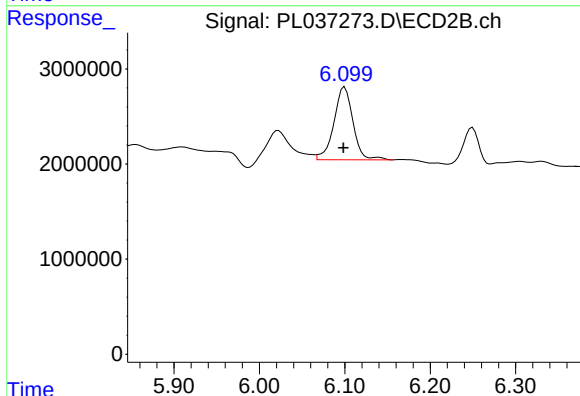


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.002 min
Response: 11904599
Conc: 24.84 ng/ml

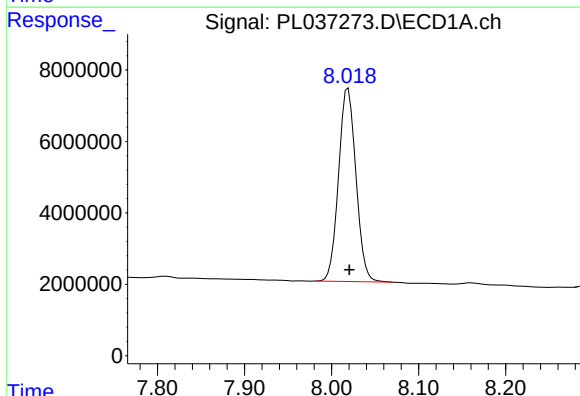

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.002 min
Response: 75098287
Conc: 12.45 ng/ml

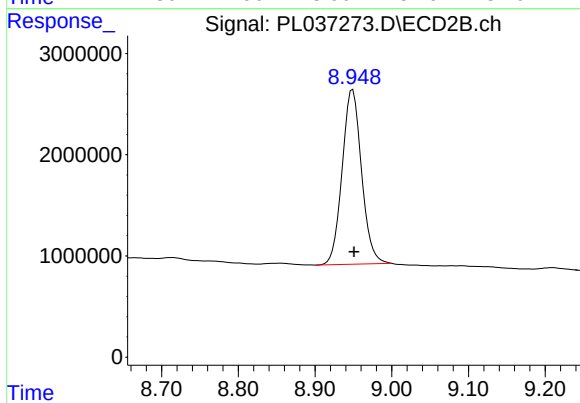

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 30423001
Conc: 15.33 ng/ml