

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 05:24
 Operator : UA\AJ
 Sample : J3594-05
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:47:28 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	87560818	29429572	11.069	10.637
28)	SA Decachlor...	8.019	8.949	51523689	19117178	8.539	9.636
Target Compounds							
10)	B gamma-Chl...	5.165f	0.000	14420418	0	1.540	N.D. #
13)	MA Dieldrin	5.580	0.000	7648534	0	0.864	N.D. #
23)	Chlordane-1	4.130	0.000	9345540	0	30.436	N.D. #
25)	Chlordane-3	5.165	0.000	14420418	0	13.567	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 05:24
Operator : UA\AJ
Sample : J3594-05
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:47:28 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

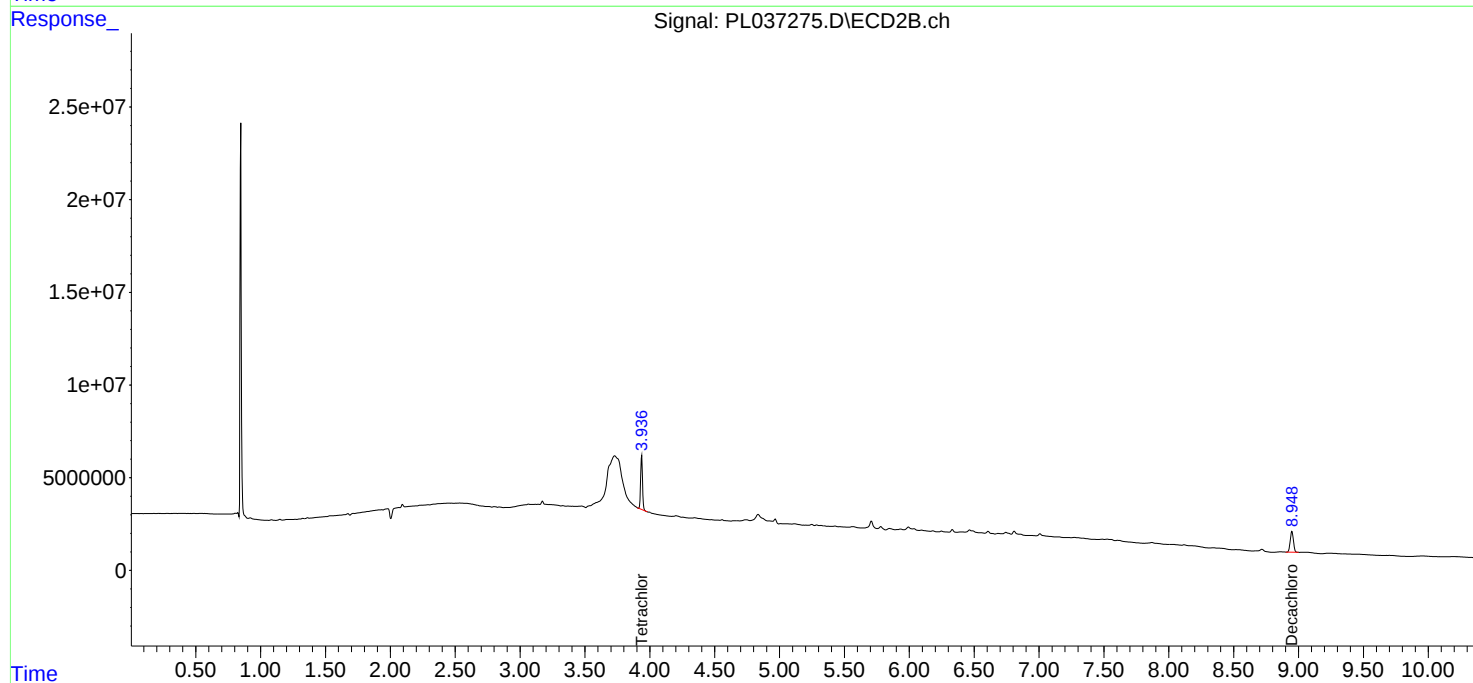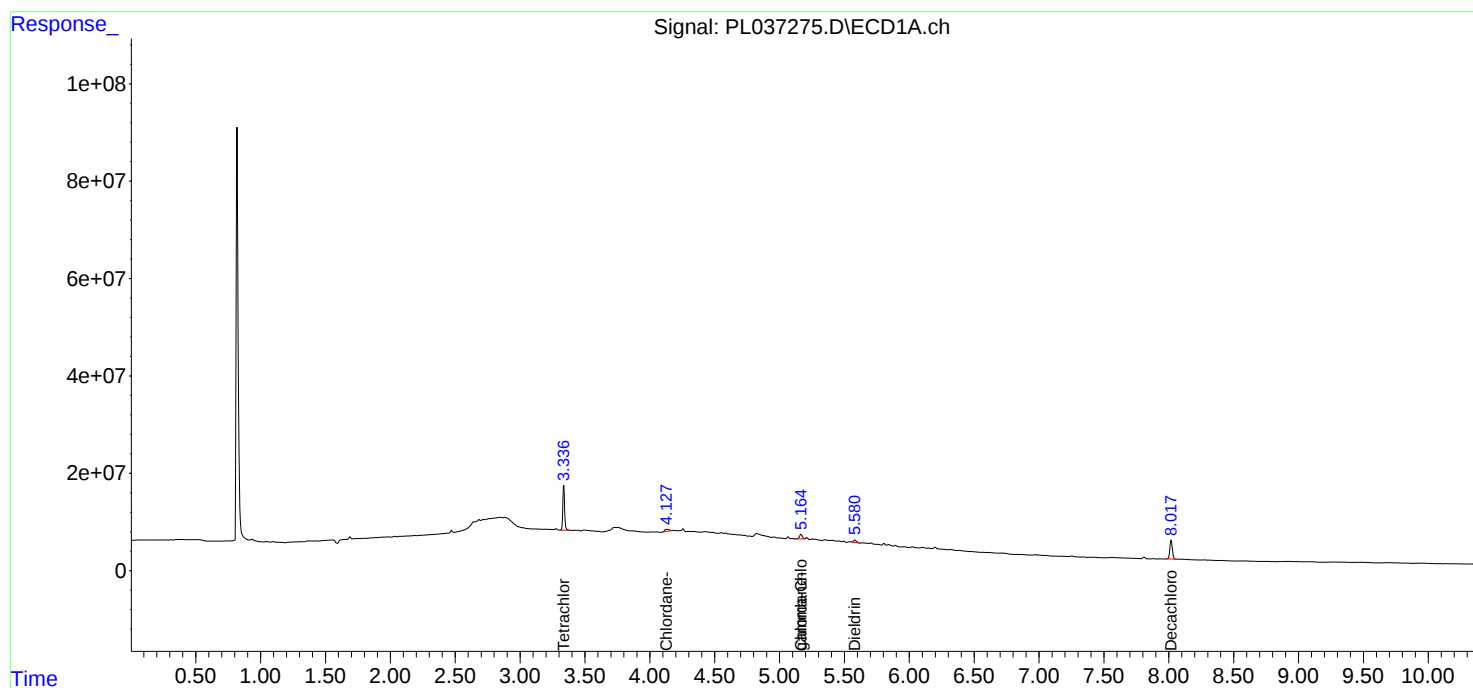


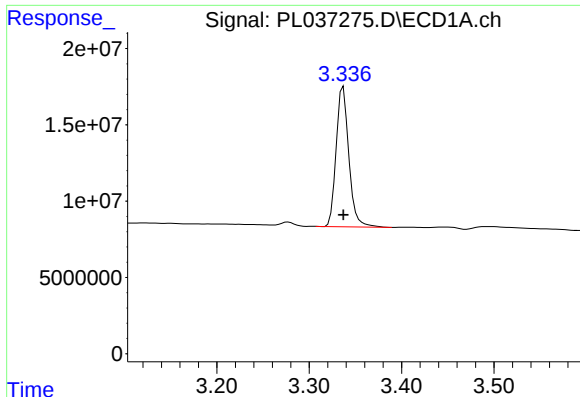

#1 Tetrachloro-m-xylene


R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 87560818
Conc: 11.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

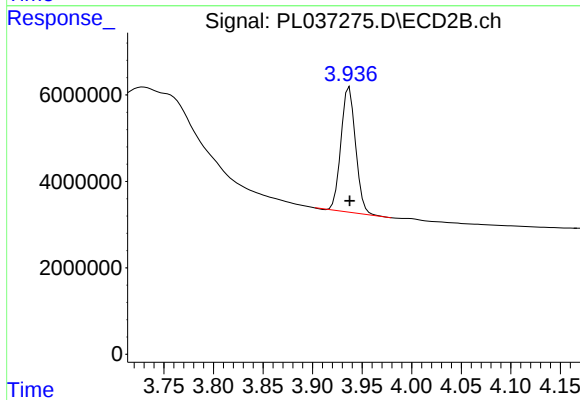


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 29429572
Conc: 10.64 ng/ml

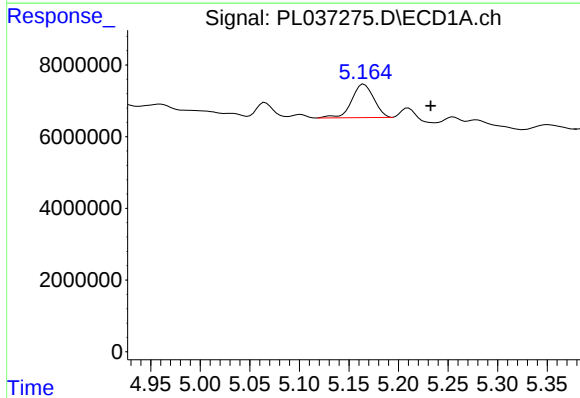


#10 gamma-Chlordane

R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 14420418
Conc: 1.54 ng/ml

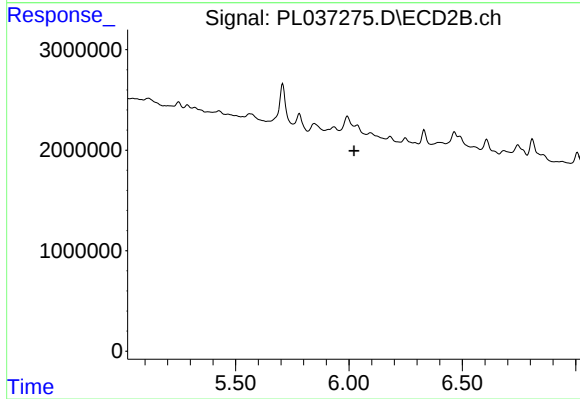

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

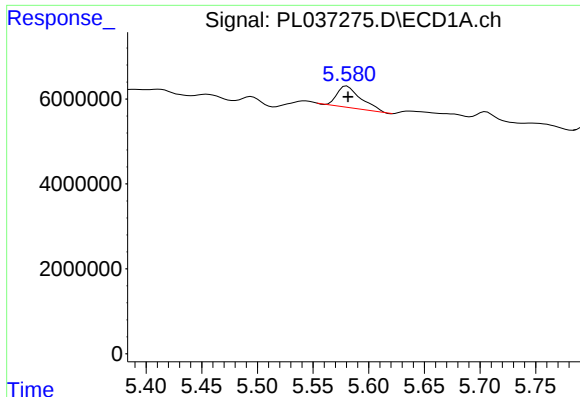

#13 Dieldrin


R.T.: 5.580 min
Delta R.T.: 0.000 min
Response: 7648534
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

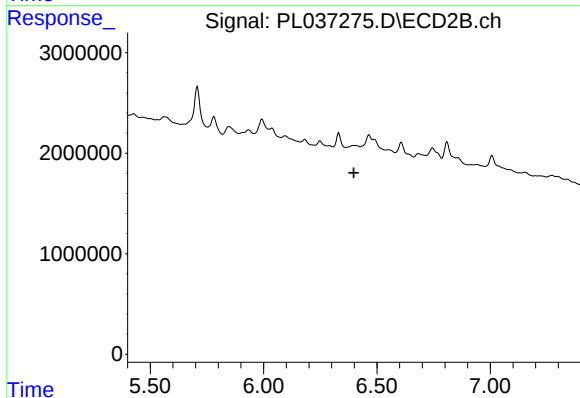


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

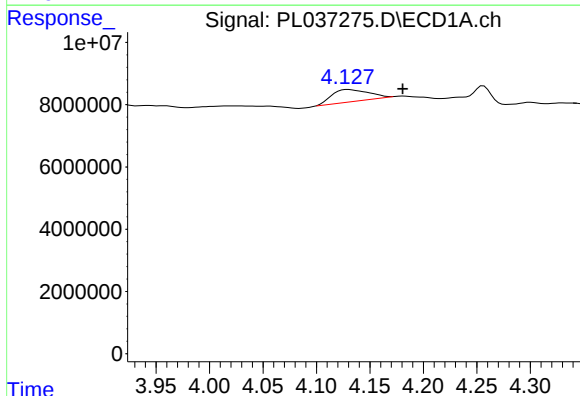


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: -0.051 min
Response: 9345540
Conc: 30.44 ng/ml

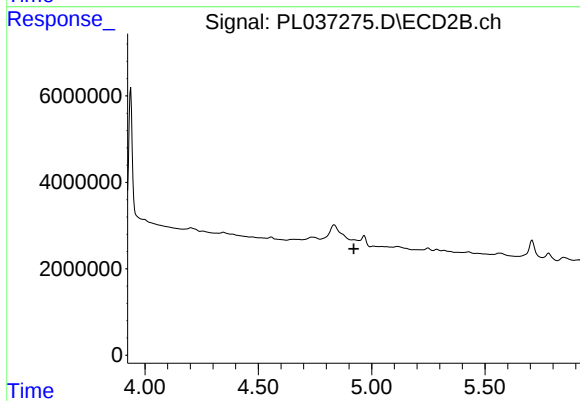

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

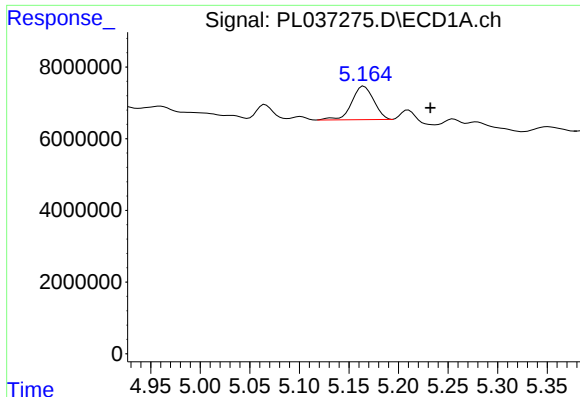

#25 Chlordane-3


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 14420418
Conc: 13.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

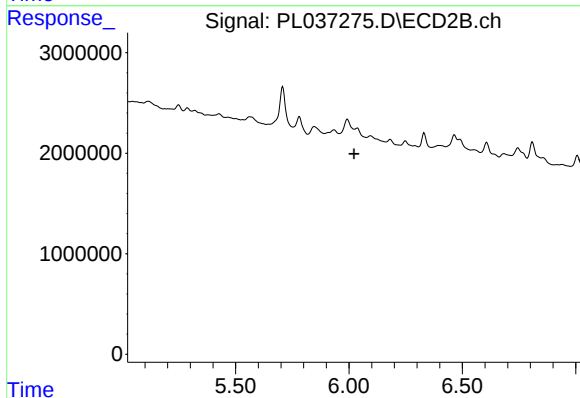


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

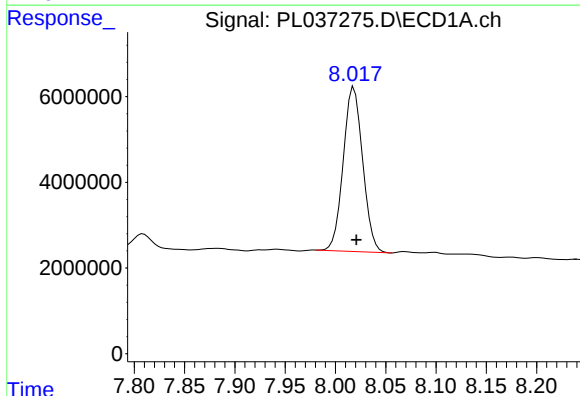

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.002 min
Response: 51523689
Conc: 8.54 ng/ml

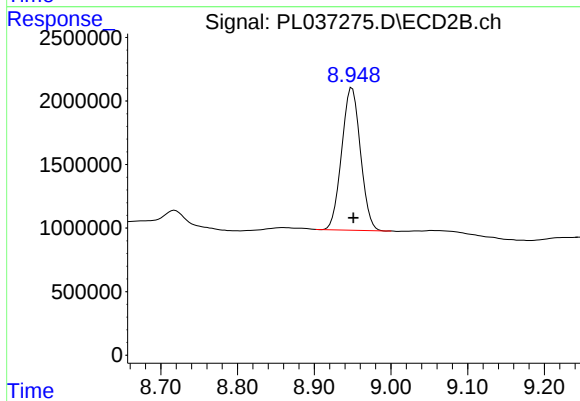

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 19117178
Conc: 9.64 ng/ml