

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 07:31
 Operator : UA\AJ
 Sample : J3603-13
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:49:02 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	80043306	29365586	10.119	10.614
28)	SA Decachlor...	8.018	8.948	57983902	21982202	9.609	11.080
Target Compounds							
8)	B Heptachlo...	4.956f	0.000	3889540	0	0.415	N.D. #
10)	B gamma-Chl...	5.165f	0.000	18789719	0	2.006	N.D. #
23)	Chlordane-1	4.132	0.000	8386883	0	27.314	N.D. #
25)	Chlordane-3	5.165	0.000	18789719	0	17.677	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 07:31
Operator : UA\AJ
Sample : J3603-13
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:49:02 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

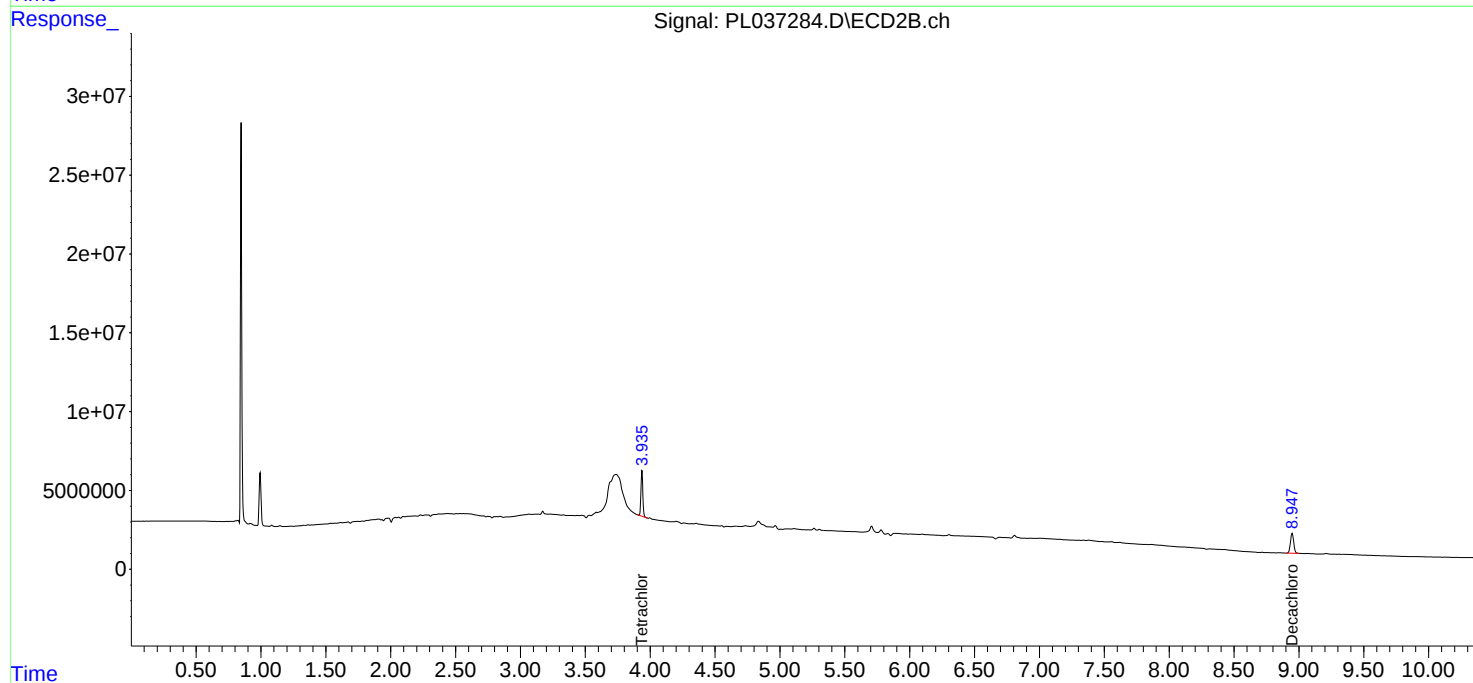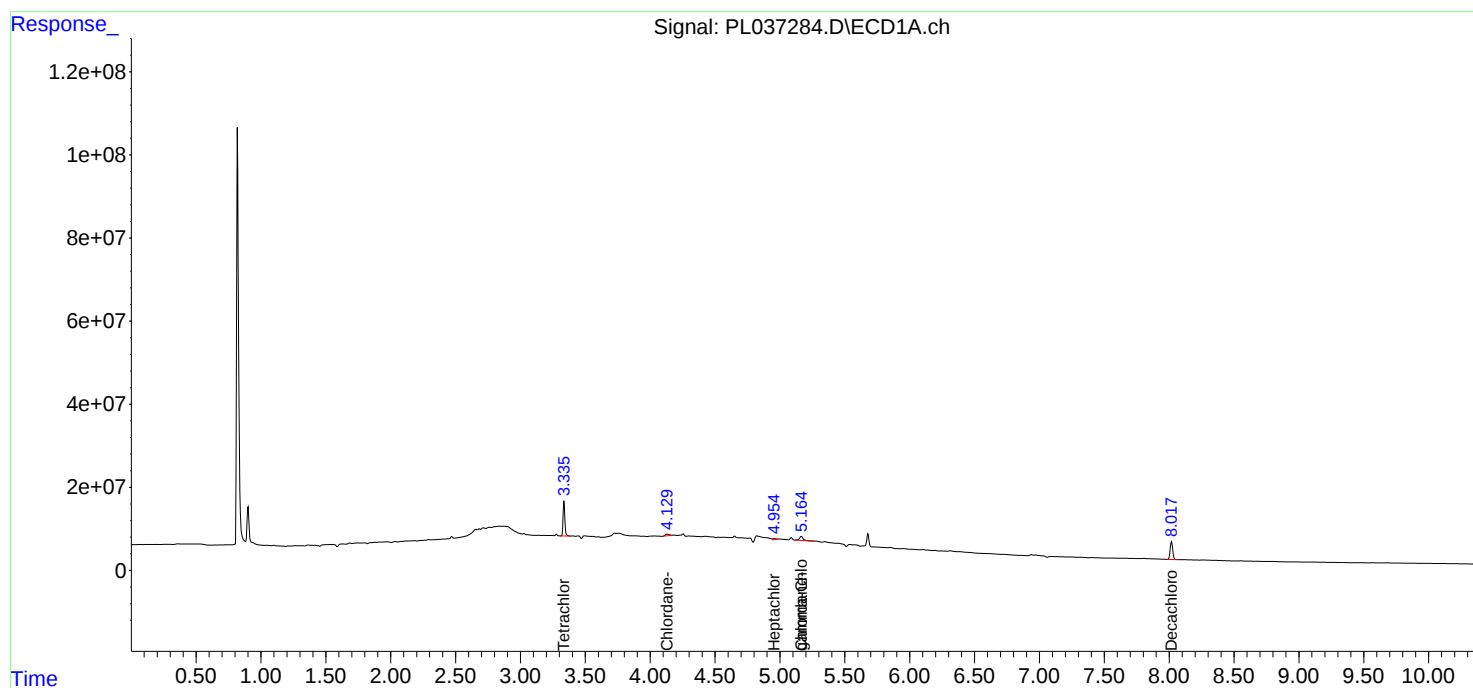


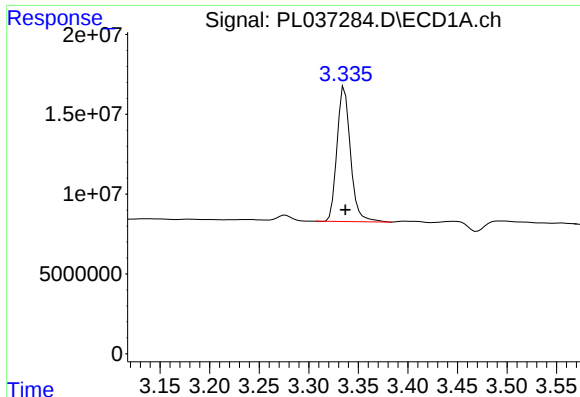

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 80043306
Conc: 10.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

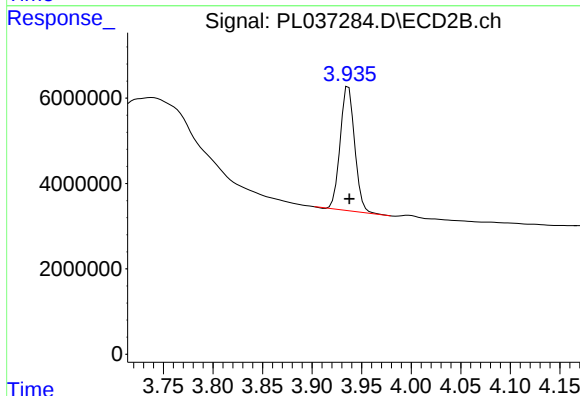


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 29365586
Conc: 10.61 ng/ml

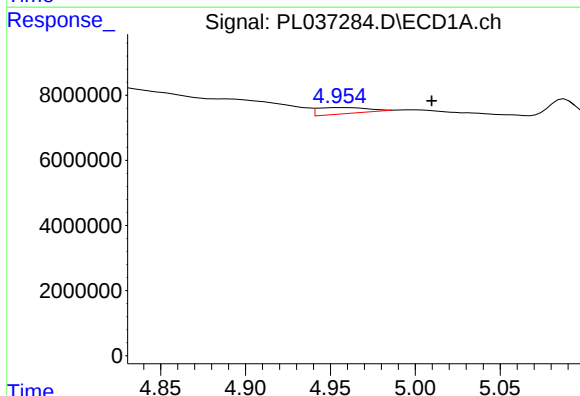


#8 Heptachlor epoxide

R.T.: 4.956 min
Delta R.T.: -0.053 min
Response: 3889540
Conc: 0.42 ng/ml

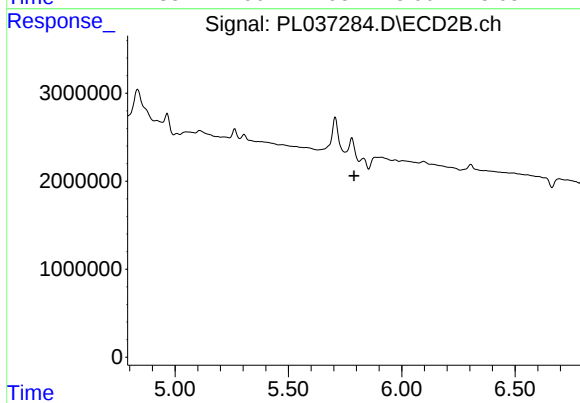

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.790 min
Response: 0
Conc: N.D.

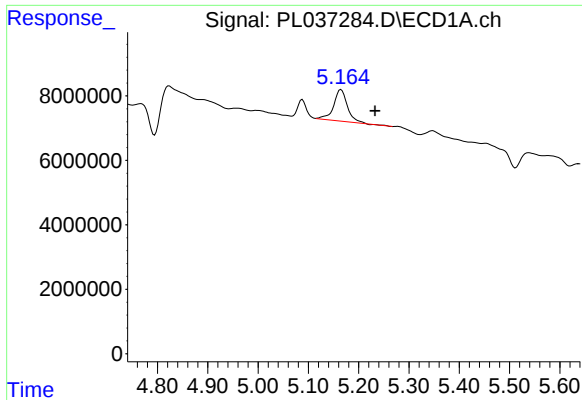

#10 gamma-Chlordane


R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 18789719
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

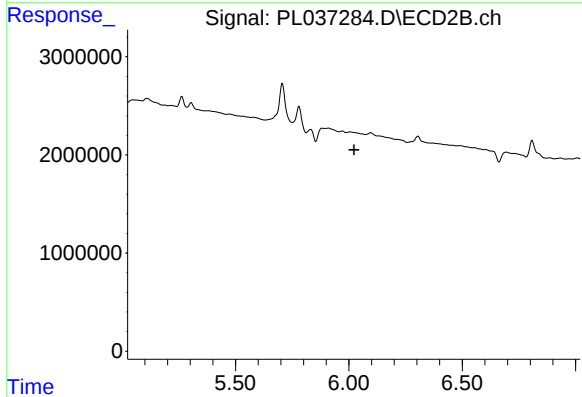


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

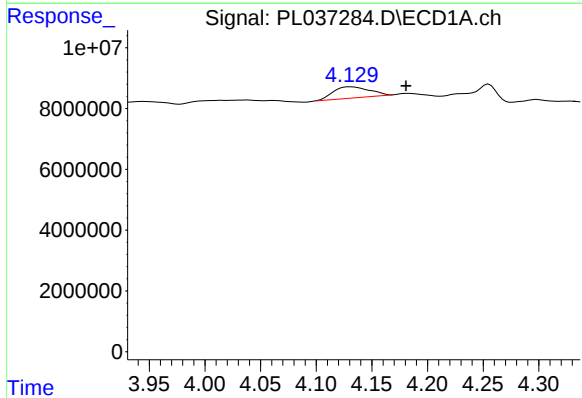


#23 Chlordane-1

R.T.: 4.132 min
Delta R.T.: -0.049 min
Response: 8386883
Conc: 27.31 ng/ml

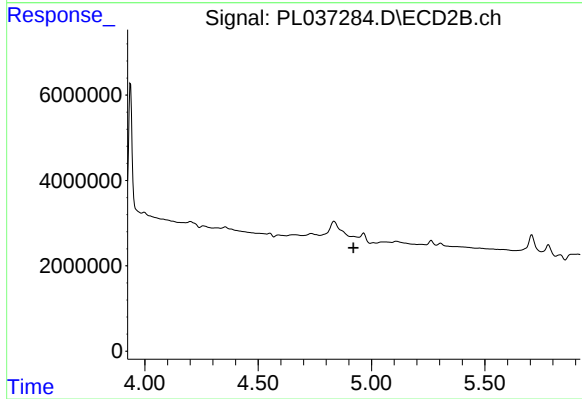

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

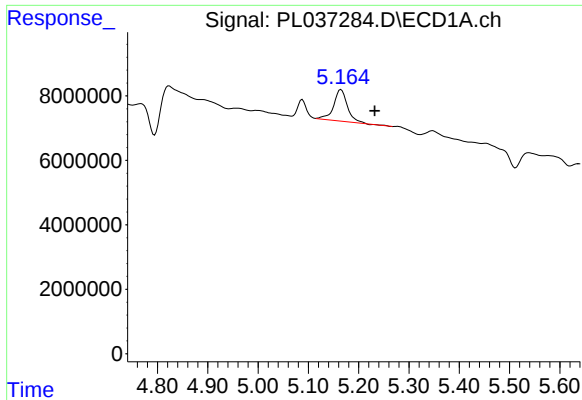

#25 Chlordane-3


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 18789719
Conc: 17.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

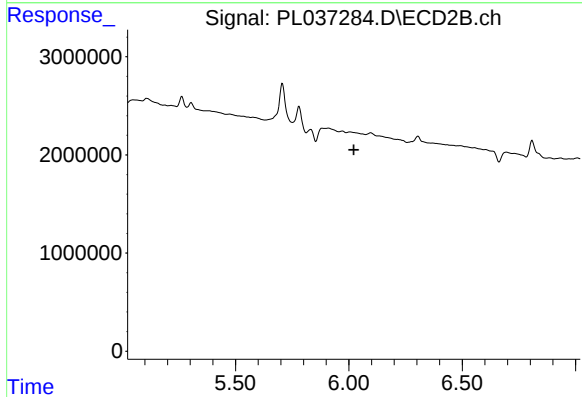


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

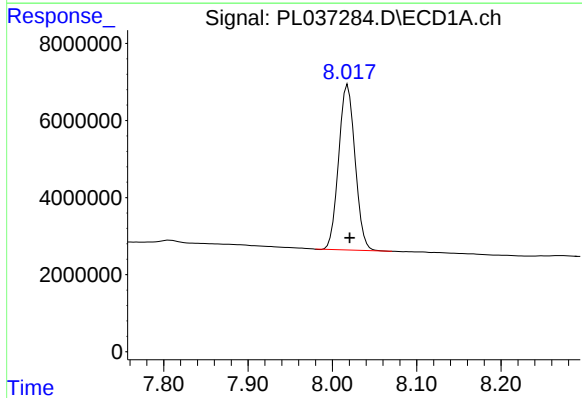

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.002 min
Response: 57983902
Conc: 9.61 ng/ml

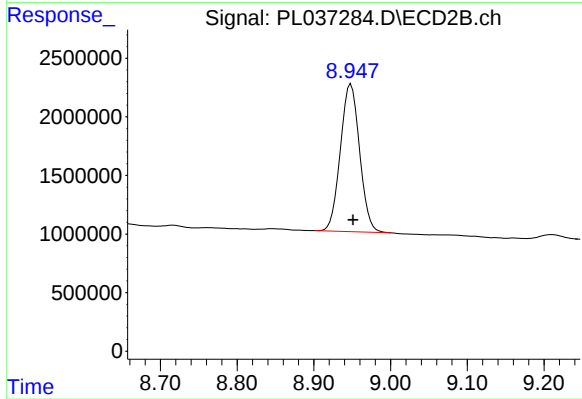

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 21982202
Conc: 11.08 ng/ml