

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 09:23
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 09:41:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	130.4E6	46424371	16.489	16.779
28)	SA Decachlor...	8.018	8.948	122.6E6	44469808	20.311	22.415
Target Compounds							
6)	B beta-BHC	4.256f	0.000	7956061	0	1.744	N.D. #
10)	B gamma-Chl...	5.165f	0.000	25533729	0	2.726	N.D. #
14)	MA Endrin	5.853	0.000	11963302	0	1.519	N.D. #
23)	Chlordane-1	4.116	0.000	20937410	0	69.348	N.D. #
25)	Chlordane-3	5.165	0.000	25533729	0	24.022	N.D. #
27)	Chlordane-5	5.853	0.000	11963302	0	92.288	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 09:23
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 09:41:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

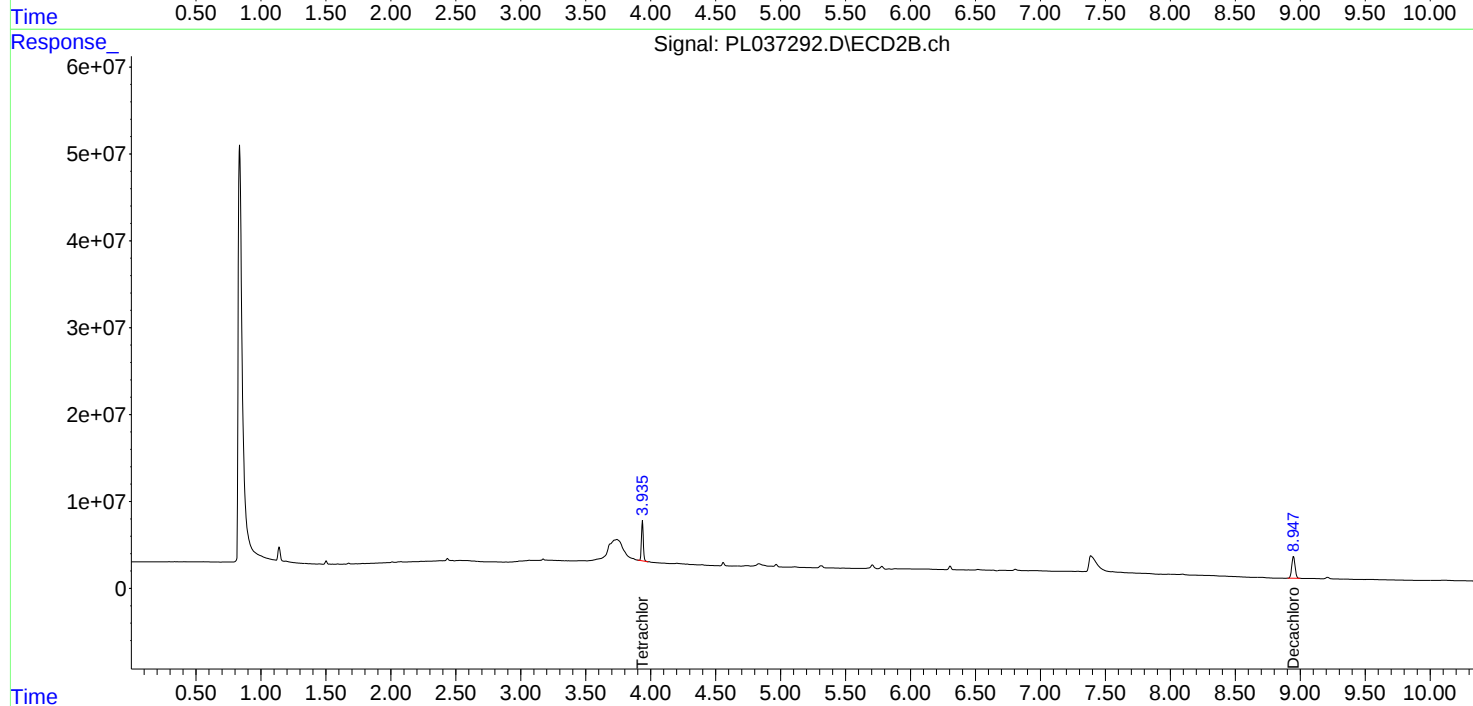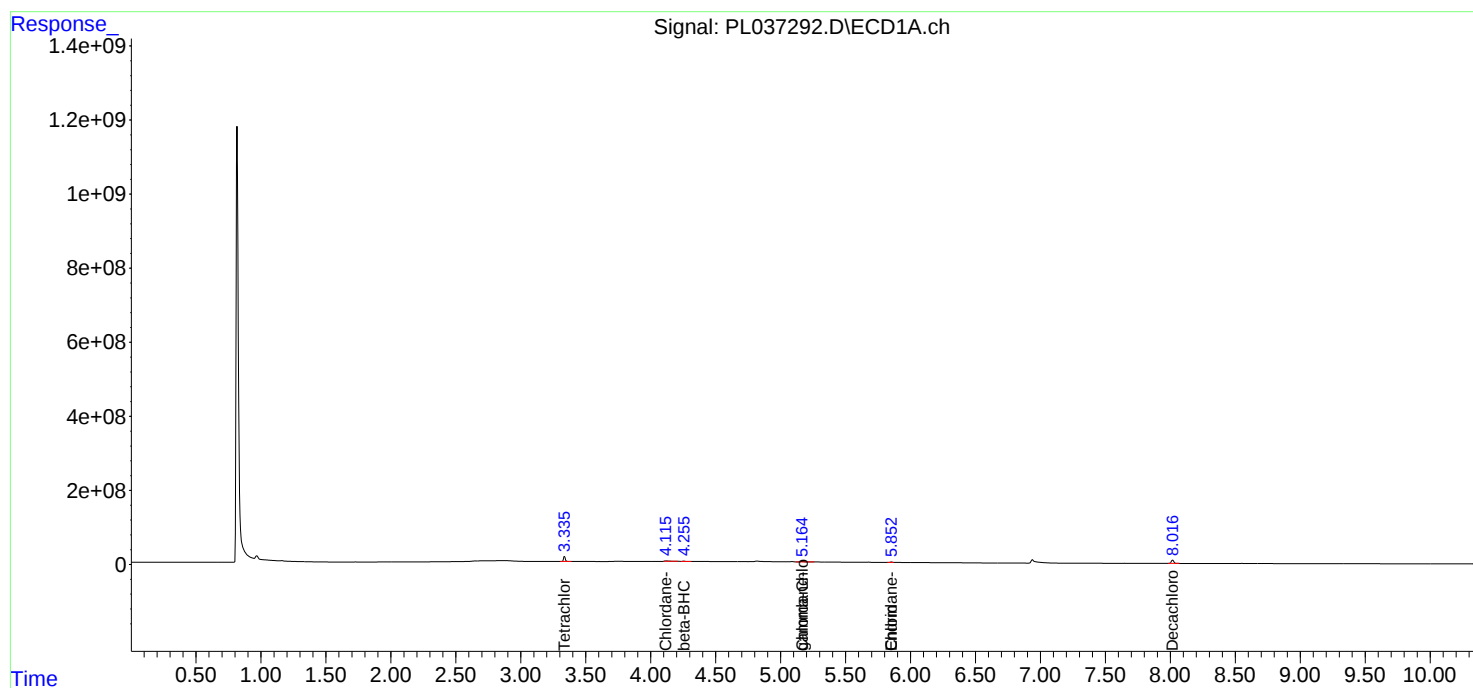


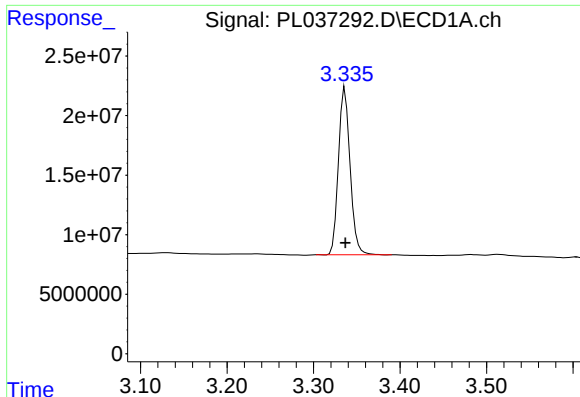

#1 Tetrachloro-m-xylene


R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 130436668
Conc: 16.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

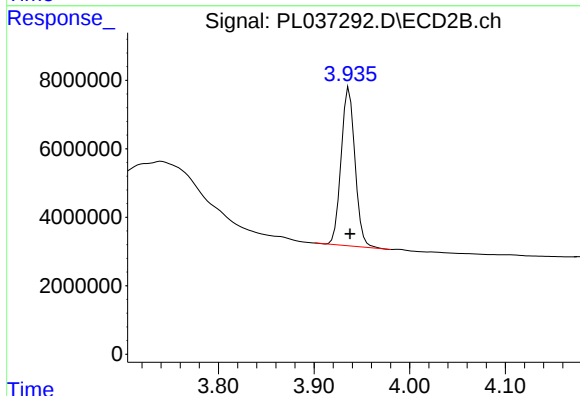


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 46424371
Conc: 16.78 ng/ml

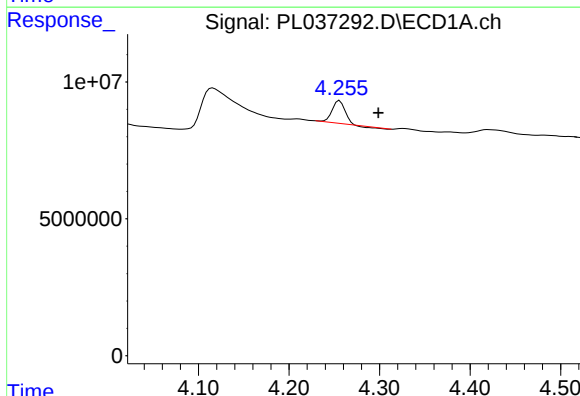


#6 beta-BHC

R.T.: 4.256 min
Delta R.T.: -0.043 min
Response: 7956061
Conc: 1.74 ng/ml

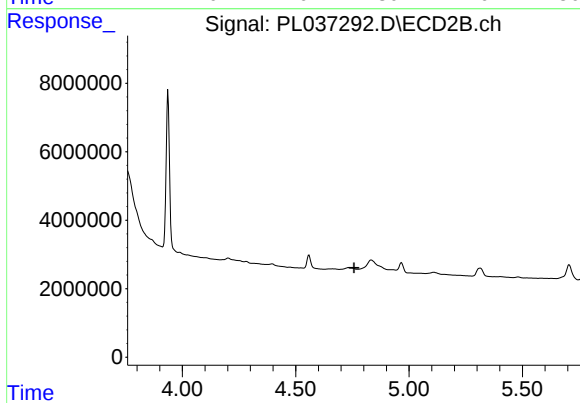

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

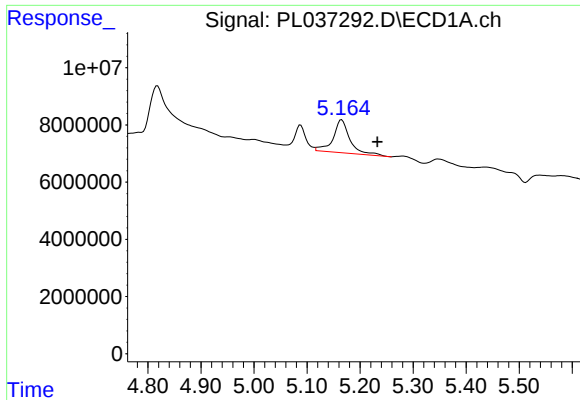

#10 gamma-Chlordane


R.T.: 5.165 min
Delta R.T.: -0.067 min
Response: 25533729
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

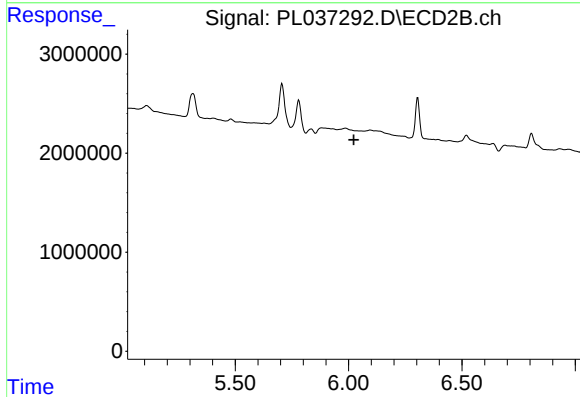


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

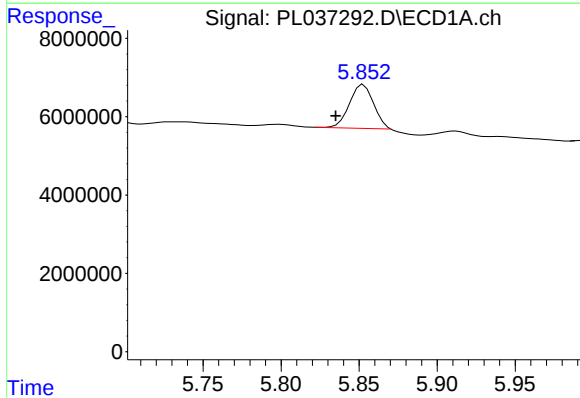


#14 Endrin

R.T.: 5.853 min
Delta R.T.: 0.018 min
Response: 11963302
Conc: 1.52 ng/ml

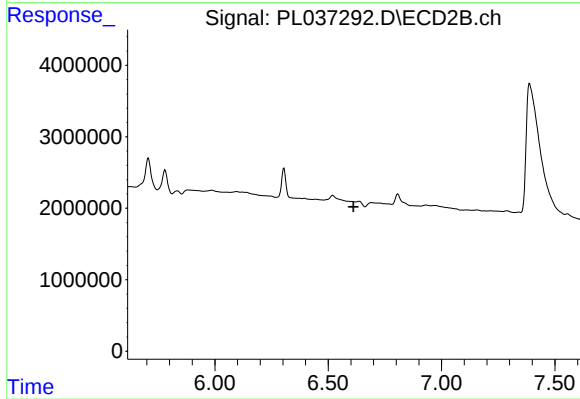

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

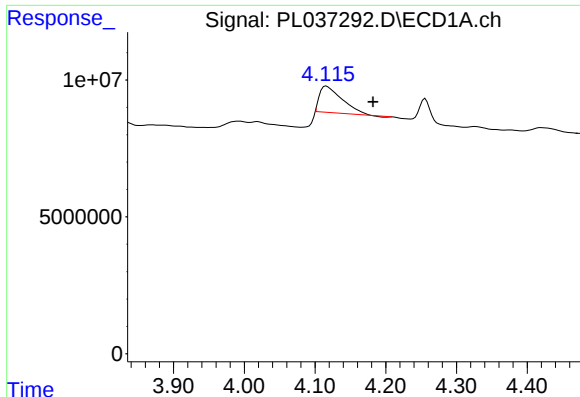

#23 Chlordane-1


R.T.: 4.116 min
Delta R.T.: -0.066 min
Response: 20937410
Conc: 69.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

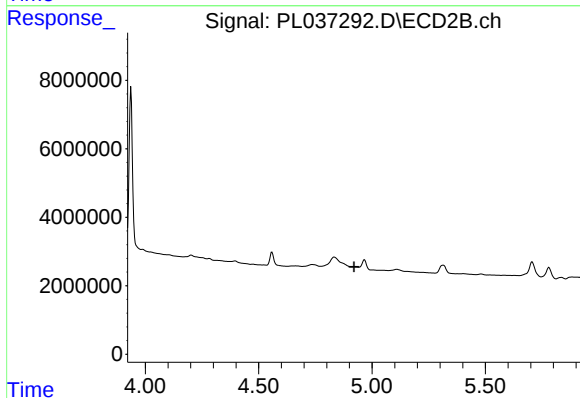


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

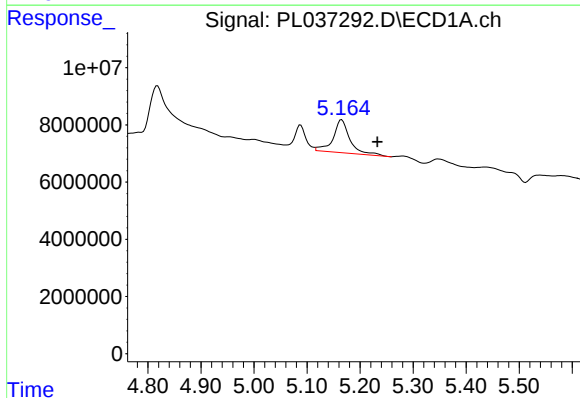


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: -0.068 min
Response: 25533729
Conc: 24.02 ng/ml

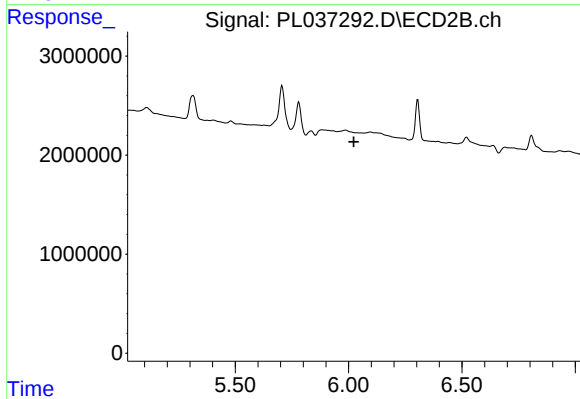

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

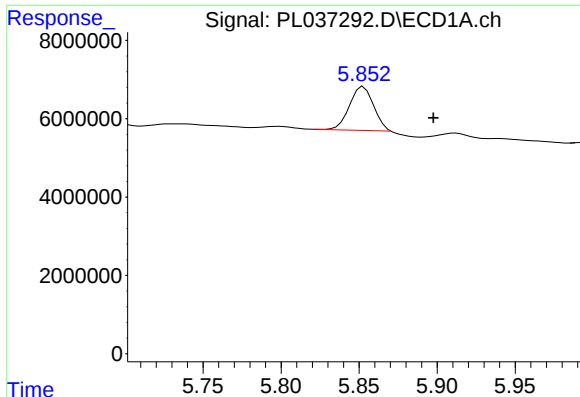

#27 Chlordane-5


R.T.: 5.853 min
Delta R.T.: -0.045 min
Response: 11963302
Conc: 92.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

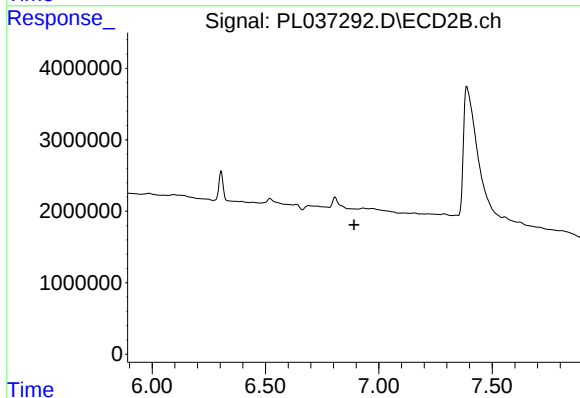


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

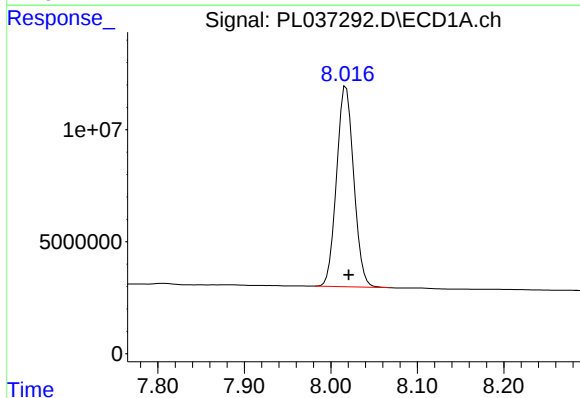

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: -0.003 min
Response: 122555938
Conc: 20.31 ng/ml

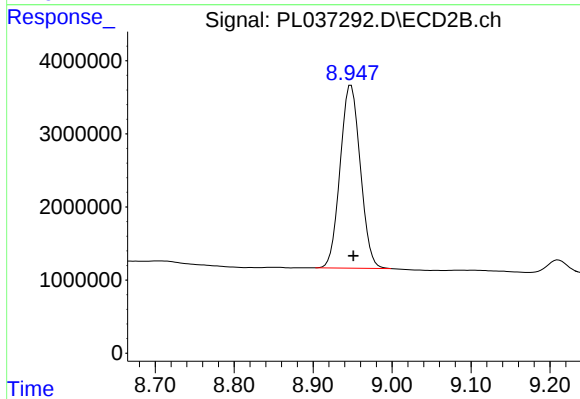

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 44469808
Conc: 22.41 ng/ml