

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 15:20
 Operator : UA\AJ
 Sample : J3245-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-061918-B

Manual Integrations
 APPROVED

ugo
 6/22/2018 1:59:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 03:48:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.936	102.1E6	33915441	12.905	12.258m
28)	SA Decachlor...	8.020	8.950	64200274	25230723	10.640	12.717
Target Compounds							
10)	B gamma-Chl...	5.231	6.020	12354045	4664423	1.319	1.656m#
11)	B alpha-Chl...	5.288	6.099	13482716	7240267	1.485	2.515 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 15:20
Operator : UA\AJ
Sample : J3245-11
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-02-061918-B


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 03:48:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

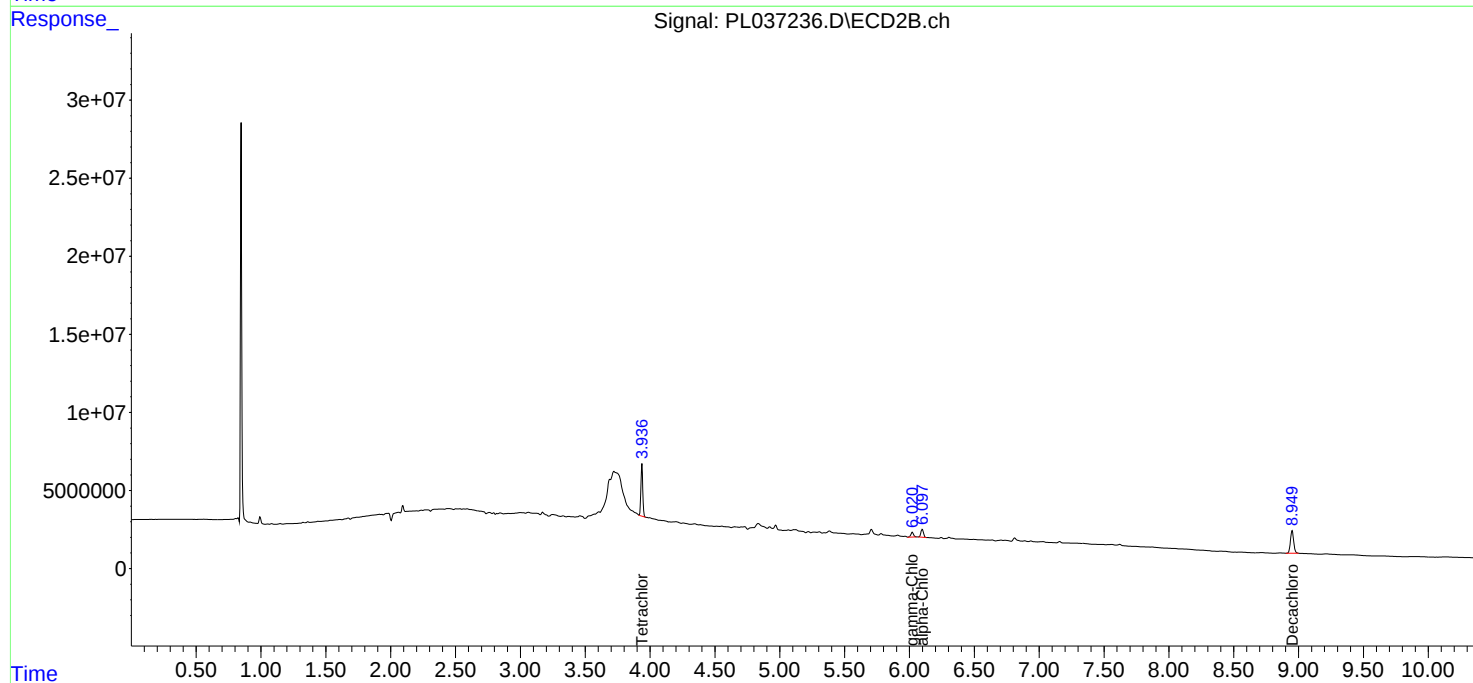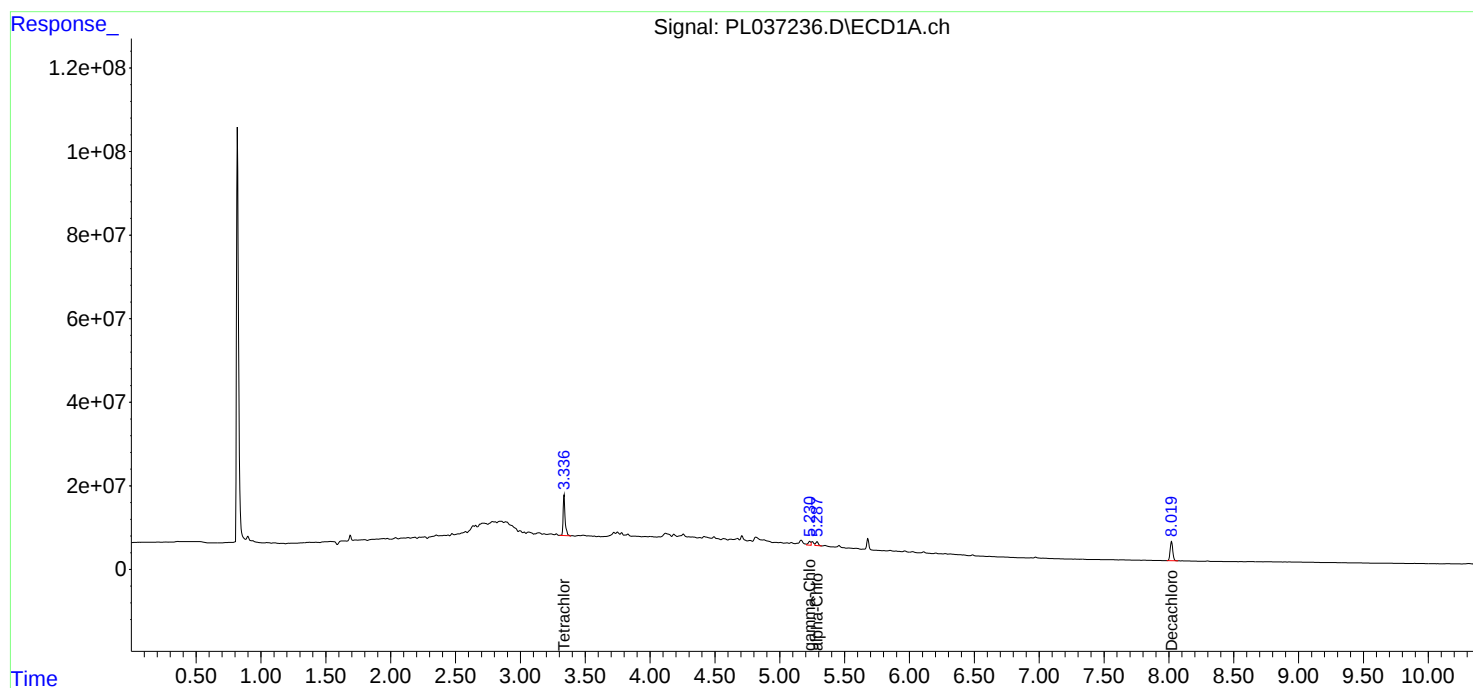

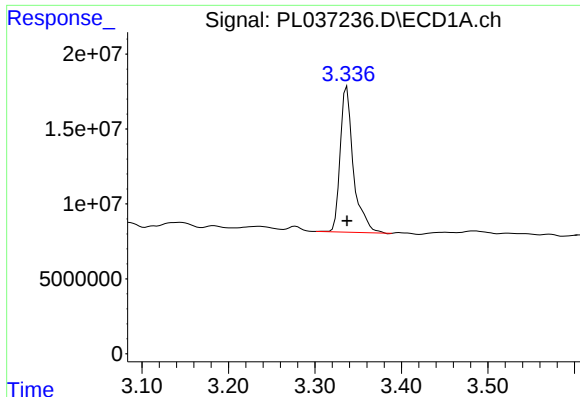


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 102083033
Conc: 12.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-061918-B


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:23 PM

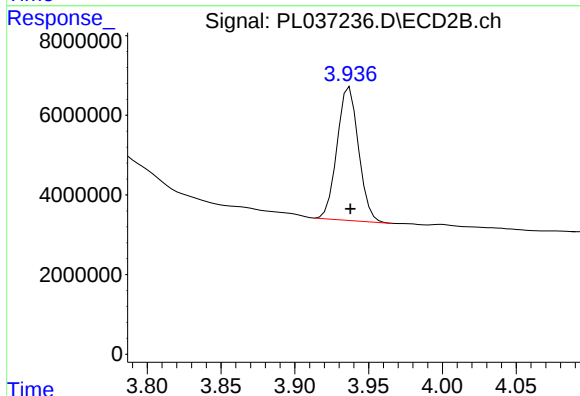


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 33915441
Conc: 12.26 ng/ml m

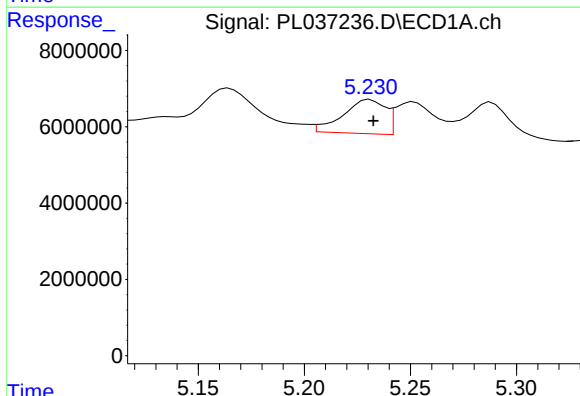


#10 gamma-Chlordane

R.T.: 5.231 min
Delta R.T.: -0.001 min
Response: 12354045
Conc: 1.32 ng/ml

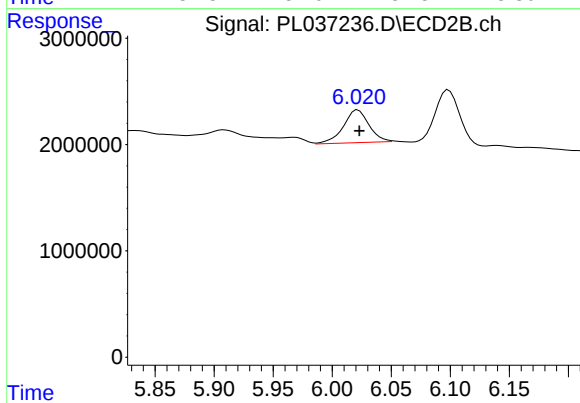

#10 gamma-Chlordane

R.T.: 6.020 min
Delta R.T.: -0.003 min
Response: 4664423
Conc: 1.66 ng/ml m

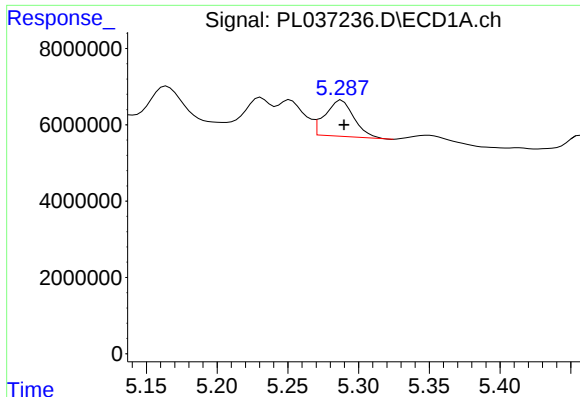


#11 alpha-Chlordane

R.T.: 5.288 min
Delta R.T.: -0.002 min
Response: 13482716
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-061918-B


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:23 PM

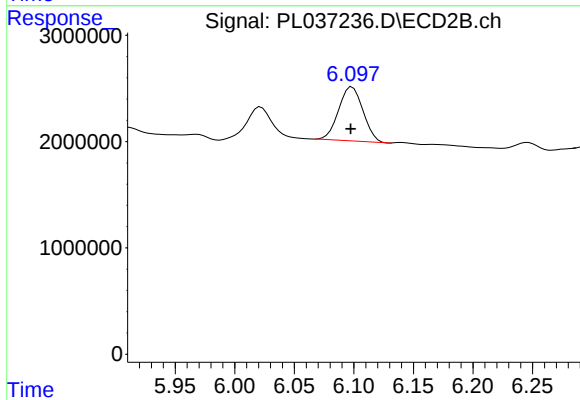


#11 alpha-Chlordane

R.T.: 6.099 min
Delta R.T.: 0.001 min
Response: 7240267
Conc: 2.52 ng/ml

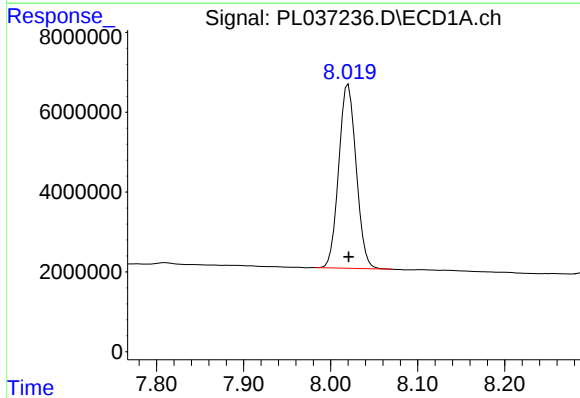

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 64200274
Conc: 10.64 ng/ml

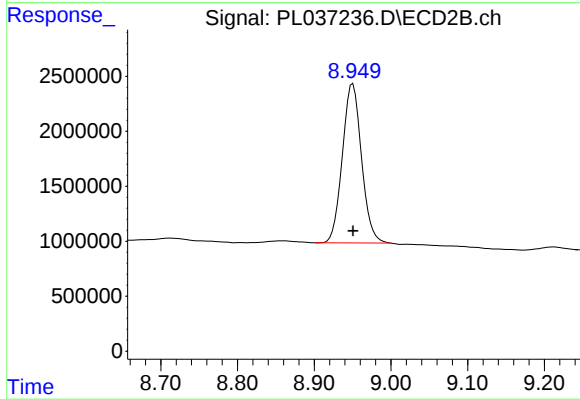

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 25230723
Conc: 12.72 ng/ml