

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2018 15:34
 Operator : UA\AJ
 Sample : J3245-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-061918-C

Manual Integrations
 APPROVED

ugo
 6/22/2018 1:59:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 03:48:33 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.337	3.937	90179501	30193945	11.400	10.913
28)	SA Decachlor...	8.020	8.951	62546636	24079316	10.366	12.137
Target Compounds							
10)	B gamma-Chl...	5.230	6.021	5611059	4013625	0.599m	1.425m#
11)	B alpha-Chl...	5.287	6.098	10442463	5513991	1.150m	1.916m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2018 15:34
Operator : UA\AJ
Sample : J3245-13
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-061918-C


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 03:48:33 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

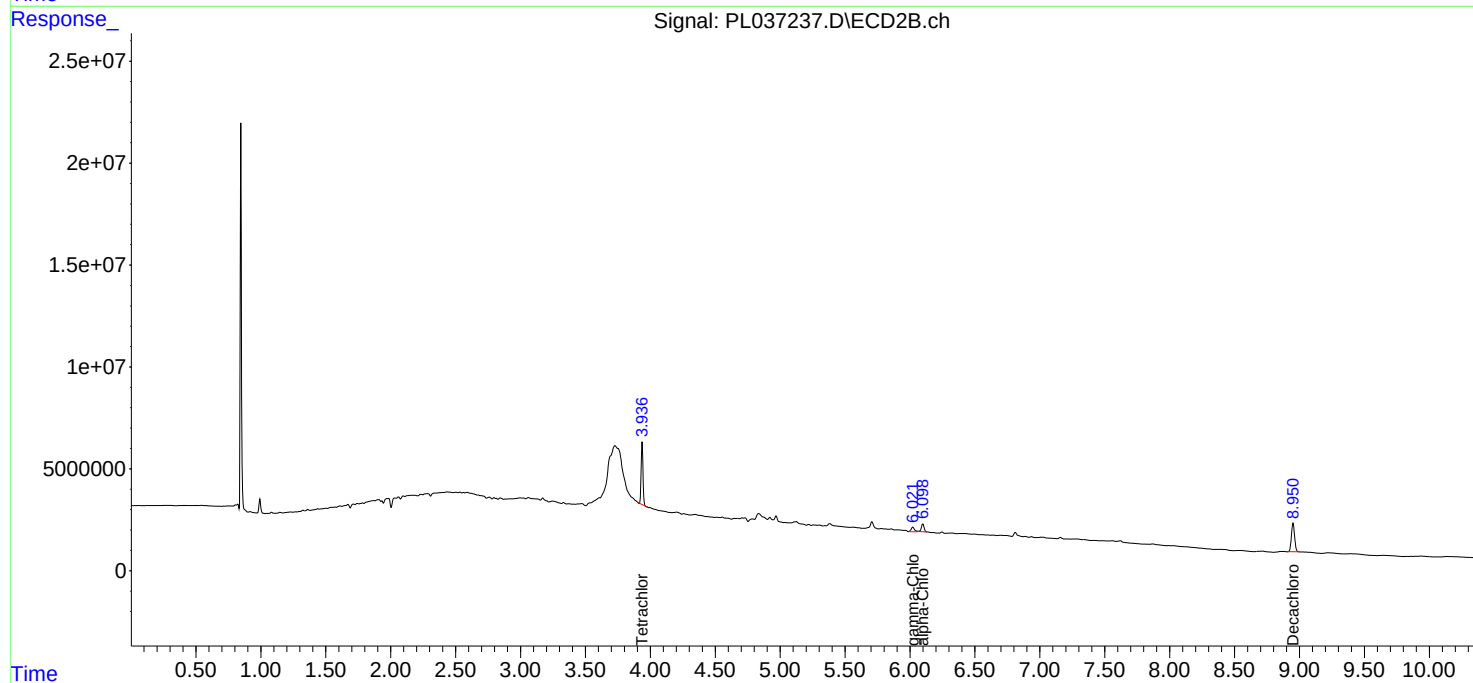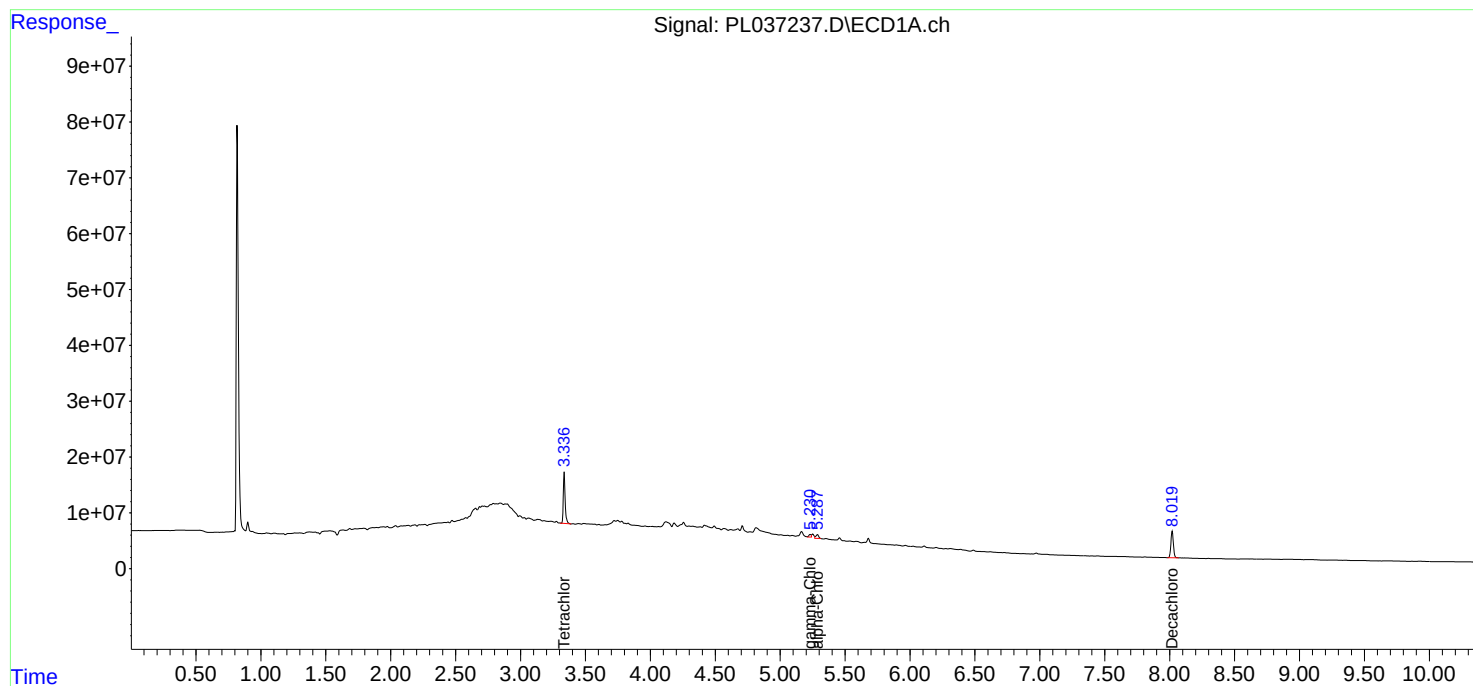

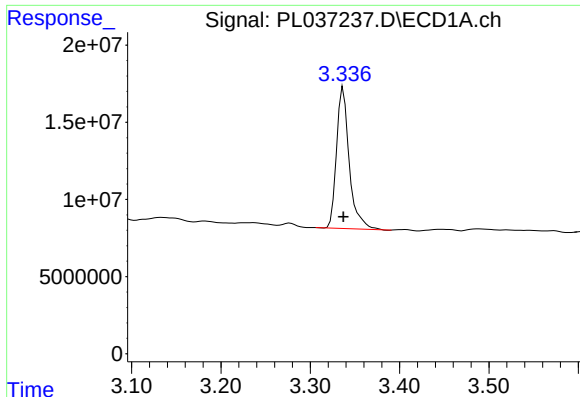


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: 0.000 min
Response: 90179501
Conc: 11.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-061918-C


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:11 PM

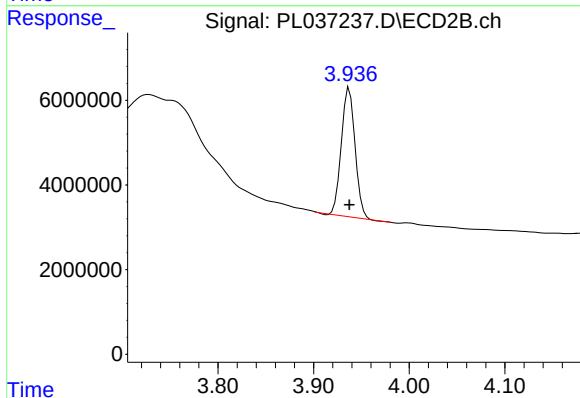


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 30193945
Conc: 10.91 ng/ml

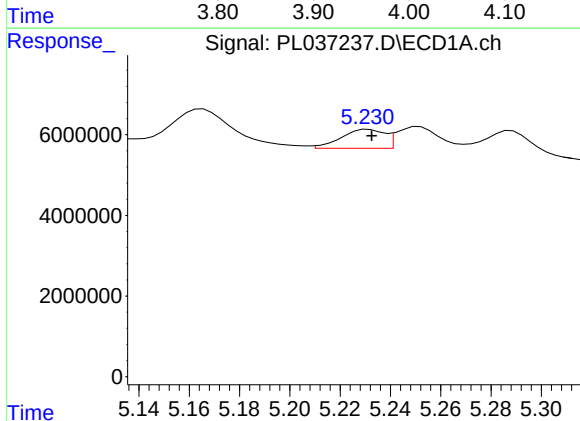


#10 gamma-Chlordane

R.T.: 5.230 min
Delta R.T.: -0.003 min
Response: 5611059
Conc: 0.60 ng/ml m

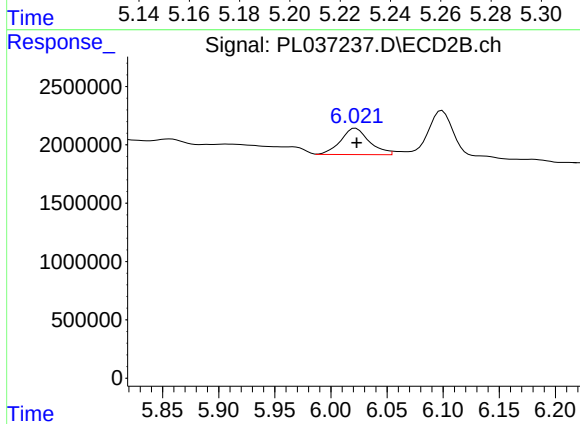

#10 gamma-Chlordane

R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 4013625
Conc: 1.43 ng/ml m

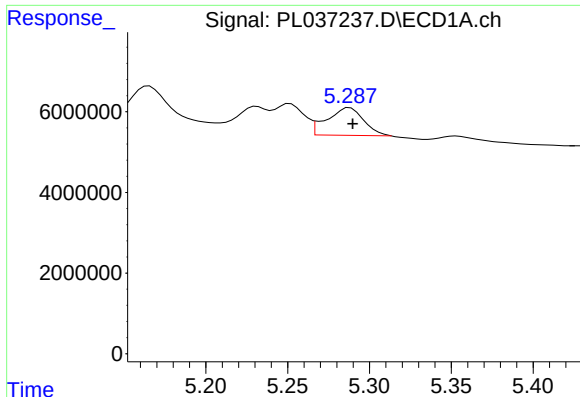


#11 alpha-Chlordane

R.T.: 5.287 min
Delta R.T.: -0.003 min
Response: 10442463
Conc: 1.15 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-061918-C


Manual Integrations
APPROVED

ugo
6/22/2018 1:59:11 PM

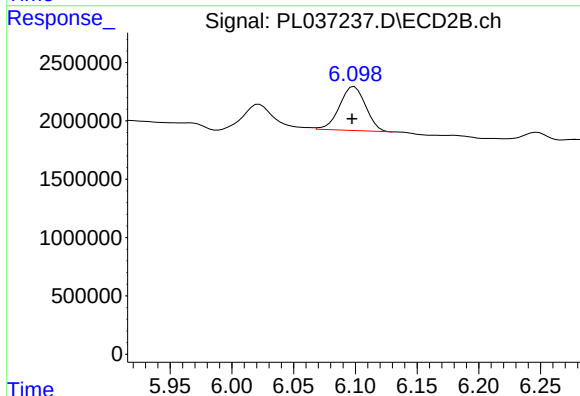


#11 alpha-Chlordane

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 5513991
Conc: 1.92 ng/ml m

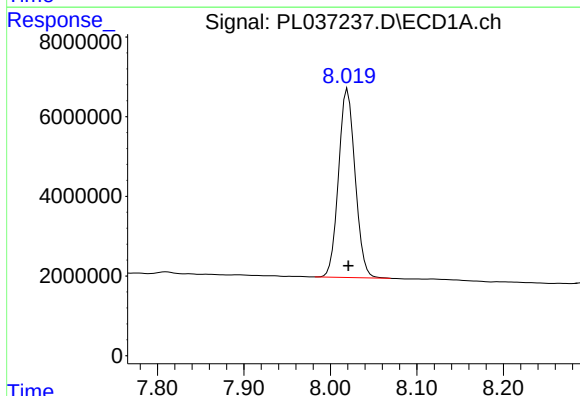

#28 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: 0.000 min
Response: 62546636
Conc: 10.37 ng/ml

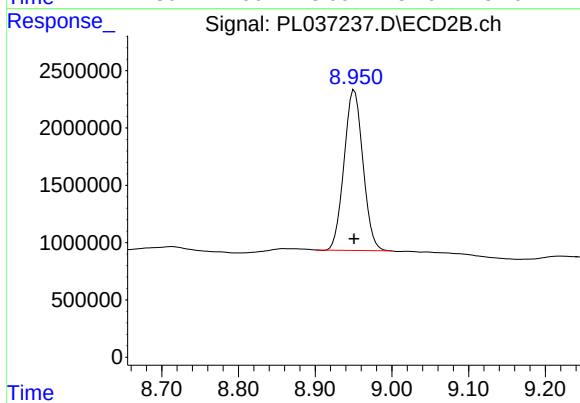

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 24079316
Conc: 12.14 ng/ml