

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 05:38
 Operator : UA\AJ
 Sample : J3603-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 26KV-TP-9

Manual Integrations
 APPROVED

ugo
 6/22/2018 1:58:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:47:37 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	69593094	24527527	8.798	8.865
28)	SA Decachlor...	8.019	8.948	52793031	19550154	8.749	9.854
Target Compounds							
12)	B 4,4'-DDE	5.457	6.248	12080583	4043377	1.368	1.589m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 05:38
Operator : UA\AJ
Sample : J3603-15
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:47:37 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

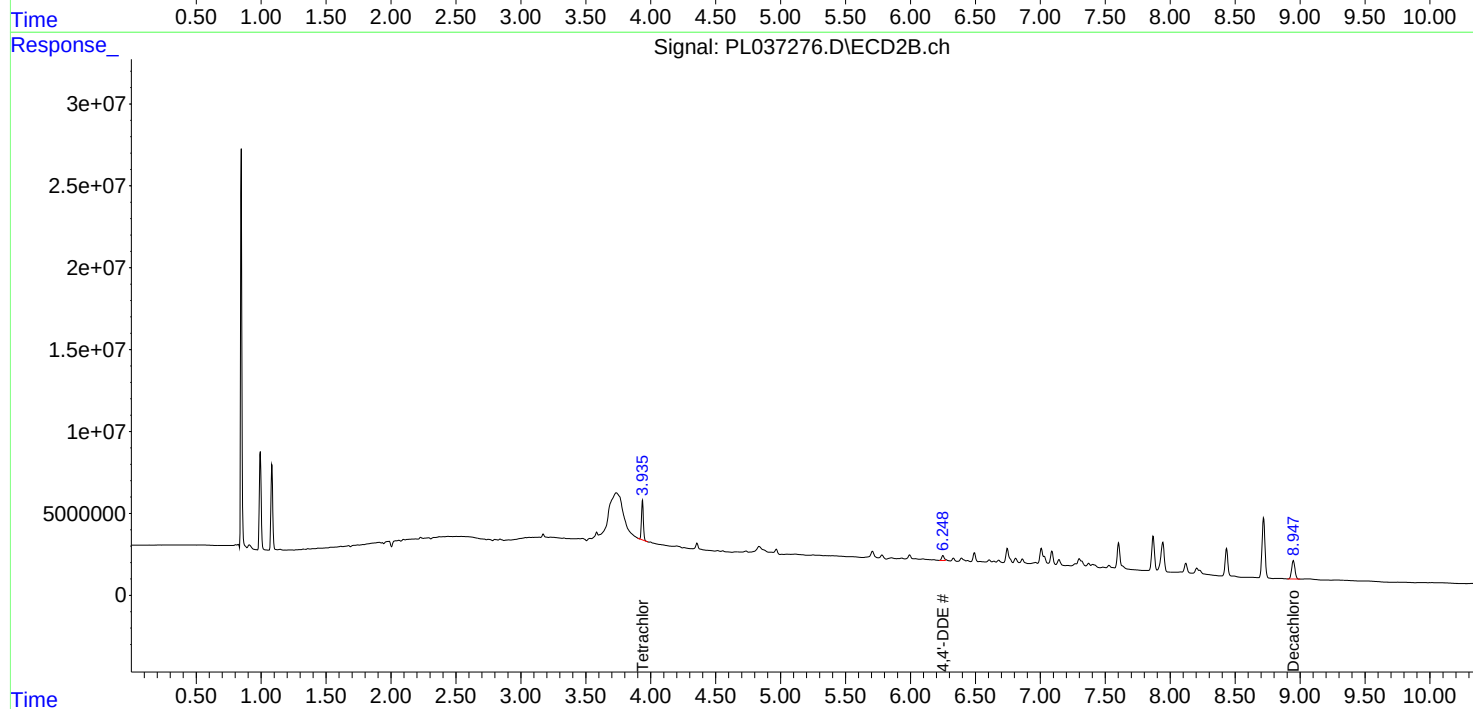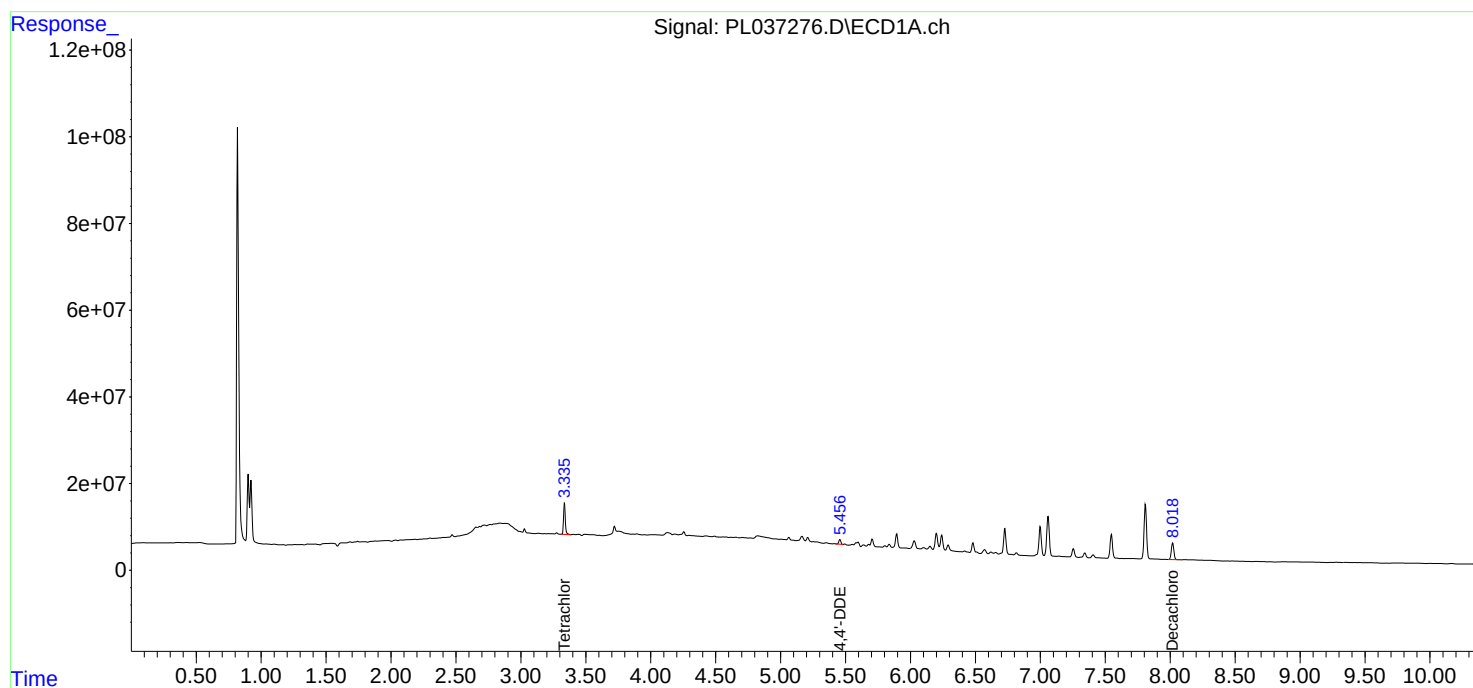

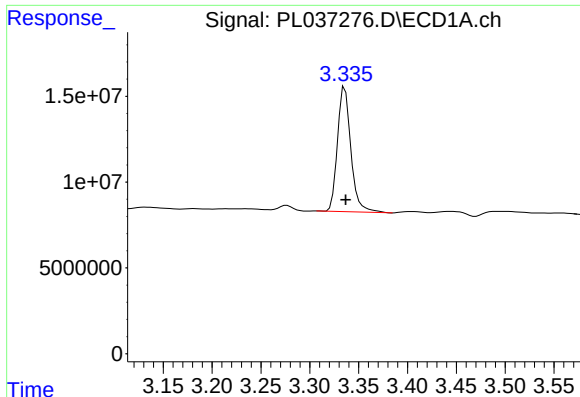


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 69593094
Conc: 8.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:27 PM

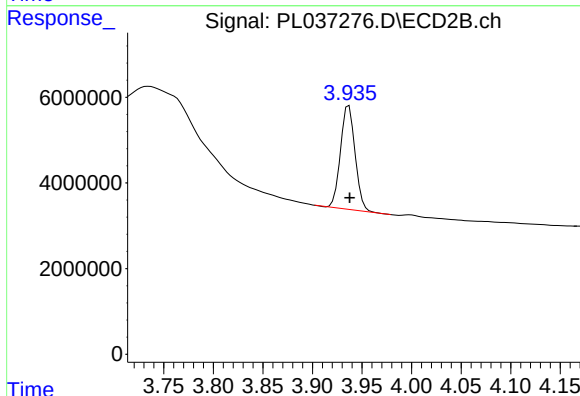


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 24527527
Conc: 8.87 ng/ml

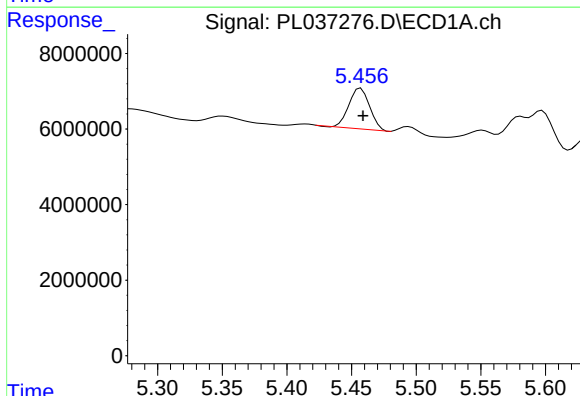


#12 4,4'-DDE

R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 12080583
Conc: 1.37 ng/ml

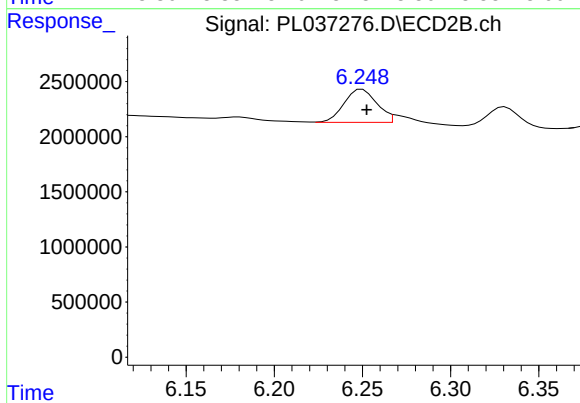

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.004 min
Response: 4043377
Conc: 1.59 ng/ml m

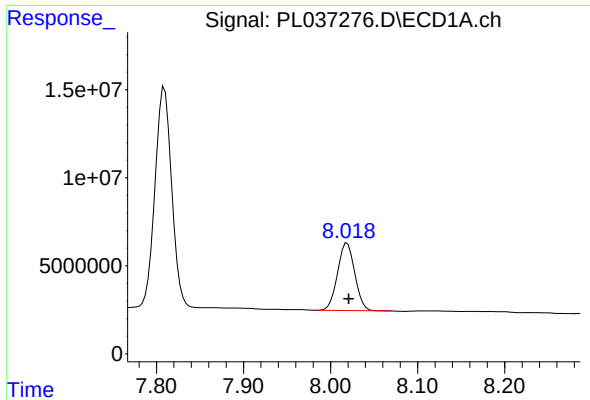

#28 Decachlorobiphenyl

R.T.: 8.019 min

Delta R.T.: -0.002 min


Response: 52793031

Conc: 8.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-9

Manual Integrations
APPROVED

ugo
6/22/2018 1:58:27 PM

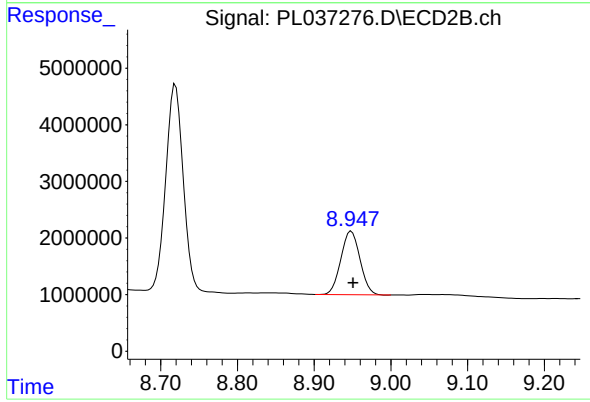

#28 Decachlorobiphenyl

R.T.: 8.948 min

Delta R.T.: -0.003 min

Response: 19550154

Conc: 9.85 ng/ml