

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 06:06
 Operator : UA\AJ
 Sample : J3603-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 26KV-TP-3

Manual Integrations
 APPROVED

ugo
 6/22/2018 1:58:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:47:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	76344553	26754315	9.651	9.670
28)	SA Decachlor...	8.017	8.948	47357511	18433156	7.848	9.291
Target Compounds							
12)	B 4,4'-DDE	5.455	6.249	19883458	6422315	2.251m	2.524

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 06:06
Operator : UA\AJ
Sample : J3603-05
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
26KV-TP-3


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:47:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

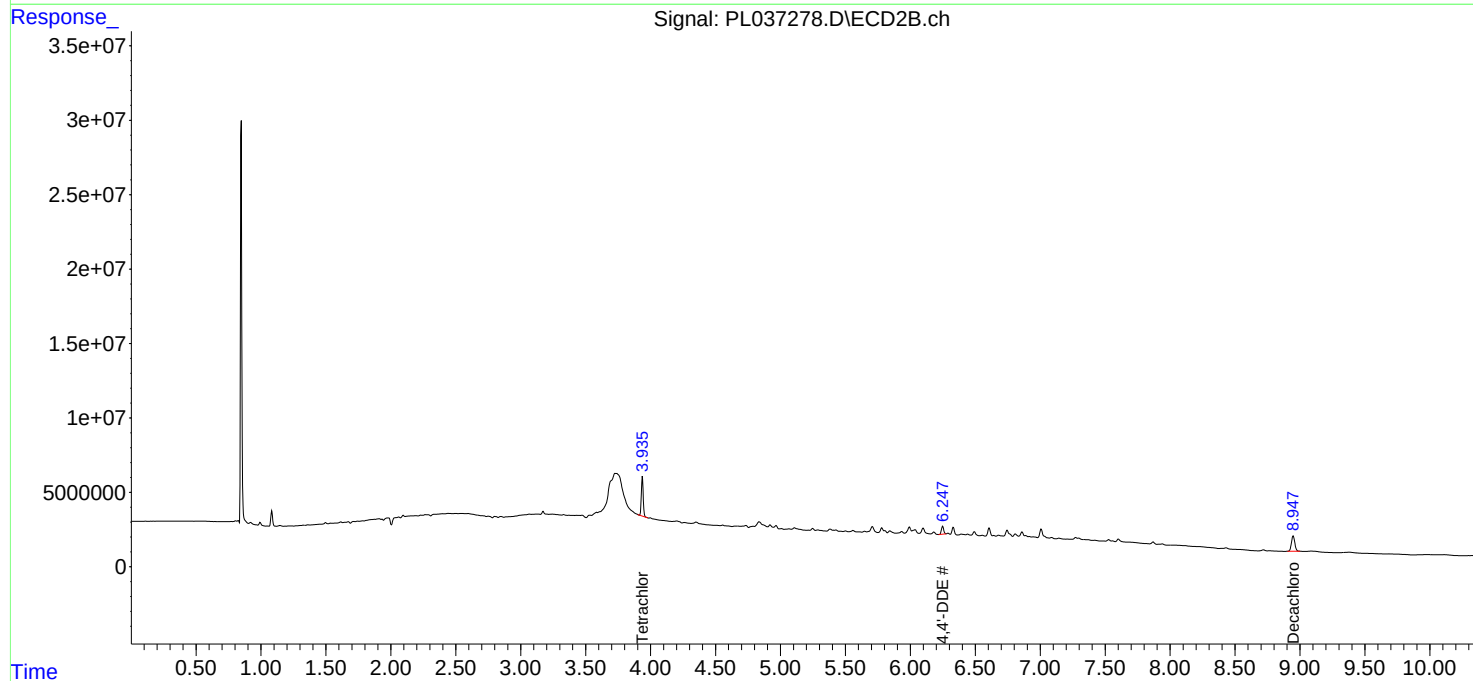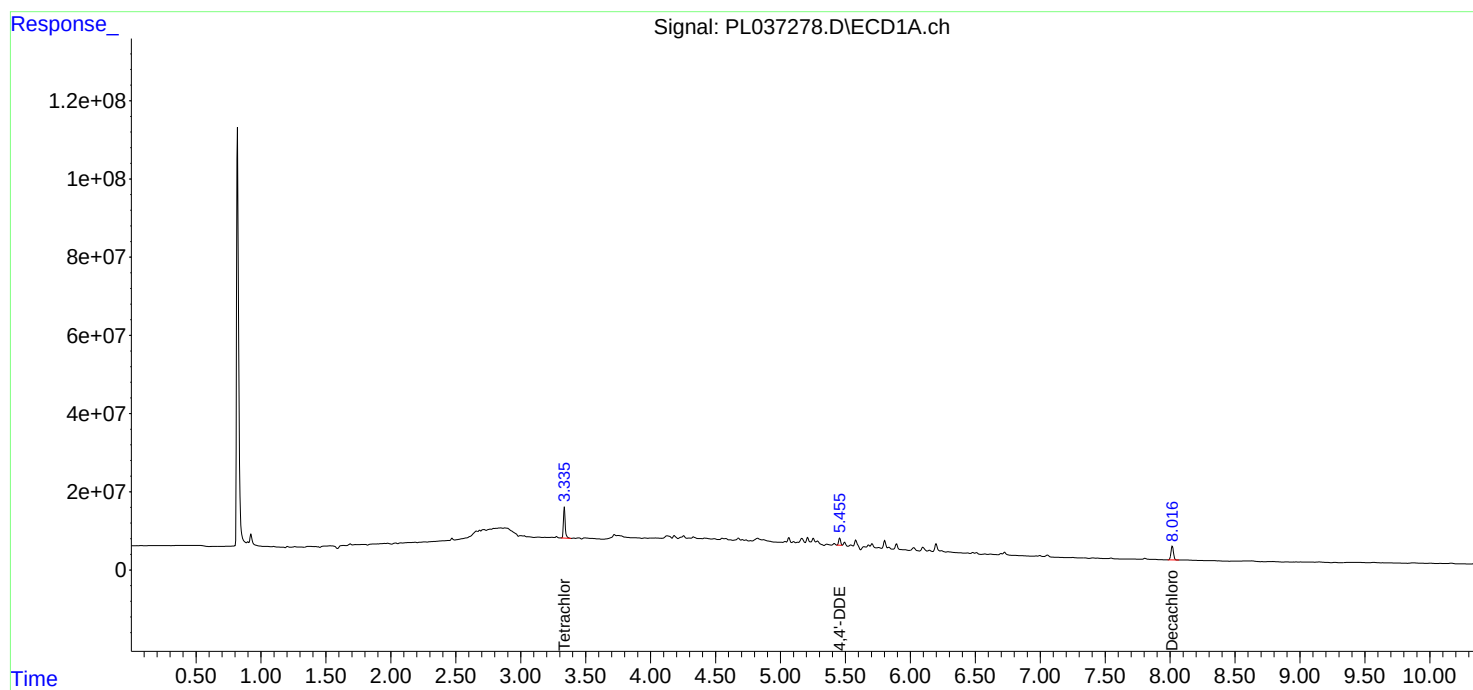

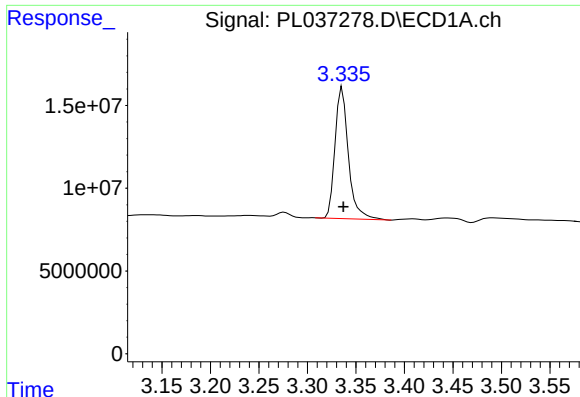


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.001 min
Response: 76344553
Conc: 9.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-3


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:23 PM

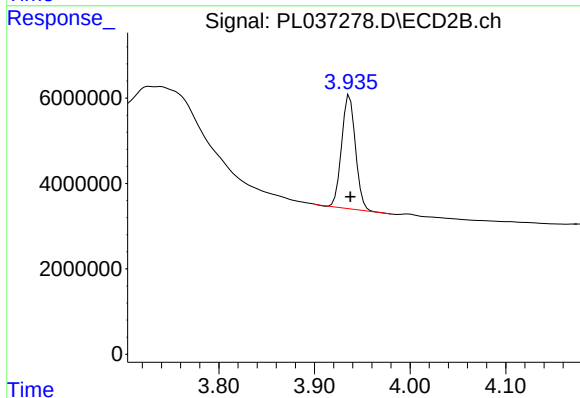


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 26754315
Conc: 9.67 ng/ml

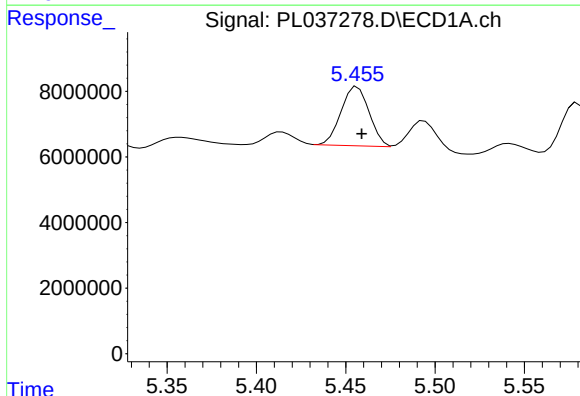


#12 4,4'-DDE

R.T.: 5.455 min
Delta R.T.: -0.004 min
Response: 19883458
Conc: 2.25 ng/ml m

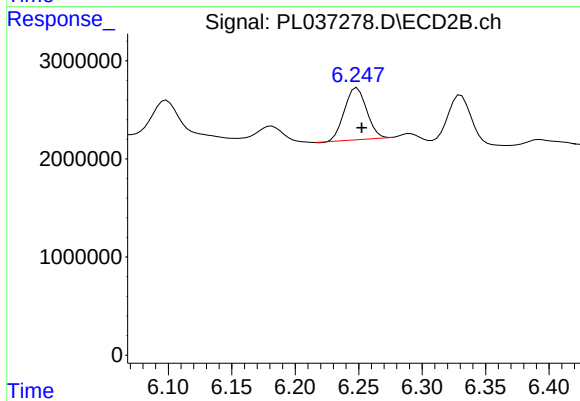

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.004 min
Response: 6422315
Conc: 2.52 ng/ml

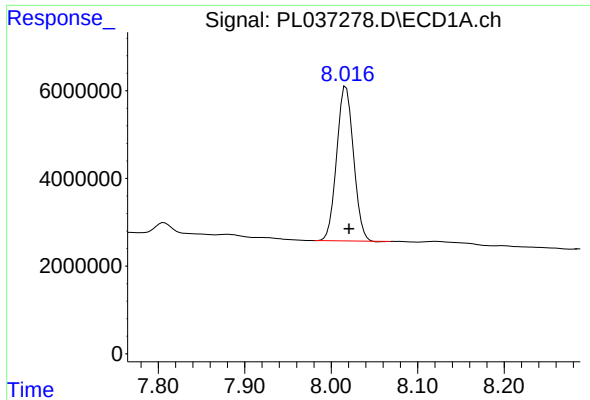


#28 Decachlorobiphenyl

R.T.: 8.017 min
Delta R.T.: -0.003 min
Response: 47357511
Conc: 7.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-3

Manual Integrations
APPROVED

ugo
6/22/2018 1:58:23 PM

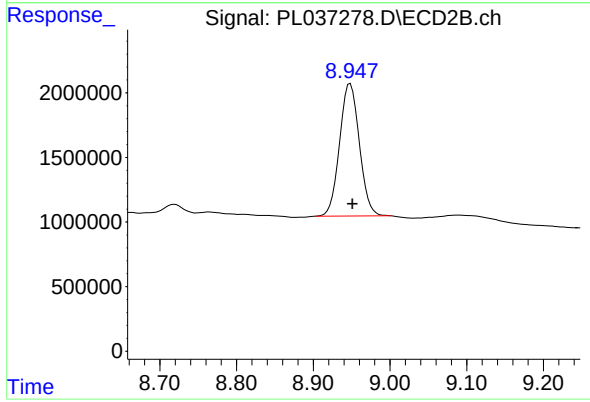

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 18433156
Conc: 9.29 ng/ml