

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
 Data File : PL037280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2018 06:34
 Operator : UA\AJ
 Sample : J3603-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 26KV-TP-1

Manual Integrations
 APPROVED

ugo
 6/22/2018 1:58:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 07:48:22 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	82445286	26174872	10.423	9.461
28)	SA Decachlor...	8.018	8.948	48939067	18889132	8.110	9.521
Target Compounds							
12)	B 4,4'-DDE	5.456	6.248	8422080	1899222	0.954	0.746m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062118\
Data File : PL037280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2018 06:34
Operator : UA\AJ
Sample : J3603-01
Misc :
ALS Vial : 61 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
26KV-TP-1


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 07:48:22 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

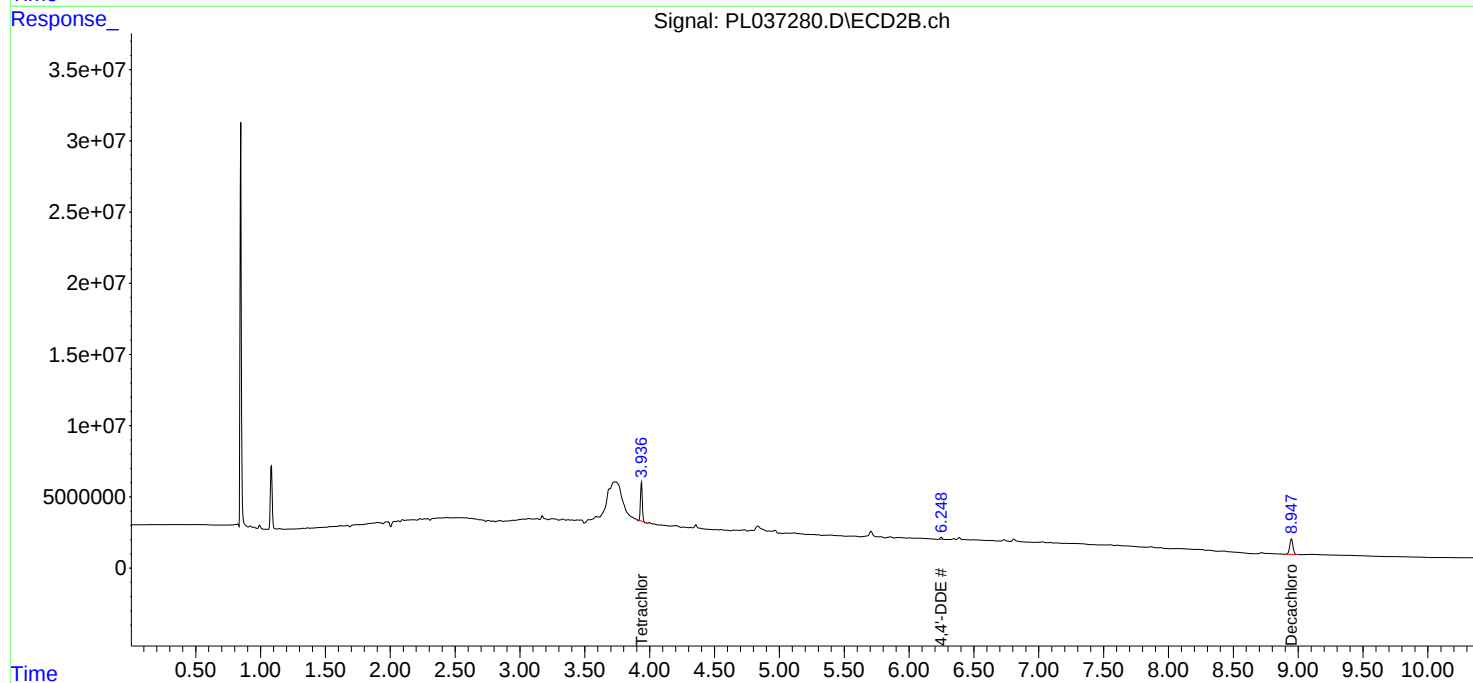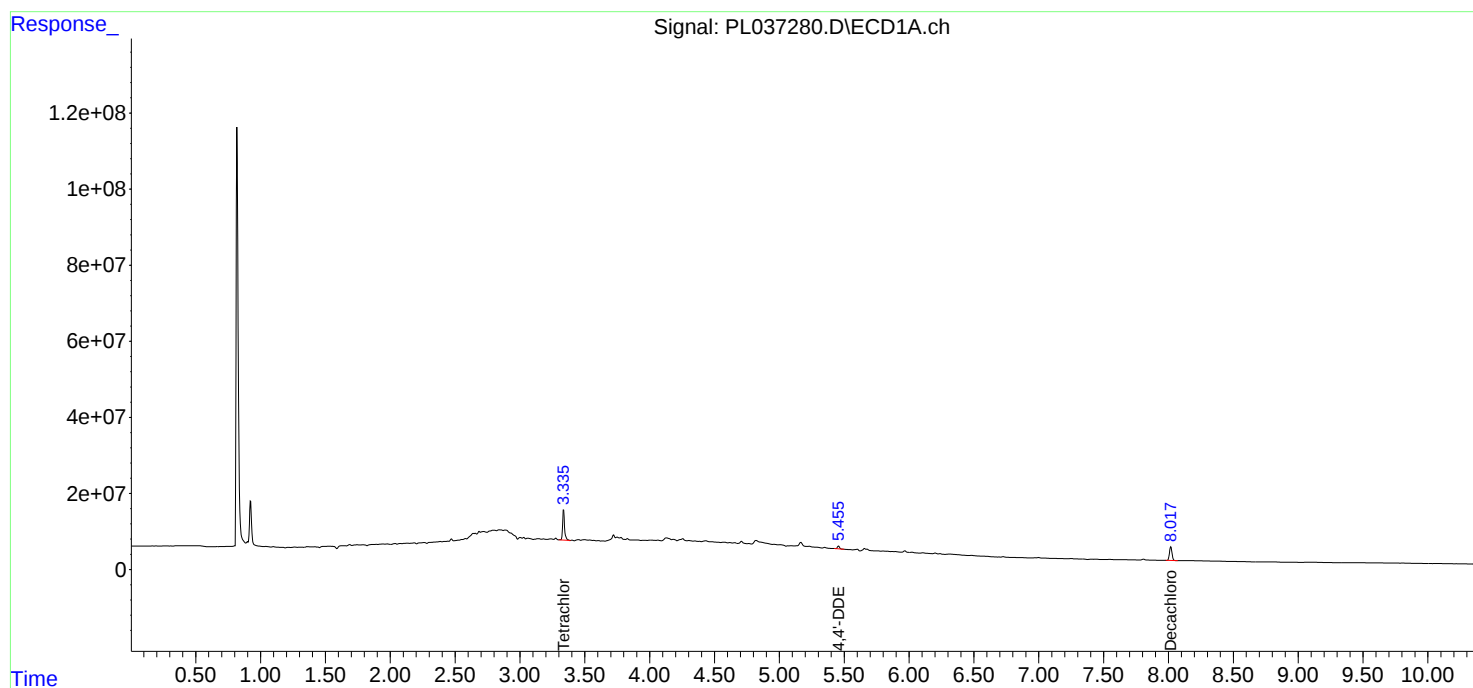

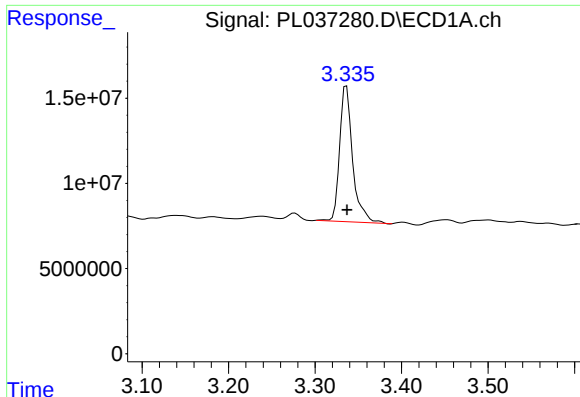


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 82445286
Conc: 10.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-1


Manual Integrations
APPROVED

ugo
6/22/2018 1:58:19 PM

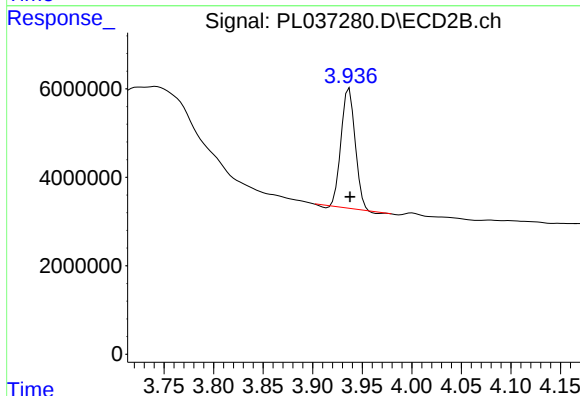


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 26174872
Conc: 9.46 ng/ml

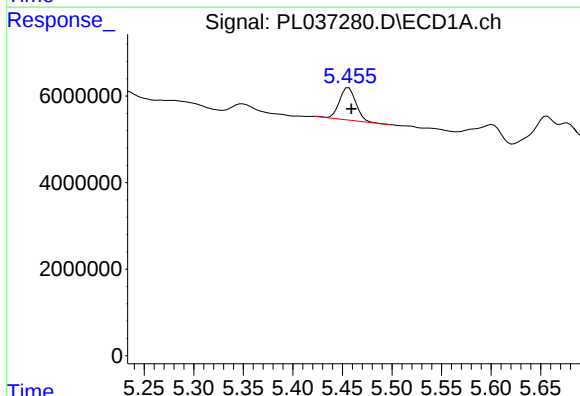


#12 4,4'-DDE

R.T.: 5.456 min
Delta R.T.: -0.003 min
Response: 8422080
Conc: 0.95 ng/ml

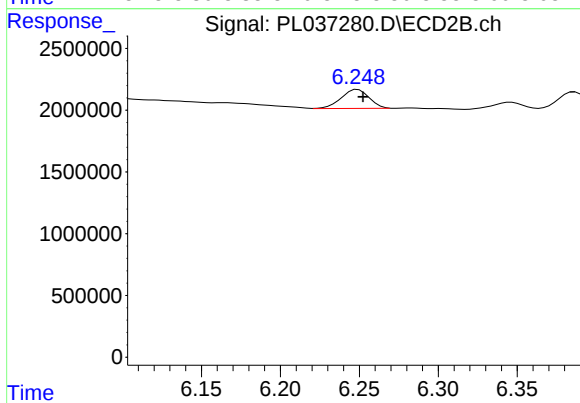

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.005 min
Response: 1899222
Conc: 0.75 ng/ml m

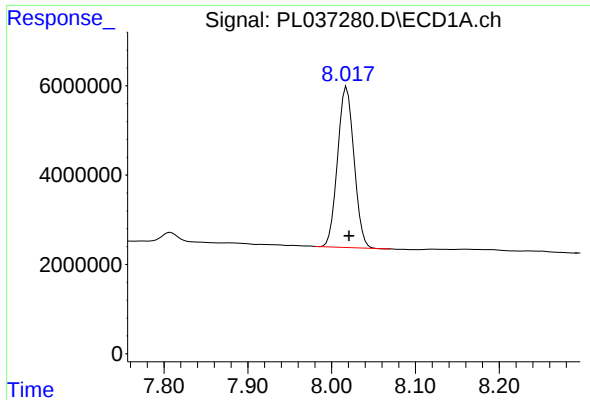

#28 Decachlorobiphenyl

R.T.: 8.018 min

Delta R.T.: -0.003 min


Response: 48939067

Conc: 8.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
26KV-TP-1

Manual Integrations
APPROVED

ugo
6/22/2018 1:58:19 PM

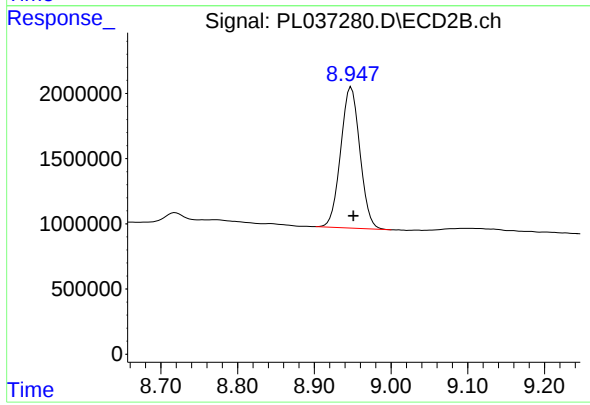

#28 Decachlorobiphenyl

R.T.: 8.948 min

Delta R.T.: -0.003 min

Response: 18889132

Conc: 9.52 ng/ml