

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070222\
 Data File : PL076214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2022 10:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:49:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.630	14656066	37058243	19.378	19.539
28)	SA Decachlor...	11.631	10.370	14214793	33787235	22.589	21.999
Target Compounds							
7)	B delta-BHC	0.000	6.395	0	563707	N.D.	0.250 #
8)	B Heptachlo...	8.121	7.055	873961	282767	1.098	0.147 #
11)	B alpha-Chl...	0.000	7.379f	0	346229	N.D.	0.181 #
13)	MA Dieldrin	0.000	7.742	0	259061	N.D.	0.144 #
14)	MA Endrin	0.000	8.056f	0	560611	N.D.	0.369 #
15)	B Endosulfa...	9.300	0.000	295256	0	0.465	N.D. #
17)	MA 4,4'-DDT	0.000	8.453	0	142454	N.D.	0.096 #
21)	B Endrin ke...	10.182f	0.000	2839075	0	3.939	N.D. #
26)	Chlordane-4	0.000	7.379f	0	346229	N.D.	1.837 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070222\
Data File : PL076214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2022 10:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:49:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

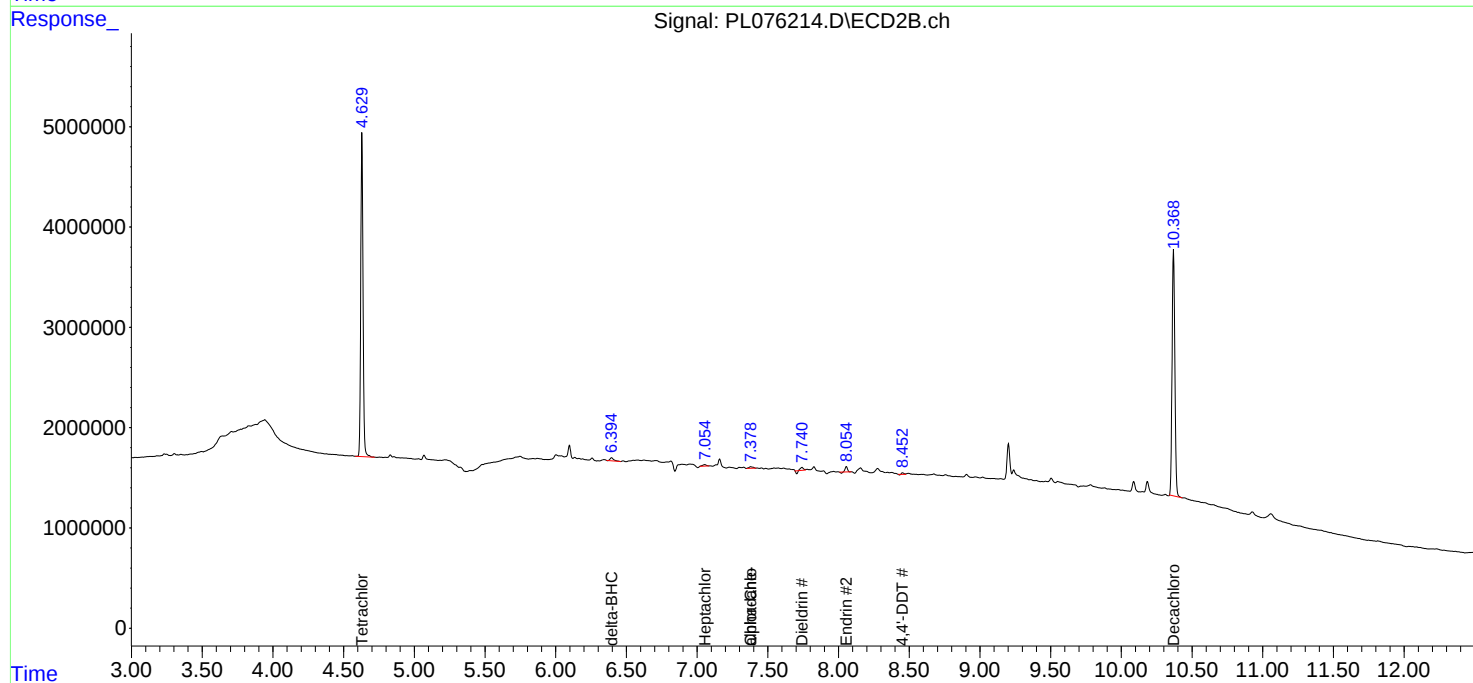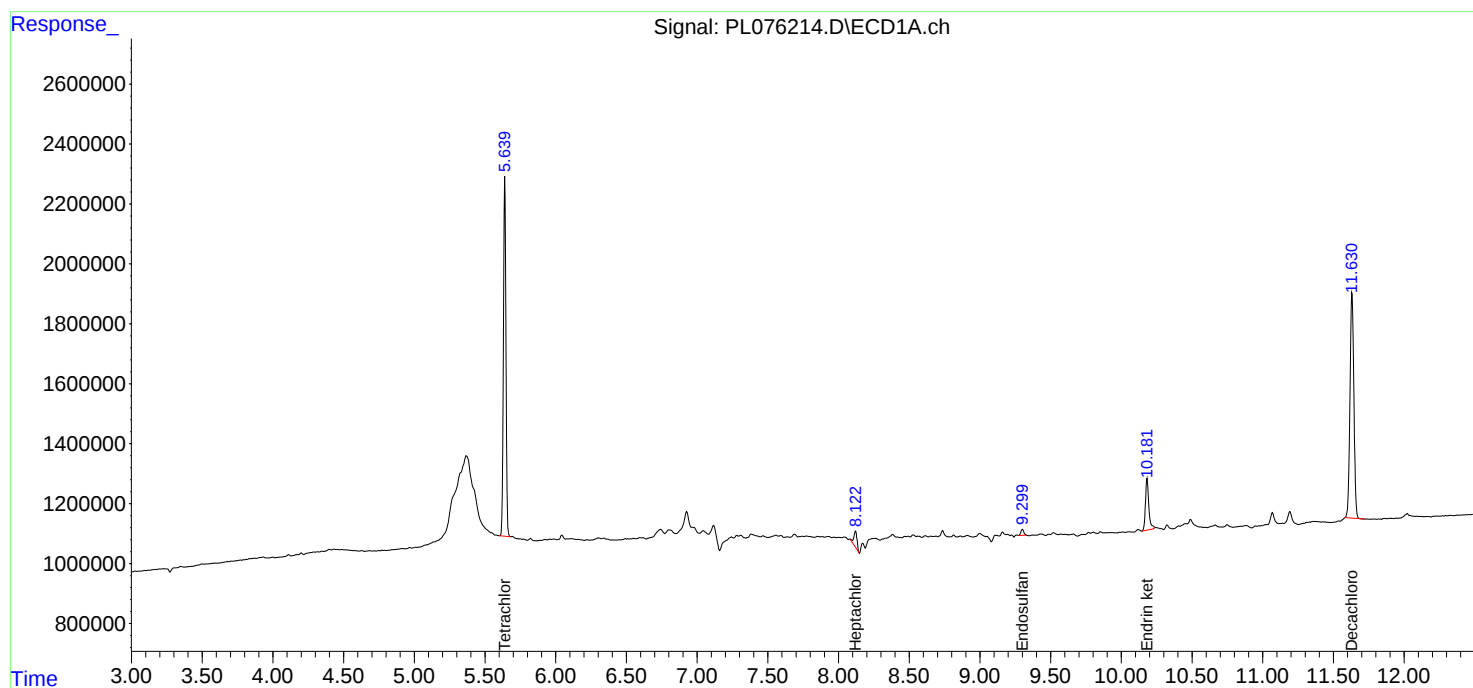


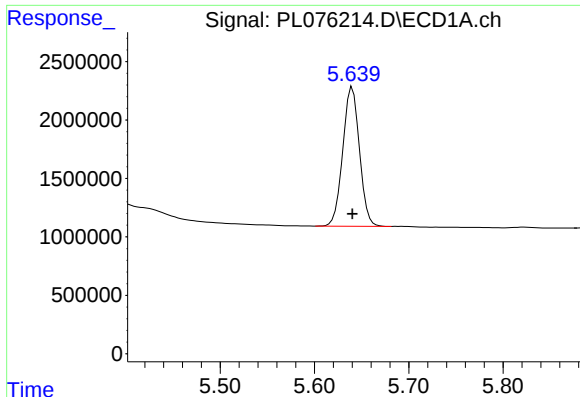

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 14656066
Conc: 19.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

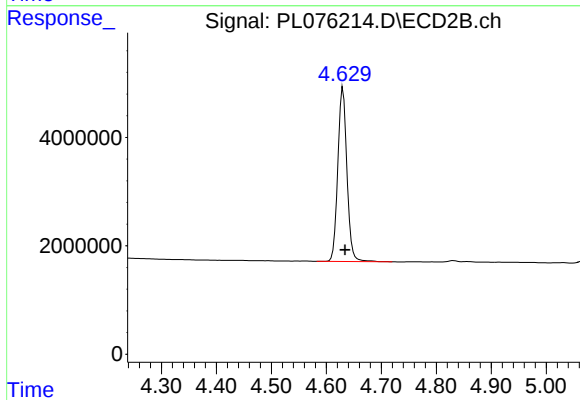


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: -0.004 min
Response: 37058243
Conc: 19.54 ng/ml

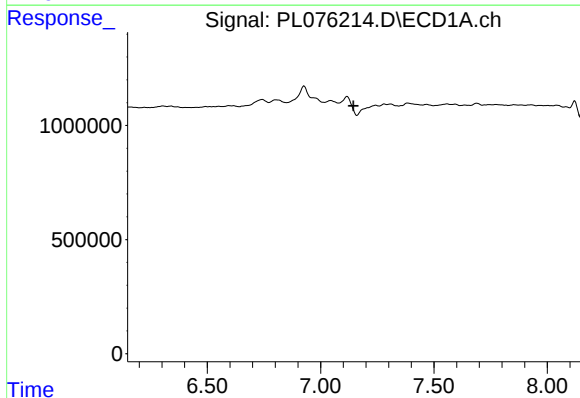


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

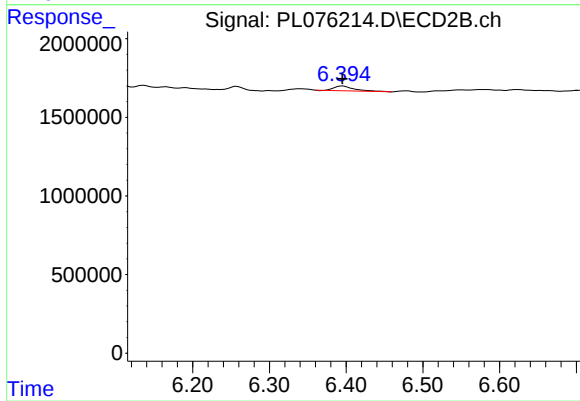

#7 delta-BHC


R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 563707
Conc: 0.25 ng/ml

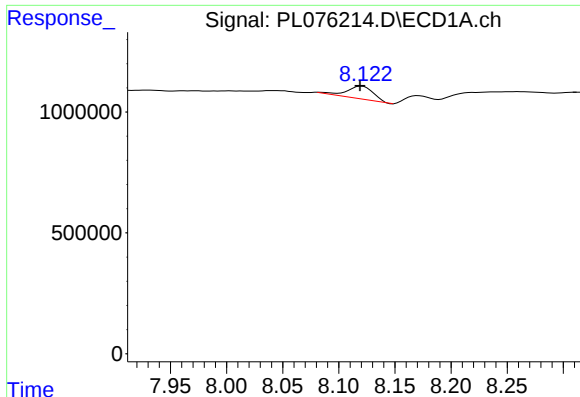

#8 Heptachlor epoxide


R.T.: 8.121 min
Delta R.T.: 0.002 min
Response: 873961
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

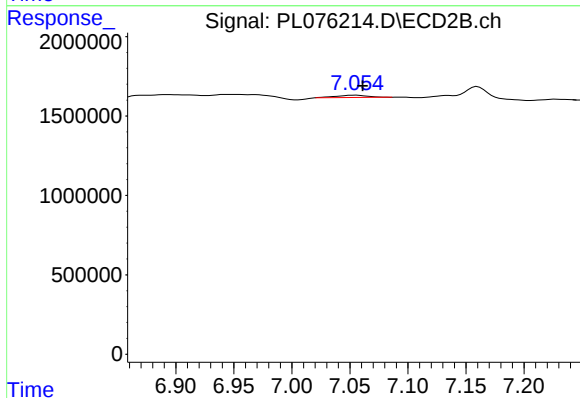


#8 Heptachlor epoxide

R.T.: 7.055 min
Delta R.T.: -0.006 min
Response: 282767
Conc: 0.15 ng/ml

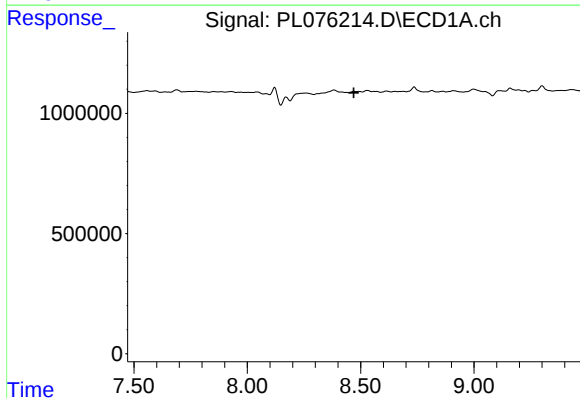


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.470 min
Response: 0
Conc: N.D.

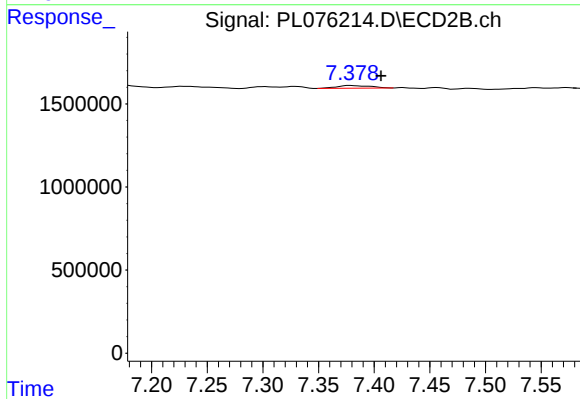

#11 alpha-Chlordane


R.T.: 7.379 min
Delta R.T.: -0.027 min
Response: 346229
Conc: 0.18 ng/ml

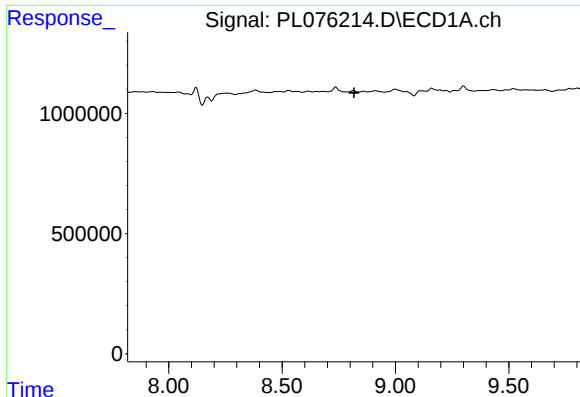

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

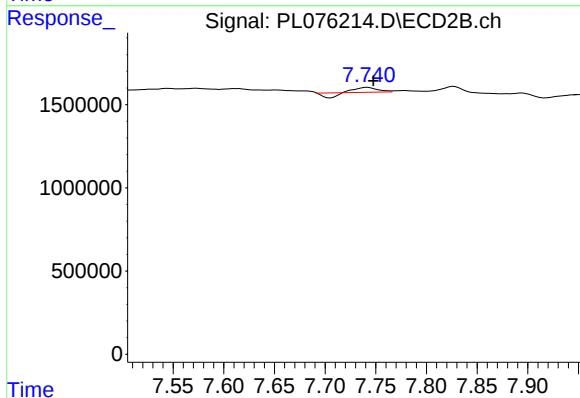


#13 Dieldrin

R.T.: 7.742 min
Delta R.T.: -0.006 min
Response: 259061
Conc: 0.14 ng/ml

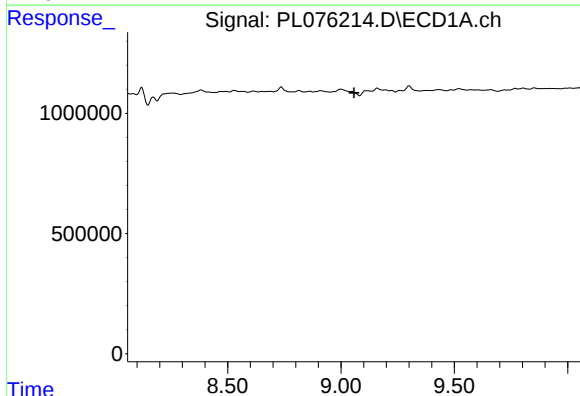


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

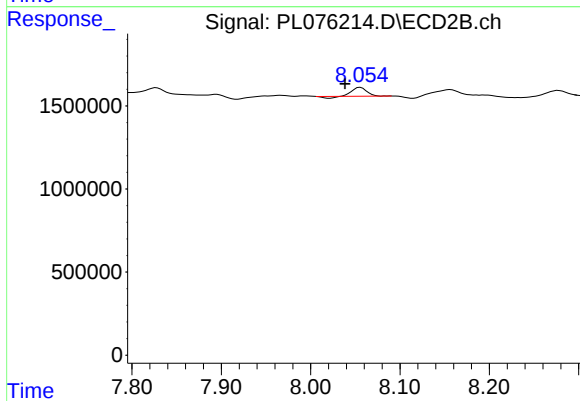

#14 Endrin


R.T.: 8.056 min
Delta R.T.: 0.017 min
Response: 560611
Conc: 0.37 ng/ml

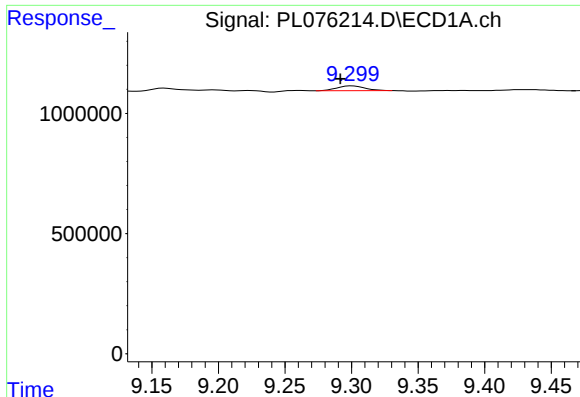

#15 Endosulfan II


R.T.: 9.300 min
Delta R.T.: 0.009 min
Response: 295256
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

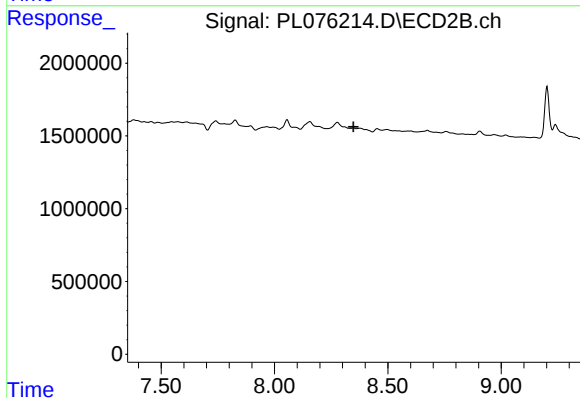


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

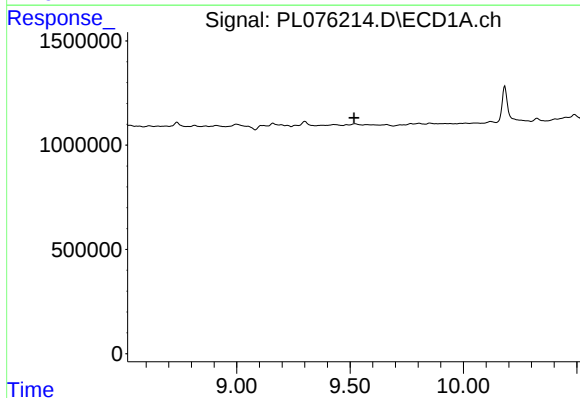


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.518 min
Response: 0
Conc: N.D.

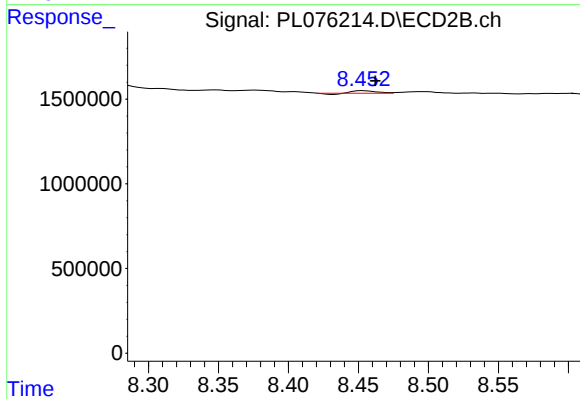

#17 4,4'-DDT


R.T.: 8.453 min
Delta R.T.: -0.009 min
Response: 142454
Conc: 0.10 ng/ml

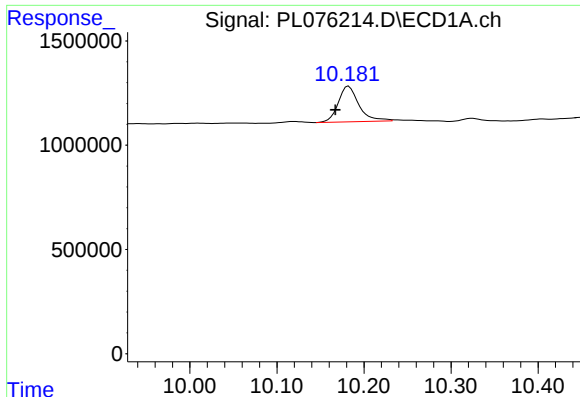

#21 Endrin ketone


R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 2839075
Conc: 3.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

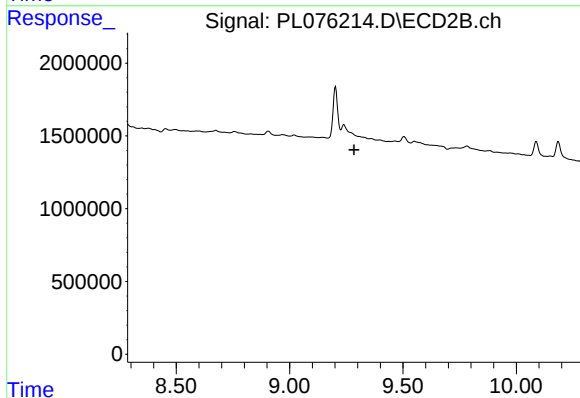


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

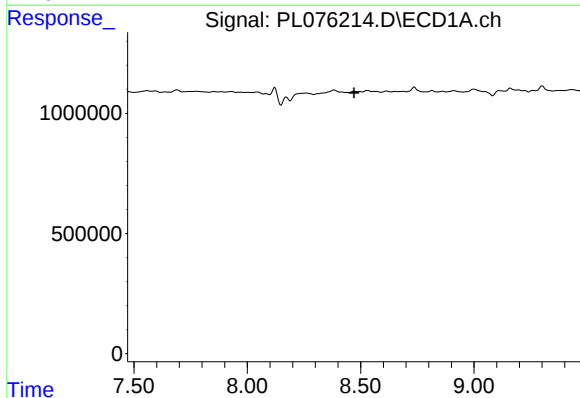


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

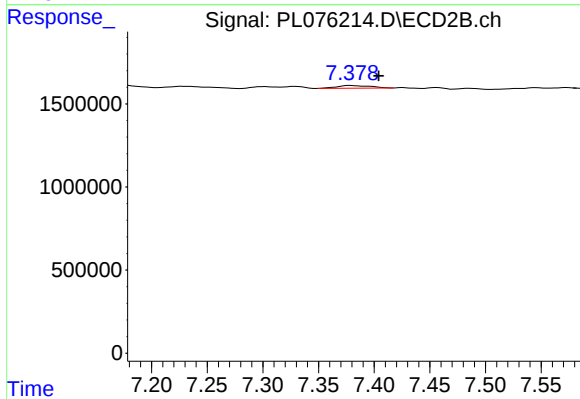

#26 Chlordane-4


R.T.: 7.379 min
Delta R.T.: -0.025 min
Response: 346229
Conc: 1.84 ng/ml

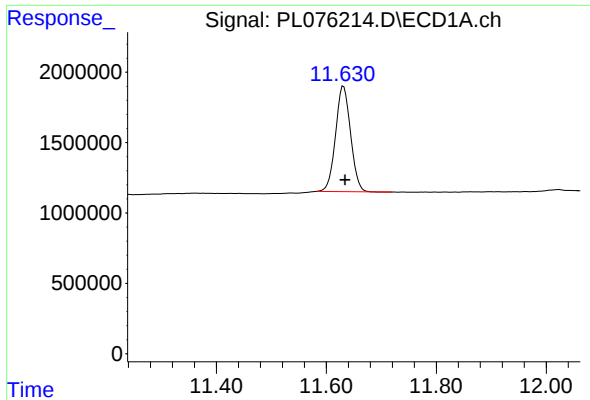

#28 Decachlorobiphenyl

R.T.: 11.631 min
Delta R.T.: -0.003 min
Response: 14214793
Conc: 22.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

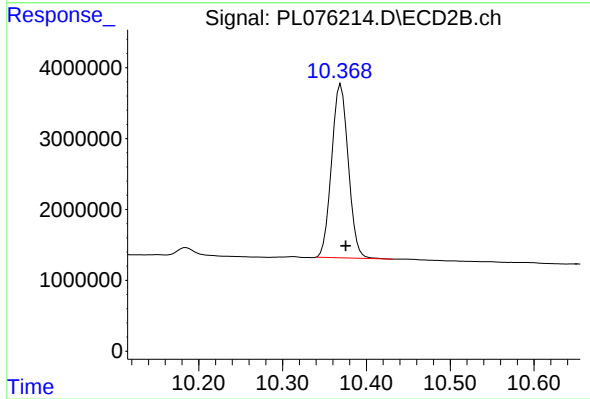

#28 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: -0.006 min
Response: 33787235
Conc: 22.00 ng/ml