

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070222\
 Data File : PL076219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2022 13:17
 Operator : AR\AJ
 Sample : PB145979BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:50:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.630	13001269	32497038	17.190	17.134
28)	SA Decachlor...	11.633	10.370	12696387	30502454	20.177	19.860
Target Compounds							
7)	B delta-BHC	0.000	6.392	0	644690	N.D.	0.285 #
8)	B Heptachlo...	8.122	0.000	604453	0	0.759	N.D. #
11)	B alpha-Chl...	0.000	7.378f	0	265981	N.D.	0.139 #
13)	MA Dieldrin	0.000	7.754	0	121414	N.D.	0.067 #
14)	MA Endrin	0.000	8.056f	0	1338280	N.D.	0.881 #
15)	B Endosulfa...	9.302	0.000	319548	0	0.504	N.D. #
18)	B Endrin al...	0.000	8.529	0	244297	N.D.	0.205 #
21)	B Endrin ke...	10.183f	0.000	2757759	0	3.826	N.D. #
24)	Chlordane-2	0.000	6.637	0	89303	N.D.	1.284 #
26)	Chlordane-4	0.000	7.378f	0	265981	N.D.	1.411 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070222\
Data File : PL076219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2022 13:17
Operator : AR\AJ
Sample : PB145979BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:50:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

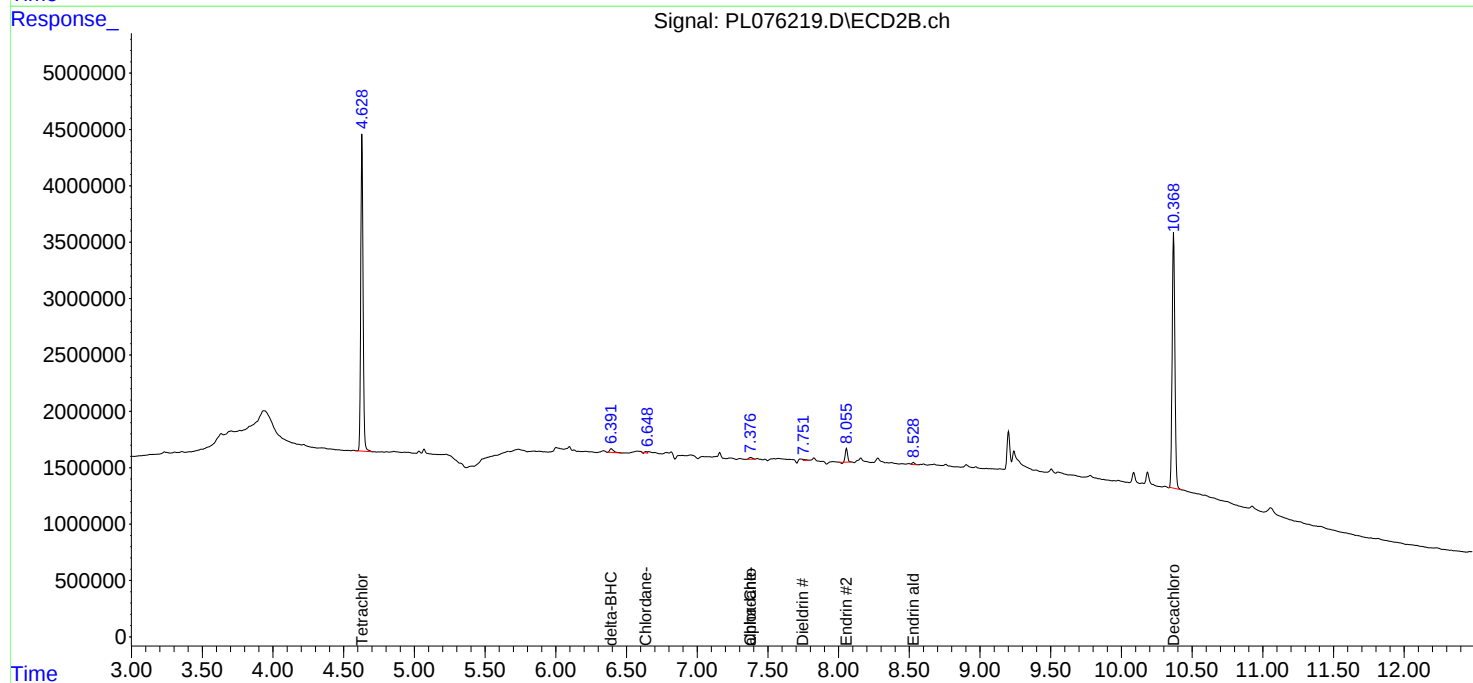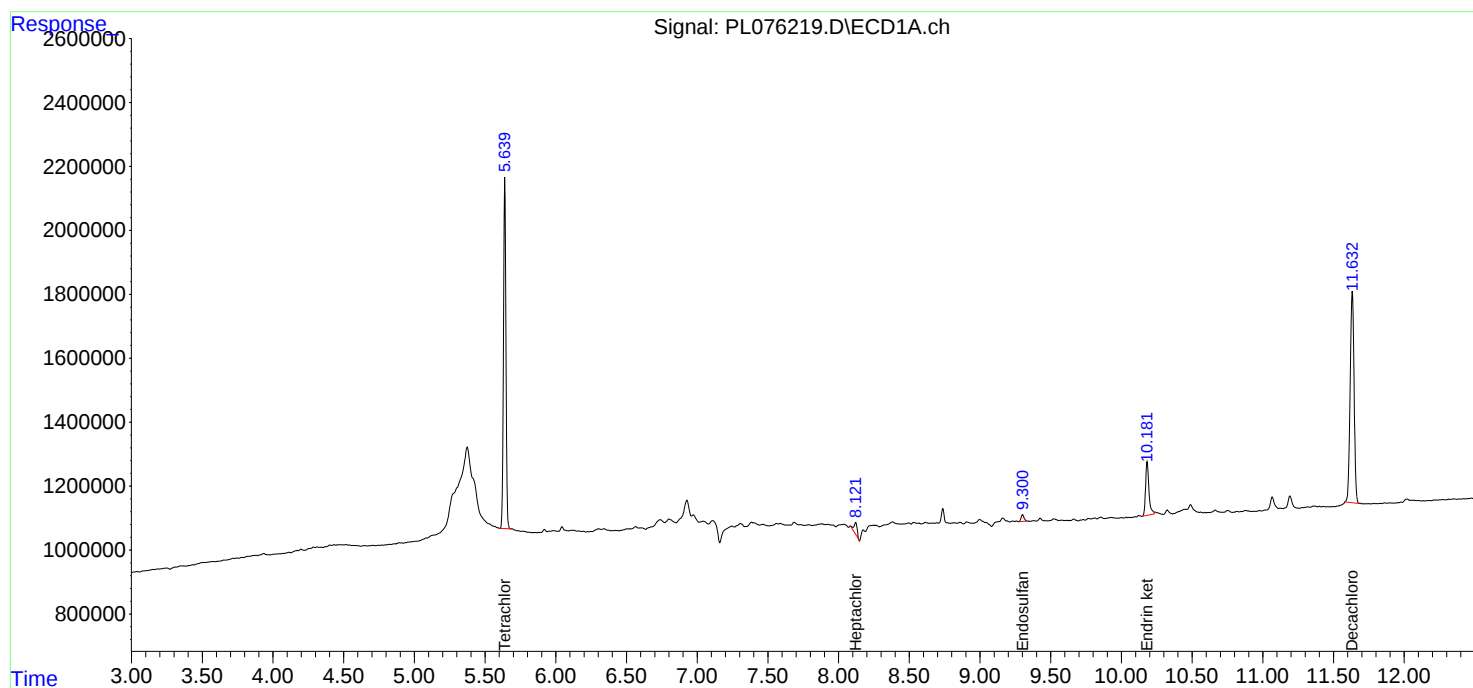


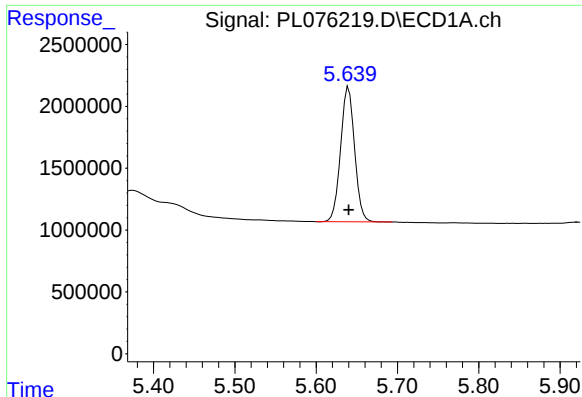

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 13001269
Conc: 17.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

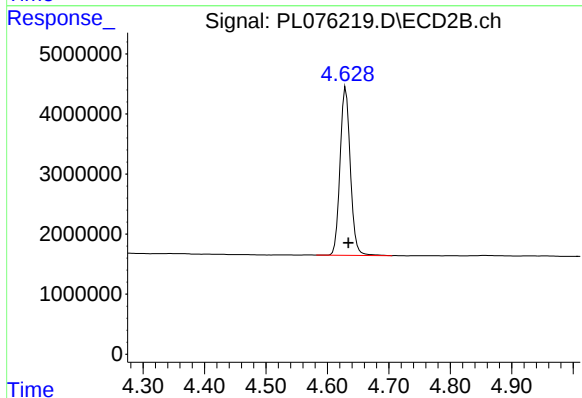


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: -0.004 min
Response: 32497038
Conc: 17.13 ng/ml

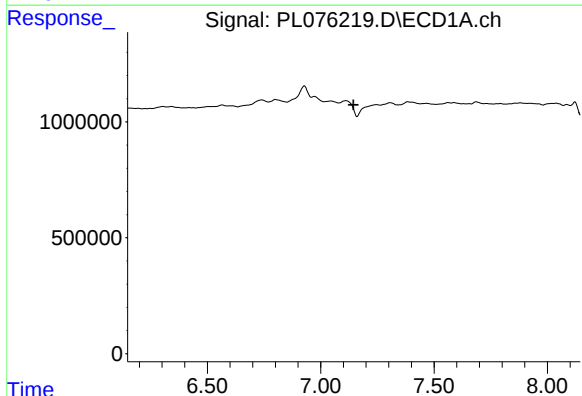


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

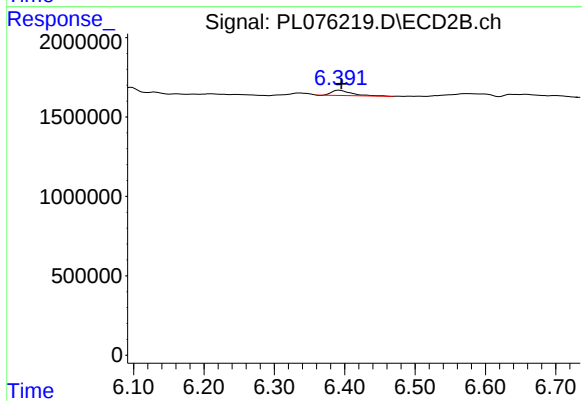

#7 delta-BHC


R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 644690
Conc: 0.29 ng/ml

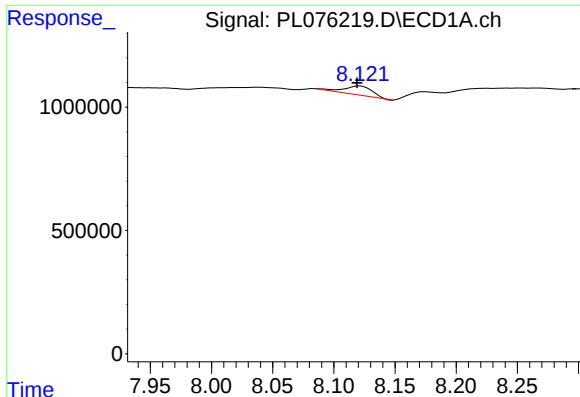

#8 Heptachlor epoxide


R.T.: 8.122 min
Delta R.T.: 0.003 min
Response: 604453
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

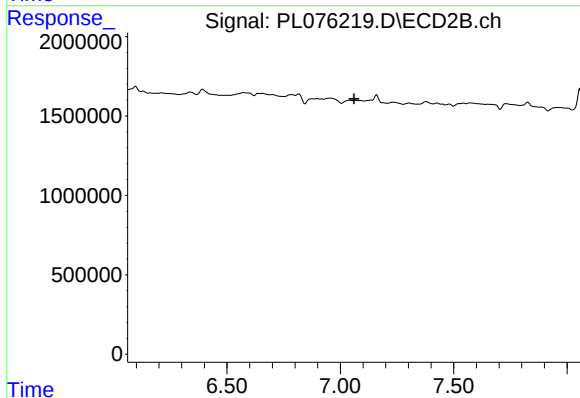


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.061 min
Response: 0
Conc: N.D.

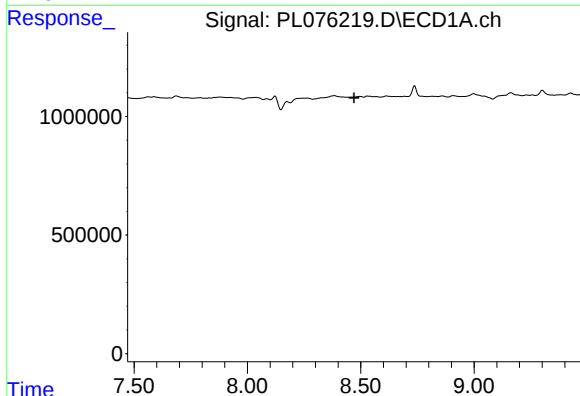


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.470 min
Response: 0
Conc: N.D.

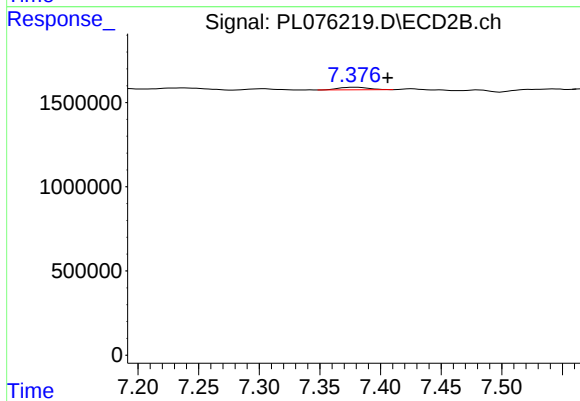

#11 alpha-Chlordane


R.T.: 7.378 min
Delta R.T.: -0.029 min
Response: 265981
Conc: 0.14 ng/ml

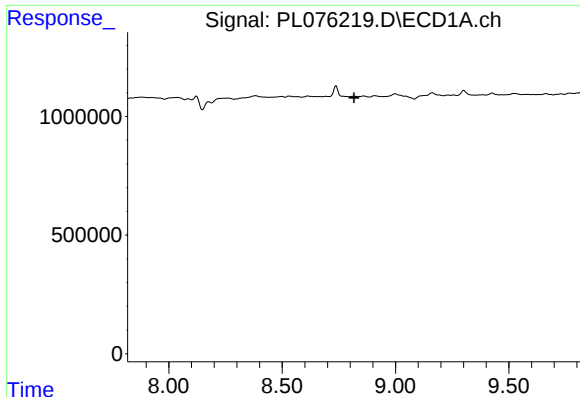

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

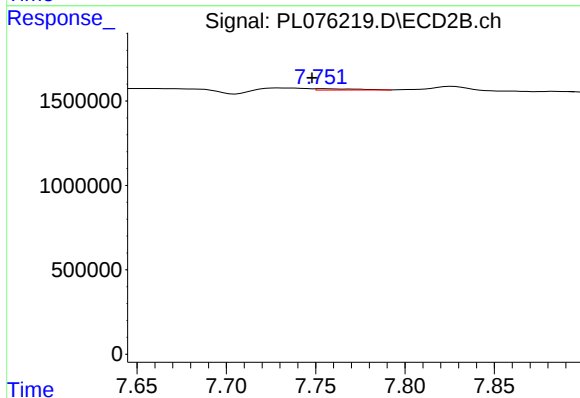


#13 Dieldrin

R.T.: 7.754 min
Delta R.T.: 0.006 min
Response: 121414
Conc: 0.07 ng/ml

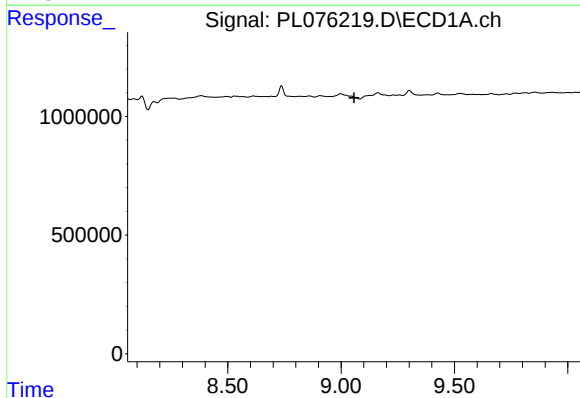


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

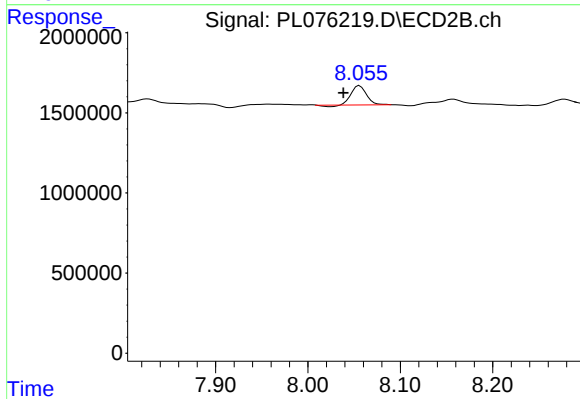

#14 Endrin


R.T.: 8.056 min
Delta R.T.: 0.018 min
Response: 1338280
Conc: 0.88 ng/ml

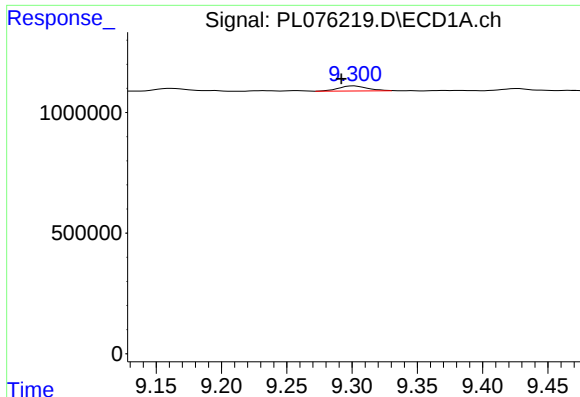

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.010 min
Response: 319548
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

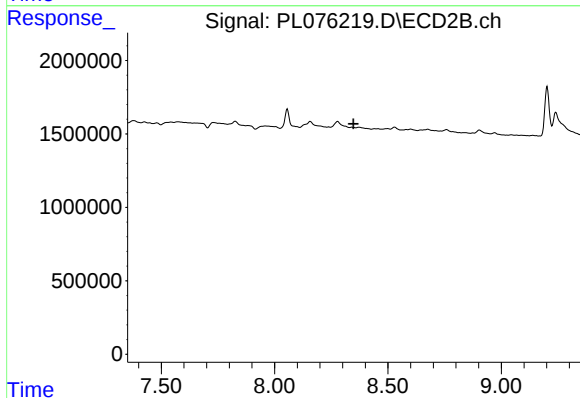


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

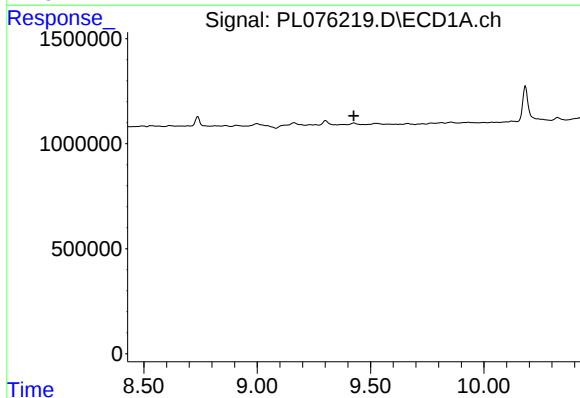


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.426 min
Response: 0
Conc: N.D.

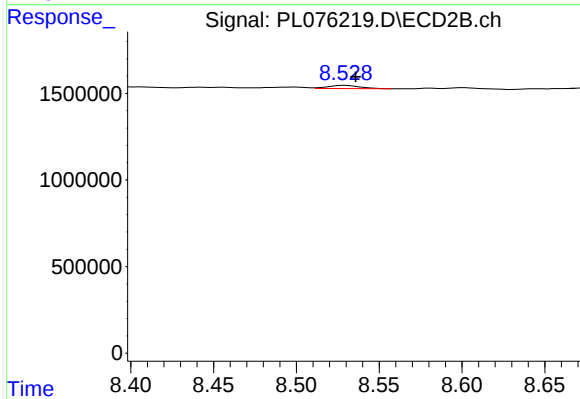

#18 Endrin aldehyde


R.T.: 8.529 min
Delta R.T.: -0.006 min
Response: 244297
Conc: 0.20 ng/ml

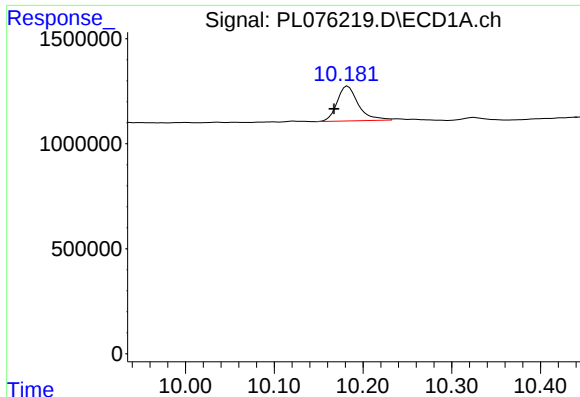

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.015 min
Response: 2757759
Conc: 3.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

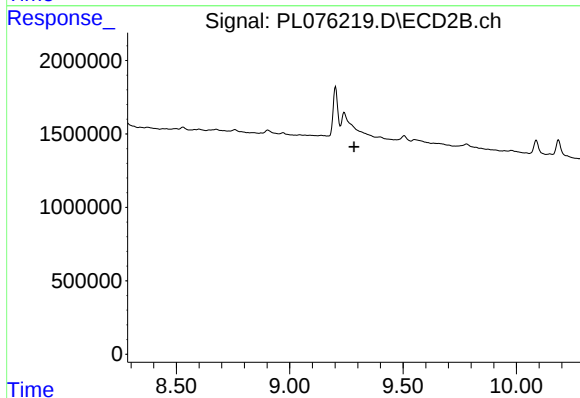


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

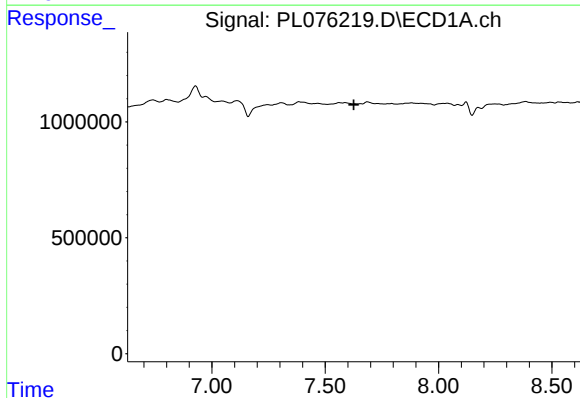


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.627 min
Response: 0
Conc: N.D.

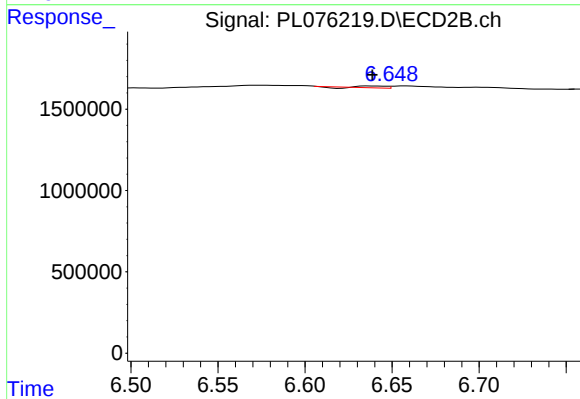

#24 Chlordane-2


R.T.: 6.637 min
Delta R.T.: -0.002 min
Response: 89303
Conc: 1.28 ng/ml

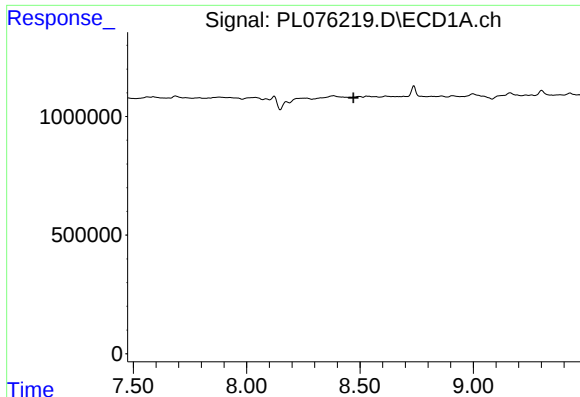

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

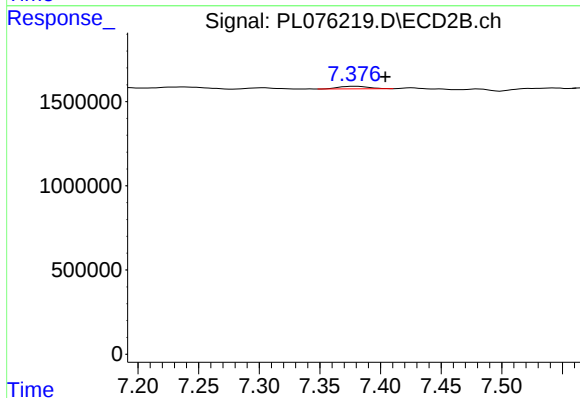


#26 Chlordane-4

R.T.: 7.378 min
Delta R.T.: -0.027 min
Response: 265981
Conc: 1.41 ng/ml

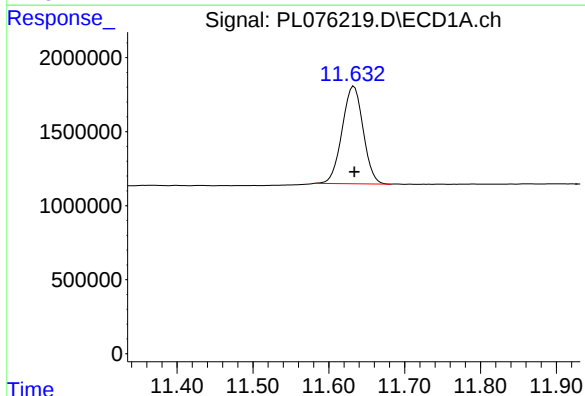

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 12696387
Conc: 20.18 ng/ml

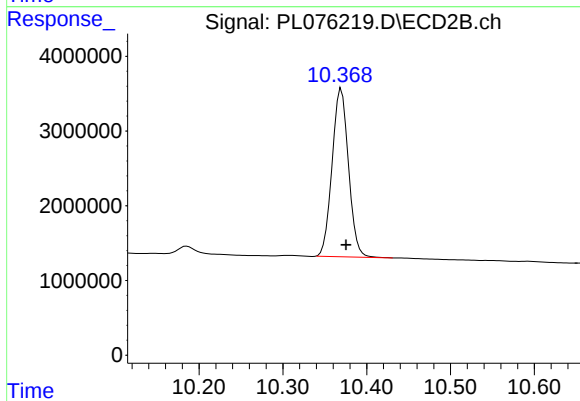

#28 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: -0.006 min
Response: 30502454
Conc: 19.86 ng/ml