

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070918\
 Data File : PL037791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2018 14:57
 Operator : AJ\SJ
 Sample : J3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURCHARGE-SP-3

Manual Integrations
 APPROVED

Sohil
 7/10/2018 1:41:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:31:04 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	59998385	22381611	7.585	8.090
28)	SA Decachlor...	8.010	8.946	69657842	24535384	11.544	12.367
Target Compounds							
12)	B 4,4'-DDE	5.450	6.248	59951084	20595728	6.788	8.094

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070918\
Data File : PL037791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2018 14:57
Operator : AJ\SJ
Sample : J3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-3


Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:31:04 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

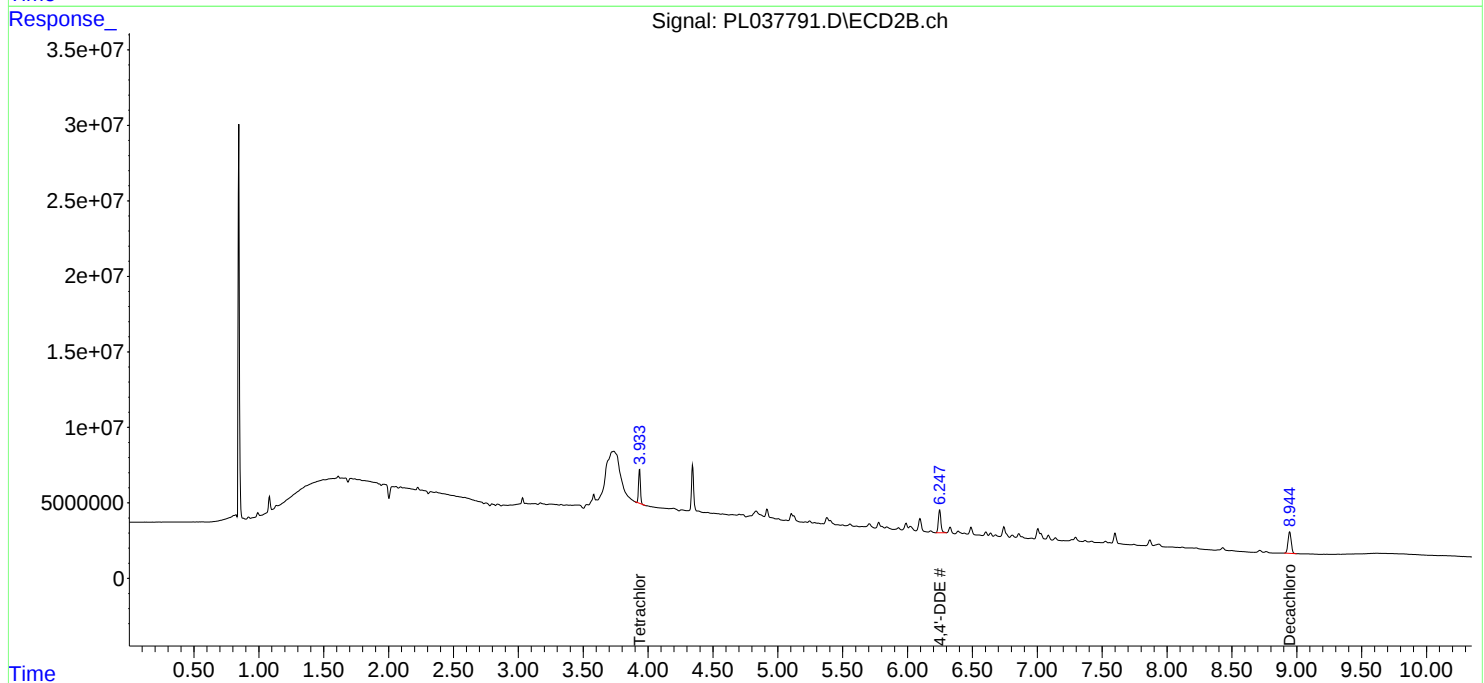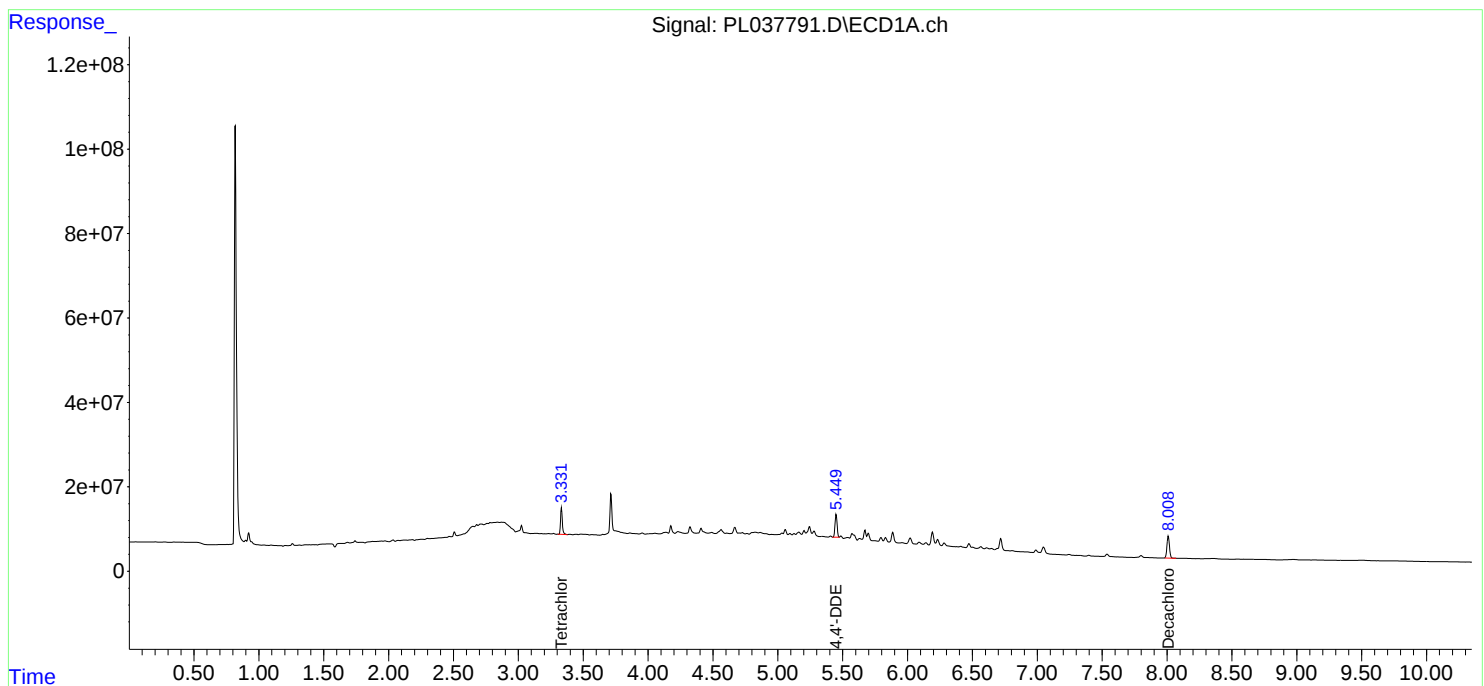

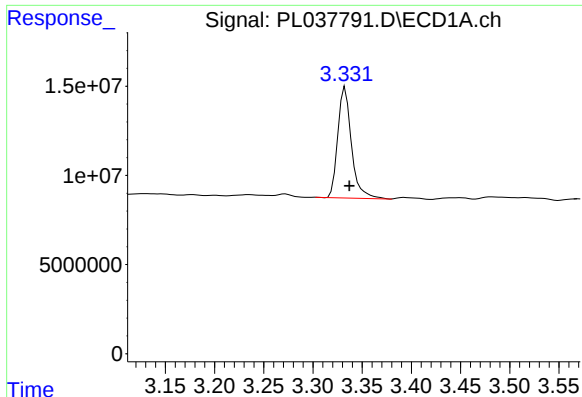


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 59998385
Conc: 7.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-3


Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:21 PM

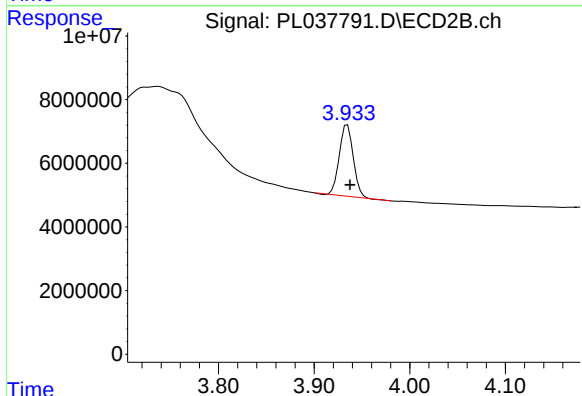


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 22381611
Conc: 8.09 ng/ml

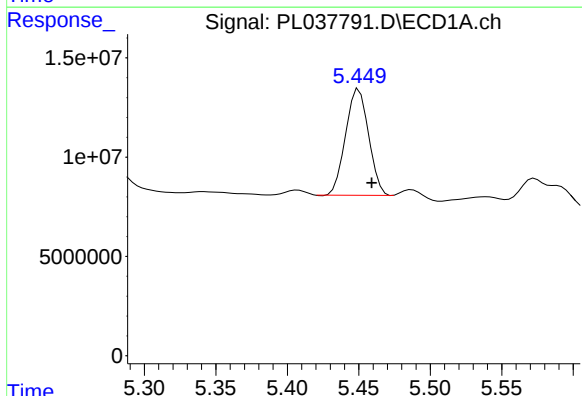


#12 4,4'-DDE

R.T.: 5.450 min
Delta R.T.: -0.009 min
Response: 59951084
Conc: 6.79 ng/ml

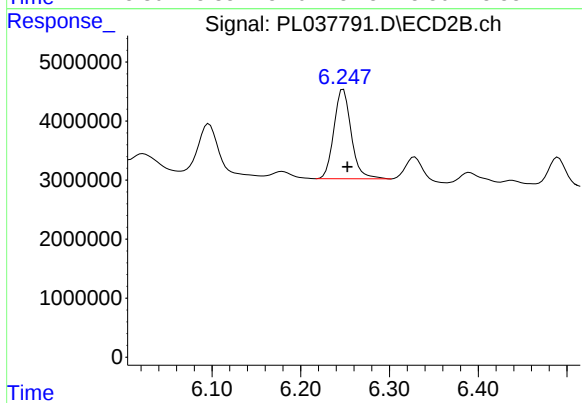

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.004 min
Response: 20595728
Conc: 8.09 ng/ml

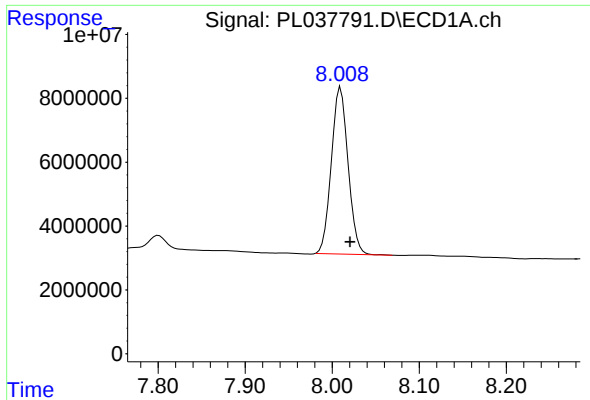


#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 69657842
Conc: 11.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-3

Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:21 PM

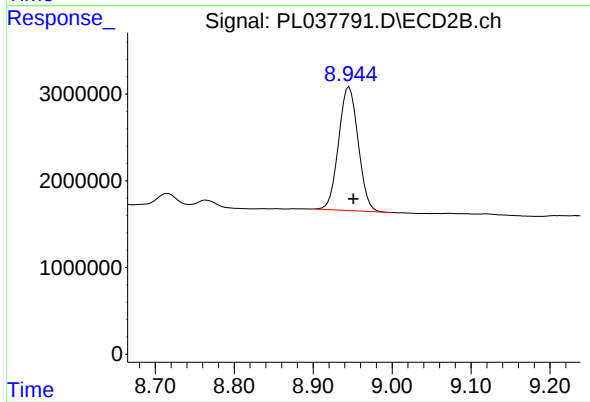

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.005 min
Response: 24535384
Conc: 12.37 ng/ml