

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070918\
 Data File : PL037794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2018 15:39
 Operator : AJ\SJ
 Sample : J3879-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURCHARGE-SP-6

Manual Integrations
 APPROVED

Sohil
 7/10/2018 1:41:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:31:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	81195520	27632234	10.265	9.987
28)	SA Decachlor...	8.010	8.945	77213170	27193999	12.796	13.707
Target Compounds							
12)	B 4,4'-DDE	5.450	6.248	75208183	23228914	8.515	9.128

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070918\
Data File : PL037794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2018 15:39
Operator : AJ\SJ
Sample : J3879-11
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-6


Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:31:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

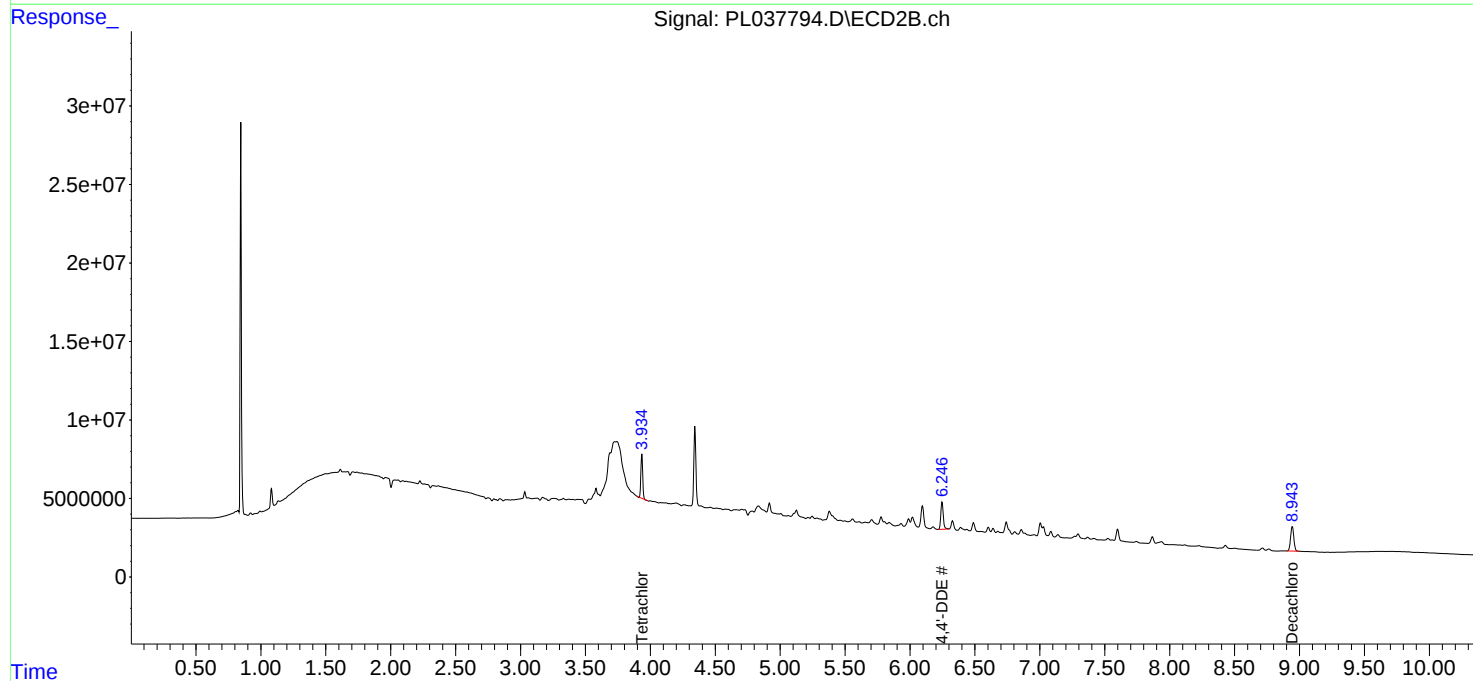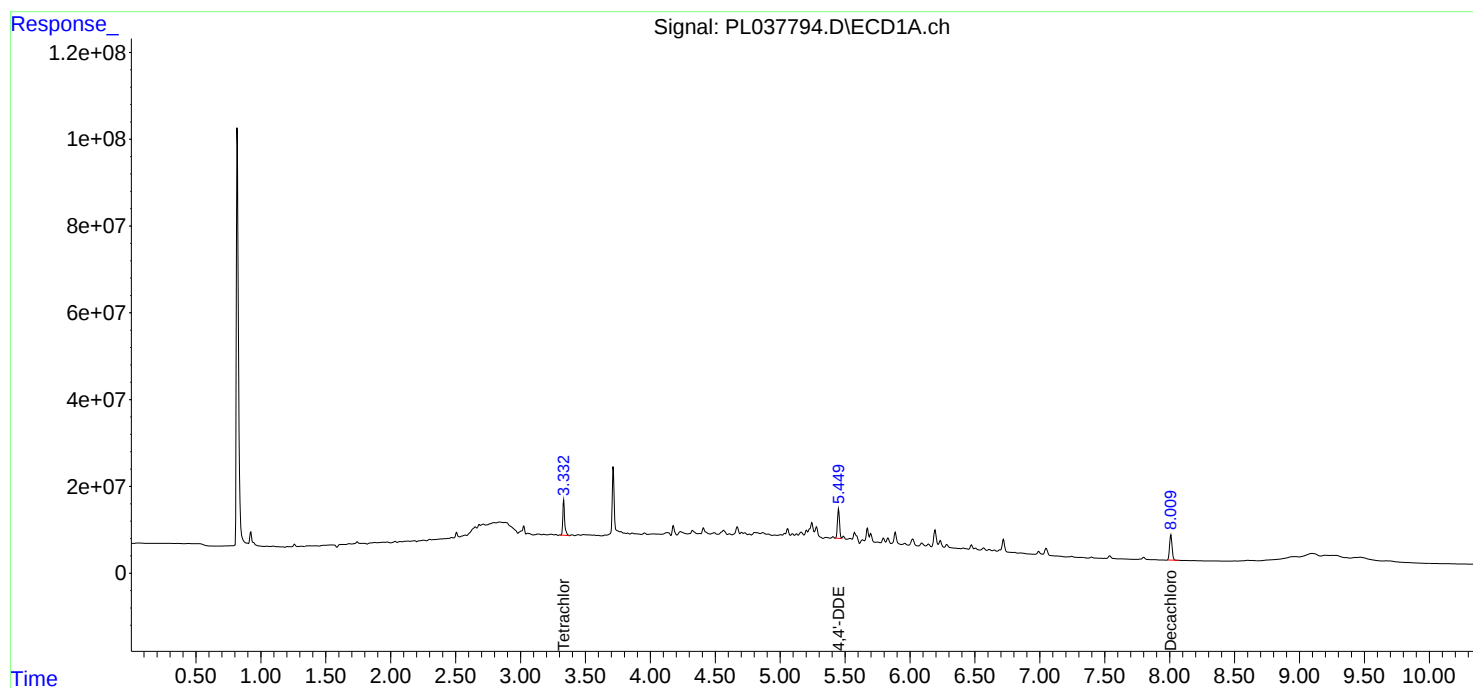

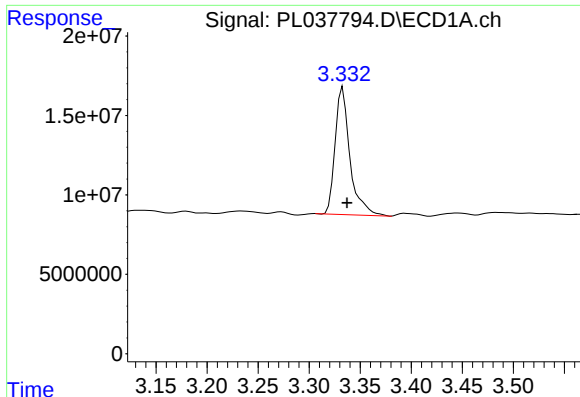


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 81195520
Conc: 10.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-6


Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:22 PM

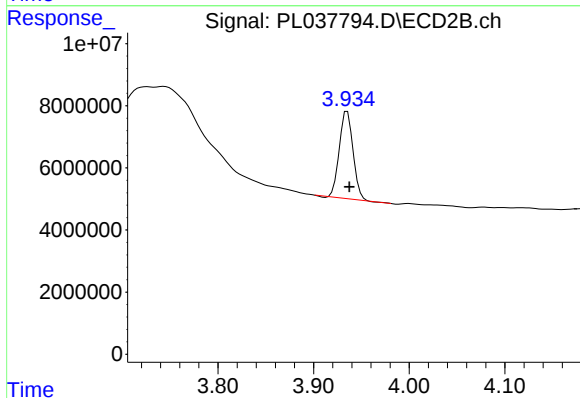


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 27632234
Conc: 9.99 ng/ml

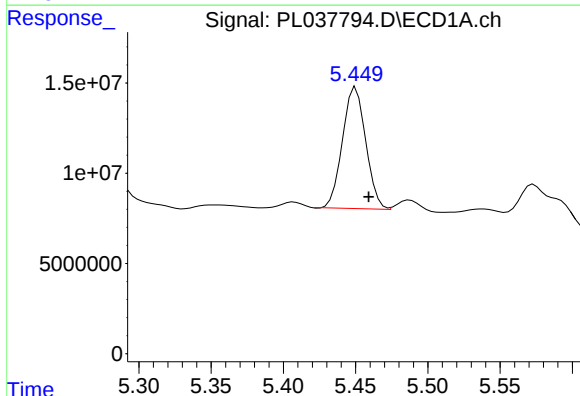


#12 4,4'-DDE

R.T.: 5.450 min
Delta R.T.: -0.009 min
Response: 75208183
Conc: 8.51 ng/ml

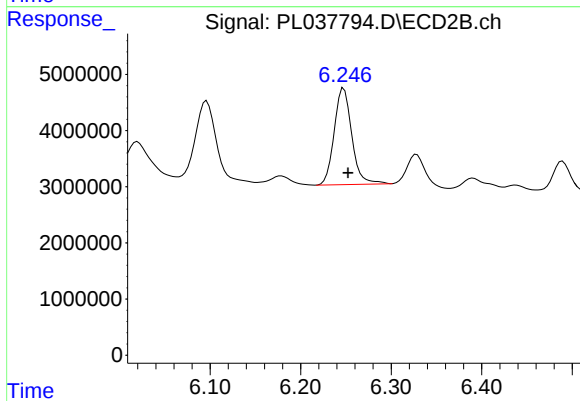

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.005 min
Response: 23228914
Conc: 9.13 ng/ml

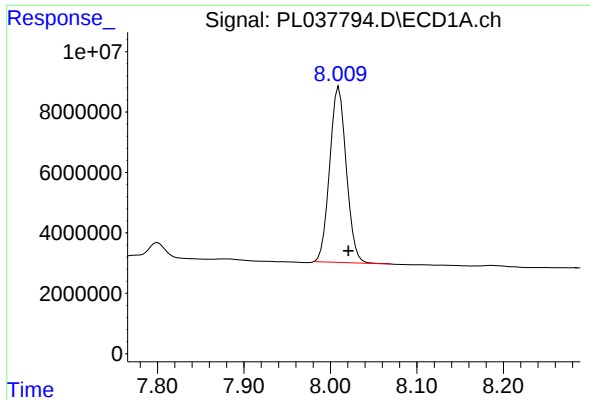


#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 77213170
Conc: 12.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-6

Manual Integrations
APPROVED

Sohil
7/10/2018 1:41:22 PM

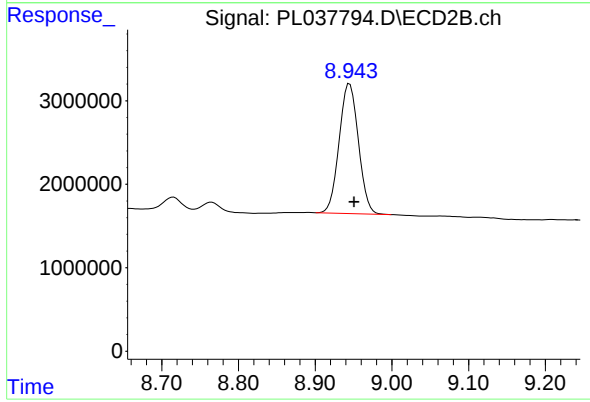

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 27193999
Conc: 13.71 ng/ml