

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
 Data File : PL076772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 16:16
 Operator : AR\AJ
 Sample : N3927-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RVE-80

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
 Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:53:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.642	24534501	64801908	23.773	21.847
2)	SA Decachlor...	8.911	7.750	20205694	54699391	22.910m	21.311

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
Data File : PL076772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 16:16
Operator : AR\AJ
Sample : N3927-07
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RVE-80


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:53:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

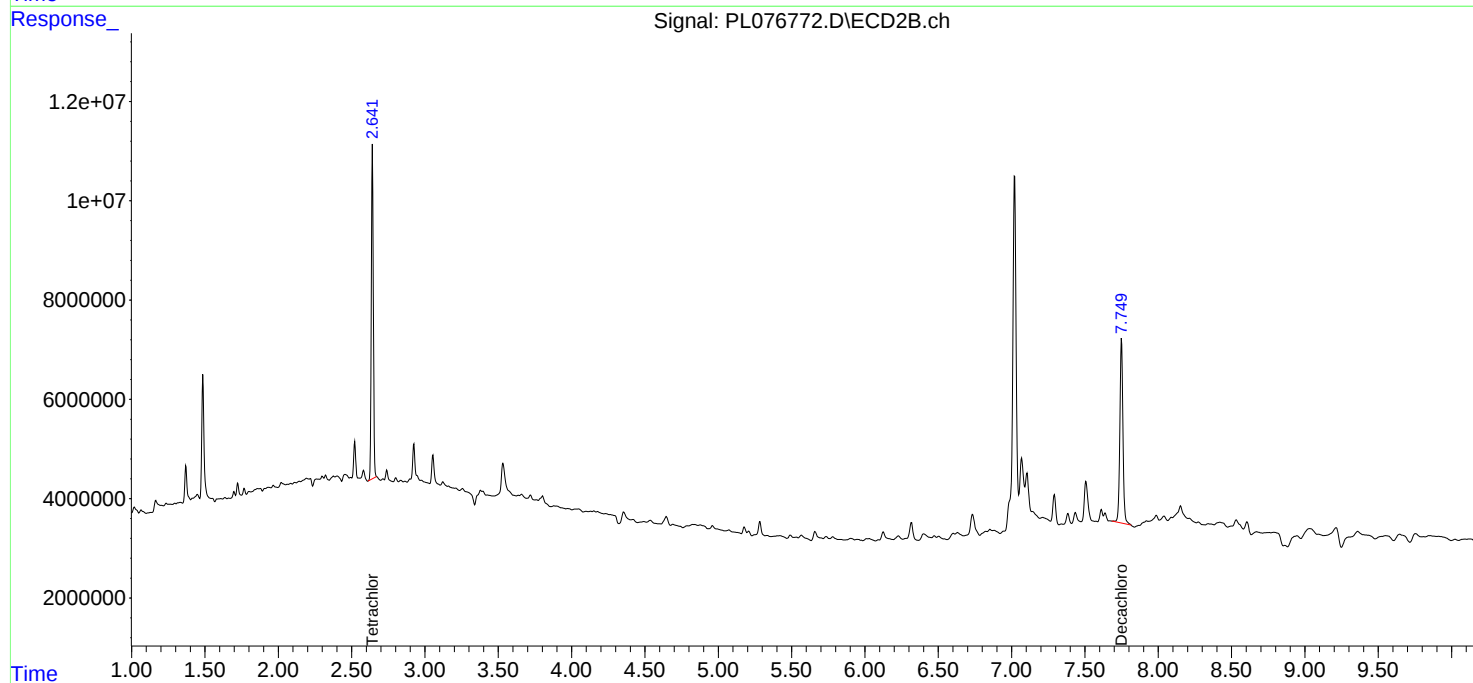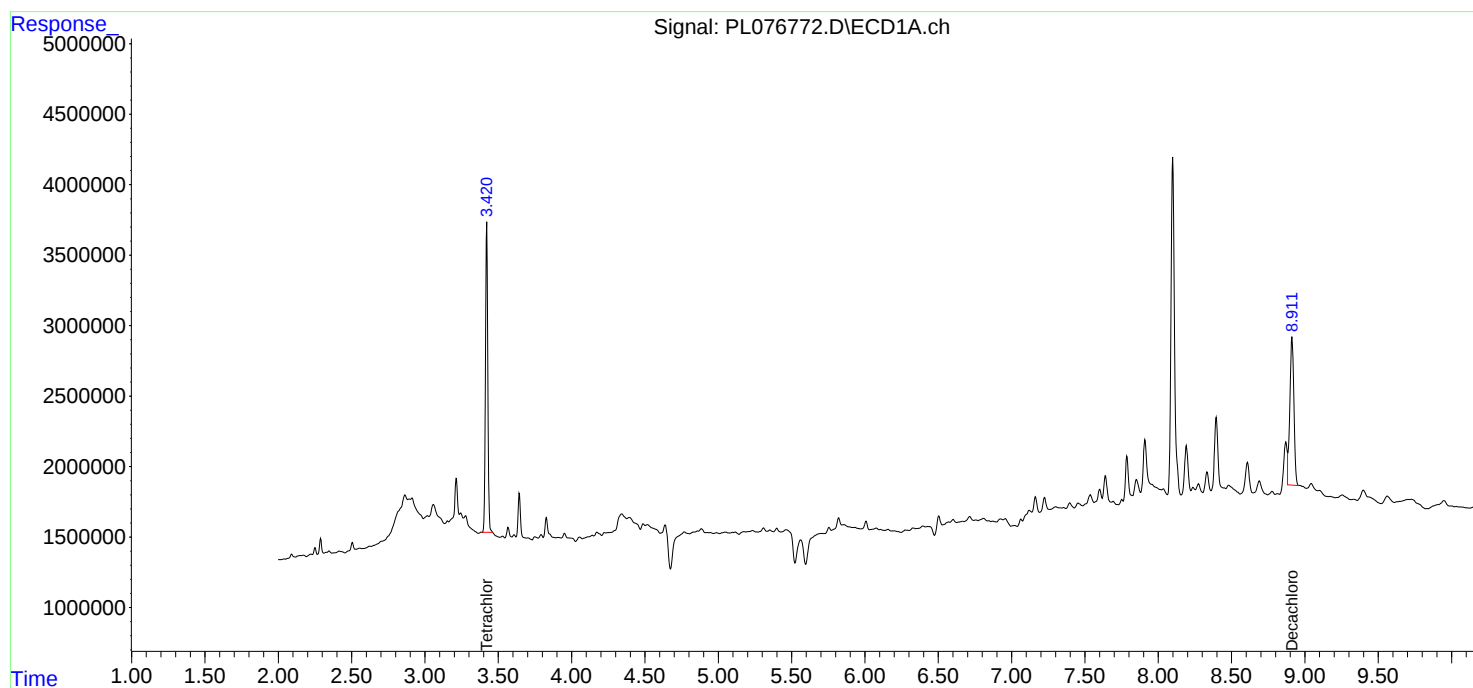

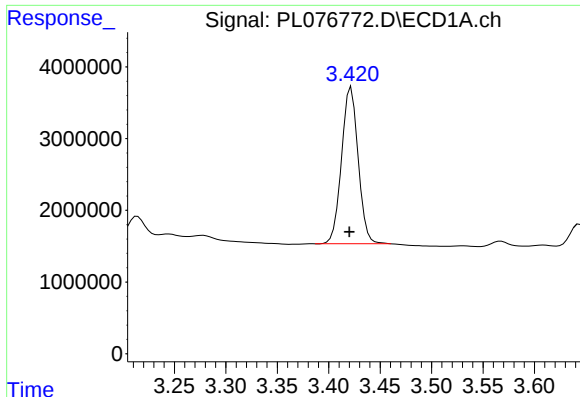


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: 0.002 min
Response: 24534501
Conc: 23.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
RVE-80


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

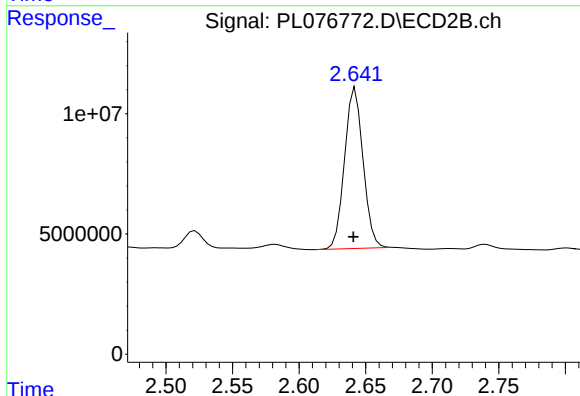


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.002 min
Response: 64801908
Conc: 21.85 ng/ml

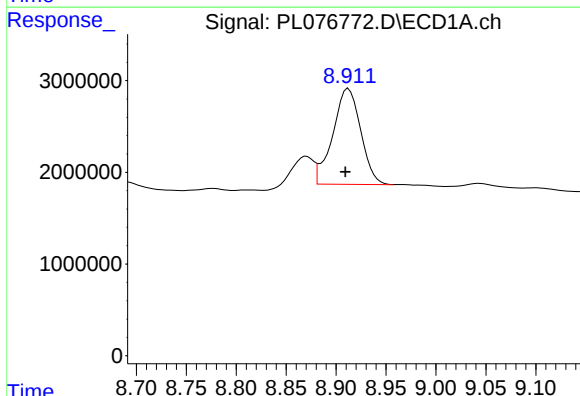

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.002 min
Response: 20205694
Conc: 22.91 ng/ml m

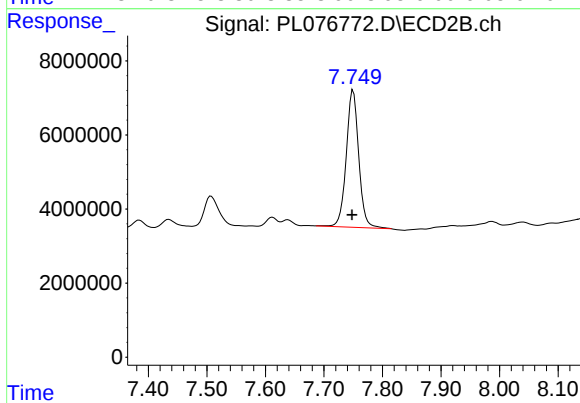

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 54699391
Conc: 21.31 ng/ml