

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
 Data File : PL076792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 22:02
 Operator : AR\AJ
 Sample : N3953-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 IRV-OILY-WATER

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
 Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:59:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.642	13178672	43319074	12.770	14.604m
28)	SA Decachlor...	8.912	7.747	5790230	14570771	6.565	5.677m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
Data File : PL076792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 22:02
Operator : AR\AJ
Sample : N3953-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
IRV-OILY-WATER


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:59:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

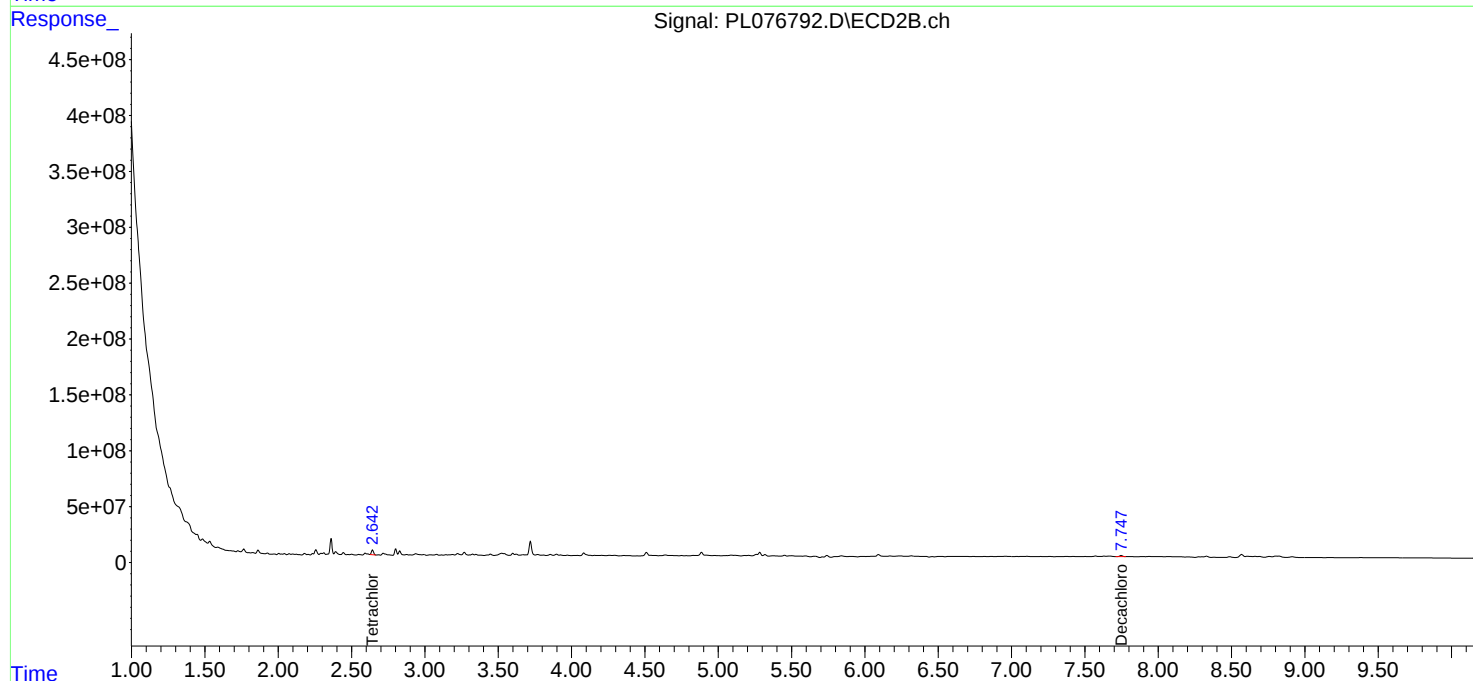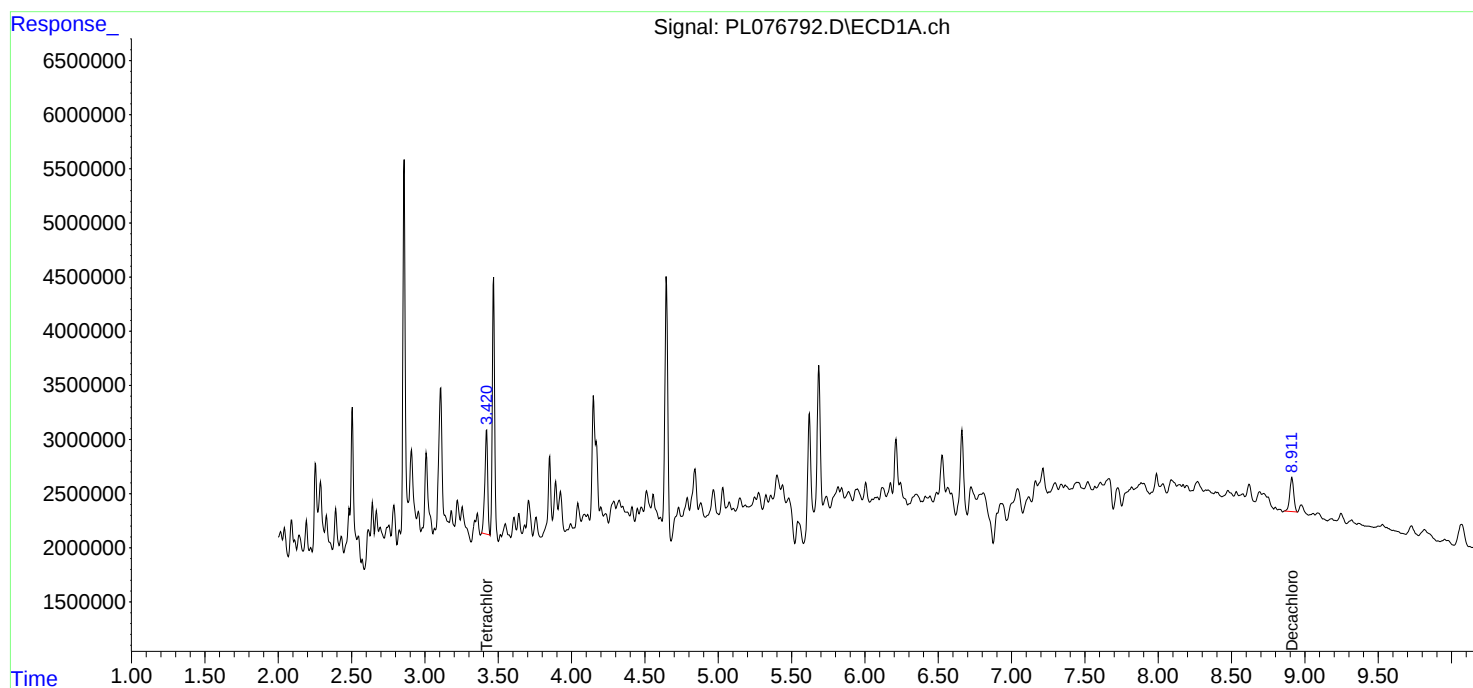

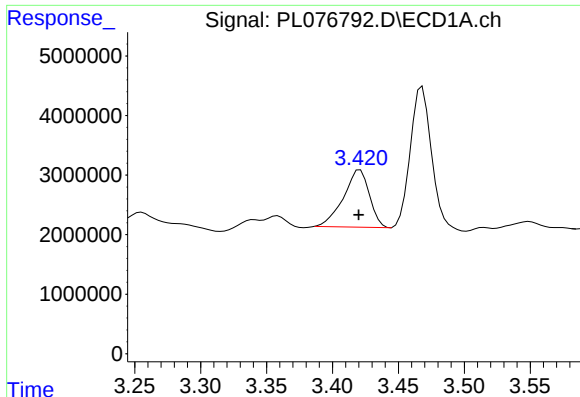


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.001 min
Response: 13178672
Conc: 12.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
IRV-OILY-WATER


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

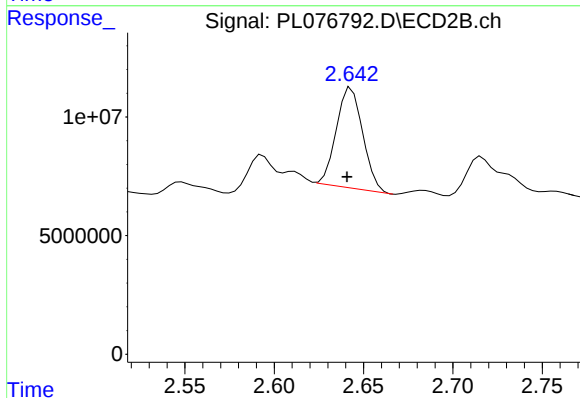


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.001 min
Response: 43319074
Conc: 14.60 ng/ml m

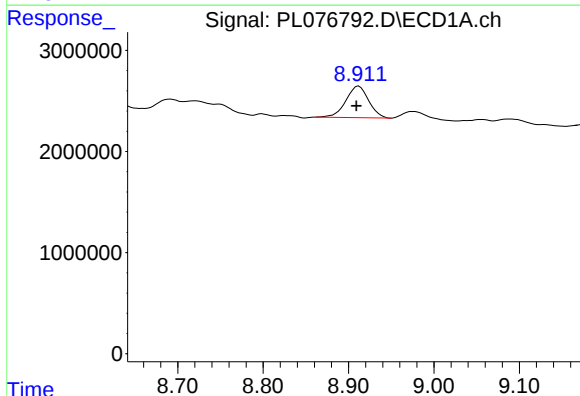

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.003 min
Response: 5790230
Conc: 6.57 ng/ml

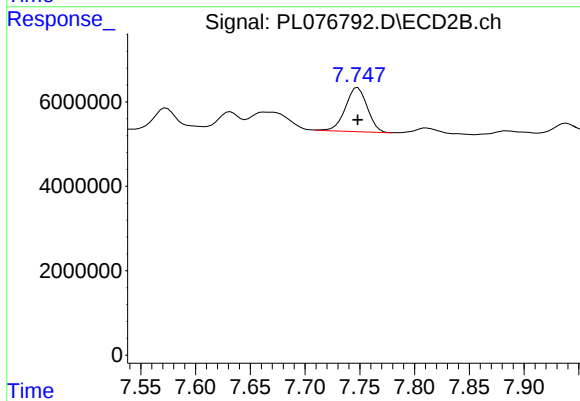

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: -0.001 min
Response: 14570771
Conc: 5.68 ng/ml m