

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
 Data File : PL076793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 22:16
 Operator : AR\AJ
 Sample : N3964-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HMGP-WATER-1

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
 Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:00:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.419	2.641	19635508	31335570	19.026m	10.564m#
2) SA Decachlor...	8.912	7.749	12473110	30853368	14.143	12.020

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
Data File : PL076793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 22:16
Operator : AR\AJ
Sample : N3964-07
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HMGP-WATER-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:00:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

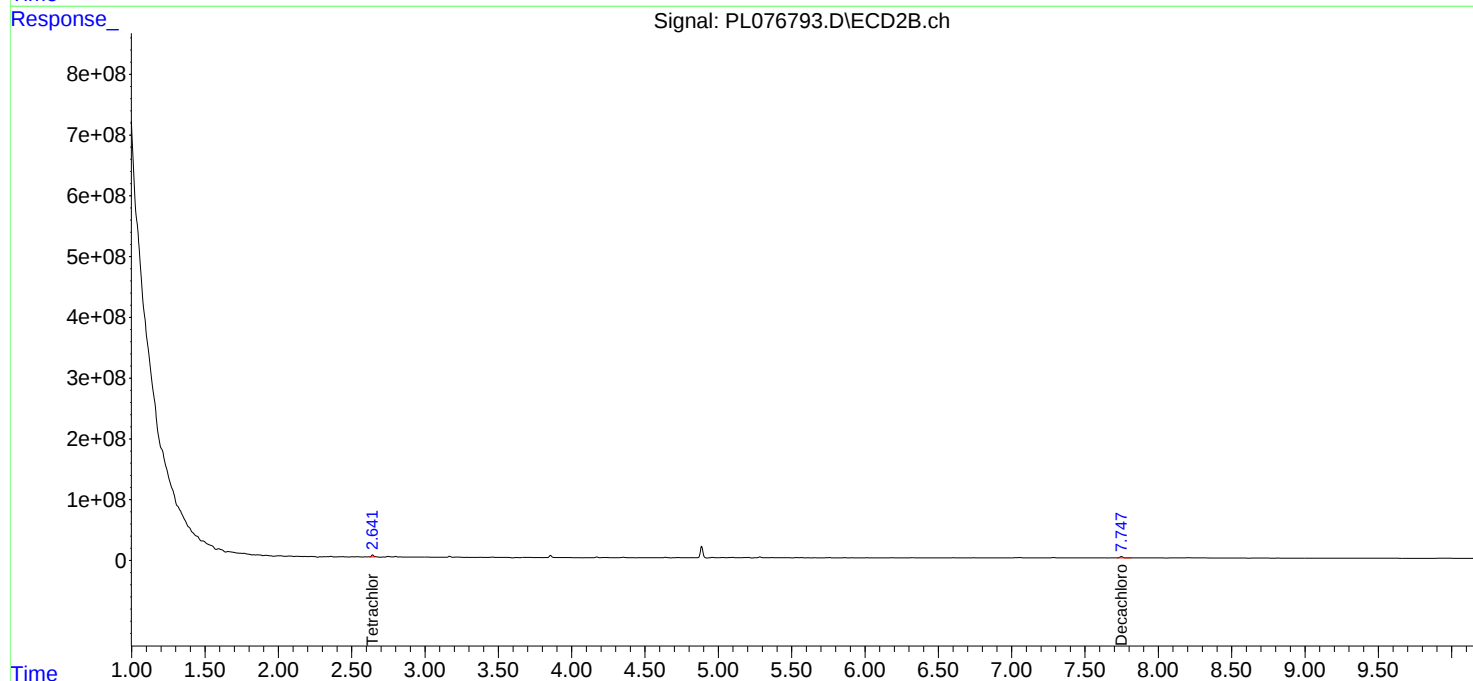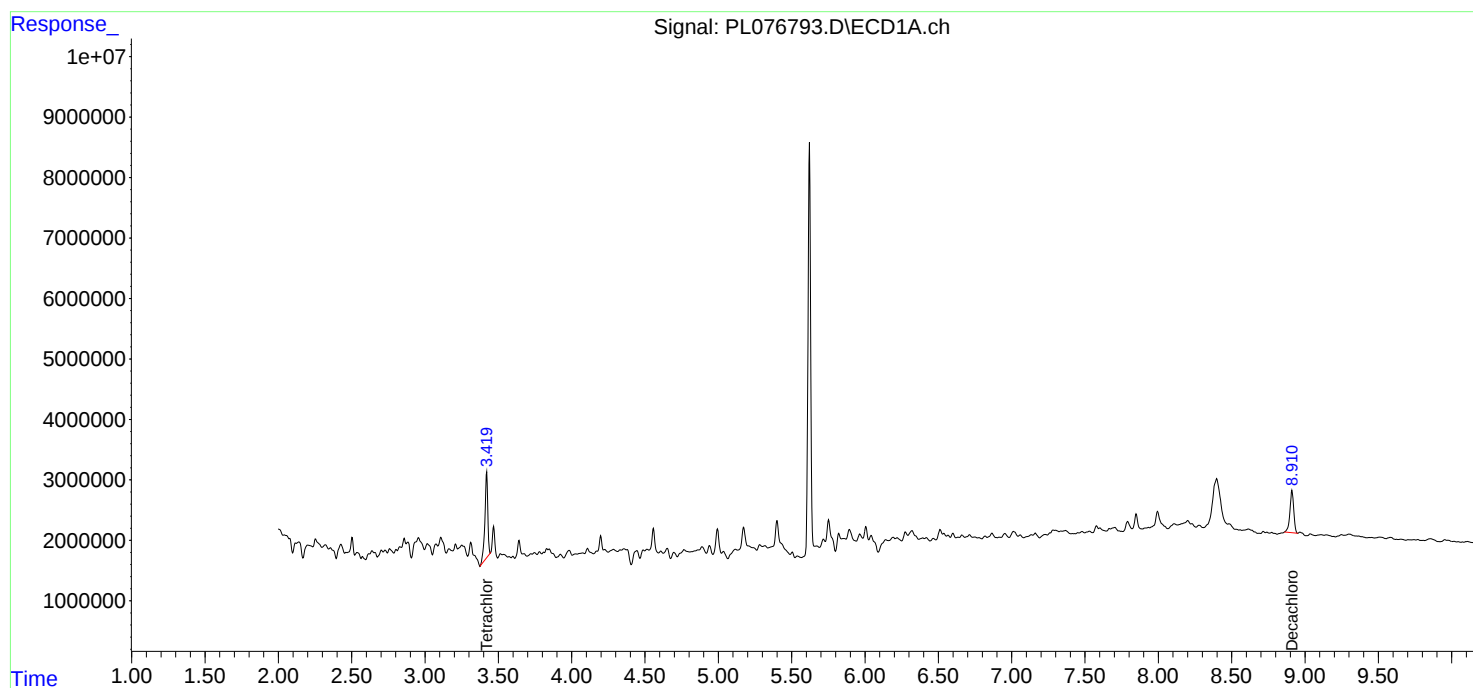

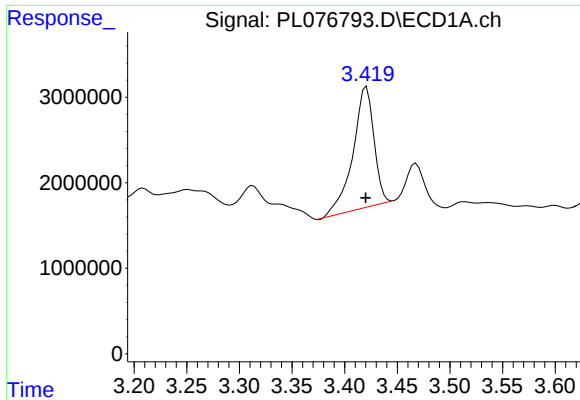


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 19635508
Conc: 19.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
HMGP-WATER-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

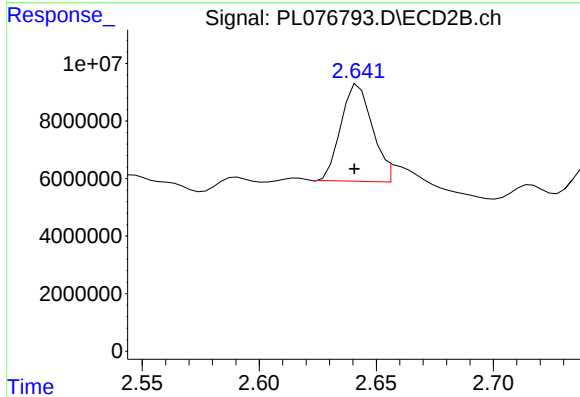


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 31335570
Conc: 10.56 ng/ml m

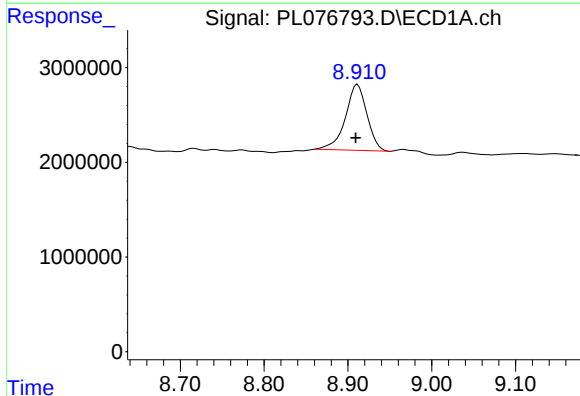

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.002 min
Response: 12473110
Conc: 14.14 ng/ml

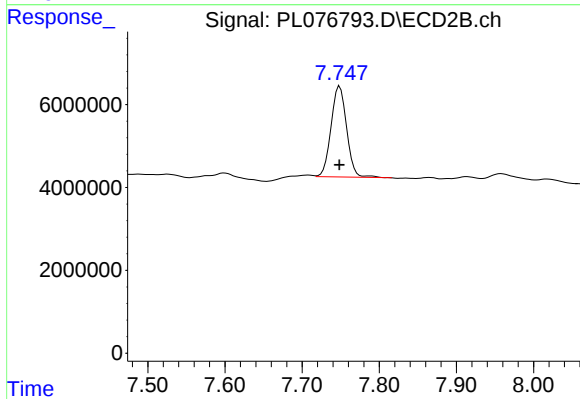

#28 Decachlorobiphenyl

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 30853368
Conc: 12.02 ng/ml