

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
 Data File : PL076794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 22:30
 Operator : AR\AJ
 Sample : N3964-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HMGP-WATER-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
 Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:00:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.414	2.642	16264484	33218730	15.760m	11.199m#
28) SA Decachlor...	8.909	7.748	12701480	35135727	14.402m	13.689

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073022\
Data File : PL076794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 22:30
Operator : AR\AJ
Sample : N3964-08
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
HMGP-WATER-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:00:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

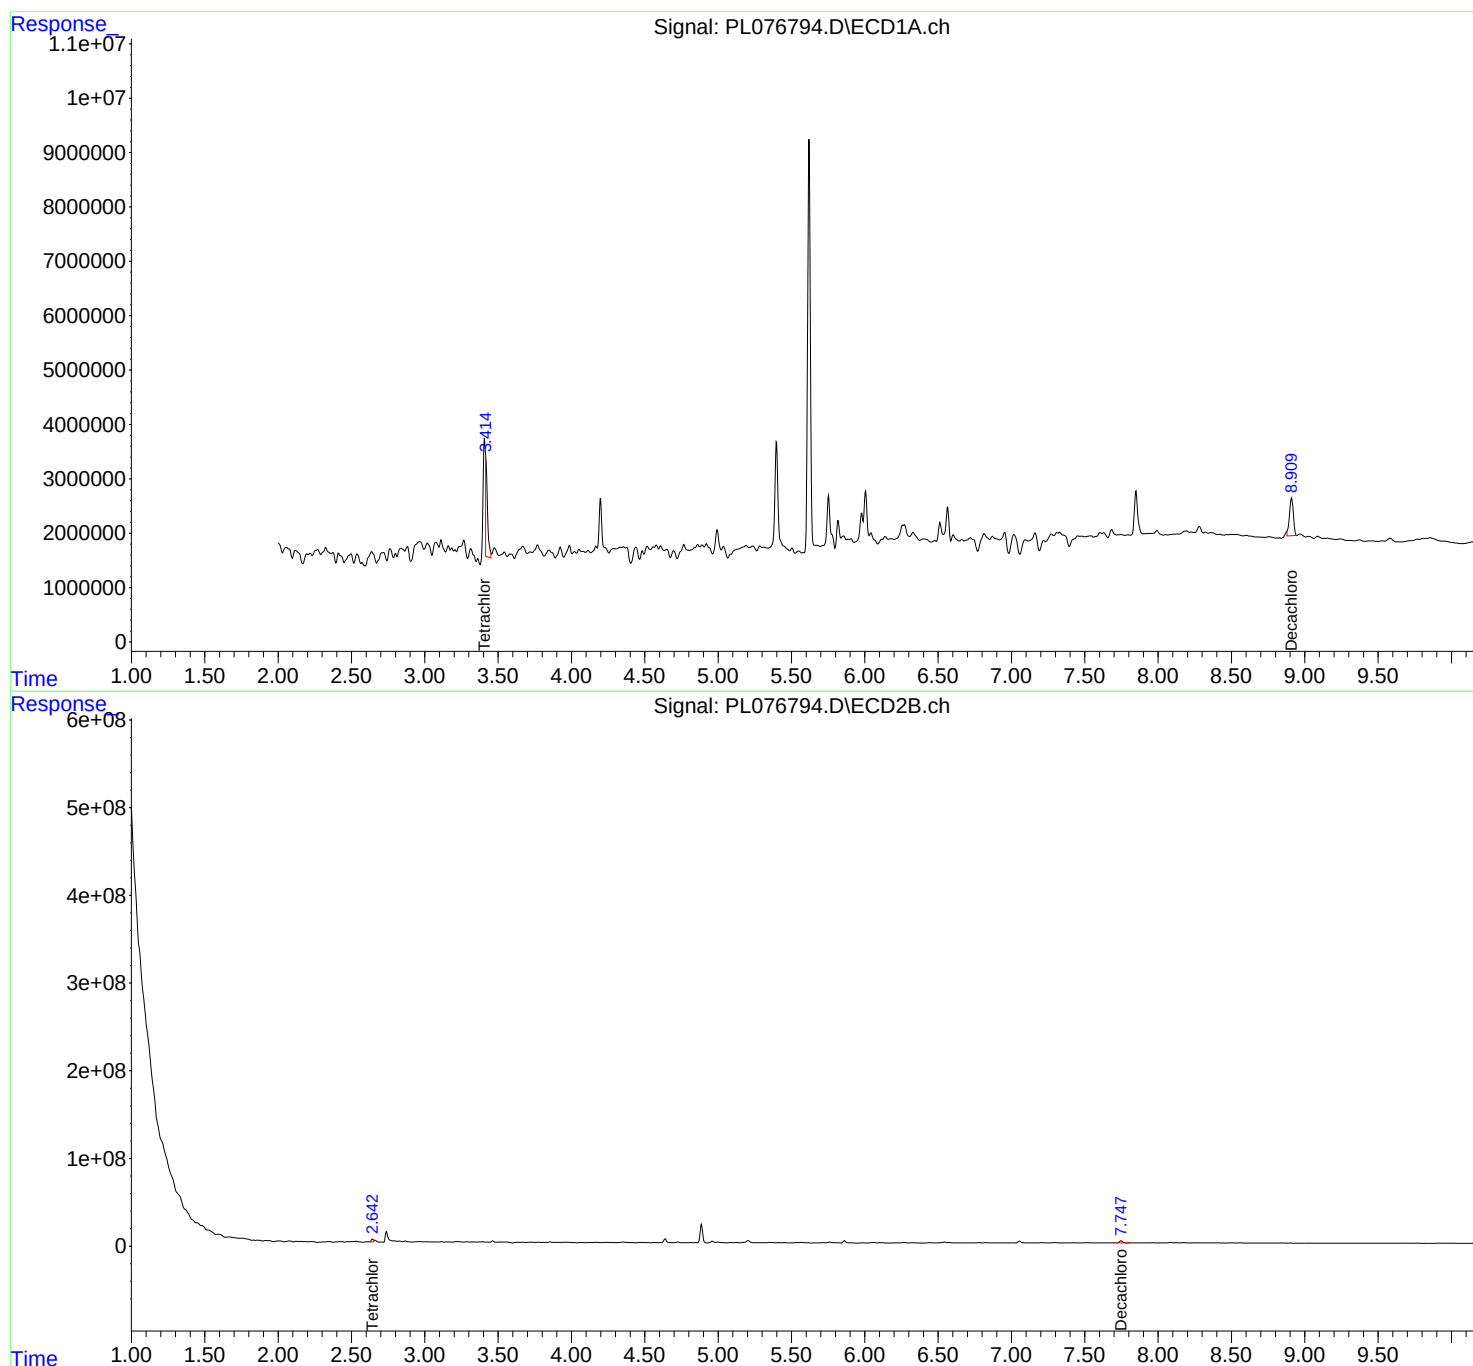

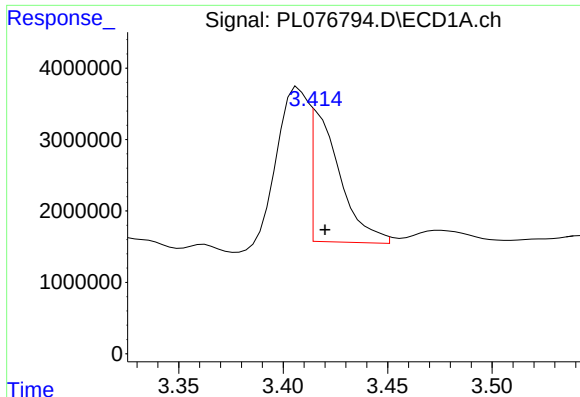


#1 Tetrachloro-m-xylene

R.T.: 3.414 min
Delta R.T.: -0.006 min
Response: 16264484
Conc: 15.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
HMGP-WATER-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/01/2022
Supervised By :mohammad ahmed 08/01/2022

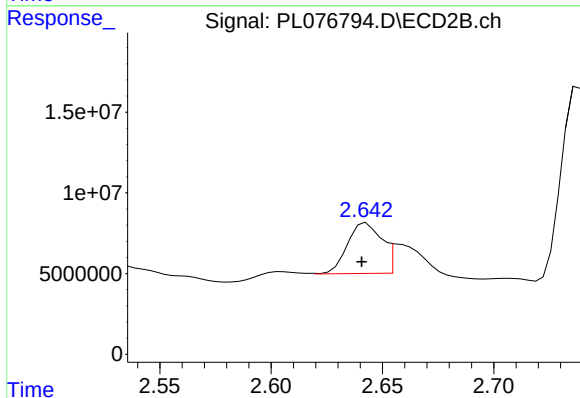


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.000 min
Response: 33218730
Conc: 11.20 ng/ml m

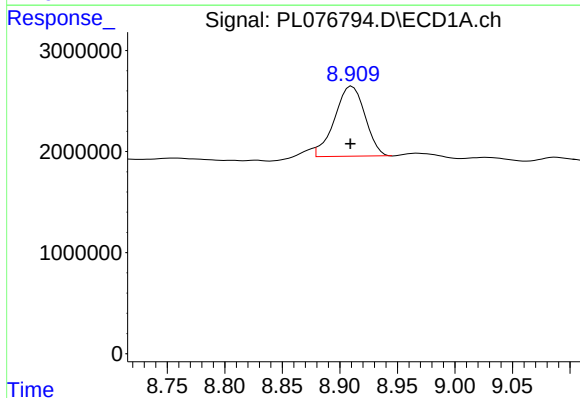

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.000 min
Response: 12701480
Conc: 14.40 ng/ml m

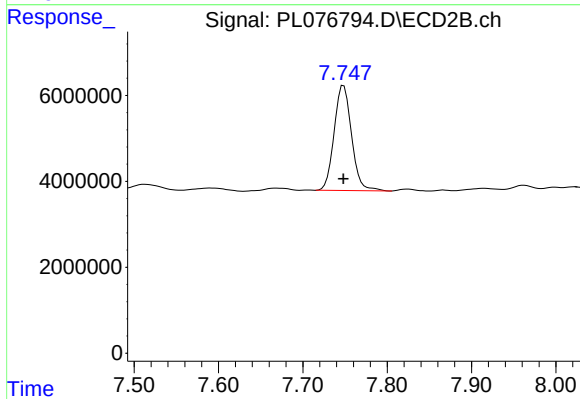

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 35135727
Conc: 13.69 ng/ml